
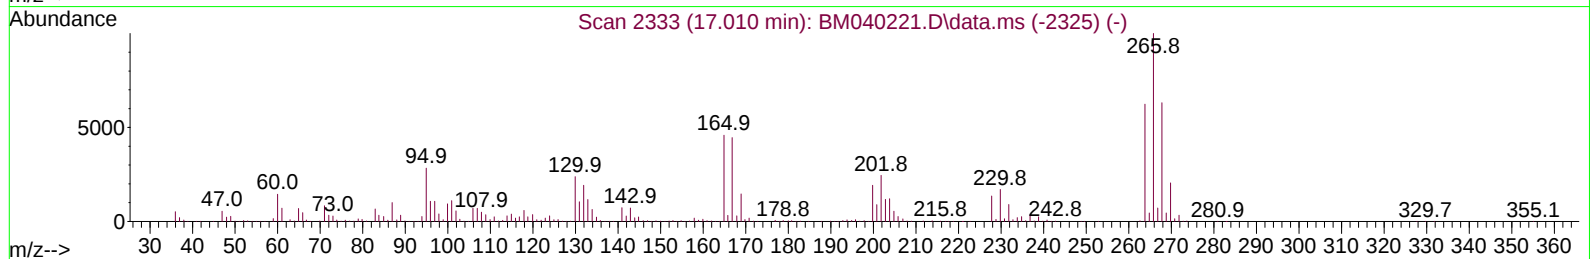
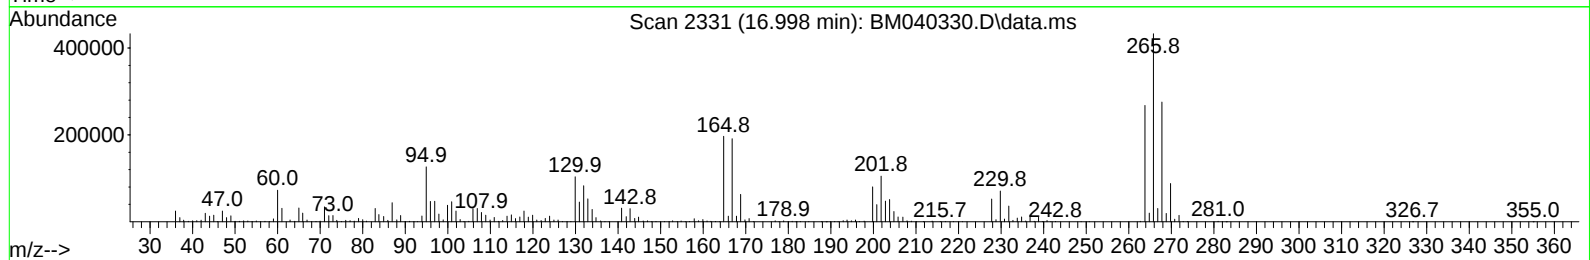


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040330.D
Acq On : 21 Jun 2023 11:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 05:29:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 15:54:19 2023
Response via : Initial Calibration

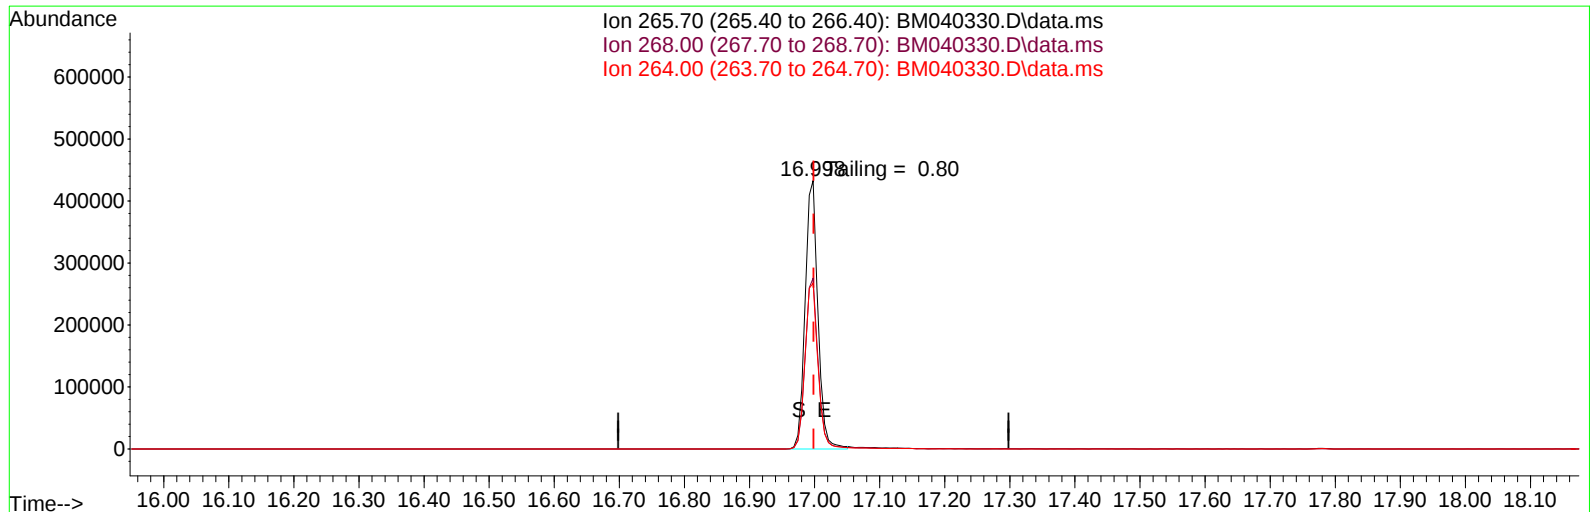

TIC: BM040330.D\data.ms

(70) Pentachlorophenol (C)




16.998min (-0.000) 0.00 ng

response 601786

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.64
264.00	62.30	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040330.D
Acq On : 21 Jun 2023 11:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 05:29:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 15:54:19 2023
Response via : Initial Calibration

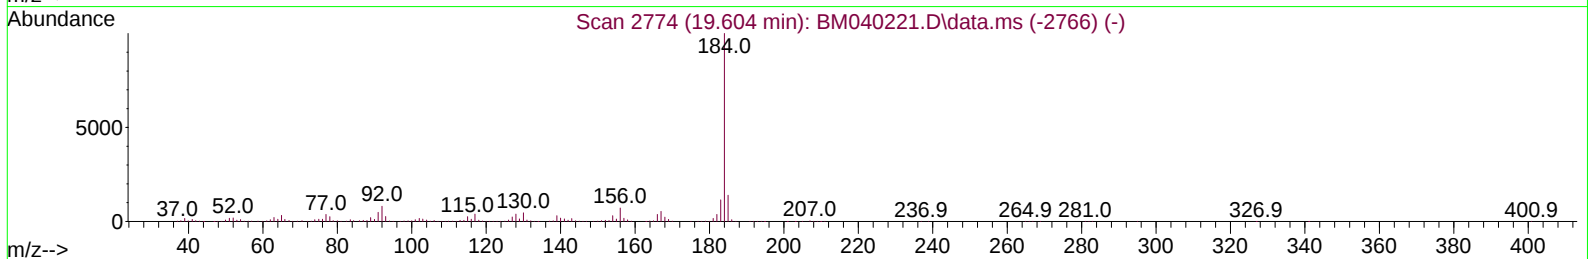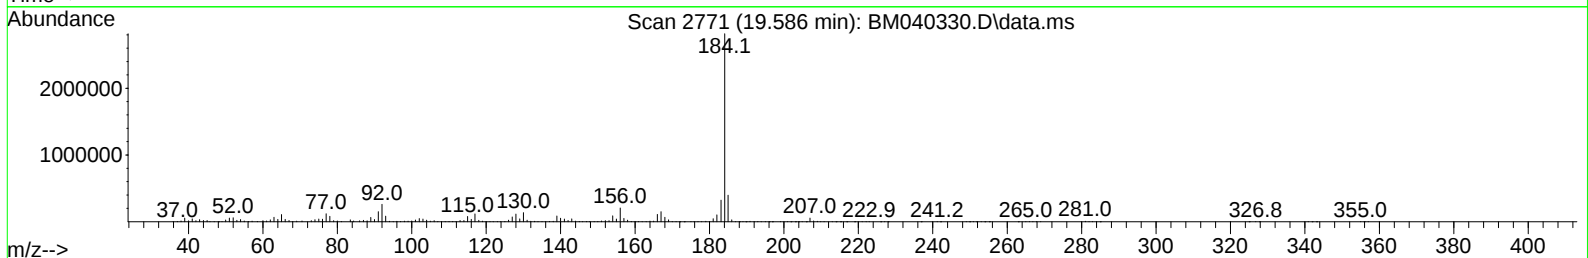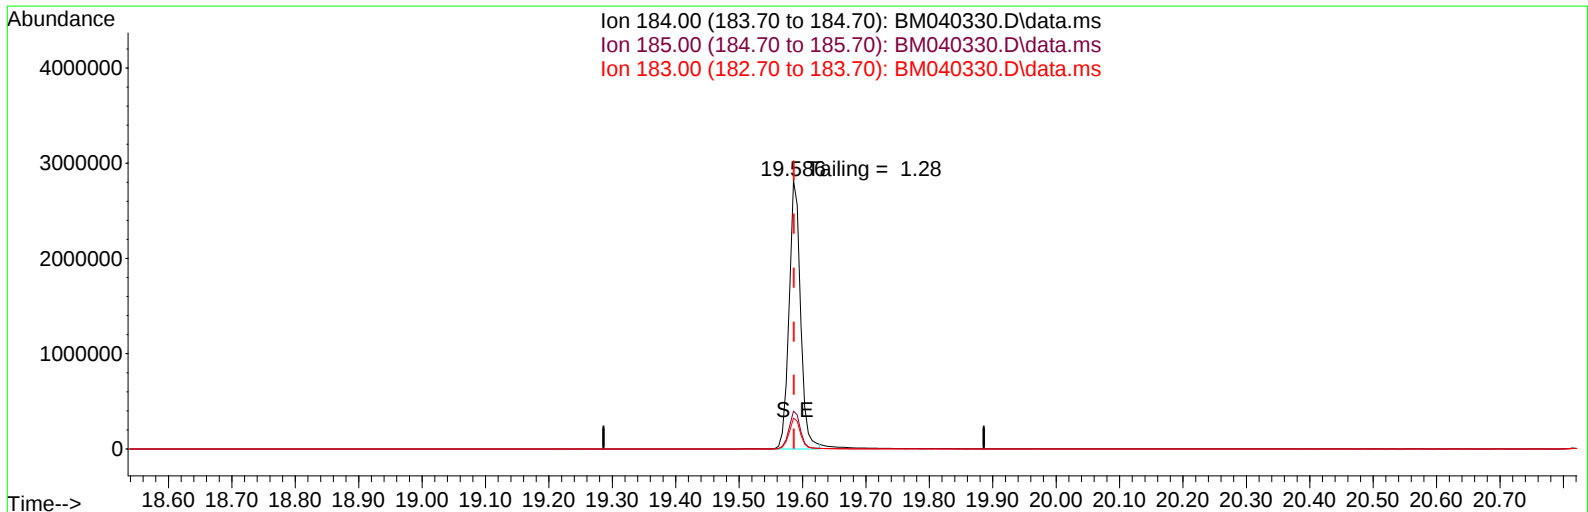

TIC: BM040330.D\data.ms

(77) Benzidine**19.586min (-0.000) 60819.00 ng****response 3658348**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.14
183.00	11.50	11.47
0.00	0.00	0.00