

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
 Data File : BM040334.D
 Acq On : 21 Jun 2023 14:29
 Operator : MA/JU
 Sample : PB153189BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153189BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	293	299	306	rBV	1820911	2414097	21.71%	4.012%
2	5.516	372	379	392	rBV	4508623	6233568	56.05%	10.359%
3	7.128	645	653	665	rBV	4033881	6293442	56.59%	10.458%
4	7.963	788	795	804	rBV	1079947	1686178	15.16%	2.802%
5	9.133	985	994	1008	rBV	3470136	5745265	51.66%	9.547%
6	10.775	1265	1273	1283	rBV	1381710	2307464	20.75%	3.834%
7	13.227	1682	1690	1703	rBV	7979515	11121568	100.00%	18.482%
8	14.598	1917	1923	1936	rBV	1757756	2586546	23.26%	4.298%
9	16.086	2170	2176	2199	rBV	3081041	4249461	38.21%	7.062%
10	17.345	2383	2390	2400	rBV	1756209	2530650	22.75%	4.205%
11	18.239	2539	2542	2552	rBV3	66384	170739	1.54%	0.284%
12	19.962	2829	2835	2844	rBV	9664702	10790476	97.02%	17.931%
13	21.521	3095	3100	3105	rBV	1676747	2098777	18.87%	3.488%
14	23.938	3506	3511	3519	rVB2	1027005	1948439	17.52%	3.238%




Sum of corrected areas: 60176670

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040334.D
Acq On : 21 Jun 2023 14:29
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153189BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

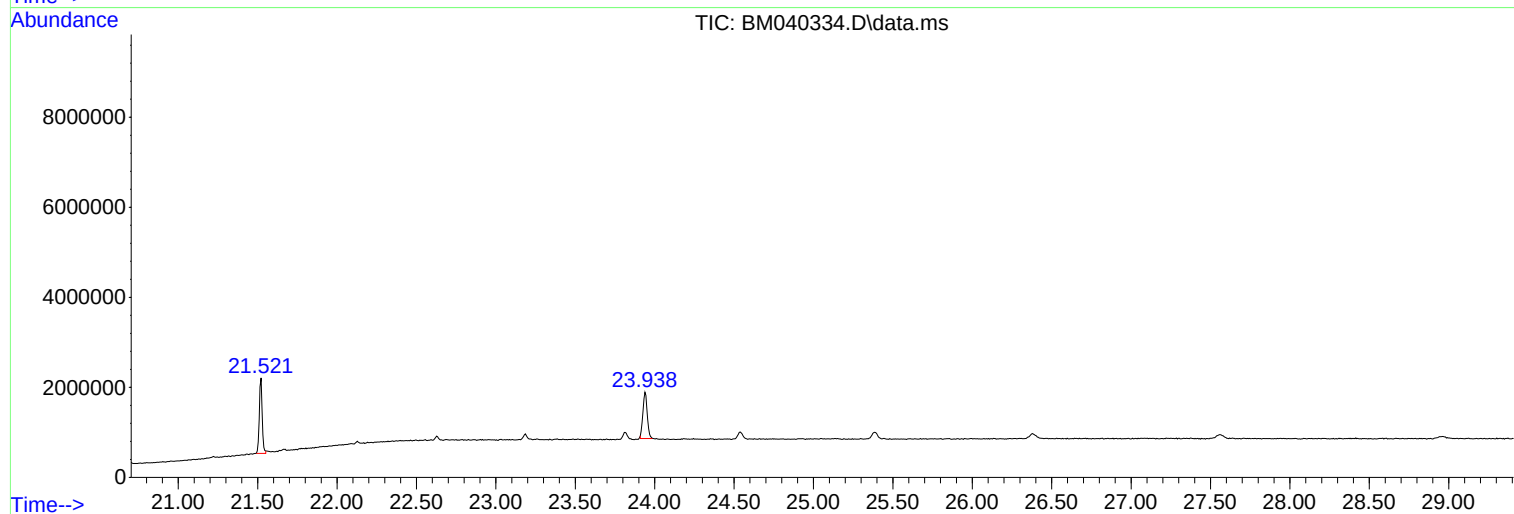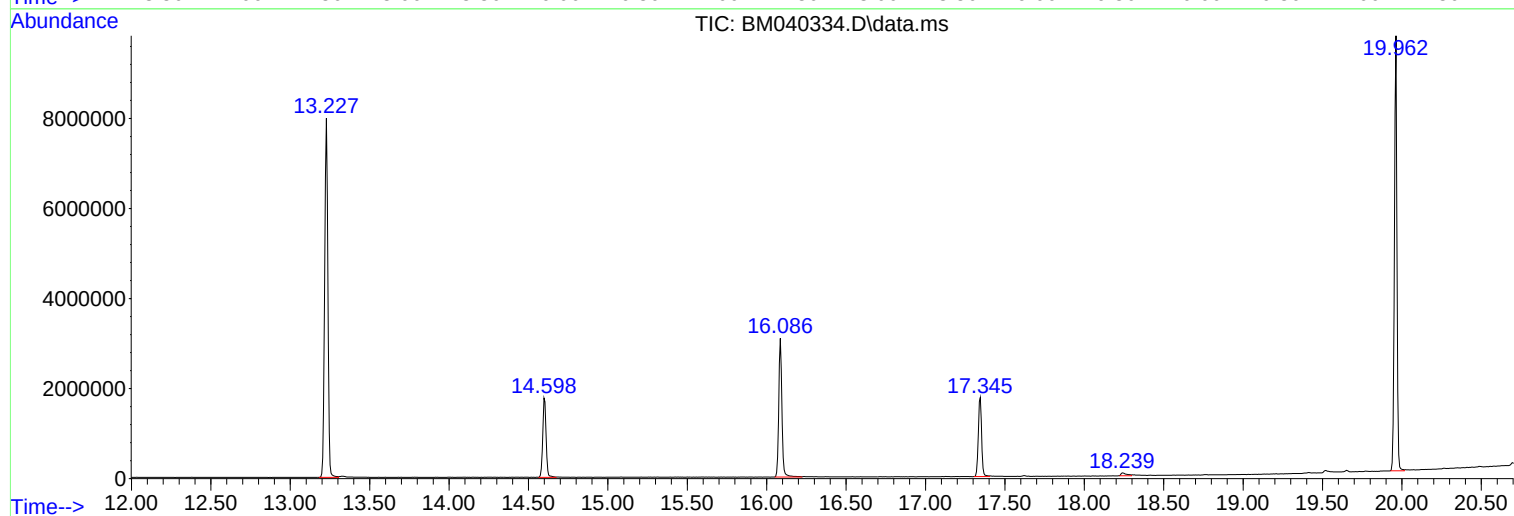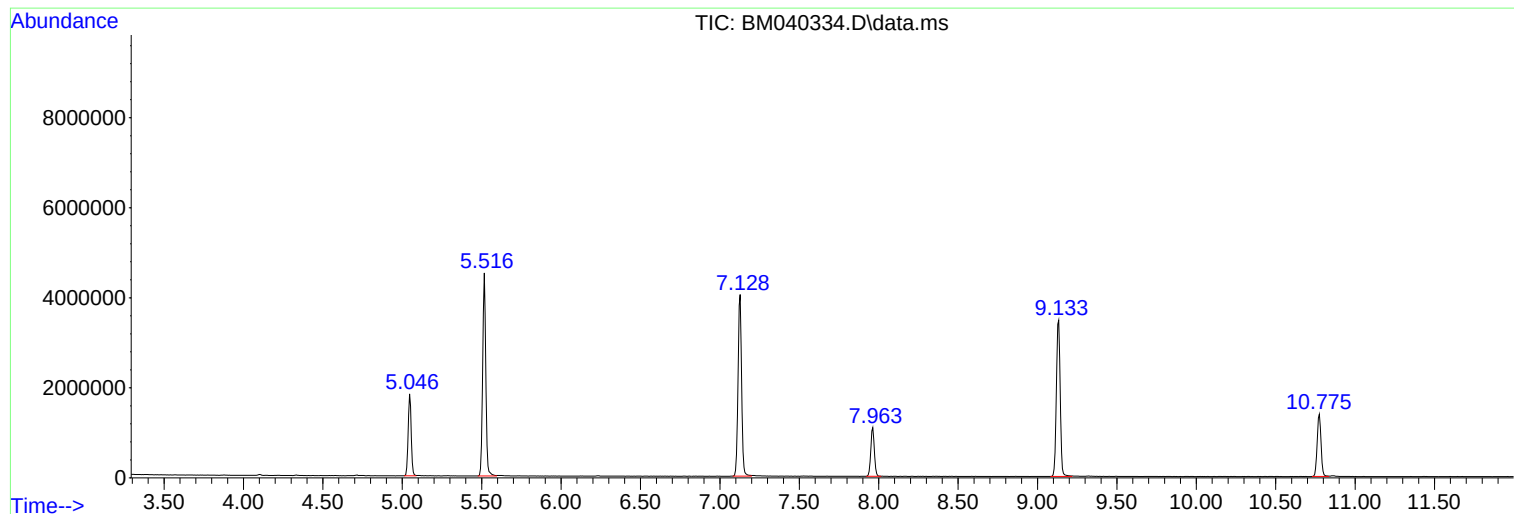

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040334.D
Acq On : 21 Jun 2023 14:29
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB153189BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.046	28.63 ng	2414100	1,4-Dichlorobenzene-d4	7.963	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

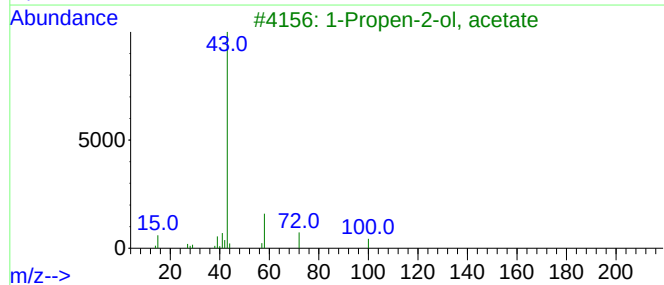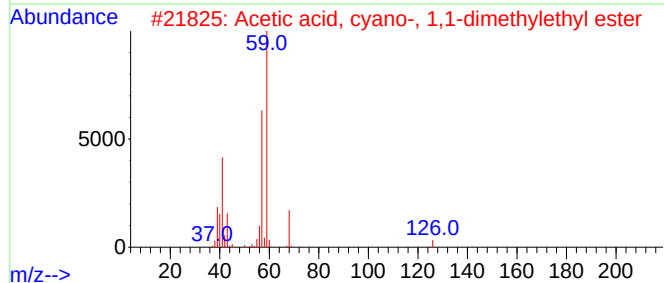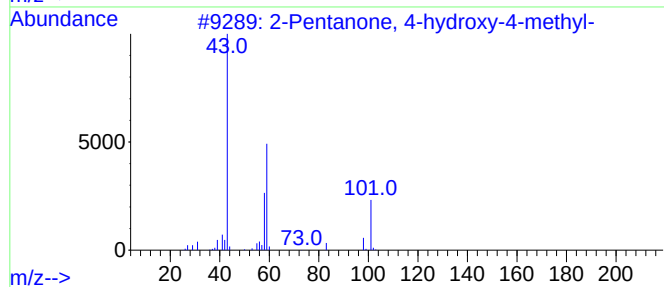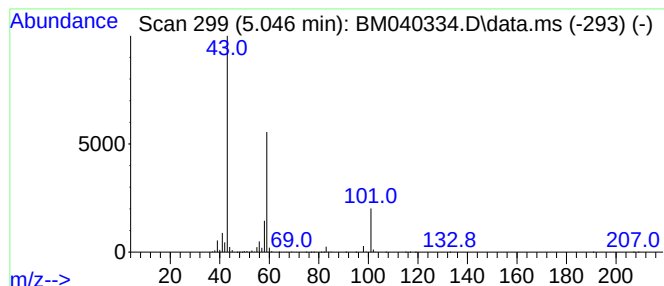

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040334.D
Acq On : 21 Jun 2023 14:29
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153189BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.046	28.6	ng	2414100	1	7.963	1686180	20.0