

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
 Data File : BM040337.D
 Acq On : 21 Jun 2023 16:39
 Operator : MA/JU
 Sample : PB153484BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153484BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	293	299	307	rBV	2225322	2909552	20.87%	3.926%
2	5.516	372	379	393	rBV	5399044	7532825	54.03%	10.163%
3	7.128	642	653	665	rBV	4854083	7709608	55.30%	10.402%
4	7.963	788	795	804	rBV	1243712	1983375	14.23%	2.676%
5	9.134	985	994	1016	rBV	4295623	7000812	50.22%	9.445%
6	10.775	1265	1273	1283	rBV	1695171	2816297	20.20%	3.800%
7	13.227	1683	1690	1704	rBV	9882571	13941276	100.00%	18.810%
8	14.598	1915	1923	1938	rBV	2233087	3298664	23.66%	4.451%
9	16.086	2169	2176	2189	rBV	4050612	5498321	39.44%	7.418%
10	17.345	2383	2390	2400	rBV	2362050	3226618	23.14%	4.353%
11	18.239	2538	2542	2551	rBV3	73870	163015	1.17%	0.220%
12	19.515	2756	2759	2770	rBV3	70492	169054	1.21%	0.228%
13	19.962	2829	2835	2845	rBV	11791719	13387677	96.03%	18.063%
14	21.521	3095	3100	3105	rBV	1866525	2345311	16.82%	3.164%
15	23.944	3506	3512	3519	rVB2	1073016	2135632	15.32%	2.881%




Sum of corrected areas: 74118037

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040337.D
Acq On : 21 Jun 2023 16:39
Operator : MA/JU
Sample : PB153484BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

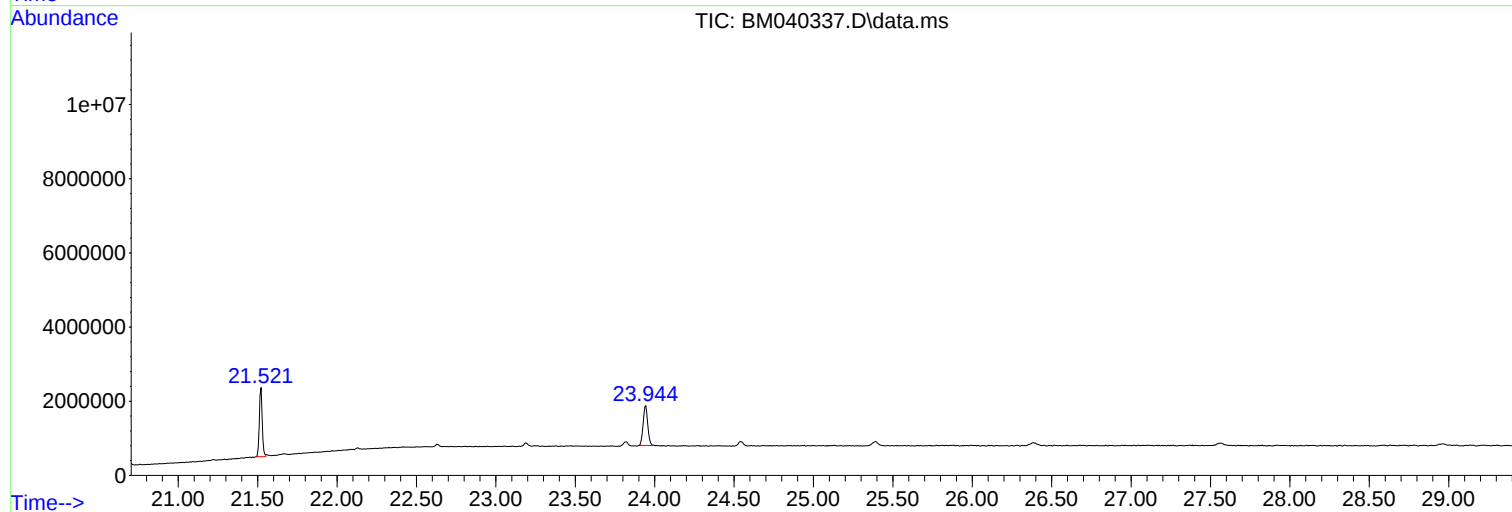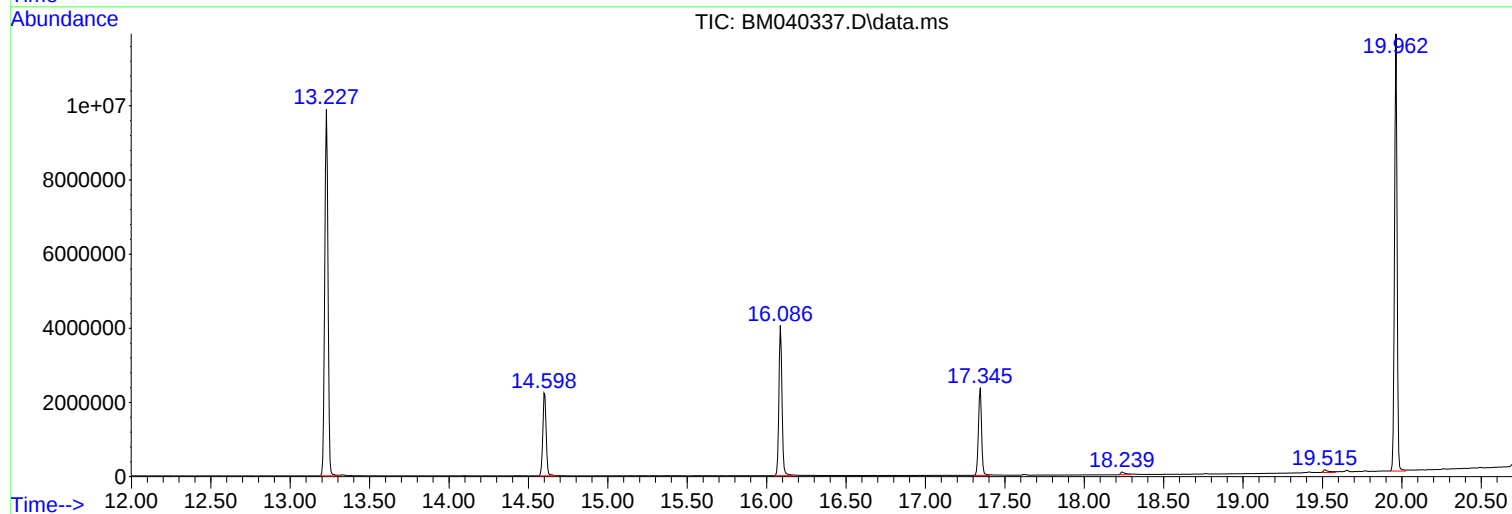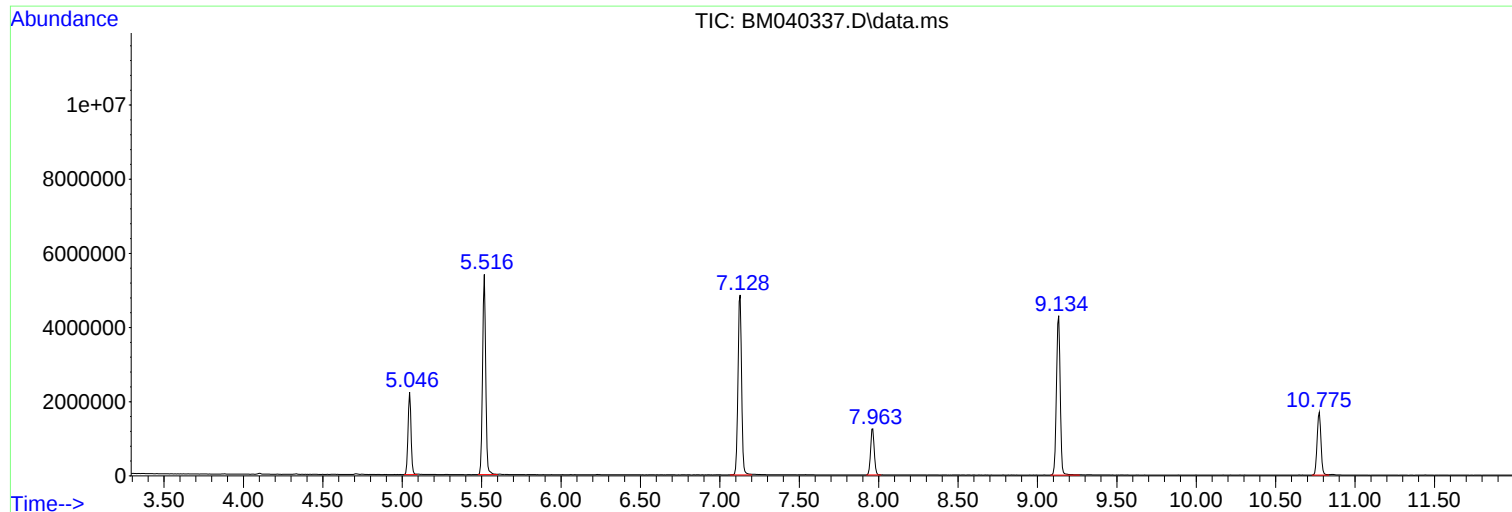

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040337.D
Acq On : 21 Jun 2023 16:39
Operator : MA/JU
Sample : PB153484BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153484BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.
5.046	29.34 ng	2909550	1,4-Dichlorobenzene-d4		7.963

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17	
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10	
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9	
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	

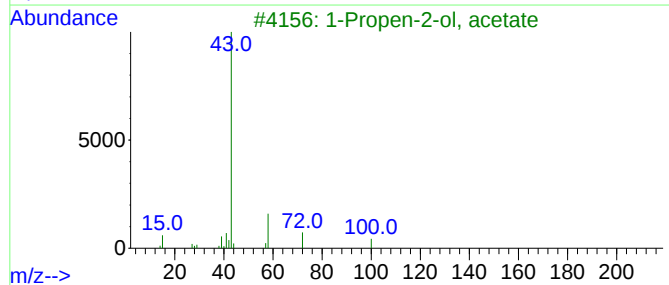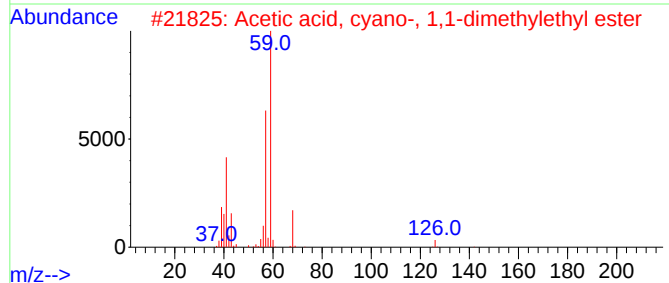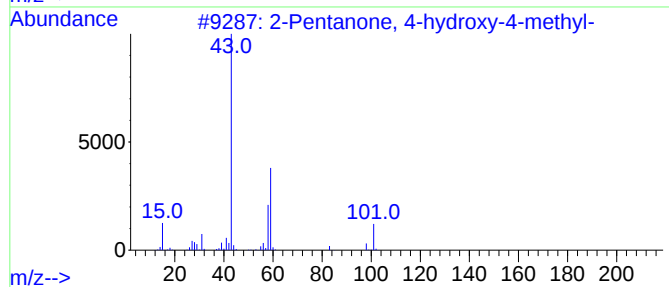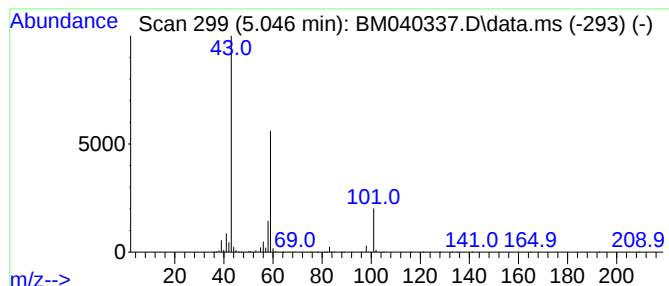

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040337.D
Acq On : 21 Jun 2023 16:39
Operator : MA/JU
Sample : PB153484BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.046	29.3	ng	2909550	1	7.963	1983380	20.0