

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
 Data File : BM040339.D
 Acq On : 21 Jun 2023 17:52
 Operator : MA/JU
 Sample : 03047-09RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-41RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	33	37	47	rVB	88688	112875	1.54%	0.243%
2	4.434	190	195	207	rBV	652761	882125	12.02%	1.902%
3	5.046	293	299	315	rVB	2883345	3815143	51.99%	8.226%
4	5.516	372	379	391	rBV	1172306	1780980	24.27%	3.840%
5	6.134	478	484	493	rBV	313295	455960	6.21%	0.983%
6	7.122	641	652	664	rBV	695784	1137866	15.51%	2.453%
7	7.957	786	794	803	rBV	1214178	1944764	26.50%	4.193%
8	9.128	985	993	1010	rBV	2352933	3839383	52.32%	8.278%
9	10.769	1264	1272	1283	rBV	1582182	2686457	36.61%	5.792%
10	13.228	1680	1690	1704	rBV	5046826	7338120	100.00%	15.822%
11	14.598	1917	1923	1936	rBV	2042648	2950309	40.21%	6.361%
12	15.957	2145	2154	2166	rBV	1071917	1501192	20.46%	3.237%
13	16.086	2169	2176	2192	rBV	1799706	2587687	35.26%	5.579%
14	16.516	2245	2249	2254	rVB	72600	93769	1.28%	0.202%
15	17.345	2383	2390	2401	rBV	1998259	2871768	39.13%	6.192%
16	18.233	2536	2541	2550	rBV	286899	568754	7.75%	1.226%
17	18.304	2550	2553	2560	rVB	52773	99924	1.36%	0.215%
18	19.509	2754	2758	2771	rBV3	94594	222195	3.03%	0.479%
19	19.956	2829	2834	2842	rBV	4953081	6133541	83.58%	13.225%
20	21.221	3045	3049	3055	rBV	398327	521689	7.11%	1.125%
21	21.521	3095	3100	3110	rBV	1706633	2315647	31.56%	4.993%
22	23.939	3505	3511	3522	rVB	1312901	2519236	34.33%	5.432%


Sum of corrected areas: 46379384

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040339.D
Acq On : 21 Jun 2023 17:52
Operator : MA/JU
Sample : 03047-09RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-41RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

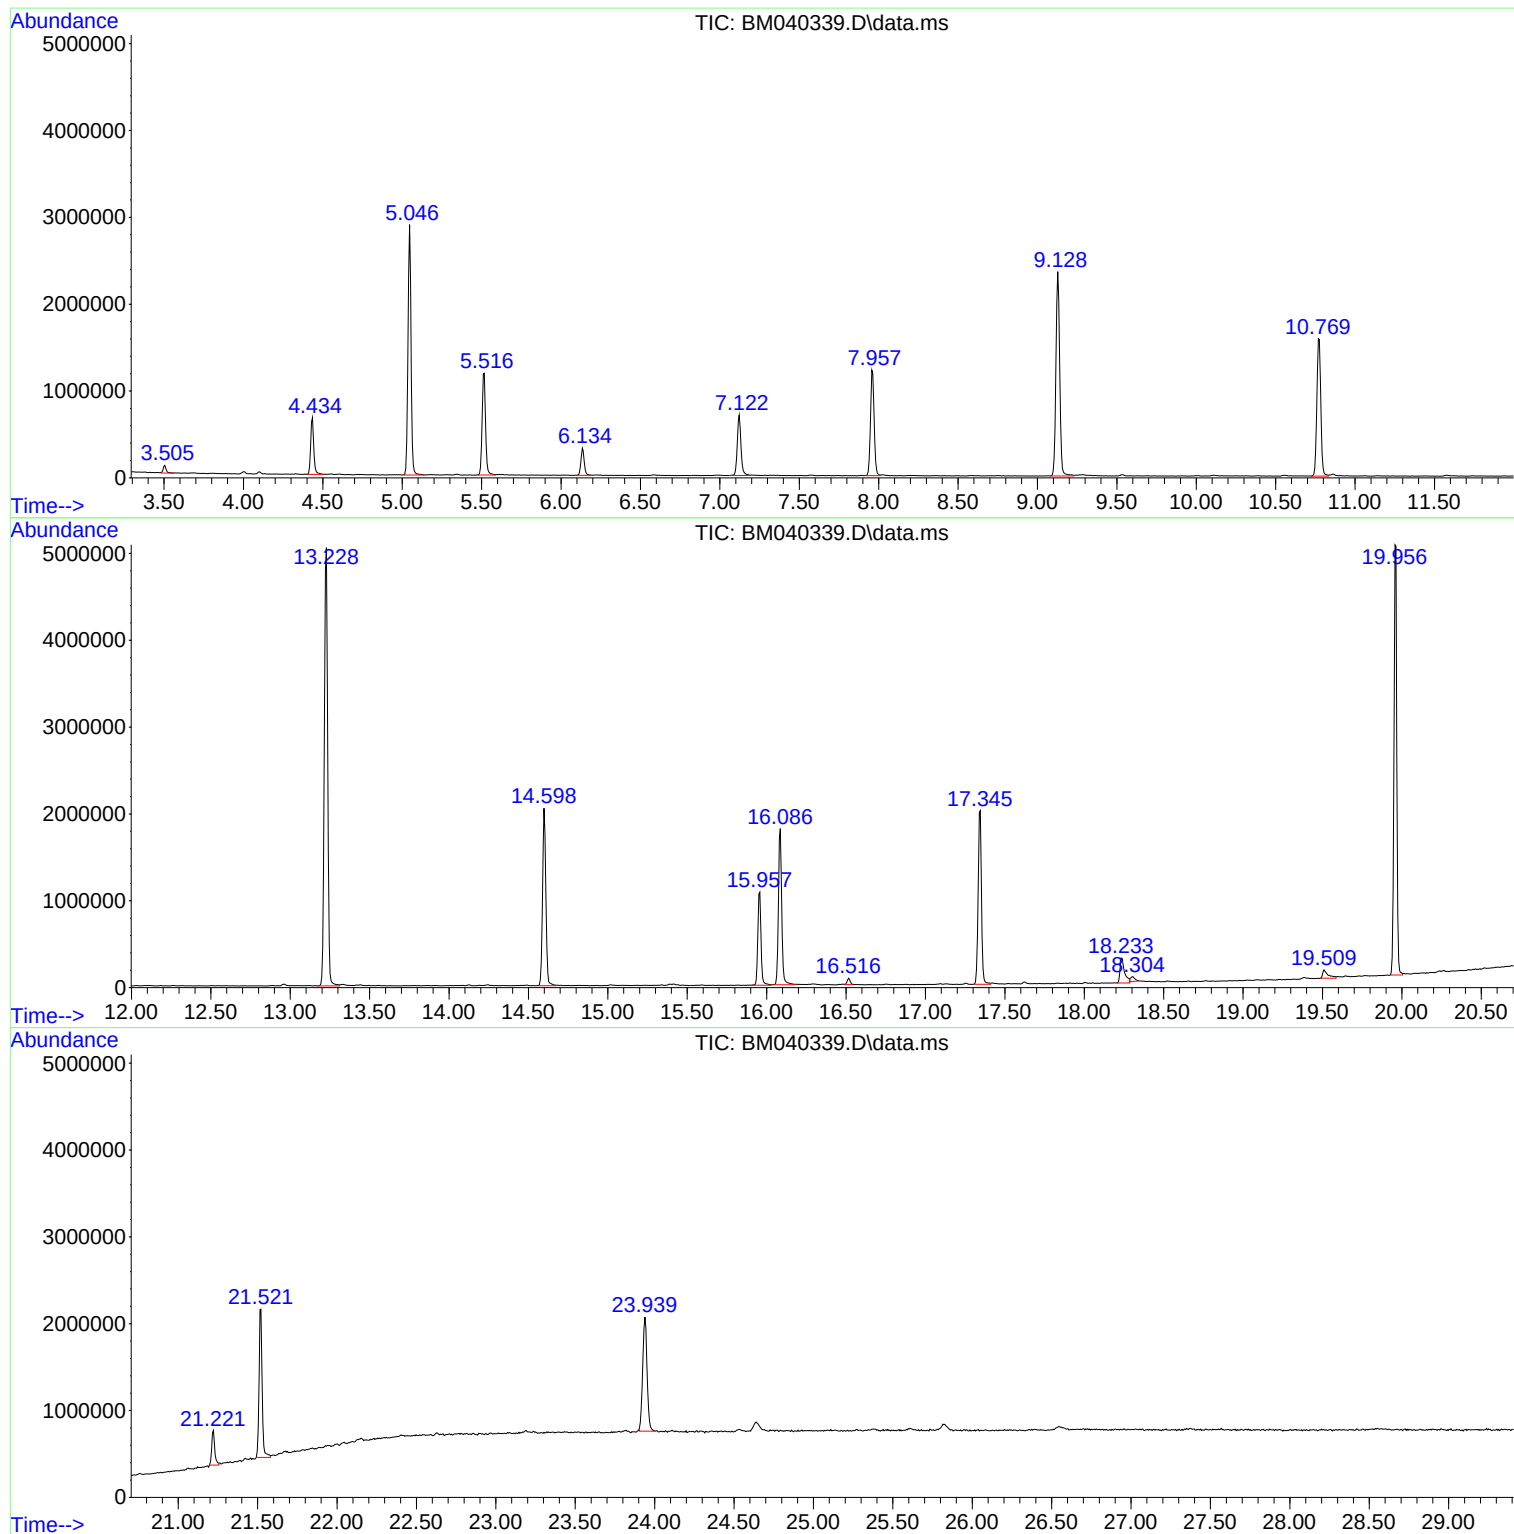

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040339.D
Acq On : 21 Jun 2023 17:52
Operator : MA/JU
Sample : 03047-09RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-41RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040339.D
Acq On : 21 Jun 2023 17:52
Operator : MA/JU
Sample : 03047-09RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-41RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------