

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062123\  
 Data File : BM040342.D  
 Acq On : 21 Jun 2023 19:42  
 Operator : MA/JU  
 Sample : 03069-11RE  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 TWP08RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM061323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040342.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.434       | 189           | 195         | 208          | rBV      | 1296681        | 1757020       | 10.59%          | 2.167%        |
| 2         | 5.046       | 293           | 299         | 316          | rBV      | 4853196        | 6759845       | 40.73%          | 8.337%        |
| 3         | 5.516       | 372           | 379         | 392          | rBV      | 2832741        | 4047271       | 24.39%          | 4.991%        |
| 4         | 6.134       | 478           | 484         | 494          | rBV      | 612166         | 876574        | 5.28%           | 1.081%        |
| 5         | 7.122       | 641           | 652         | 665          | rBV      | 1744147        | 2719869       | 16.39%          | 3.354%        |
| 6         | 7.957       | 787           | 794         | 799          | rBV      | 1245640        | 1945106       | 11.72%          | 2.399%        |
| 7         | 8.010       | 799           | 803         | 813          | rVB      | 569465         | 907108        | 5.47%           | 1.119%        |
| 8         | 9.134       | 985           | 994         | 1006         | rBV      | 4610670        | 7648471       | 46.09%          | 9.432%        |
| 9         | 10.769      | 1264          | 1272        | 1283         | rBV      | 1597931        | 2718318       | 16.38%          | 3.352%        |
| 10        | 13.228      | 1682          | 1690        | 1704         | rBV      | 11492307       | 15673385      | 94.45%          | 19.329%       |
| 11        | 13.445      | 1721          | 1727        | 1736         | rVB      | 127794         | 187035        | 1.13%           | 0.231%        |
| 12        | 14.598      | 1916          | 1923        | 1936         | rBV      | 2234163        | 3163816       | 19.06%          | 3.902%        |
| 13        | 15.951      | 2148          | 2153        | 2168         | rVB      | 192077         | 280335        | 1.69%           | 0.346%        |
| 14        | 16.086      | 2168          | 2176        | 2194         | rBV      | 5021096        | 6918065       | 41.69%          | 8.532%        |
| 15        | 17.339      | 2383          | 2389        | 2397         | rBV      | 2407683        | 3358709       | 20.24%          | 4.142%        |
| 16        | 18.233      | 2536          | 2541        | 2550         | rBV      | 187534         | 342483        | 2.06%           | 0.422%        |
| 17        | 19.962      | 2829          | 2835        | 2846         | rBV      | 14459034       | 16595231      | 100.00%         | 20.466%       |
| 18        | 21.515      | 3095          | 3099        | 3106         | rBV      | 2135846        | 2680642       | 16.15%          | 3.306%        |
| 19        | 23.939      | 3505          | 3511        | 3520         | rVB      | 1284959        | 2507520       | 15.11%          | 3.092%        |


Sum of corrected areas: 81086803

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062123\  
Data File : BM040342.D  
Acq On : 21 Jun 2023 19:42  
Operator : MA/JU  
Sample : 03069-11RE  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TWP08RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM061323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

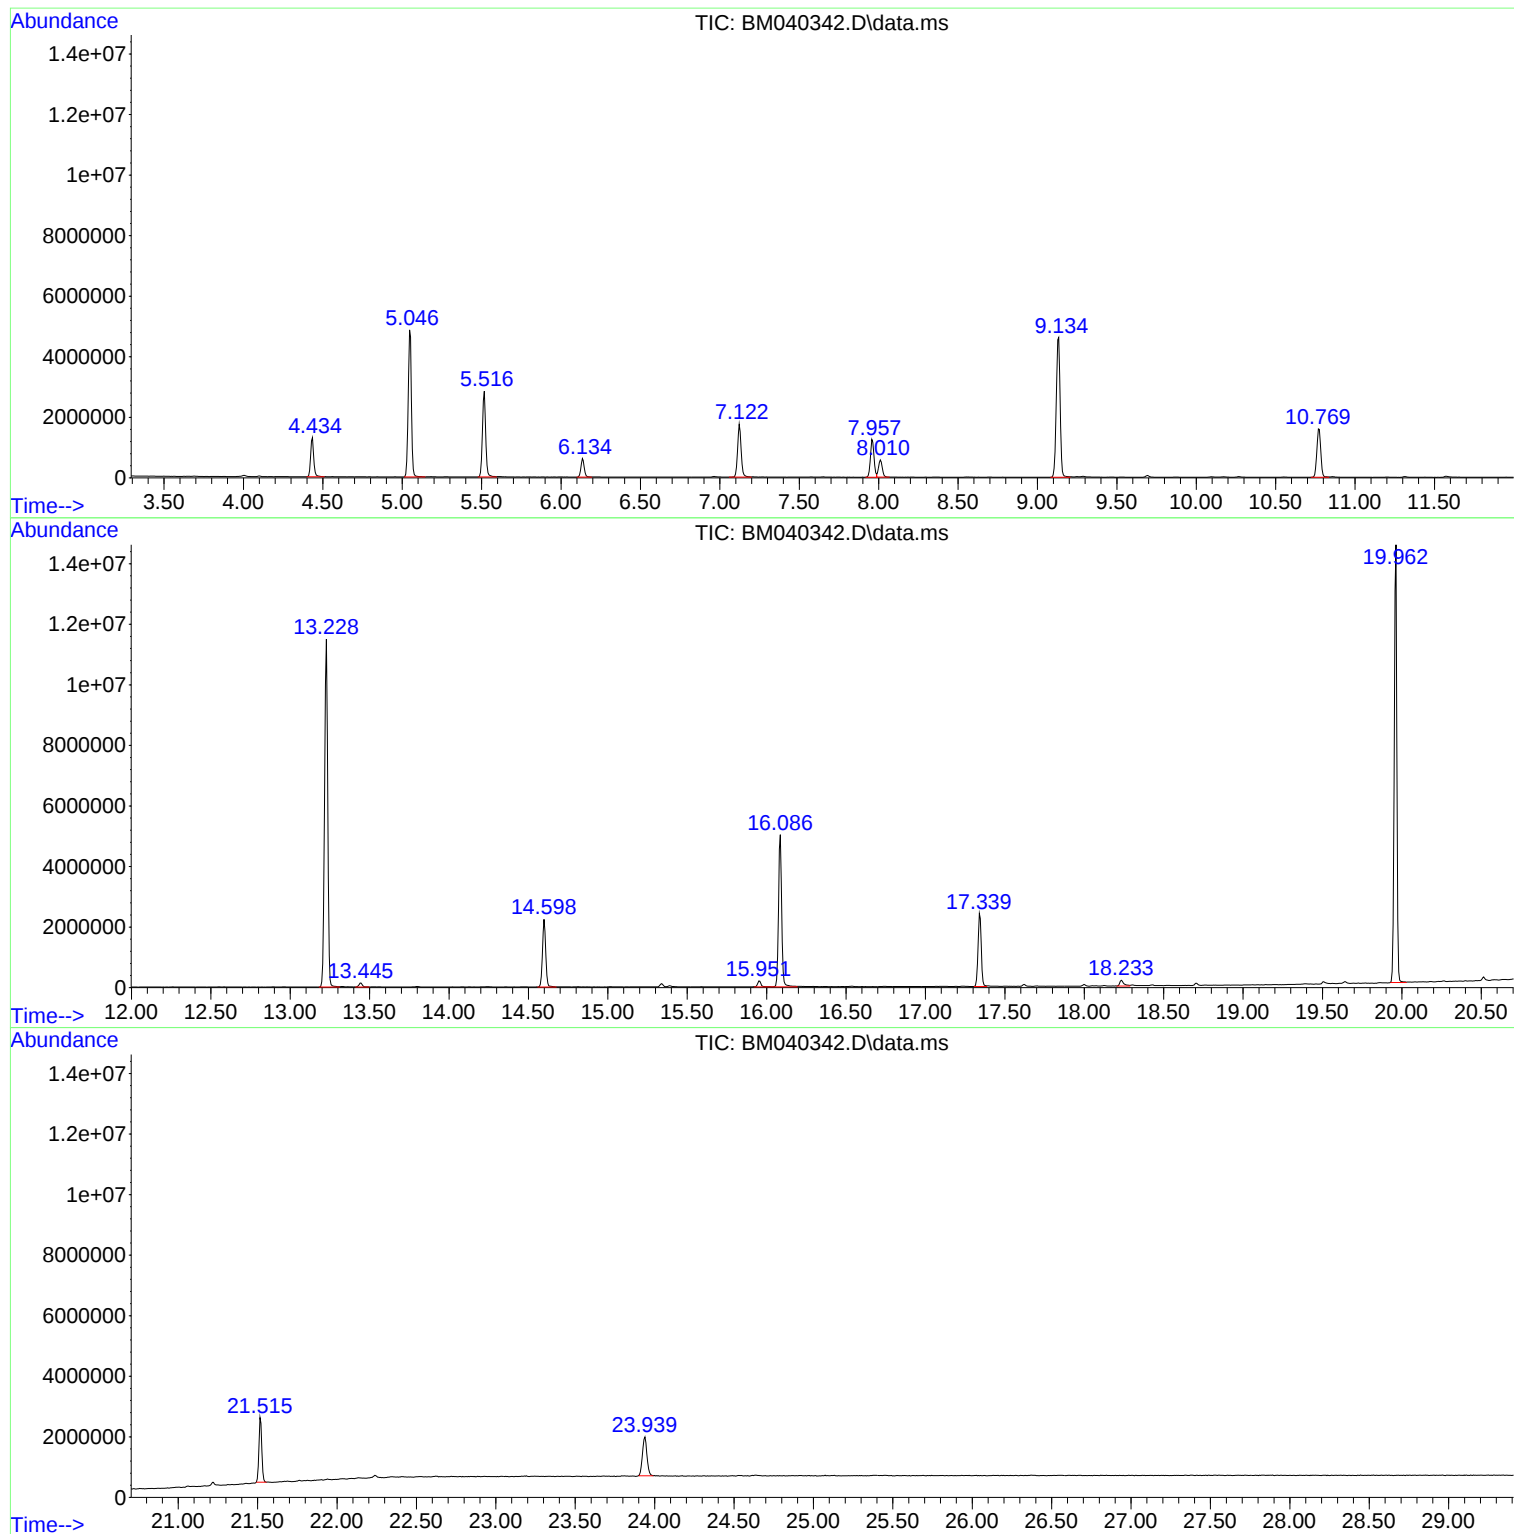

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062123\  
Data File : BM040342.D  
Acq On : 21 Jun 2023 19:42  
Operator : MA/JU  
Sample : 03069-11RE  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TWP08RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM061323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM062123\  
Data File : BM040342.D  
Acq On : 21 Jun 2023 19:42  
Operator : MA/JU  
Sample : 03069-11RE  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
TWP08RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM061323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|