

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040344.D
Acq On : 21 Jun 2023 20:56
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153189BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	293	299	307	rBV	1995235	2633560	21.85%	3.995%
2	5.516	372	379	393	rBV	4746788	6690071	55.50%	10.148%
3	7.122	644	652	667	rBV	4221568	6738175	55.90%	10.221%
4	7.957	788	794	804	rBV	1245761	1967544	16.32%	2.984%
5	9.128	985	993	1015	rBV	3727572	6220807	51.61%	9.436%
6	10.769	1263	1272	1283	rBV	1586476	2687519	22.30%	4.076%
7	13.227	1682	1690	1704	rBV	8652476	12054134	100.00%	18.284%
8	14.598	1915	1923	1940	rBV	2081184	3004420	24.92%	4.557%
9	16.086	2169	2176	2193	rBV	3263722	4548846	37.74%	6.900%
10	17.339	2383	2389	2403	rBV	1993275	2902217	24.08%	4.402%
11	19.962	2829	2835	2851	rBV	10465176	11968102	99.29%	18.153%
12	21.515	3095	3099	3108	rBV	1690307	2243813	18.61%	3.403%
13	23.939	3505	3511	3522	rVB2	1193620	2268533	18.82%	3.441%




Sum of corrected areas: 65927741

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040344.D
Acq On : 21 Jun 2023 20:56
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153189BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

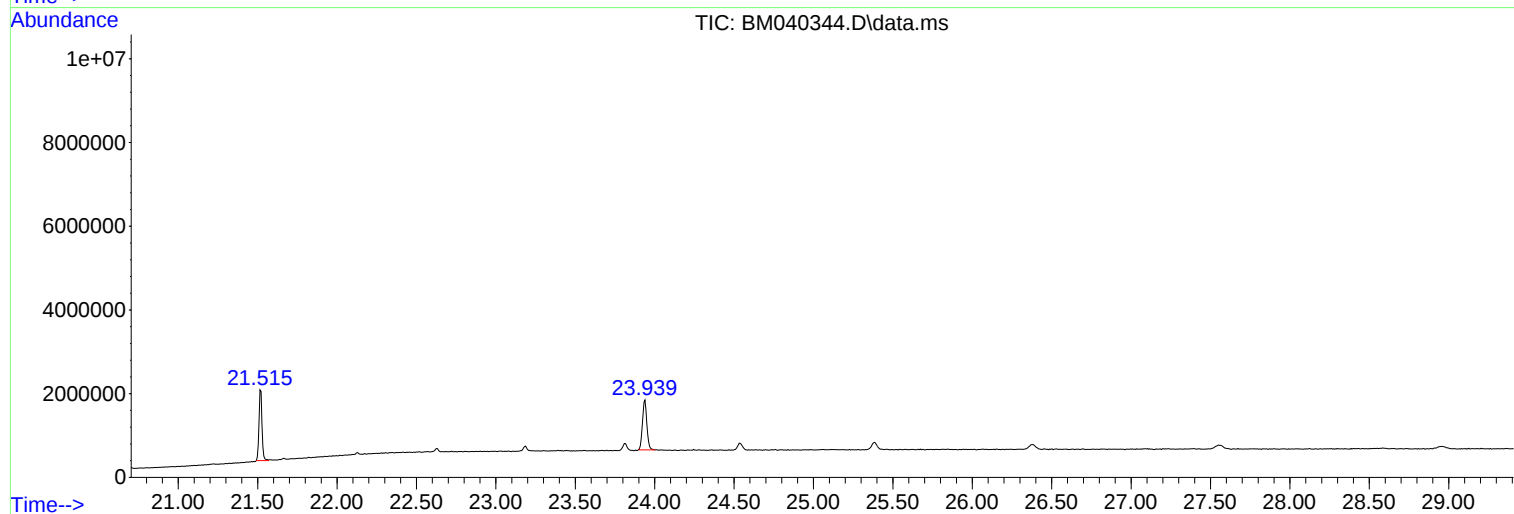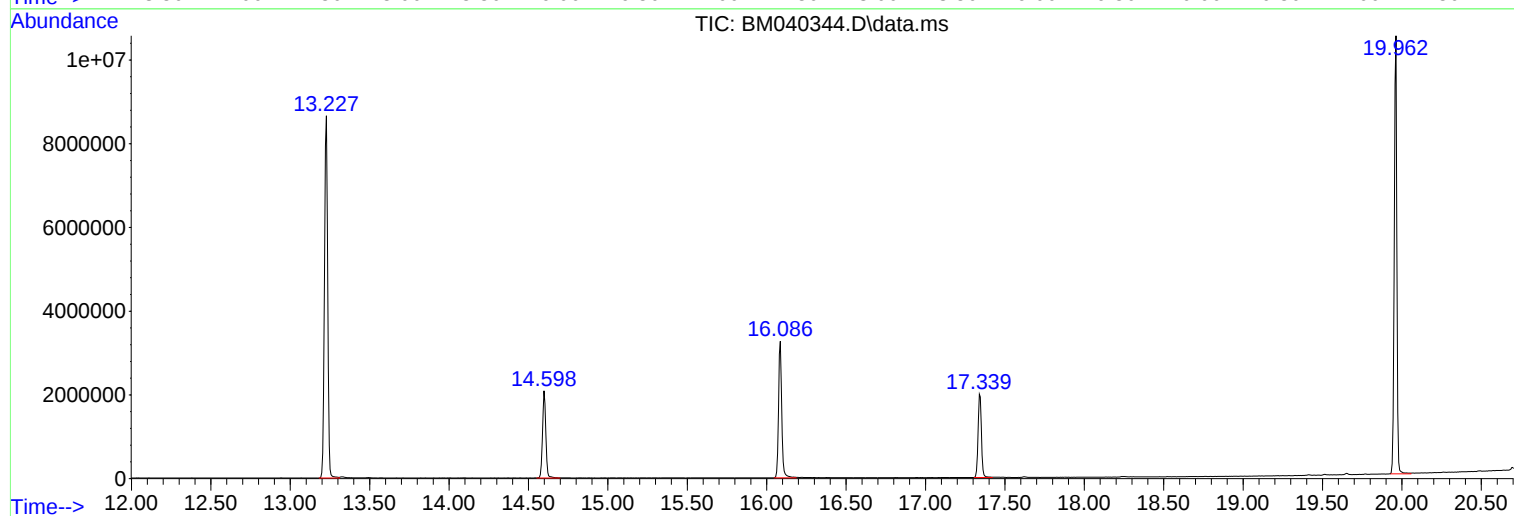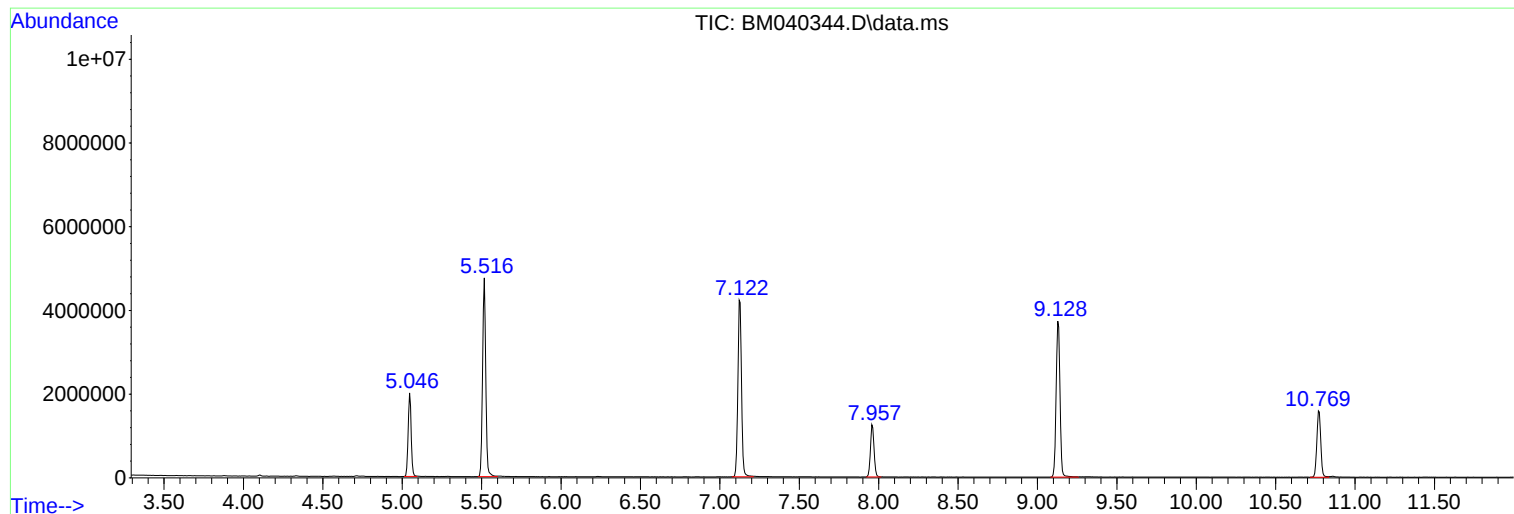

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040344.D
Acq On : 21 Jun 2023 20:56
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153189BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.046	26.77 ng	2633560	1,4-Dichlorobenzene-d4	7.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

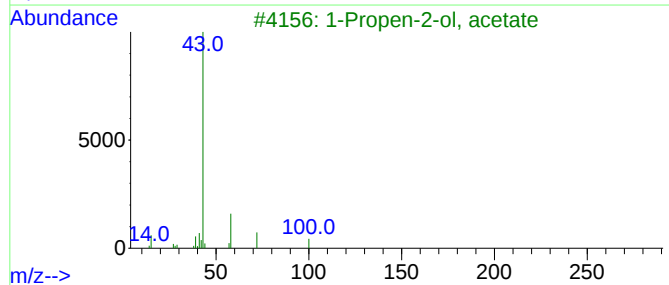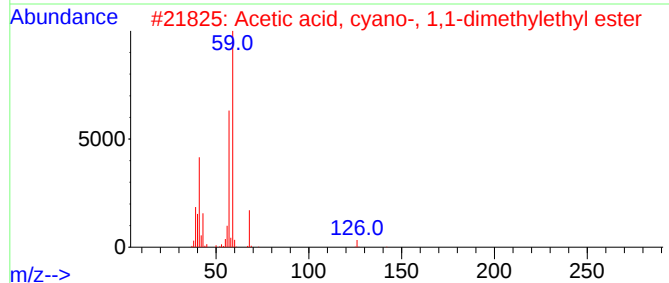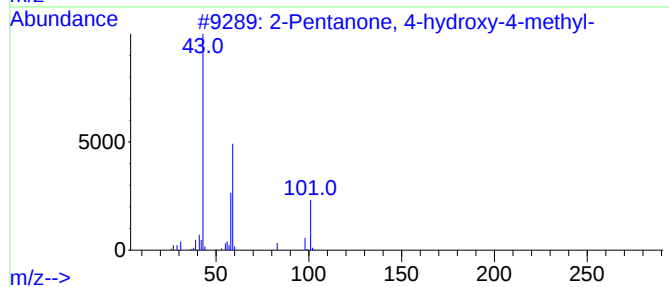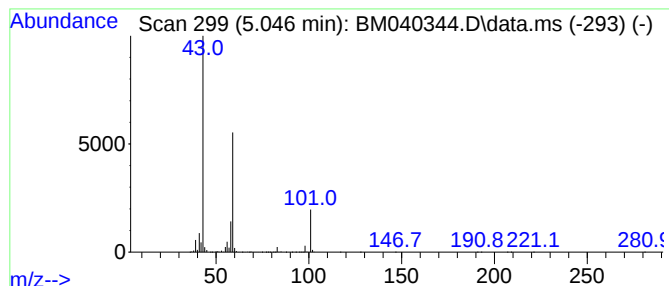

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040344.D
Acq On : 21 Jun 2023 20:56
Operator : MA/JU
Sample : PB153189BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153189BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.046	26.8	ng	2633560	1	7.957	1967540	20.0