


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
 Data File : BM040330.D
 Acq On : 21 Jun 2023 11:20
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 21 15:54:19 2023

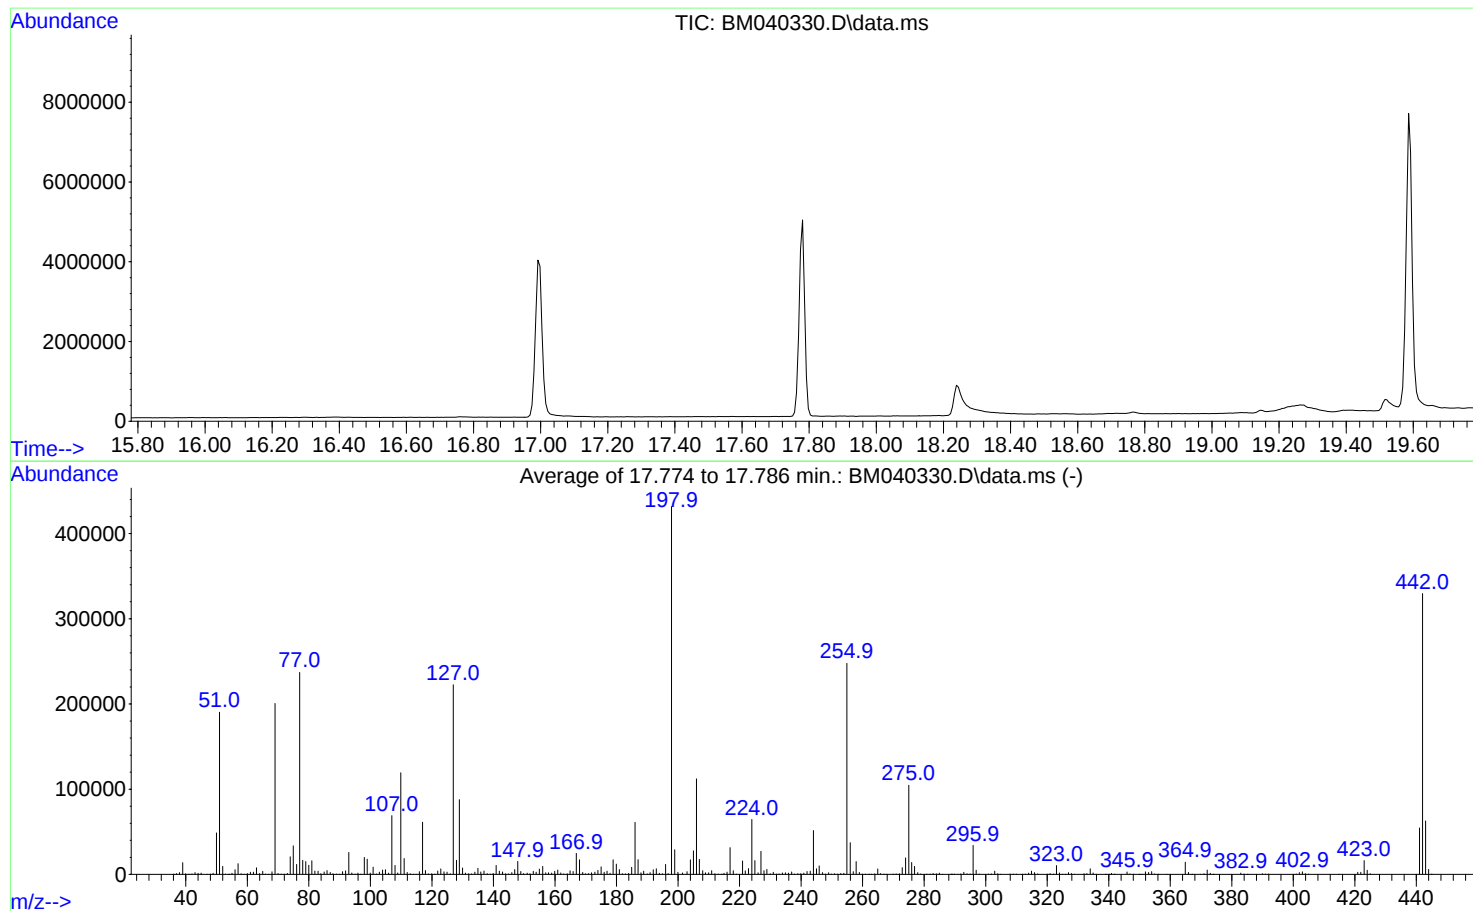




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	190169	PASS
68	69	0.00	2	1.5	3106	PASS
69	198	0.00	100	46.5	200662	PASS
70	69	0.00	2	0.6	1137	PASS
127	198	10	80	51.6	222604	PASS
197	198	0.00	2	0.2	1015	PASS
198	198	100	100	100.0	431765	PASS
199	198	5	9	6.7	28859	PASS
275	198	10	60	24.2	104549	PASS
365	198	1	100	3.3	14378	PASS
441	198	0.01	100	12.6	54523	PASS
442	442	50	100	100.0	329536	PASS
443	442	15	24	19.0	62677	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040330.D
Acq On : 21 Jun 2023 11:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 22 05:29:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 15:54:19 2023
Response via : Initial Calibration

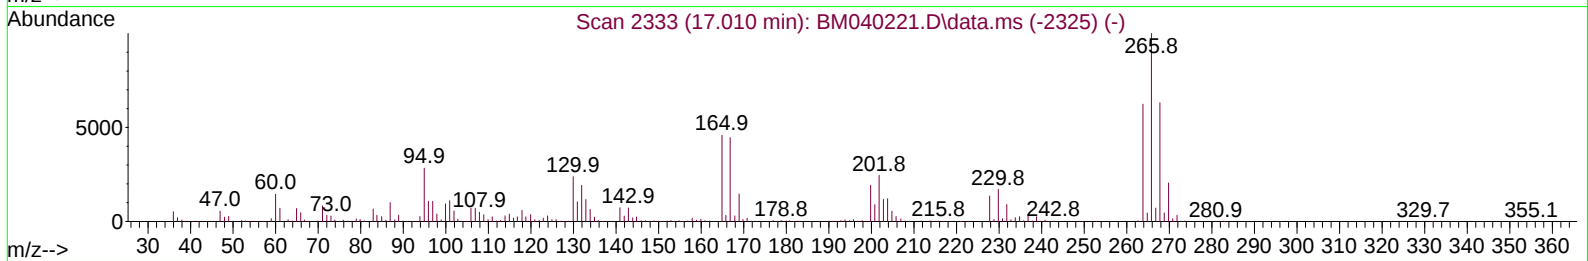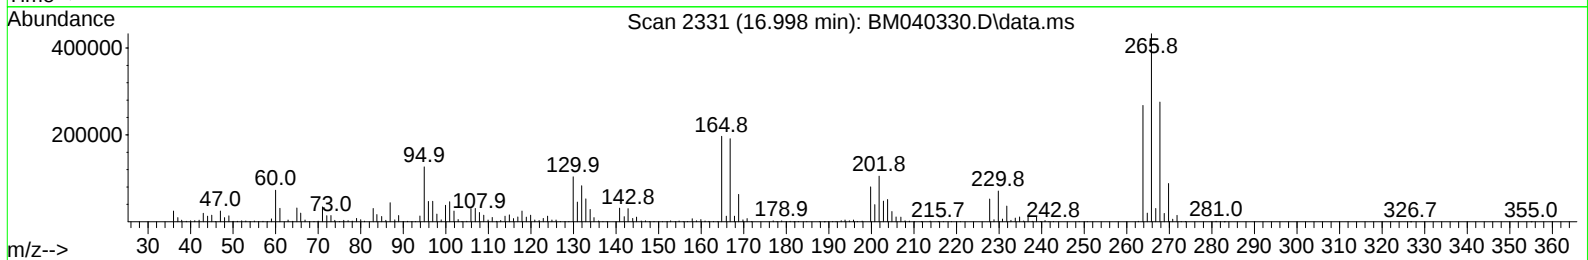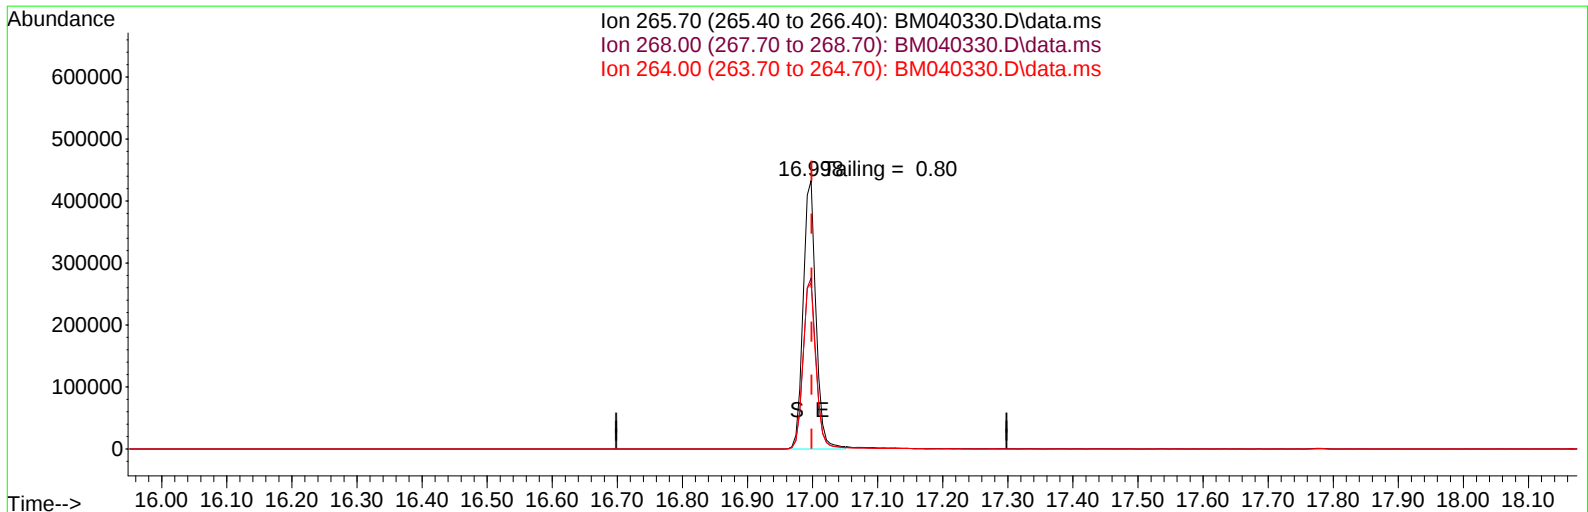

TIC: BM040330.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 0.00 ng




response 601786

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.64
264.00	62.30	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062123\
Data File : BM040330.D
Acq On : 21 Jun 2023 11:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 22 05:29:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 15:54:19 2023
Response via : Initial Calibration

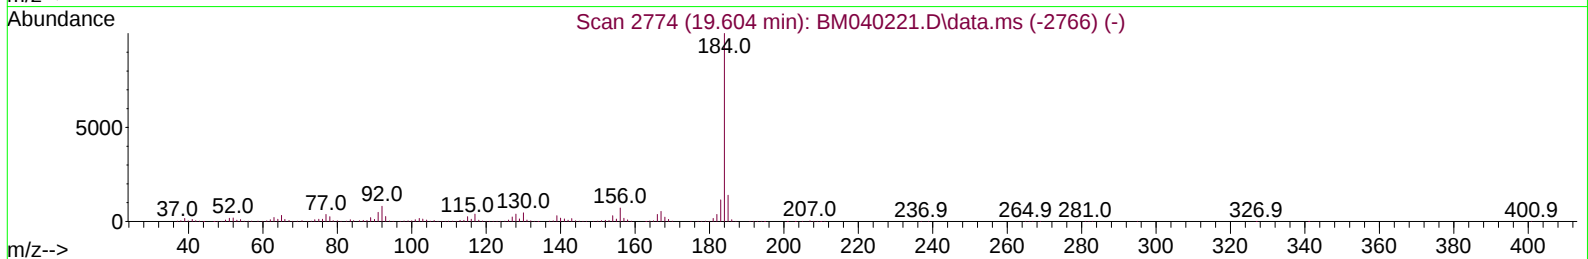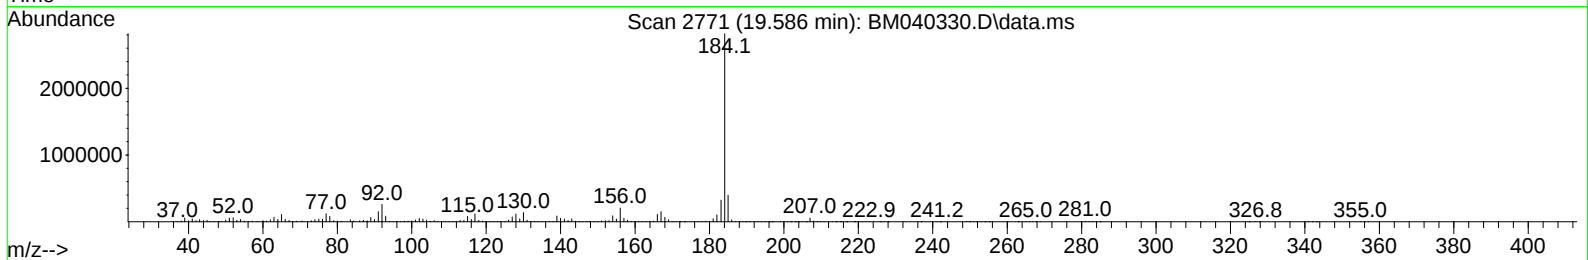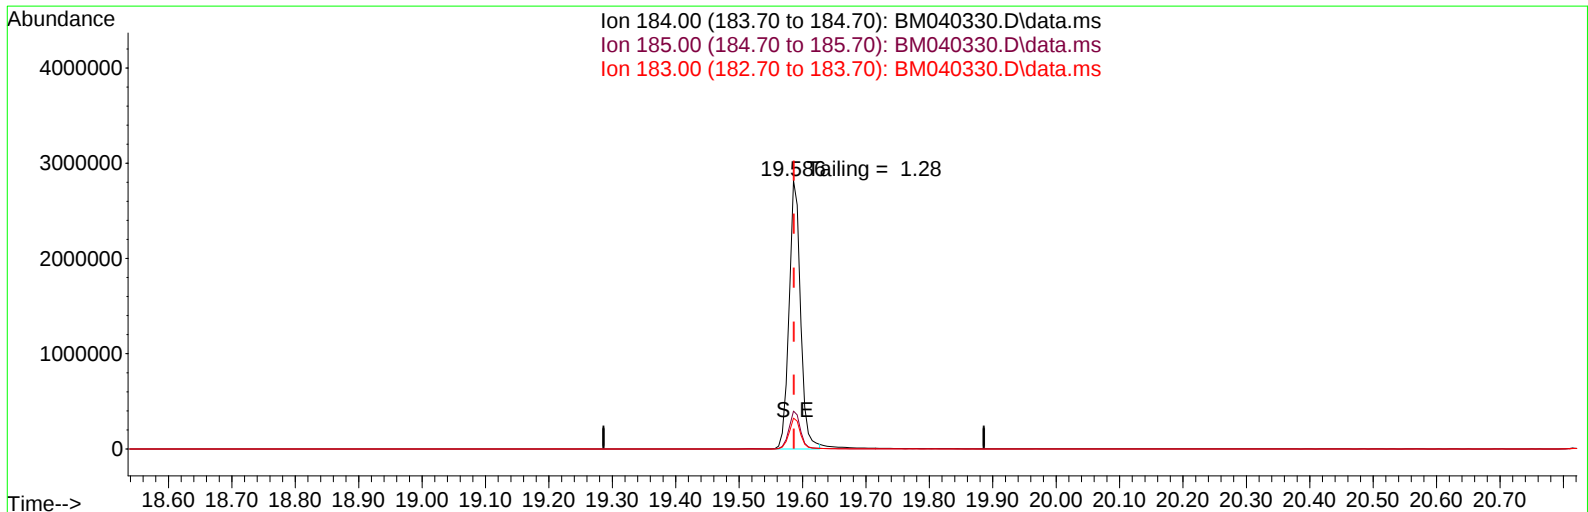

TIC: BM040330.D\data.ms

(77) Benzidine

19.586min (-0.000) 60819.00 ng

response 3658348

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.14
183.00	11.50	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2023	BNA_M	<u>BM040330.D</u>
Compound Name	Response	Retention Time
DDT	1631690	20.815
DDD	24035	20.374
DDE	529	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24564	1656254	1.48

Instrument :
BNA_M
ClientSampleId :
DFTPP