


Data Path : Z:\HPCHEM1\BNA_M\Data\BM062215\
 Data File : BM001769.D
 Acq On : 22 Jun 2015 11:18
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM061915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 05:05:14 2015

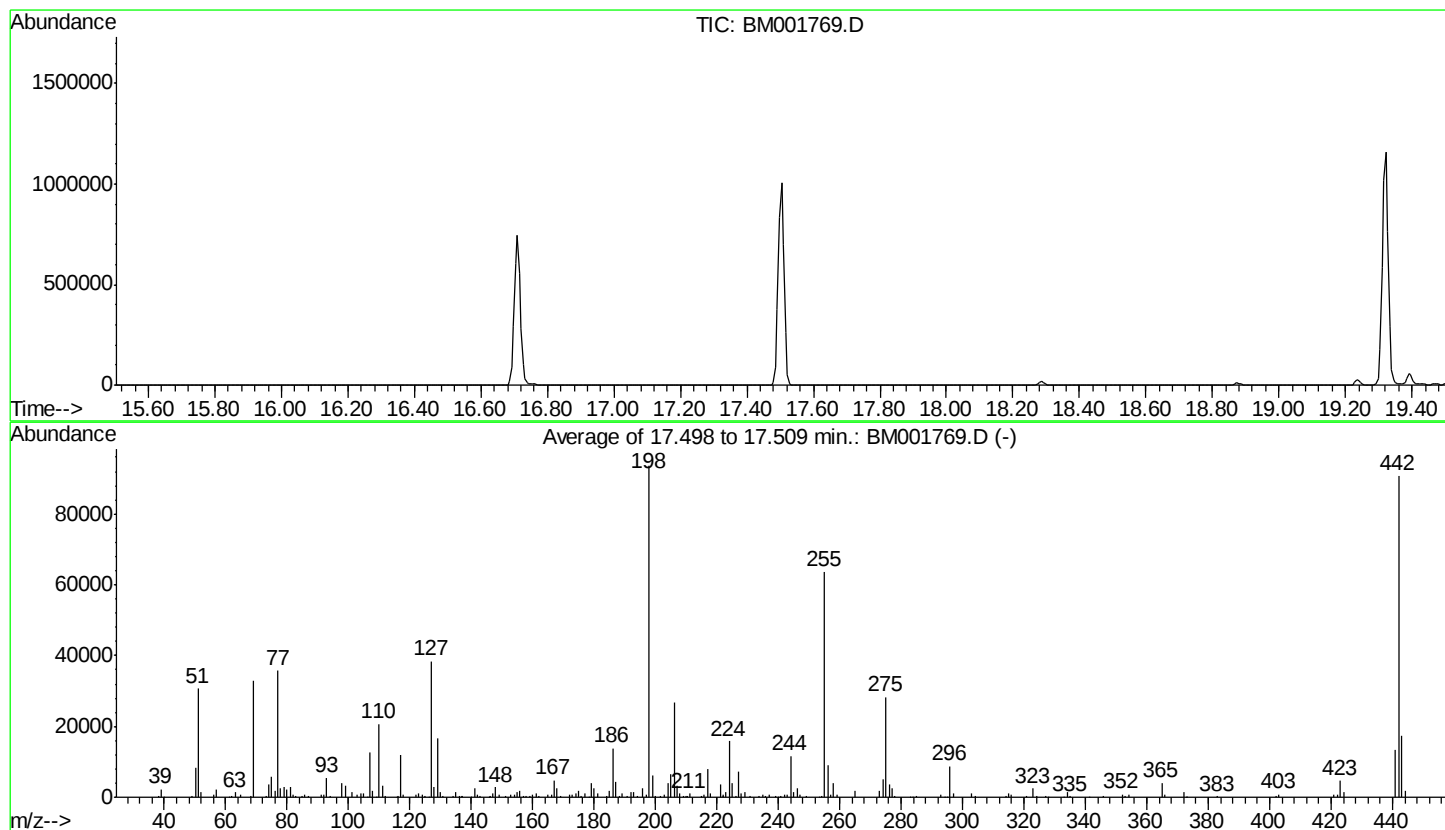

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	30626	PASS
68	69	0.00	2	1.5	511	PASS
69	198	0.00	100	35.3	33056	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	38360	PASS
197	198	0.00	2	0.7	667	PASS
198	198	100	100	100.0	93637	PASS
199	198	5	9	6.7	6293	PASS
275	198	10	60	30.3	28349	PASS
365	198	1	100	4.3	4041	PASS
441	442	0.01	24	14.6	13288	PASS
442	198	50	100	96.9	90728	PASS
443	442	15	24	19.1	17369	PASS