
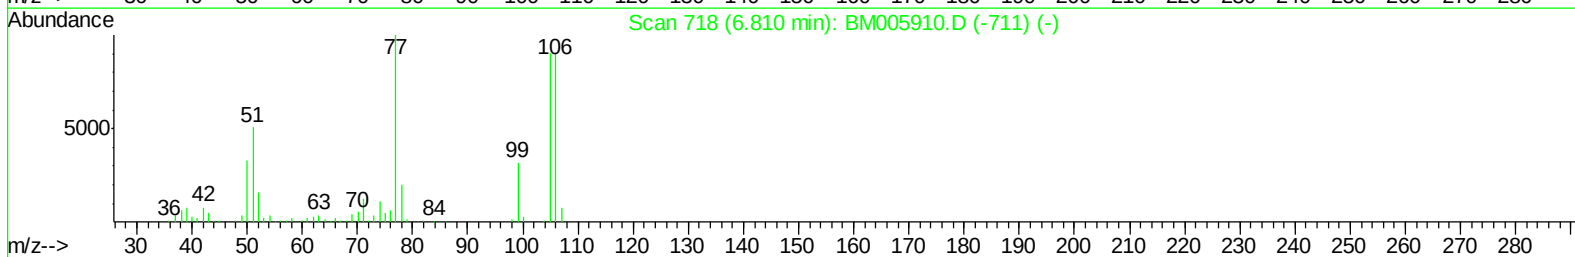
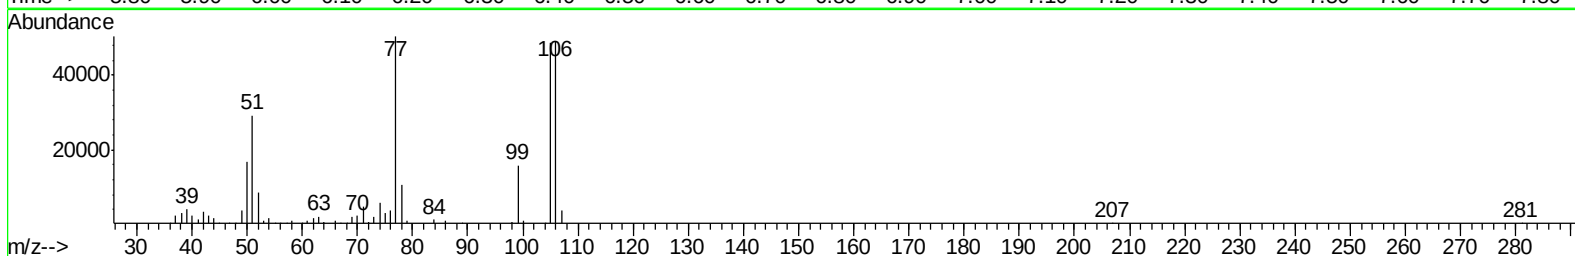


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005915.D
Acq On : 23 Jun 2016 03:13
Operator : UM/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 23 11:42:01 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 23 11:19:18 2016
Response via : Initial Calibration

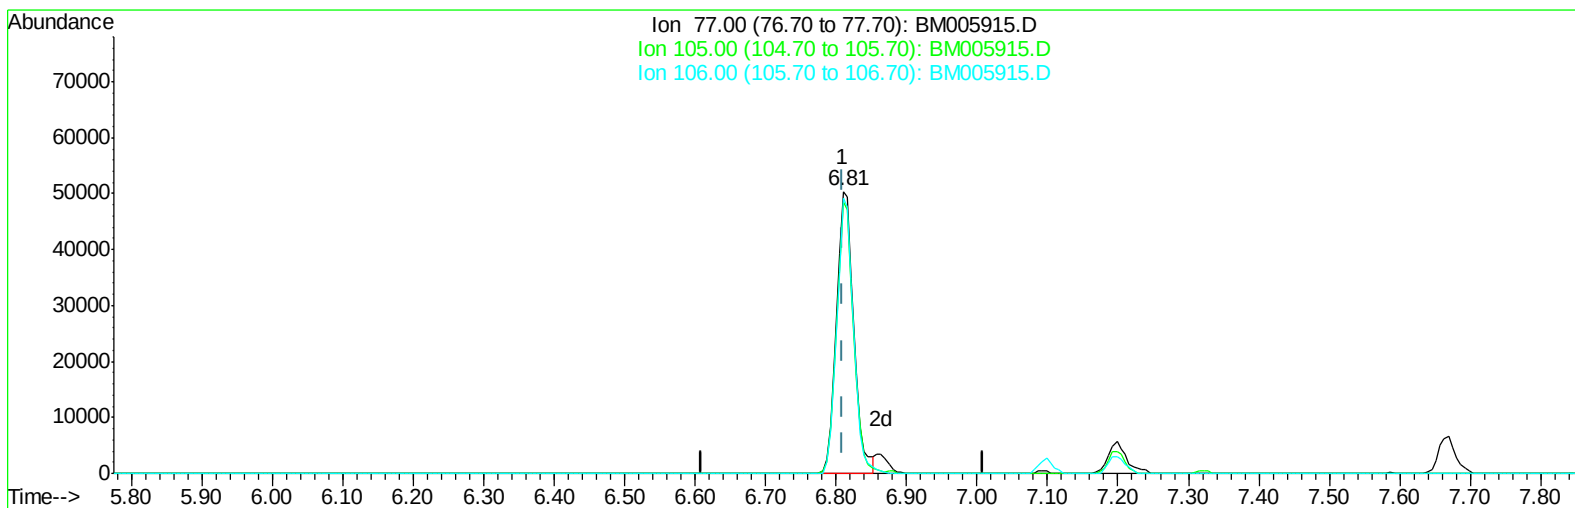

TIC: BM005915.D

(4) Benzaldehyde

6.810min (0.000) 22.66ng/ul

response 85695

Ion	Exp%	Act%
77.00	100	100
105.00	90.10	96.52
106.00	90.30	97.62
0.00	0.00	0.00