

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
 Data File : BM005930.D
 Acq On : 23 Jun 2016 14:56
 Operator : UM/SJ
 Sample : H3612-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z27

Quant Time: Jun 23 15:34:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 23 11:19:18 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	144070	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	596426	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	303838	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	672155	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	795461	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	828417	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	7987	2.21	ng/uL	0.00
5) Phenol-d5	6.83	99	312625	25.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	204461	26.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	249982	25.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	243598	25.06	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	111749	25.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	109977	23.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	216641	24.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	305001	31.68	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	627947	26.01	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	804511	26.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	66750	14.14	ng/ul	0.00
57) Fluorene-d10	15.30	176	561100	26.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	50611	15.12	ng/ul	0.00
70) Anthracene-d10	17.16	188	851886	27.82	ng/ul	0.00
76) Pyrene-d10	19.46	212	985451	26.69	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	1080794	28.96	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.77	163	196989	8.09	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005930.D
Acq On : 23 Jun 2016 14:56
Operator : UM/SJ
Sample : H3612-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z27

Quant Time: Jun 23 15:34:00 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 23 11:19:18 2016
Response via : Initial Calibration

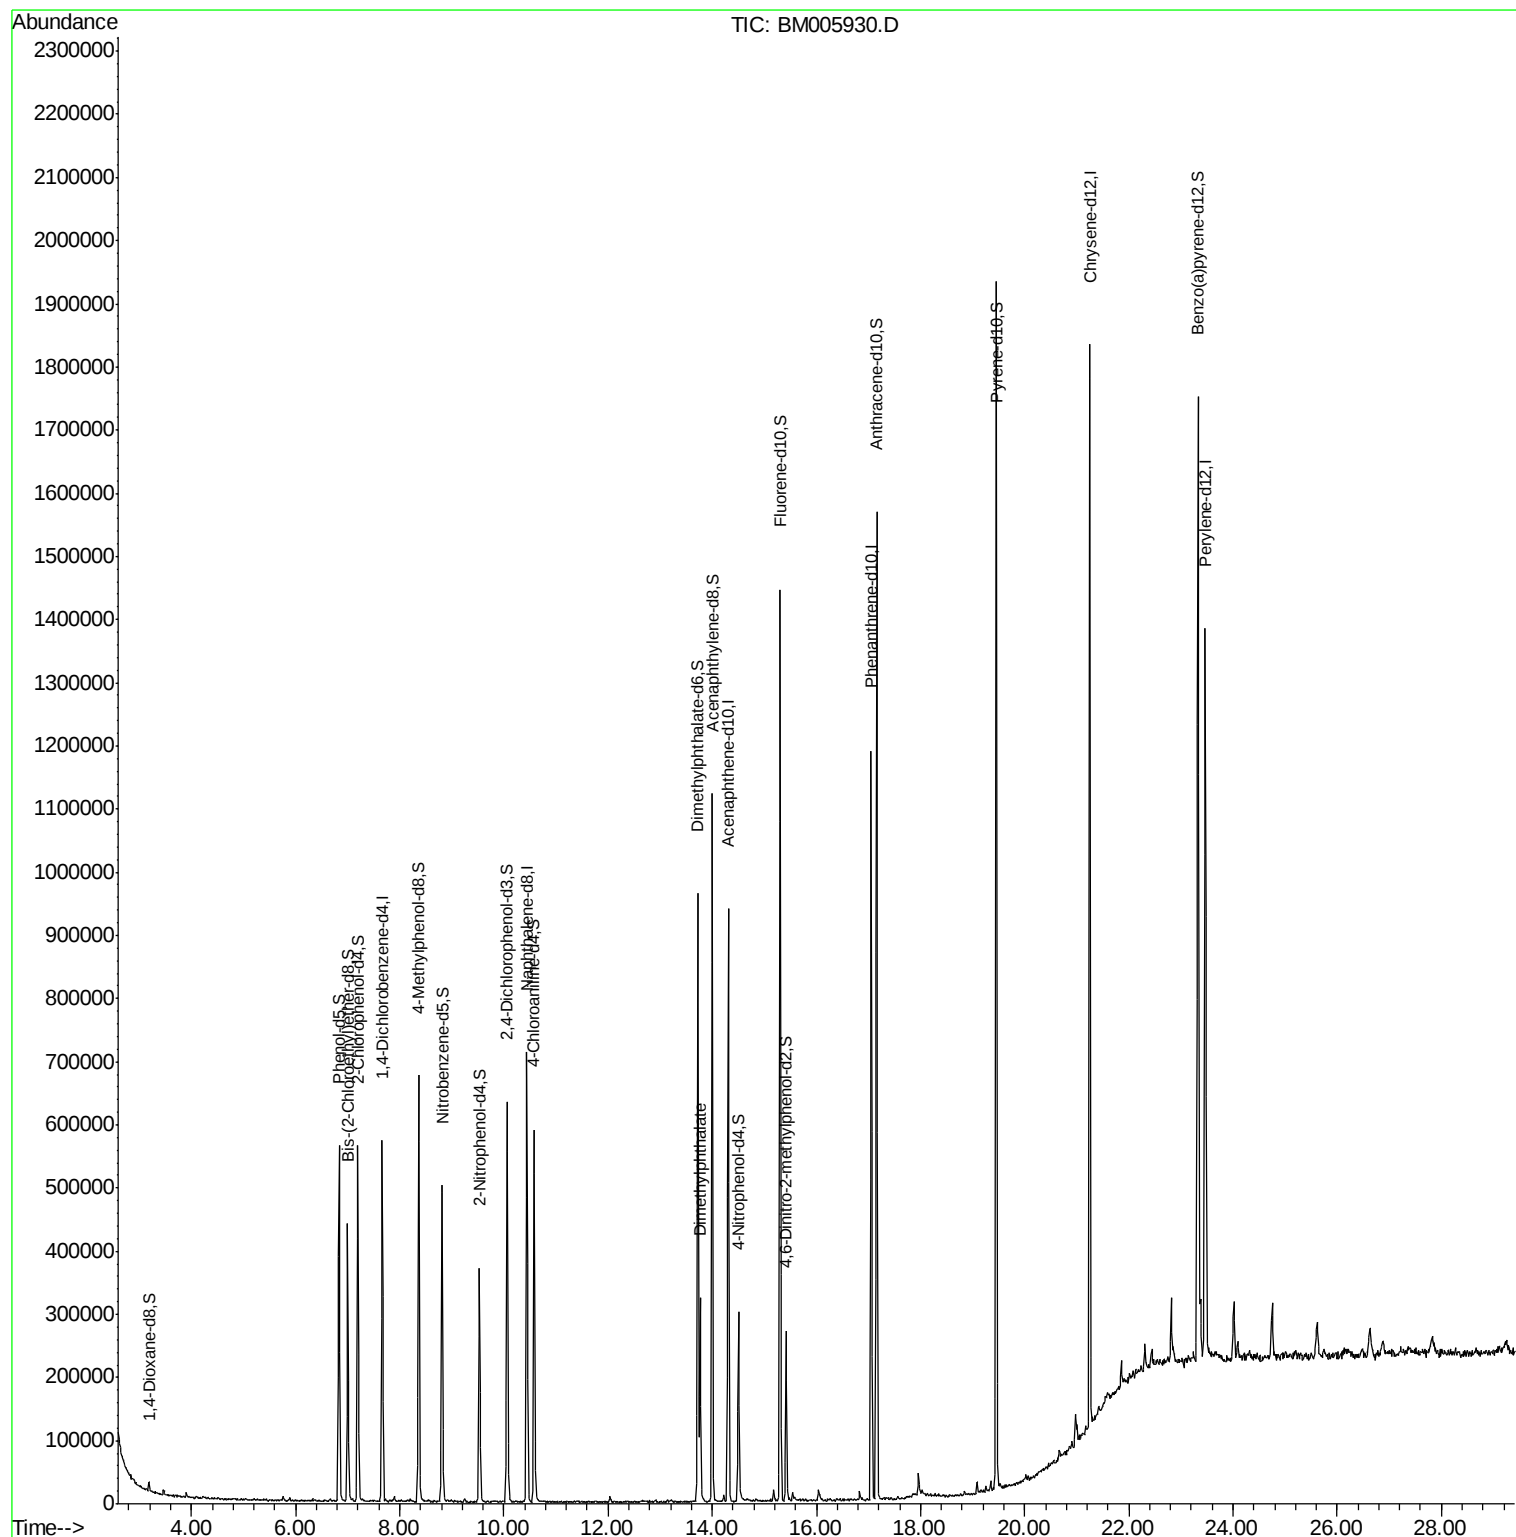

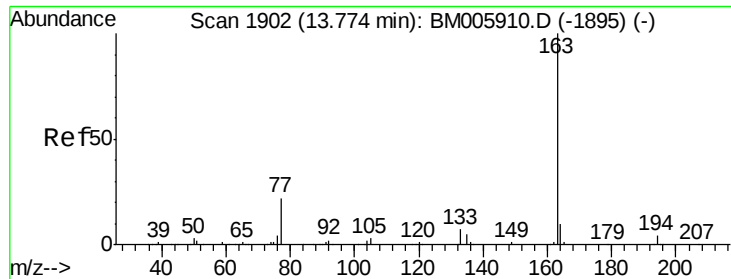

#44
 Dimethylphthalate
 Concen: 8.09 ng/ul
 RT: 13.77 min Scan# 1901
 Delta R.T. -0.01 min
 Lab File: BM005930.D
 Acq: 23 Jun 2016 14:56

Instrument :
 BNA_M
 ClientSampleId :
 D9Z27

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.1	4.7
164	10.3	7.9	11.9

