

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005931.D
 Acq On : 23 Jun 2016 15:32
 Operator : UM/SJ
 Sample : H3612-17
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z35

Quant Time: Jun 23 16:05:12 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 23 11:19:18 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	701953	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	3129968	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	1688149	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	3444156	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	3377049	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	3430071	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	39991	2.27	ng/uL	0.00
5) Phenol-d5	6.83	99	1690466	27.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	1083589	29.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	1312642	27.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	1365434	28.83	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	668811	29.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	738674	30.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	1273083	27.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	1734296	34.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	3773555	28.13	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	4700421	28.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	638873	24.37	ng/ul	0.00
57) Fluorene-d10	15.31	176	3067229	26.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	506914	29.55	ng/ul	0.00
70) Anthracene-d10	17.16	188	4388336	27.97	ng/ul	0.00
76) Pyrene-d10	19.46	212	4687940	29.91	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	4637500	30.01	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.77	163	1182880	8.74	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005931.D
Acq On : 23 Jun 2016 15:32
Operator : UM/SJ
Sample : H3612-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z35

Quant Time: Jun 23 16:05:12 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 23 11:19:18 2016
Response via : Initial Calibration

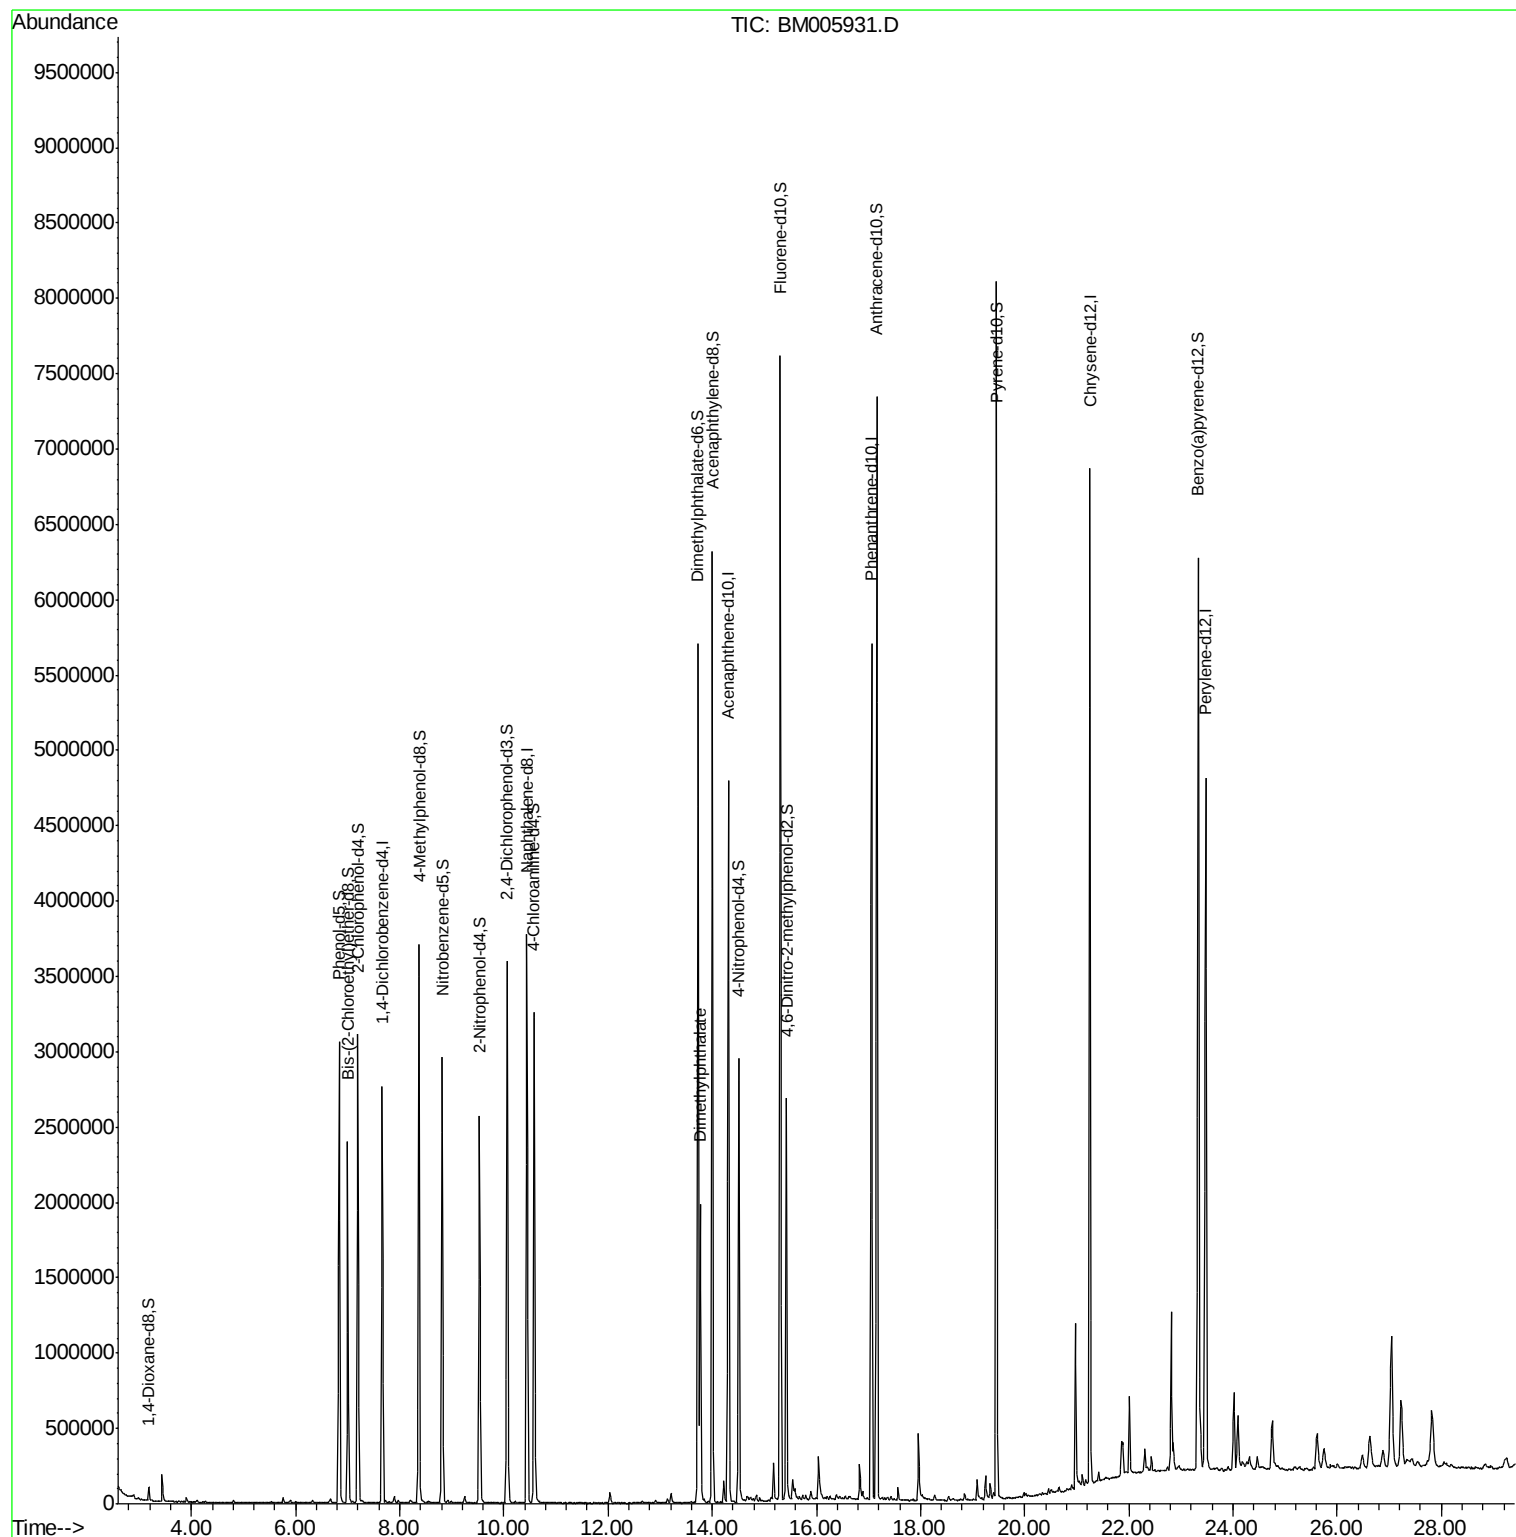

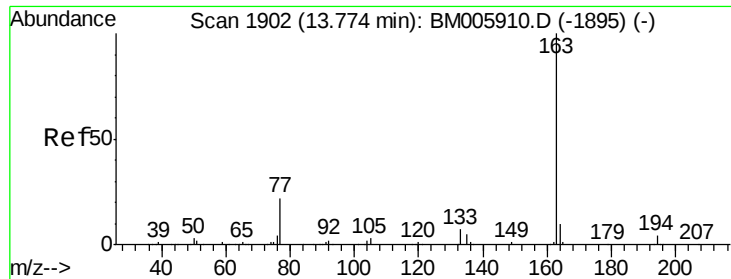

#44

Dimethylphthalate

Concen: 8.74 ng/ul

RT: 13.77 min Scan# 1902

Delta R.T. 0.00 min

Lab File: BM005931.D

Acq: 23 Jun 2016 15:32

Instrument :

BNA_M

ClientSampleId :

D9Z35


Tot Ion:163 Resp: 1182880

Ion Ratio Lower Upper

163 100

194 4.2 3.1 4.7

164 9.9 7.9 11.9

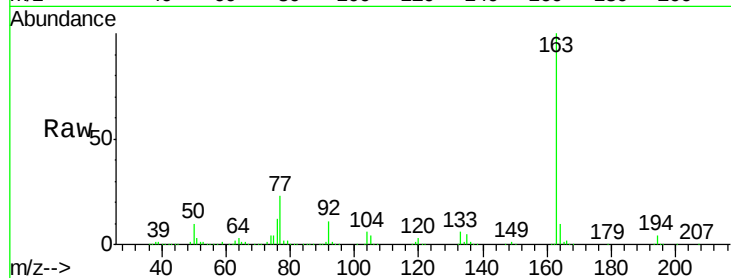

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

