

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005918.D
 Acq On : 23 Jun 2016 05:00
 Operator : UM/SJ
 Sample : H3608-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC382

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	715	722	729	rBV	291519	466059	6.99%	0.738%
2	7.004	743	751	762	rBV	963881	1520701	22.80%	2.407%
3	7.198	777	784	795	rVB	1017047	1666094	24.98%	2.637%
4	7.663	856	863	871	rBV	946629	1538867	23.07%	2.435%
5	8.363	975	982	993	rBV	797480	1316232	19.74%	2.083%
6	8.816	1050	1059	1074	rBV	1213678	2014508	30.21%	3.188%
7	9.533	1173	1181	1197	rVB	964537	1618609	24.27%	2.562%
8	10.063	1264	1271	1284	rBV	1322460	2336191	35.03%	3.697%
9	10.445	1328	1336	1349	rBV	1267028	2212729	33.18%	3.502%
10	10.580	1353	1359	1368	rBV	57324	103974	1.56%	0.165%
11	13.727	1887	1894	1910	rBV	2292895	3599401	53.97%	5.696%
12	14.004	1933	1941	1959	rVB	2684585	4278103	64.15%	6.771%
13	14.310	1986	1993	2005	rVB2	1733147	2783216	41.73%	4.405%
14	14.504	2020	2026	2038	rBV	234113	370693	5.56%	0.587%
15	15.309	2156	2163	2176	rBV	3433626	5229577	78.41%	8.276%
16	15.421	2176	2182	2195	rVV	1097101	1564274	23.45%	2.476%
17	17.056	2453	2460	2471	rBV	2258709	3333400	49.98%	5.275%
18	17.156	2471	2477	2489	rBV2	3824830	5563583	83.42%	8.805%
19	17.962	2610	2614	2620	rBV2	57587	85820	1.29%	0.136%
20	19.086	2799	2805	2809	rBV	54631	76983	1.15%	0.122%
21	19.250	2829	2833	2840	rBV2	89457	128018	1.92%	0.203%
22	19.456	2862	2868	2876	rBV2	4591062	6398118	95.93%	10.126%
23	21.250	3167	3173	3181	rBV	3304097	4185144	62.75%	6.623%
24	23.332	3519	3527	3541	rBV2	3439171	6669334	100.00%	10.555%
25	23.468	3543	3550	3562	rVB2	2098659	4127608	61.89%	6.532%


Sum of corrected areas: 63187236

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005918.D
Acq On : 23 Jun 2016 05:00
Operator : UM/SJ
Sample : H3608-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC382

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

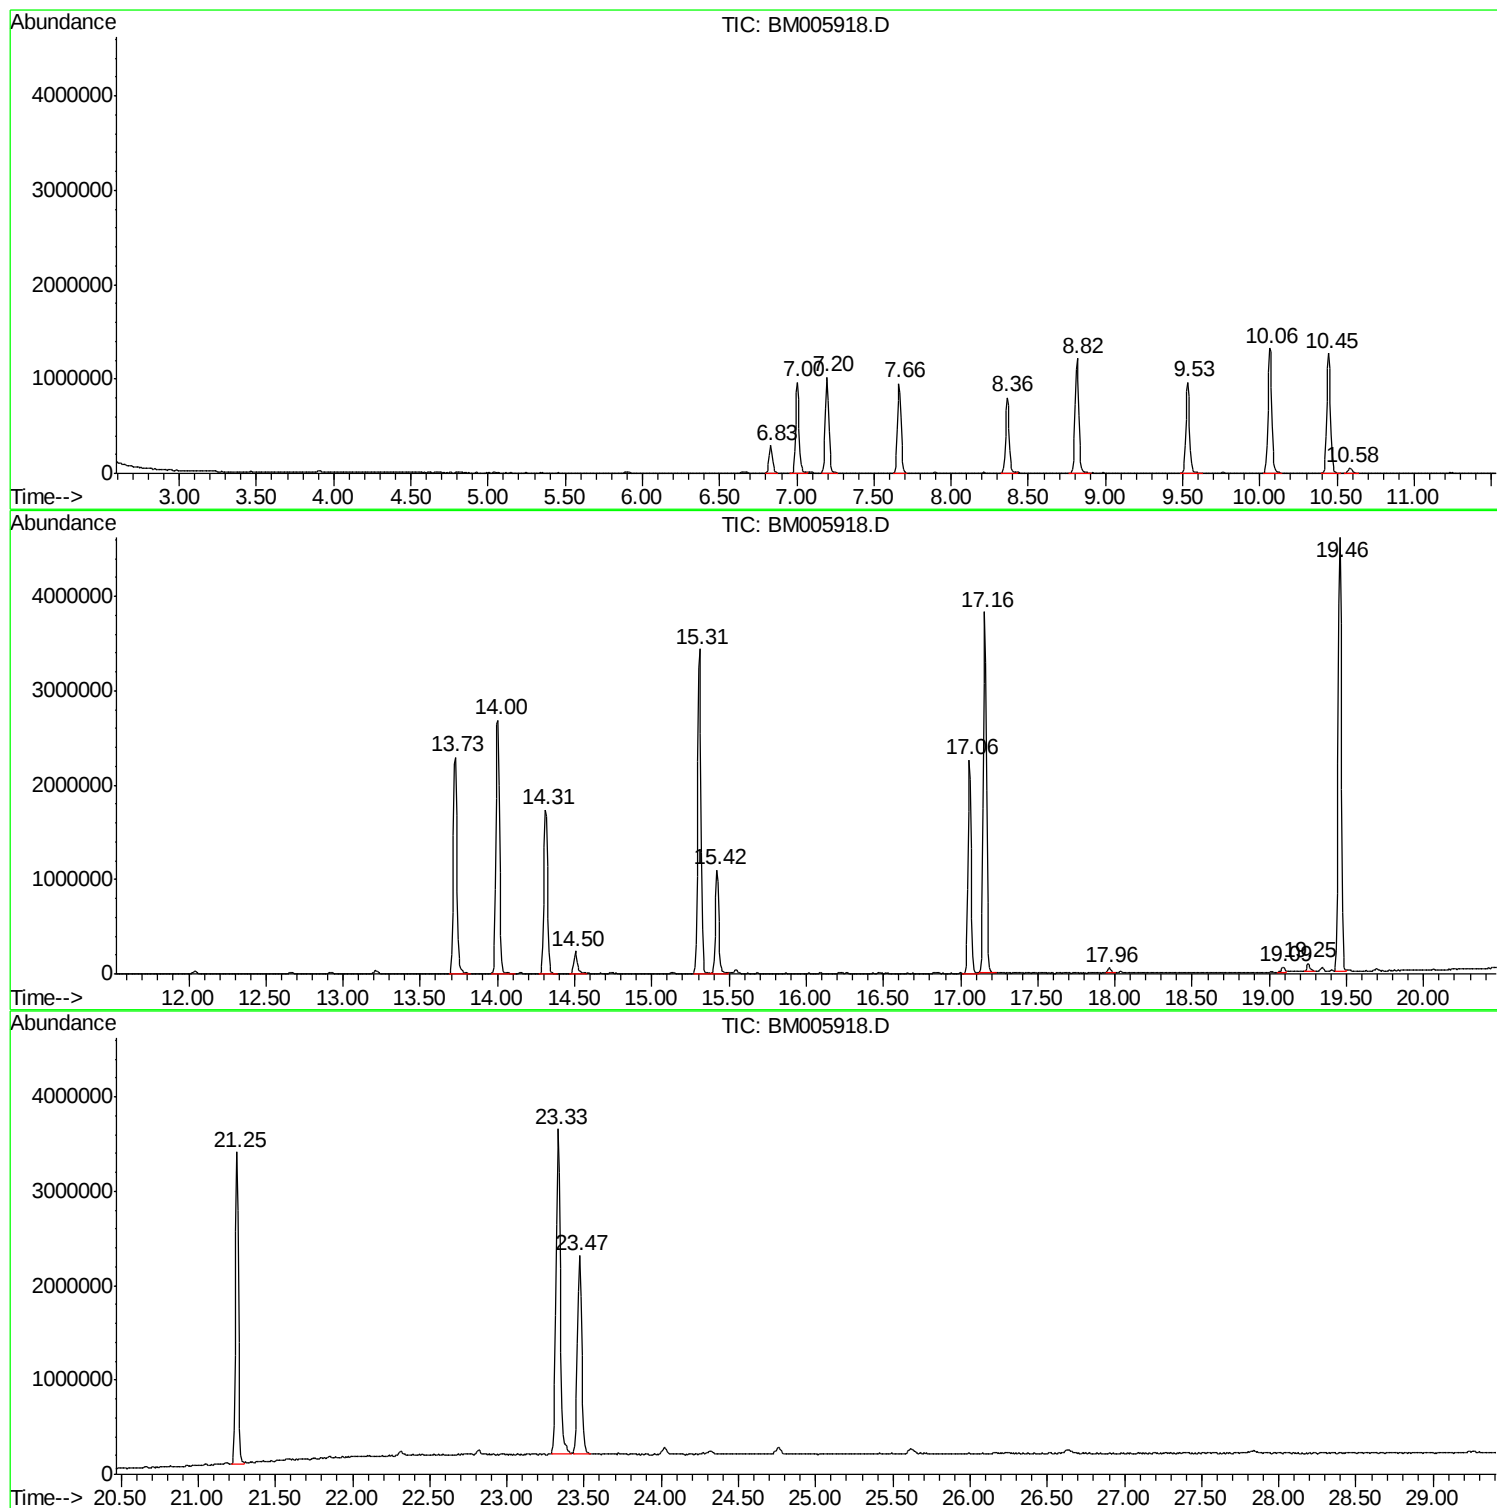

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005918.D
Acq On : 23 Jun 2016 05:00
Operator : UM/SJ
Sample : H3608-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC382

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005918.D
Acq On : 23 Jun 2016 05:00
Operator : UM/SJ
Sample : H3608-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC382

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc