

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005920.D
 Acq On : 23 Jun 2016 06:12
 Operator : UM/SJ
 Sample : H3608-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC384

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	713	722	731	rBV	332085	537540	7.68%	0.776%
2	7.004	744	751	764	rBV	997872	1634019	23.33%	2.360%
3	7.199	775	784	795	rBV	1090351	1790847	25.57%	2.587%
4	7.663	856	863	873	rBV	1154471	1915596	27.36%	2.767%
5	8.363	975	982	1003	rVB	871959	1465706	20.93%	2.117%
6	8.816	1052	1059	1072	rBV	1274945	2141593	30.58%	3.093%
7	9.534	1174	1181	1196	rBV	1027621	1731296	24.72%	2.501%
8	10.063	1262	1271	1286	rBV	1432948	2470371	35.28%	3.568%
9	10.445	1327	1336	1349	rVV	1598979	2746112	39.22%	3.967%
10	13.728	1887	1894	1910	rBV	2491536	3784973	54.05%	5.467%
11	13.998	1933	1940	1953	rBV	2794202	4517451	64.51%	6.525%
12	14.310	1986	1993	2004	rVB3	2122774	3391406	48.43%	4.899%
13	14.504	2019	2026	2037	rBV	262937	427690	6.11%	0.618%
14	15.310	2155	2163	2173	rBV	3551193	5527427	78.94%	7.984%
15	15.422	2176	2182	2194	rBV	1138259	1613293	23.04%	2.330%
16	17.057	2453	2460	2470	rBV2	2748148	3977906	56.81%	5.746%
17	17.157	2470	2477	2489	rBV2	4105111	5896851	84.21%	8.518%
18	19.086	2800	2805	2811	rBV	55747	79167	1.13%	0.114%
19	19.457	2862	2868	2878	rBV	4793045	6725060	96.04%	9.714%
20	21.251	3168	3173	3185	rBV	3652642	4919409	70.25%	7.106%
21	23.333	3520	3527	3542	rVV2	3590249	7002439	100.00%	10.115%
22	23.474	3544	3551	3563	rVB2	2610476	4934919	70.47%	7.128%


Sum of corrected areas: 69231071

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005920.D
Acq On : 23 Jun 2016 06:12
Operator : UM/SJ
Sample : H3608-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC384

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

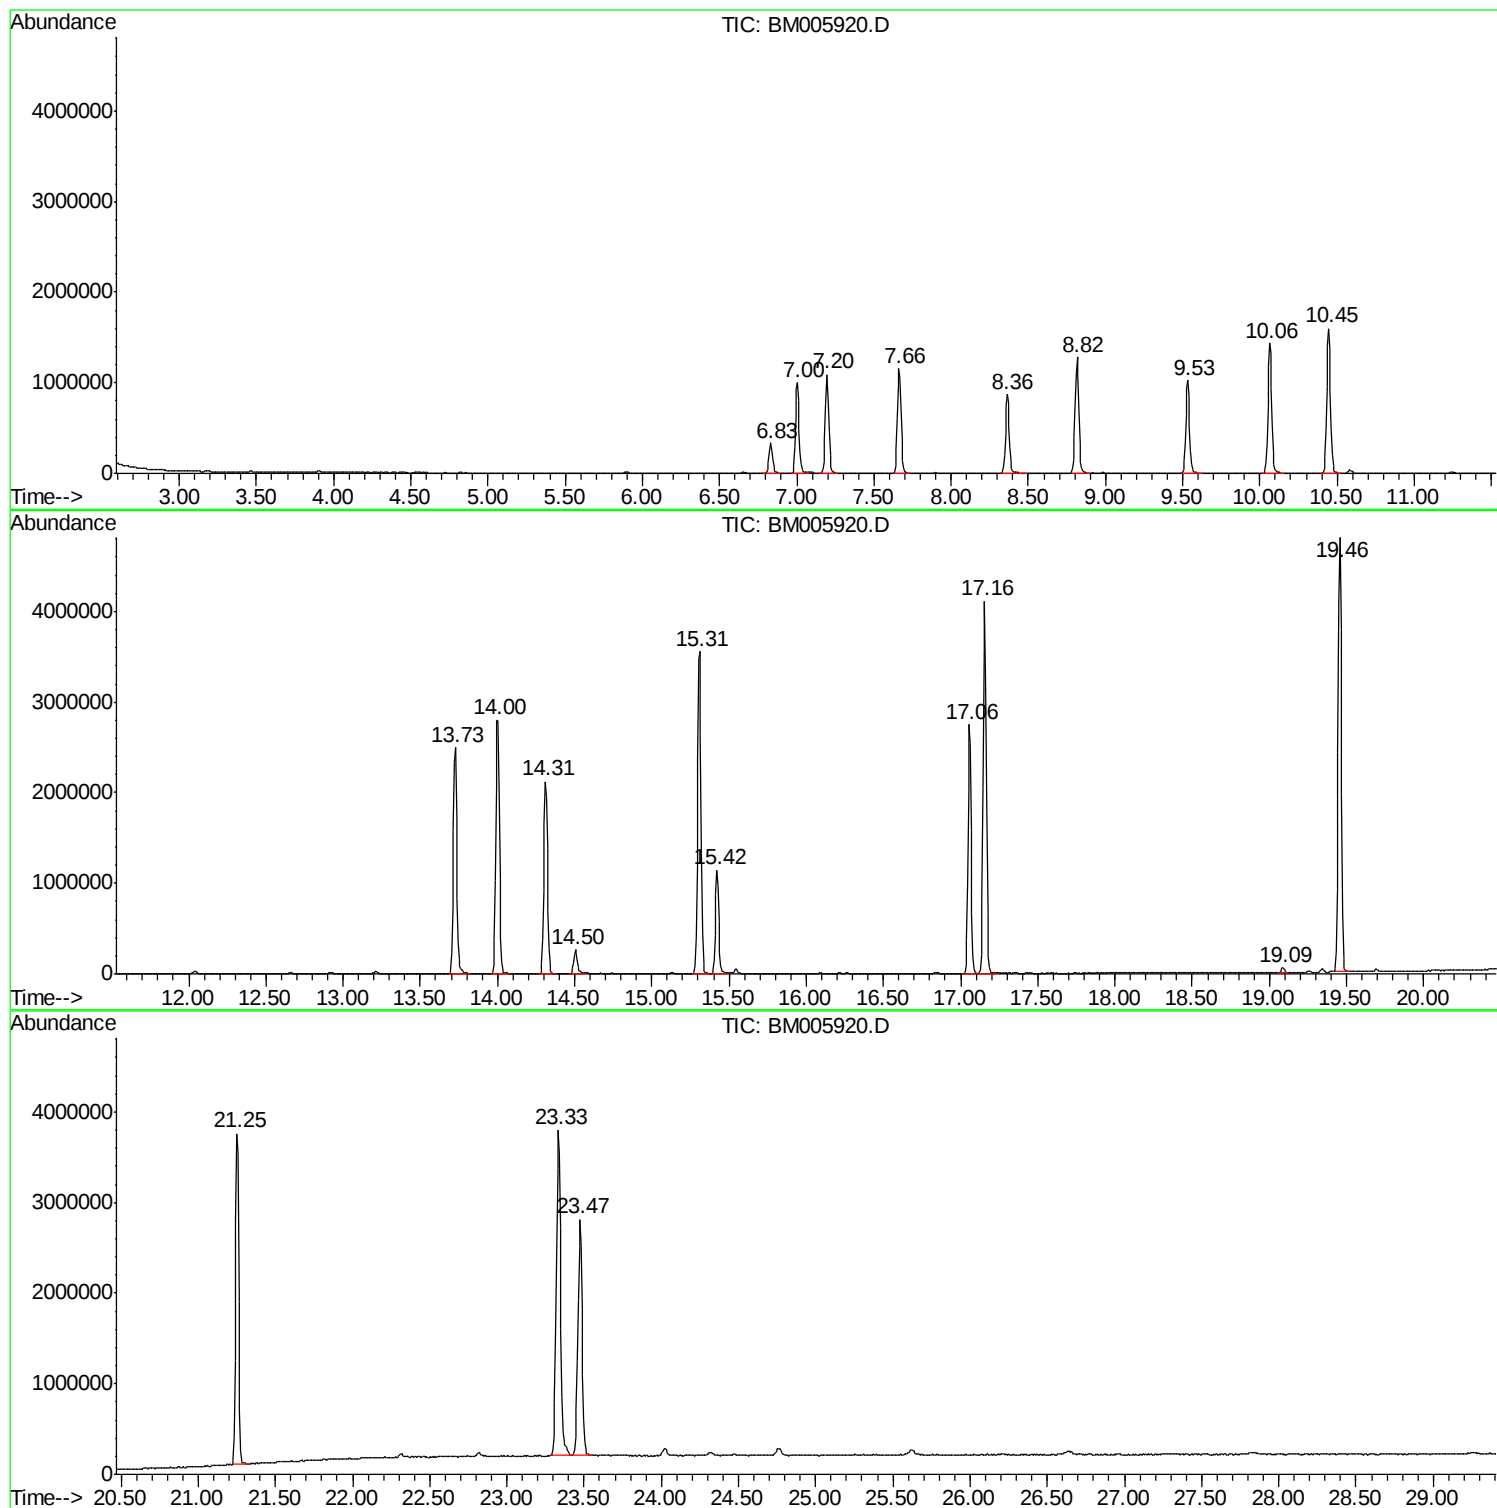

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005920.D
Acq On : 23 Jun 2016 06:12
Operator : UM/SJ
Sample : H3608-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC384

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005920.D
Acq On : 23 Jun 2016 06:12
Operator : UM/SJ
Sample : H3608-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC384

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc