

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005921.D
 Acq On : 23 Jun 2016 06:48
 Operator : UM/SJ
 Sample : H3608-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC385

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	715	722	729	rBV	408543	646704	7.71%	0.744%
2	7.004	744	751	764	rBV	1139703	1828415	21.79%	2.102%
3	7.198	775	784	799	rBV	1235214	2019581	24.07%	2.322%
4	7.663	856	863	873	rBV	1439504	2354258	28.06%	2.707%
5	8.363	974	982	992	rBV	1060035	1746705	20.82%	2.008%
6	8.816	1050	1059	1070	rBV	1437636	2453682	29.24%	2.821%
7	9.534	1173	1181	1192	rBV	1193045	2004340	23.89%	2.305%
8	10.063	1264	1271	1284	rBV	1662278	2886508	34.40%	3.319%
9	10.445	1328	1336	1348	rBV	2106173	3595913	42.85%	4.135%
10	10.581	1352	1359	1367	rBV	142392	257264	3.07%	0.296%
11	13.727	1887	1894	1910	rBV	3301096	5001204	59.60%	5.751%
12	14.004	1933	1941	1952	rBV	3569229	5677309	67.66%	6.528%
13	14.310	1986	1993	2002	rBV2	3087743	4938936	58.86%	5.679%
14	14.504	2021	2026	2038	rBV	373534	597700	7.12%	0.687%
15	15.310	2155	2163	2176	rBV	4688090	7086486	84.45%	8.148%
16	15.421	2176	2182	2196	rVV	1506448	2224733	26.51%	2.558%
17	15.551	2198	2204	2212	rVB	60831	93761	1.12%	0.108%
18	17.057	2453	2460	2469	rBV2	4080192	6065044	72.28%	6.974%
19	17.157	2469	2477	2492	rVV2	5052160	7688814	91.63%	8.841%
20	19.086	2800	2805	2810	rBV	71188	96489	1.15%	0.111%
21	19.456	2862	2868	2876	rBV2	5757740	8391473	100.00%	9.649%
22	21.256	3168	3174	3183	rBV	4643774	6359005	75.78%	7.312%
23	23.333	3520	3527	3534	rBV2	3600081	6844517	81.57%	7.870%
24	23.474	3544	3551	3563	rVB2	2832315	5614978	66.91%	6.456%
25	24.021	3640	3644	3650	rVB2	117842	224303	2.67%	0.258%
26	24.762	3766	3770	3782	rVB3	131010	270137	3.22%	0.311%


Sum of corrected areas: 86968259

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005921.D
Acq On : 23 Jun 2016 06:48
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

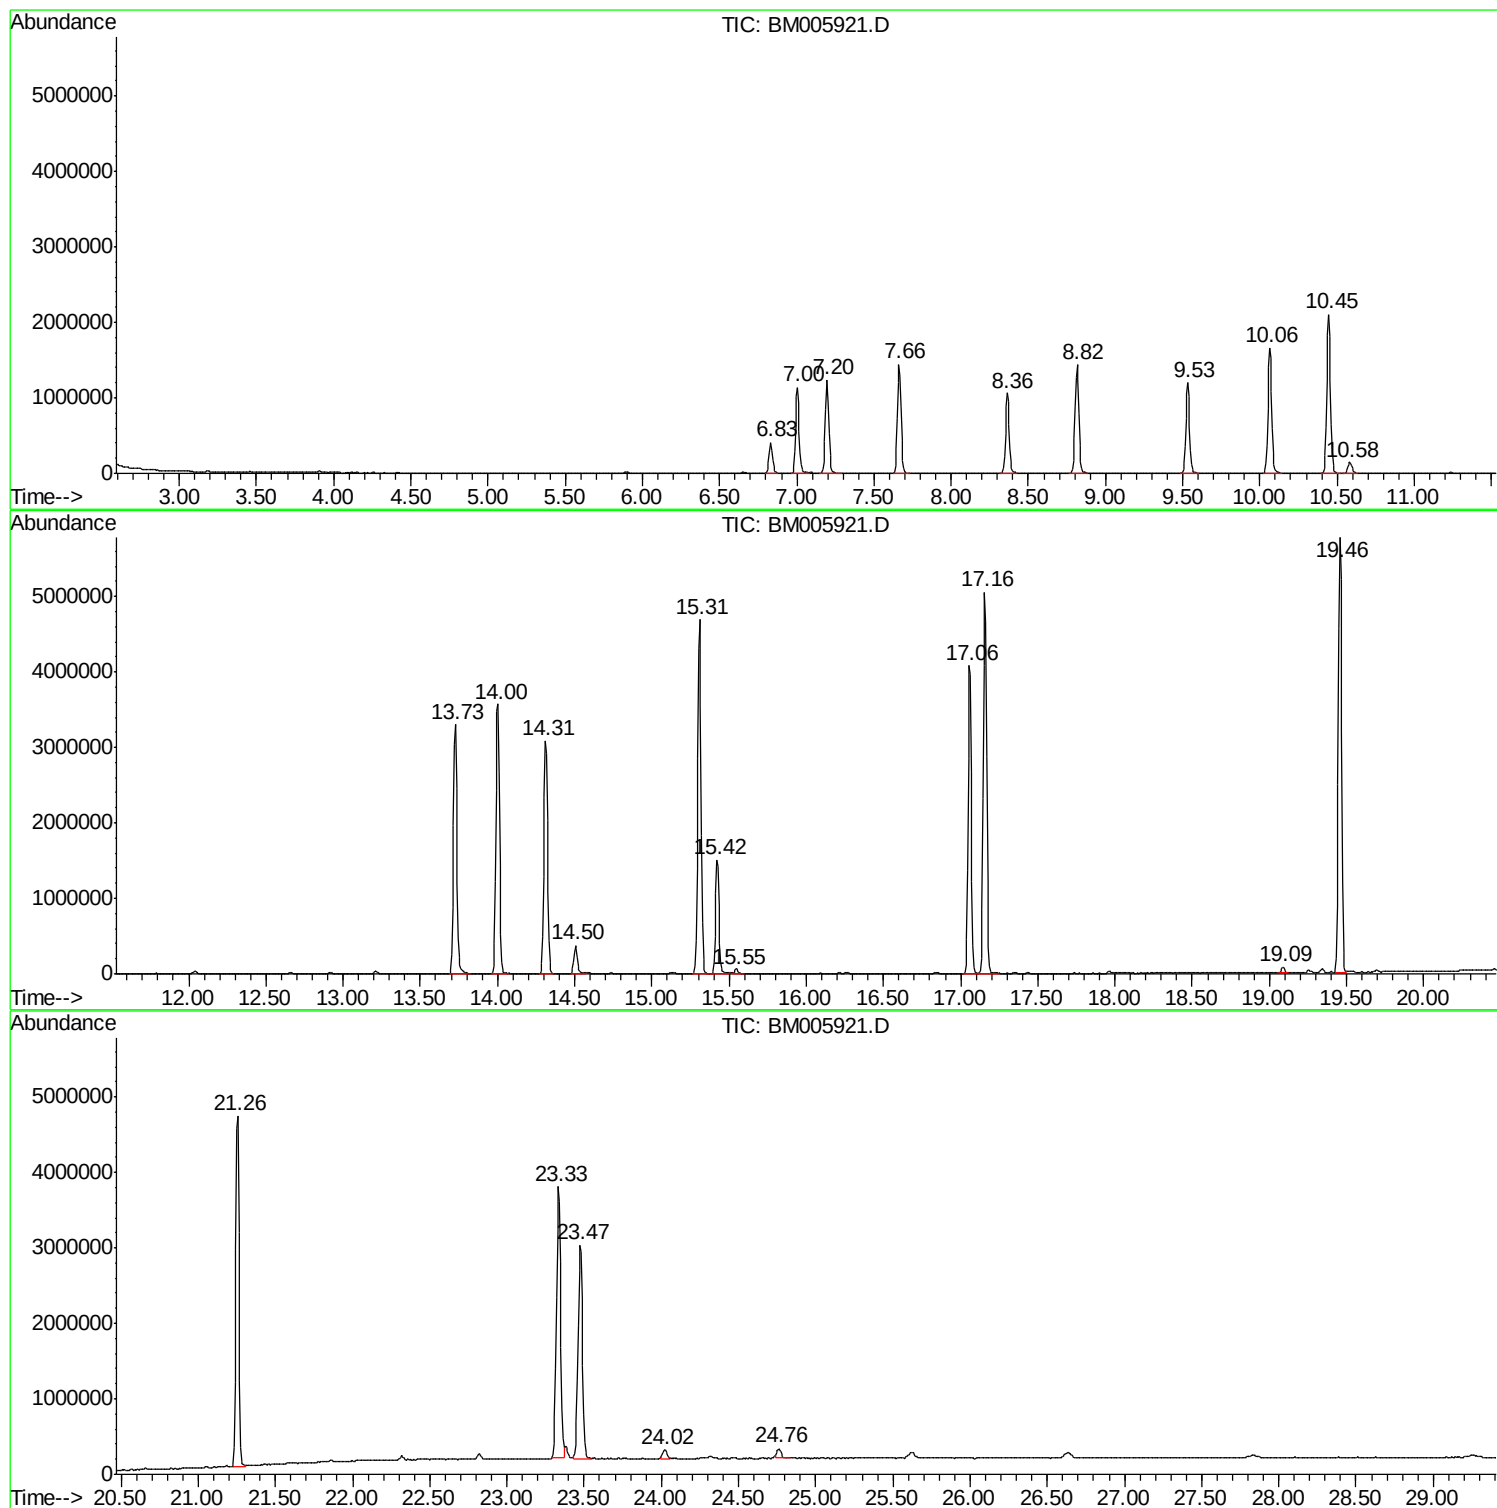

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005921.D
Acq On : 23 Jun 2016 06:48
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005921.D
Acq On : 23 Jun 2016 06:48
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc