

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005922.D
 Acq On : 23 Jun 2016 07:24
 Operator : UM/SJ
 Sample : H3608-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC392

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	715	722	733	rBV	365601	591619	8.67%	0.869%
2	7.004	744	751	763	rBV	1014612	1634047	23.95%	2.400%
3	7.198	775	784	796	rBV	1123747	1857652	27.23%	2.728%
4	7.663	856	863	873	rVB	1209457	1911618	28.02%	2.808%
5	8.363	973	982	994	rBV	939744	1543943	22.63%	2.268%
6	8.816	1051	1059	1071	rBV	1271955	2119761	31.07%	3.113%
7	9.534	1174	1181	1193	rBV	1002100	1707222	25.02%	2.507%
8	10.063	1264	1271	1287	rBV	1438881	2495336	36.58%	3.665%
9	10.445	1328	1336	1346	rBV	1562985	2711995	39.75%	3.983%
10	13.727	1886	1894	1910	rBV	2340702	3618618	53.04%	5.315%
11	13.998	1933	1940	1955	rBV	2741740	4394481	64.41%	6.454%
12	14.310	1986	1993	2002	rBV2	2090832	3299006	48.36%	4.845%
13	14.504	2020	2026	2037	rBV	273025	436270	6.39%	0.641%
14	15.310	2156	2163	2176	rBV	3410214	5320652	77.99%	7.814%
15	15.421	2176	2182	2193	rBV	1091930	1539443	22.57%	2.261%
16	17.057	2453	2460	2470	rBV2	2602551	3873262	56.77%	5.689%
17	17.157	2470	2477	2490	rVV2	3798483	5552663	81.39%	8.155%
18	19.456	2861	2868	2876	rBV2	4521644	6414990	94.03%	9.421%
19	21.250	3168	3173	3183	rBV	3751245	4843629	71.00%	7.114%
20	22.821	3436	3440	3444	rVB2	62614	88168	1.29%	0.129%
21	23.333	3519	3527	3542	rBV2	3430653	6822166	100.00%	10.019%
22	23.474	3544	3551	3564	rVB	2467030	4848949	71.08%	7.121%
23	24.021	3640	3644	3650	rVB2	120164	225187	3.30%	0.331%
24	24.762	3766	3770	3777	rVB	122909	238240	3.49%	0.350%


Sum of corrected areas: 68088917

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005922.D
Acq On : 23 Jun 2016 07:24
Operator : UM/SJ
Sample : H3608-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC392

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

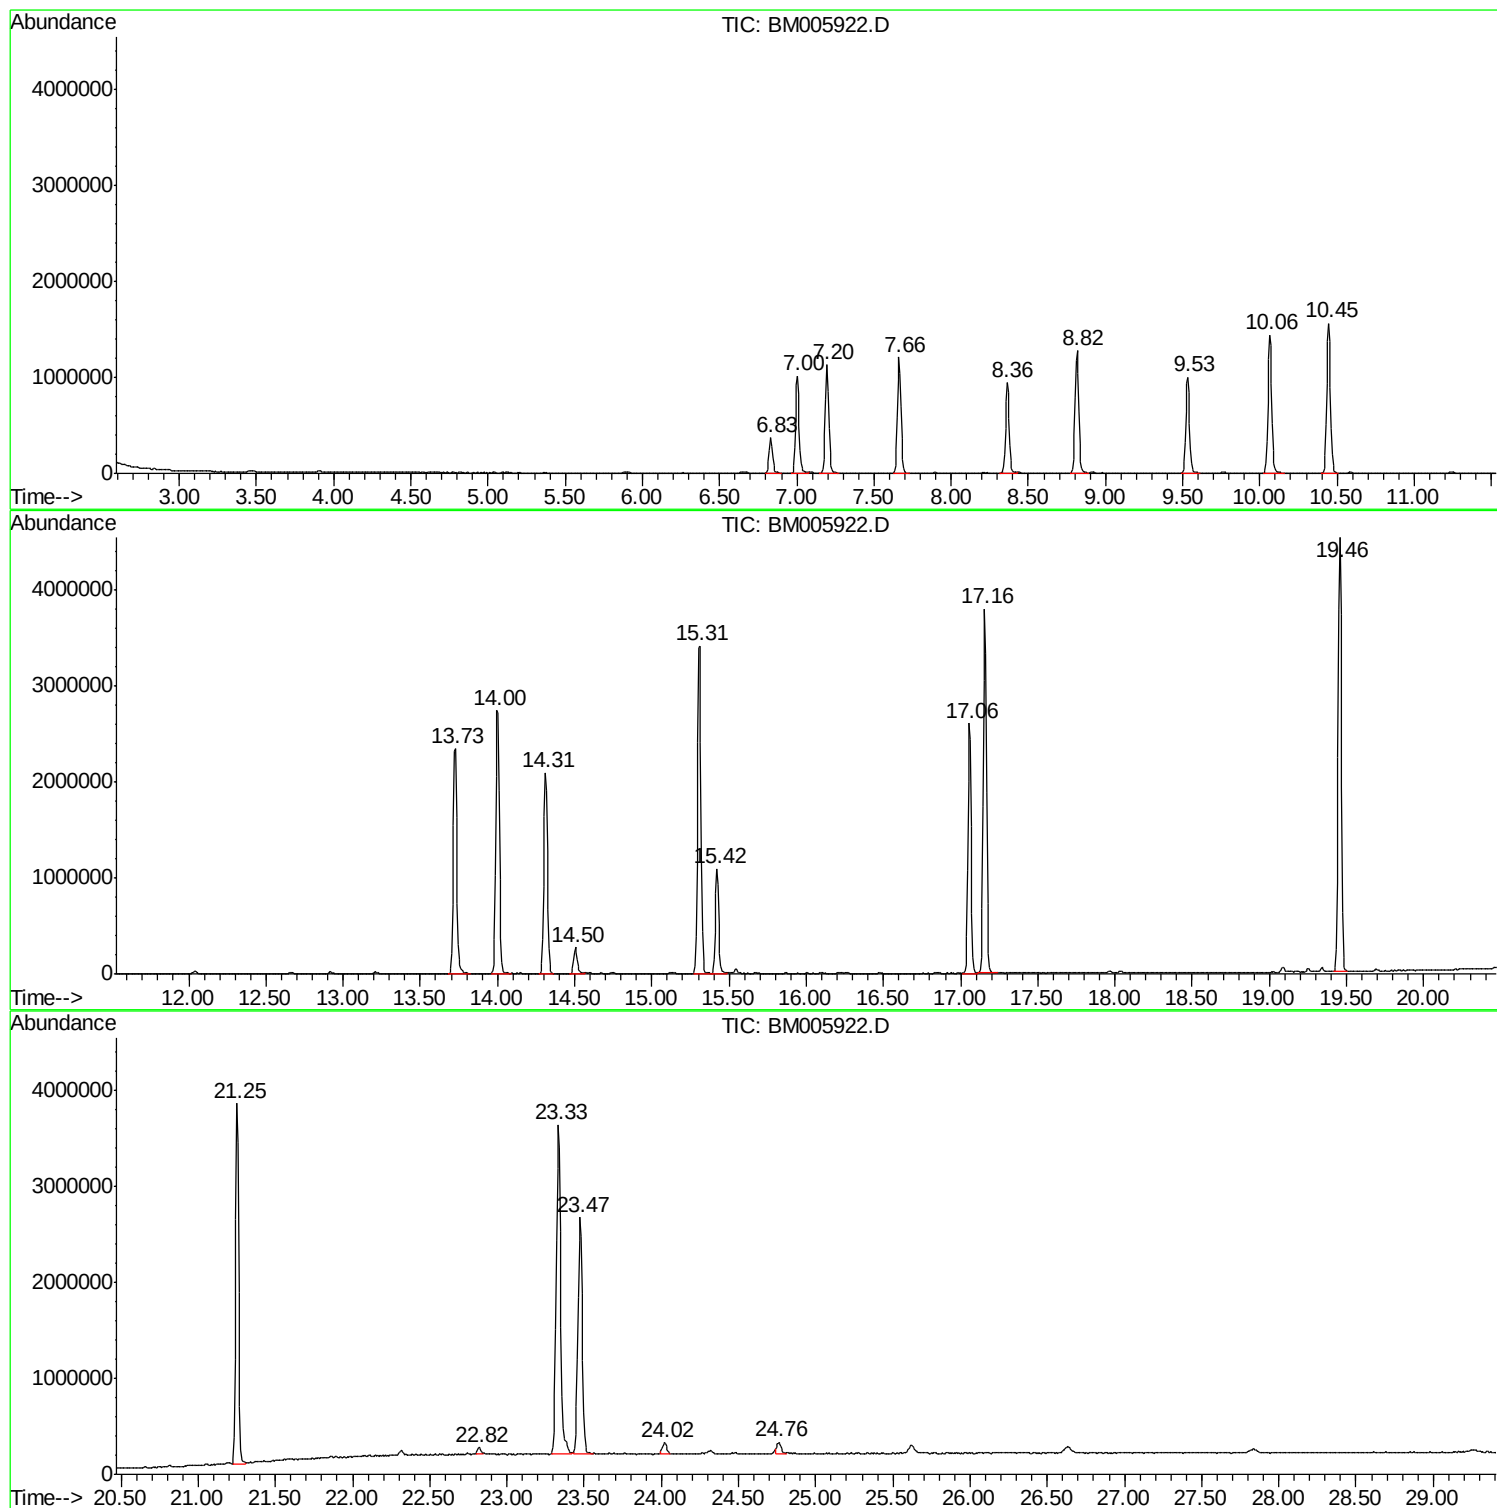

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005922.D
Acq On : 23 Jun 2016 07:24
Operator : UM/SJ
Sample : H3608-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC392

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005922.D
Acq On : 23 Jun 2016 07:24
Operator : UM/SJ
Sample : H3608-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC392

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc