

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005924.D
 Acq On : 23 Jun 2016 08:36
 Operator : UM/SJ
 Sample : H3608-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC386

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.833	716	722	730	rBV	243820	388714	5.17%	0.592%
2	7.004	744	751	762	rBV	837656	1340291	17.82%	2.040%
3	7.198	775	784	795	rBV	888731	1455339	19.35%	2.215%
4	7.663	856	863	874	rVB	1025514	1627436	21.64%	2.477%
5	8.363	974	982	998	rBV	698142	1132222	15.05%	1.723%
6	8.816	1051	1059	1073	rBV	1033201	1743300	23.18%	2.654%
7	9.533	1173	1181	1194	rBV	823180	1380228	18.35%	2.101%
8	10.063	1264	1271	1282	rBV	1191570	2023657	26.90%	3.080%
9	10.445	1328	1336	1347	rBV	1363386	2346420	31.19%	3.572%
10	13.721	1887	1893	1912	rVB	2282799	3443849	45.78%	5.242%
11	13.998	1934	1940	1955	rBV	2457462	3955760	52.59%	6.021%
12	14.309	1986	1993	2002	rVB2	1972154	3064921	40.75%	4.665%
13	14.504	2020	2026	2040	rBV	230149	379235	5.04%	0.577%
14	15.309	2155	2163	2174	rBV	3425110	5187348	68.96%	7.896%
15	15.421	2176	2182	2195	rVV	1216878	1689091	22.46%	2.571%
16	17.056	2454	2460	2469	rBV2	2519095	3795741	50.46%	5.778%
17	17.156	2470	2477	2488	rBV2	4136612	6092841	81.00%	9.274%
18	17.962	2610	2614	2623	rBV2	63095	97238	1.29%	0.148%
19	19.086	2801	2805	2811	rBV	57235	78842	1.05%	0.120%
20	19.250	2829	2833	2840	rBV2	87717	126137	1.68%	0.192%
21	19.456	2862	2868	2875	rBV2	4966092	7110505	94.53%	10.823%
22	21.250	3168	3173	3182	rBV	3746089	4892827	65.05%	7.447%
23	23.332	3519	3527	3541	rBV2	3839557	7522101	100.00%	11.450%
24	23.474	3543	3551	3562	rVV	2462252	4823705	64.13%	7.342%


Sum of corrected areas: 65697748

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005924.D
Acq On : 23 Jun 2016 08:36
Operator : UM/SJ
Sample : H3608-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC386

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

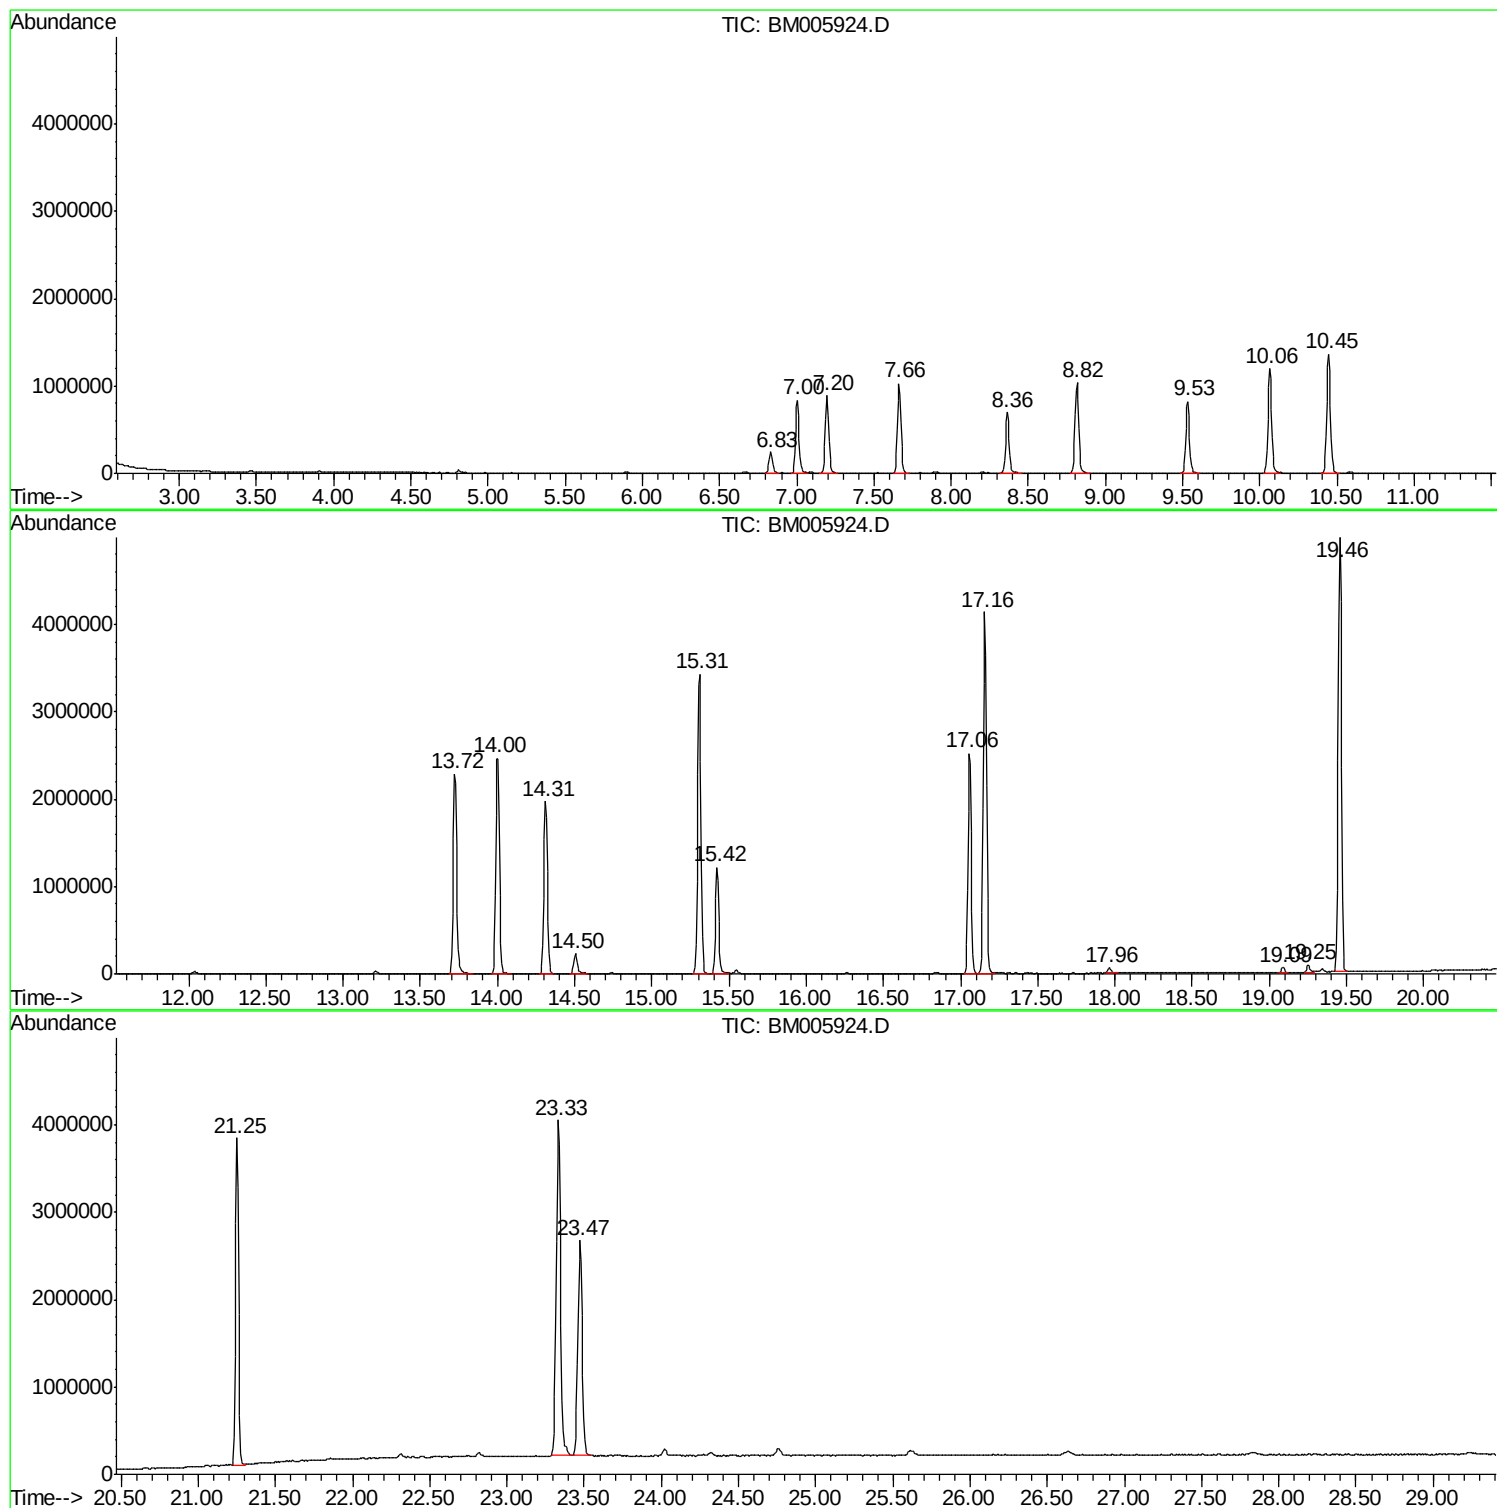

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005924.D
Acq On : 23 Jun 2016 08:36
Operator : UM/SJ
Sample : H3608-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC386

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005924.D
Acq On : 23 Jun 2016 08:36
Operator : UM/SJ
Sample : H3608-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC386

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc