

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005925.D
 Acq On : 23 Jun 2016 10:13
 Operator : UM/SJ
 Sample : H3608-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC387

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	714	722	731	rBV	273532	442538	5.88%	0.657%
2	7.004	744	751	763	rBV	888856	1428812	18.97%	2.122%
3	7.198	777	784	796	rBV	958504	1596814	21.20%	2.371%
4	7.663	855	863	873	rBV	1029688	1653150	21.95%	2.455%
5	8.363	971	982	992	rBV	748703	1254268	16.65%	1.862%
6	8.816	1051	1059	1072	rBV	1119237	1909302	25.35%	2.835%
7	9.534	1172	1181	1193	rBV	910484	1527717	20.28%	2.268%
8	10.063	1264	1271	1286	rBV	1273577	2237265	29.70%	3.322%
9	10.445	1329	1336	1349	rBV	1368531	2376429	31.55%	3.529%
10	13.727	1887	1894	1906	rBV	2318474	3583111	47.57%	5.320%
11	14.004	1933	1941	1953	rBV	2697284	4213387	55.94%	6.256%
12	14.310	1986	1993	2005	rBV2	1949768	3065323	40.70%	4.552%
13	14.504	2019	2026	2040	rBV2	253035	412283	5.47%	0.612%
14	15.310	2156	2163	2171	rBV	3428075	5281152	70.12%	7.842%
15	15.421	2176	2182	2196	rVV	1187033	1726553	22.92%	2.564%
16	17.057	2453	2460	2470	rBV2	2611331	3844051	51.04%	5.708%
17	17.157	2470	2477	2492	rVV	4064643	5979191	79.39%	8.878%
18	19.092	2800	2806	2810	rBV2	60953	94279	1.25%	0.140%
19	19.456	2862	2868	2876	rBV2	4886590	7034118	93.39%	10.445%
20	21.256	3168	3174	3184	rBV	3604341	5006602	66.47%	7.434%
21	23.339	3520	3528	3543	rVB2	3696164	7531699	100.00%	11.184%
22	23.474	3544	3551	3566	rVB	2521874	4942549	65.62%	7.339%
23	24.021	3640	3644	3650	rVB3	115526	205931	2.73%	0.306%


Sum of corrected areas: 67346524

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005925.D
Acq On : 23 Jun 2016 10:13
Operator : UM/SJ
Sample : H3608-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC387

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

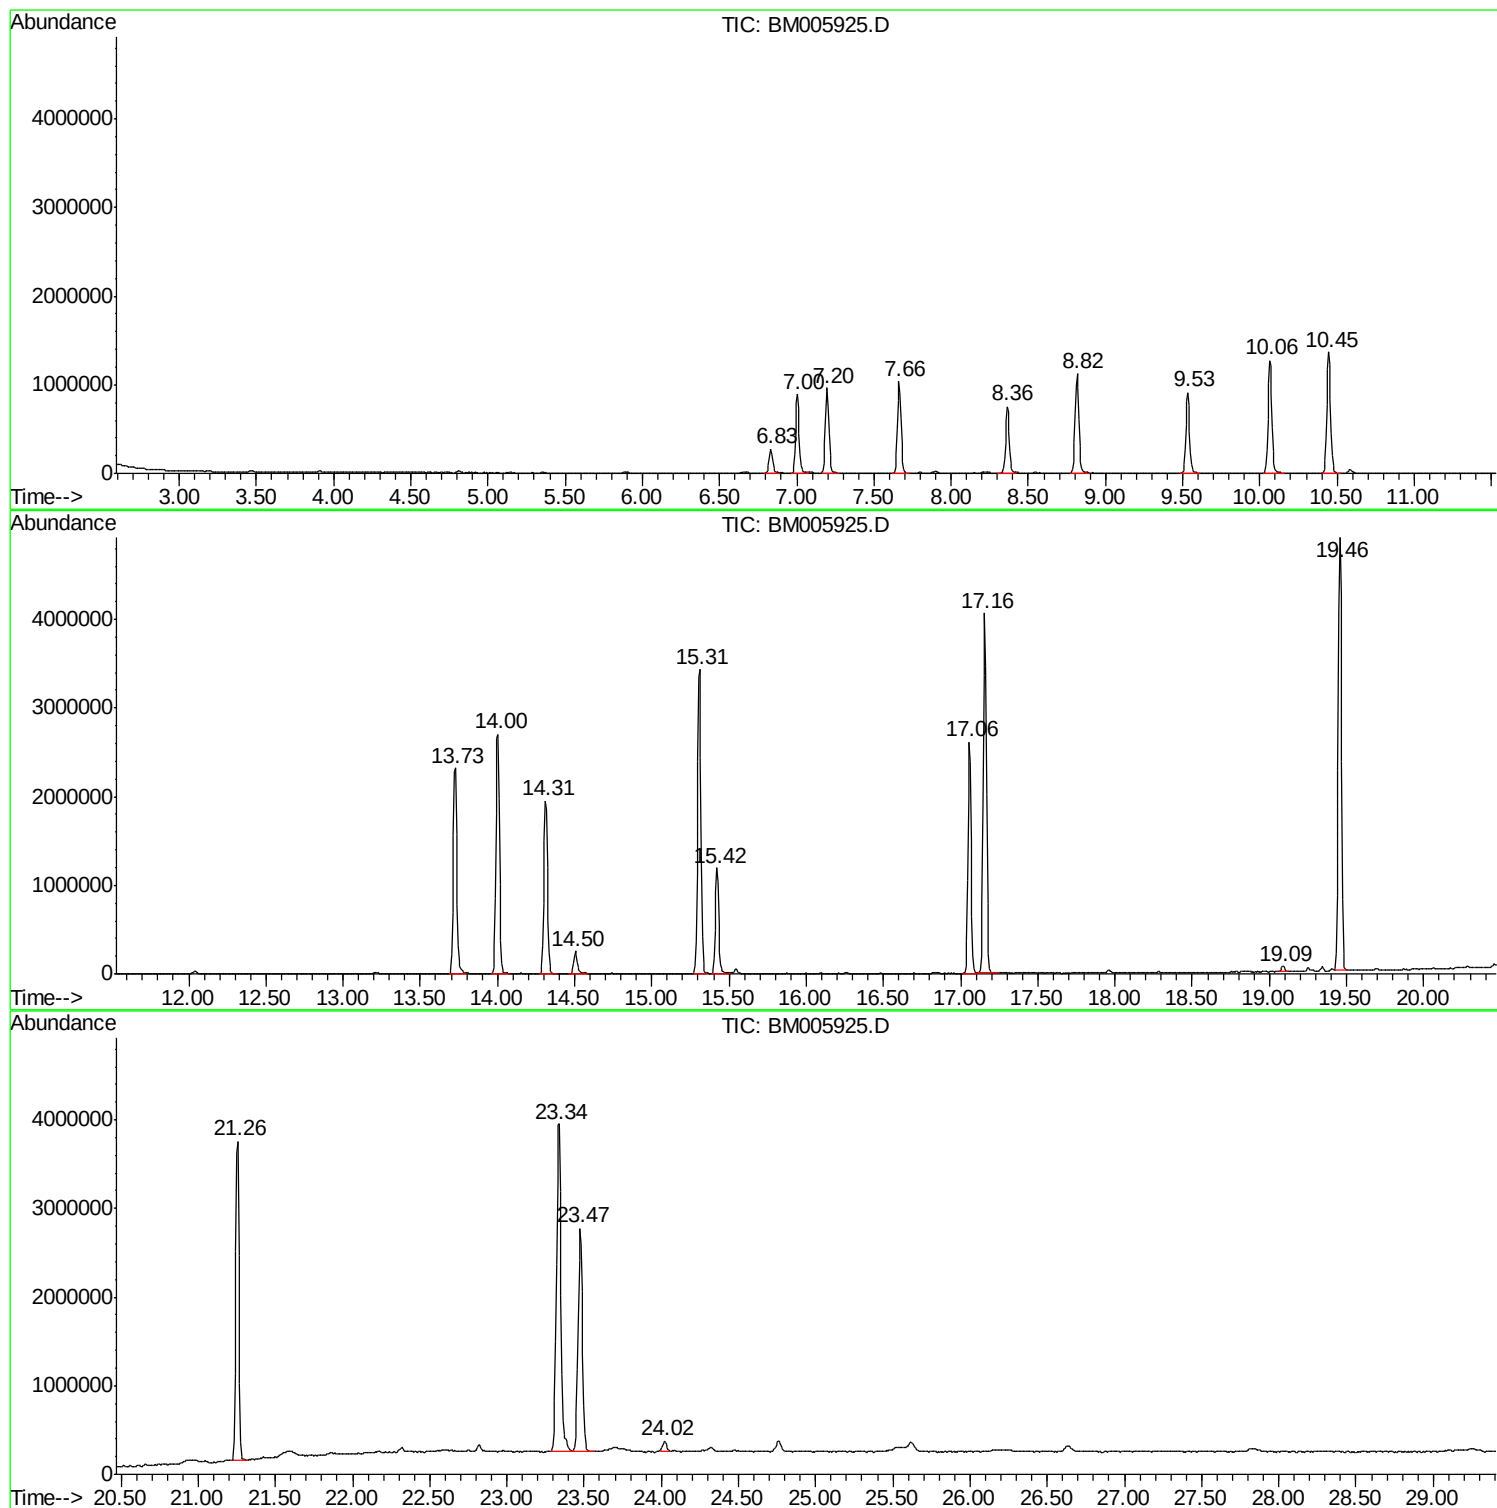

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005925.D
Acq On : 23 Jun 2016 10:13
Operator : UM/SJ
Sample : H3608-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC387

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005925.D
Acq On : 23 Jun 2016 10:13
Operator : UM/SJ
Sample : H3608-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC387

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc