

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
 Data File : BM005930.D
 Acq On : 23 Jun 2016 14:56
 Operator : UM/SJ
 Sample : H3612-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	715	722	735	rVB	561560	941379	32.85%	2.944%
2	7.004	744	751	763	rBV	439043	708262	24.71%	2.215%
3	7.192	777	783	794	rBV	562158	944901	32.97%	2.955%
4	7.663	856	863	871	rBV	571361	916524	31.98%	2.867%
5	8.363	973	982	995	rBV	675695	1123725	39.21%	3.515%
6	8.816	1050	1059	1072	rBV	499890	871192	30.40%	2.725%
7	9.534	1174	1181	1196	rVB	370517	651072	22.72%	2.036%
8	10.063	1265	1271	1285	rVB	633090	1068442	37.28%	3.342%
9	10.445	1329	1336	1345	rBV	712033	1256747	43.85%	3.931%
10	10.581	1350	1359	1374	rBV	590034	1078543	37.63%	3.373%
11	13.722	1887	1893	1898	rBV	963441	1395296	48.68%	4.364%
12	13.769	1898	1901	1909	rVB	317502	452420	15.79%	1.415%
13	13.998	1933	1940	1950	rBV	1120599	1708588	59.61%	5.344%
14	14.310	1986	1993	2004	rVB2	938346	1472144	51.36%	4.605%
15	14.504	2020	2026	2035	rBV	299766	480319	16.76%	1.502%
16	15.304	2156	2162	2170	rBV	1442340	2125770	74.17%	6.649%
17	15.421	2175	2182	2190	rBV	270288	389384	13.59%	1.218%
18	16.039	2282	2287	2300	rBV3	16665	37043	1.29%	0.116%
19	17.057	2454	2460	2469	rBV2	1185655	1688329	58.91%	5.281%
20	17.157	2470	2477	2488	rBV	1562782	2243926	78.29%	7.018%
21	17.962	2609	2614	2620	rBV4	34550	55744	1.94%	0.174%
22	19.456	2861	2868	2877	rBV	1913788	2698535	94.15%	8.440%
23	20.974	3122	3126	3129	rBV4	49561	80135	2.80%	0.251%
24	21.250	3167	3173	3181	rBV	1714734	2216042	77.32%	6.931%
25	22.815	3435	3439	3444	rBV	90161	135607	4.73%	0.424%
26	23.327	3519	3526	3533	rBV2	1518766	2866115	100.00%	8.965%
27	23.468	3543	3550	3559	rBV	1149925	2202138	76.83%	6.888%
28	24.015	3639	3643	3650	rVB2	89148	163330	5.70%	0.511%


Sum of corrected areas: 31971652

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062216\
Data File : BM005930.D
Acq On : 23 Jun 2016 14:56
Operator : UM/SJ
Sample : H3612-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
D9Z27

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

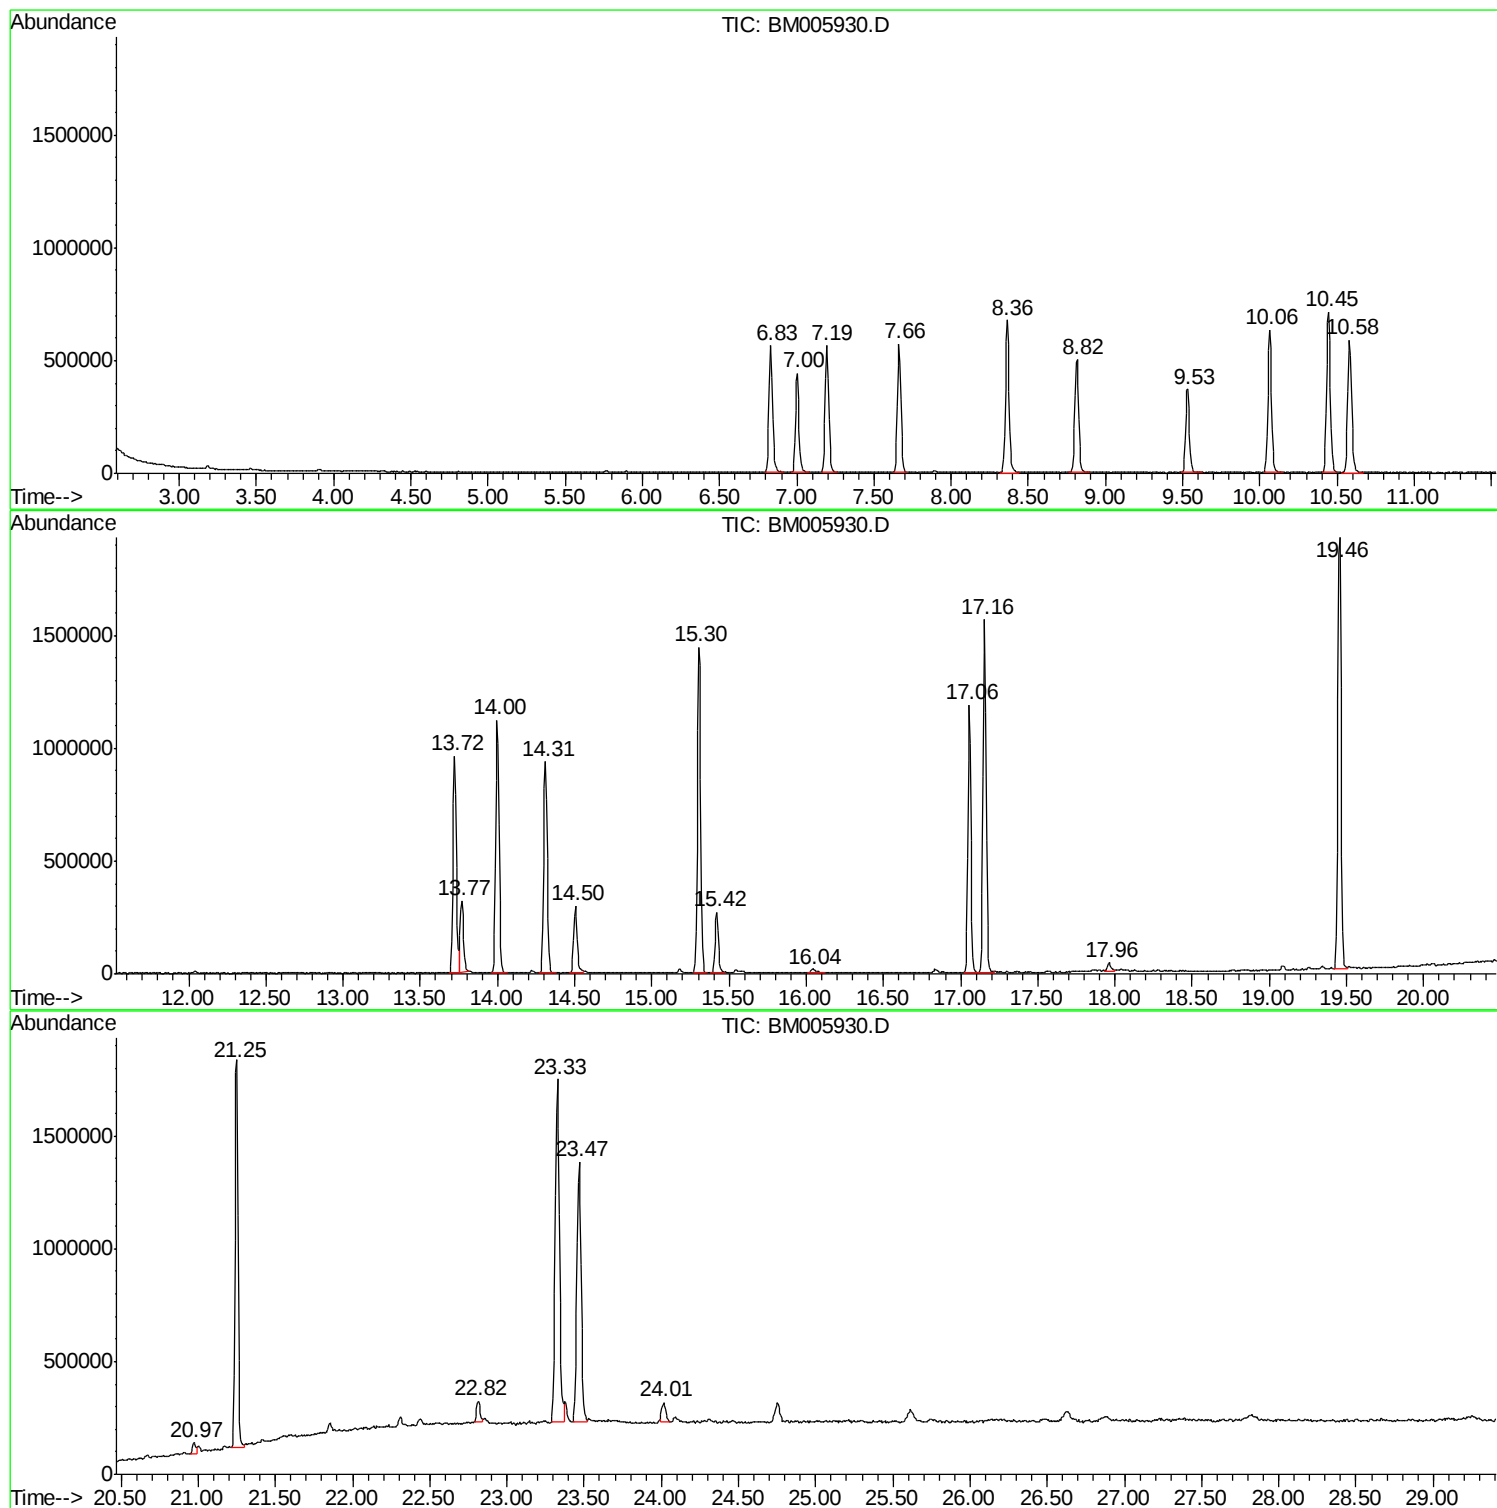

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005930.D
Acq On : 23 Jun 2016 14:56
Operator : UM/SJ
Sample : H3612-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062216\
Data File : BM005930.D
Acq On : 23 Jun 2016 14:56
Operator : UM/SJ
Sample : H3612-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z27

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc