

Data File : BM010665.D
Acq On : 22 Jun 2017 18:21
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD02044

Quant Time: Jun 23 04:06:23 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 23 01:03:57 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	63121	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	291256	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.12	164	204830	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.87	188	531861	20.00	ng/ul	0.00
75) Chrysene-d12	21.09	240	615533	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	490065	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	9001	8.17	ng/uL	0.00
5) Phenol-d5	6.65	99	104901	17.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	59270	17.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	81592	19.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	94496	18.95	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	40531	19.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	49819	20.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	101847	20.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	117902	22.20	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	362899	20.18	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	415777	19.88	ng/ul	0.00
51) 4-Nitrophenol-d4	14.33	143	60546	19.13	ng/ul	0.00
57) Fluorene-d10	15.12	176	307034	19.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	67679	20.72	ng/ul	0.00
70) Anthracene-d10	16.97	188	505907	19.70	ng/ul	0.00
76) Pyrene-d10	19.27	212	588472	20.58	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.09	264	478249	20.19	ng/ul	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.10	88	9951	8.09	ng/uL#	40
4) Benzaldehyde	6.62	77	75127	21.23	ng/ul	92
6) Phenol	6.67	94	109211	17.63	ng/ul	96
8) Bis(2-Chloroethyl)ether	6.90	93	80925	17.95	ng/ul	91
10) 2-Chlorophenol	7.03	128	79131	18.77	ng/ul	98
11) 2-Methylphenol	7.90	108	86816	18.39	ng/ul	97
12) 2,2'-oxybis(1-Chloropropan	8.00	45	50195	15.95	ng/ul#	94
14) Acetophenone	8.27	105	151024	18.55	ng/ul	93
15) N-Nitroso-di-n-propylamine	8.27	70	79277	18.07	ng/ul	95
16) 4-Methylphenol	8.23	108	98498	18.97	ng/ul	96
17) Hexachloroethane	8.52	117	38335	20.45	ng/ul#	79
20) Nitrobenzene	8.65	77	119174	19.66	ng/ul	97
21) Isophorone	9.17	82	217147	18.02	ng/ul	96
23) 2-Nitrophenol	9.35	139	50993	20.08	ng/ul	91
24) 2,4-Dimethylphenol	9.42	107	125916	19.50	ng/ul	98
25) Bis(2-Chloroethoxy)methane	9.66	93	120987	18.10	ng/ul	95
27) 2,4-Dichlorophenol	9.87	162	98522	20.08	ng/ul#	87
28) Naphthalene	10.27	128	281609	19.43	ng/ul	97
30) 4-Chloroaniline	10.39	127	114366	21.41	ng/ul	98
31) Hexachlorobutadiene	10.57	225	78697	21.27	ng/ul	93
33) 4-Chloro-3-methylphenol	11.52	107	123263	19.70	ng/ul	94
34) 2-Methylnaphthalene	11.90	142	229717	19.72	ng/ul	97
36) 1,2,4,5-Tetrachlorobenzene	12.27	216	149558	20.69	ng/ul#	96

Data File : BM010665.D
Acq On : 22 Jun 2017 18:21
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD02044

Quant Time: Jun 23 04:06:23 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 23 01:03:57 2017
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) Hexachlorocyclopentadiene	12.26	237	83574	20.11	ng/ul	96
38) 2,4,6-Trichlorophenol	12.52	196	100918	20.44	ng/ul	94
39) 2,4,5-Trichlorophenol	12.59	196	104510	20.50	ng/ul	96
40) 1,1'-Biphenyl	12.94	154	321630	20.08	ng/ul	97
41) 2-Chloronaphthalene	12.97	162	248978	19.76	ng/ul	95
42) 2-Nitroaniline	13.19	65	77250	20.96	ng/ul	96
44) Dimethylphthalate	13.59	163	349000	19.80	ng/ul	99
45) 2,6-Dinitrotoluene	13.70	165	67905	22.24	ng/ul#	78
47) Acenaphthylene	13.83	152	389807	19.57	ng/ul	99
48) 3-Nitroaniline	14.03	138	63089	20.49	ng/ul	98
49) Acenaphthene	14.18	153	265131	19.73	ng/ul	97
50) 2,4-Dinitrophenol	14.23	184	45457	20.56	ng/ul#	77
52) 4-Nitrophenol	14.34	109	94128	23.45	ng/ul#	82
53) Dibenzofuran	14.52	168	406794	19.99	ng/ul	91
54) 2,4-Dinitrotoluene	14.49	165	103015	21.75	ng/ul#	86
55) 2,3,4,6-Tetrachlorophenol	14.74	232	105464	20.45	ng/ul#	85
56) Diethylphthalate	14.97	149	367293	19.81	ng/ul	96
58) Fluorene	15.17	166	332235	19.50	ng/ul	98
59) 4-Chlorophenyl-phenylether	15.17	204	187624	20.26	ng/ul#	88
60) 4-Nitroaniline	15.20	138	72766	20.01	ng/ul	98
63) 4,6-Dinitro-2-methylphenol	15.26	198	72493	20.83	ng/ul#	98
64) N-Nitrosodiphenylamine	15.39	169	287451	19.49	ng/ul	95
65) 4-Bromophenyl-phenylether	16.07	248	120889	19.85	ng/ul	90
66) Hexachlorobenzene	16.17	284	127781	19.92	ng/ul#	82
67) Atrazine	16.36	200	131087	21.10	ng/ul	95
68) Pentachlorophenol	16.52	266	85366	18.88	ng/ul	99
69) Phenanthrene	16.91	178	549624	19.44	ng/ul	98
71) Anthracene	17.00	178	568278	19.51	ng/ul	99
72) Carbazole	17.27	167	486625	19.15	ng/ul	98
73) Di-n-butylphthalate	17.86	149	611422	18.92	ng/ul	99
74) Fluoranthene	18.94	202	705635	19.36	ng/ul#	97
77) Pyrene	19.30	202	721424	20.29	ng/ul#	97
78) Butylbenzylphthalate	20.24	149	279668	20.92	ng/ul	96
79) 3,3'-Dichlorobenzidine	21.01	252	247382	20.09	ng/ul#	98
80) Benzo(a)anthracene	21.07	228	726880	20.28	ng/ul	98
81) Bis(2-ethylhexyl)phthalate	21.03	149	408259	20.02	ng/ul#	99
82) Chrysene	21.12	228	643049	20.12	ng/ul	98
84) Di-n-octyl phthalate	21.88	149	672850	19.65	ng/ul#	95
85) Benzo(b)fluoranthene	22.59	252	670558	21.08	ng/ul	98
86) Benzo(k)fluoranthene	22.63	252	609192	20.20	ng/ul	98
88) Benzo(a)pyrene	23.13	252	587391	20.06	ng/ul	96
89) Indeno(1,2,3-cd)pyrene	25.33	276	573763	18.89	ng/ul	97
90) Dibenzo(a,h)anthracene	25.35	278	470583	18.59	ng/ul	99
91) Benzo(g,h,i)perylene	25.97	276	451432	18.67	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

ALS Vial : 2 Sample Multiplier: 1

SSTD02044

Response via : Initial Calibration

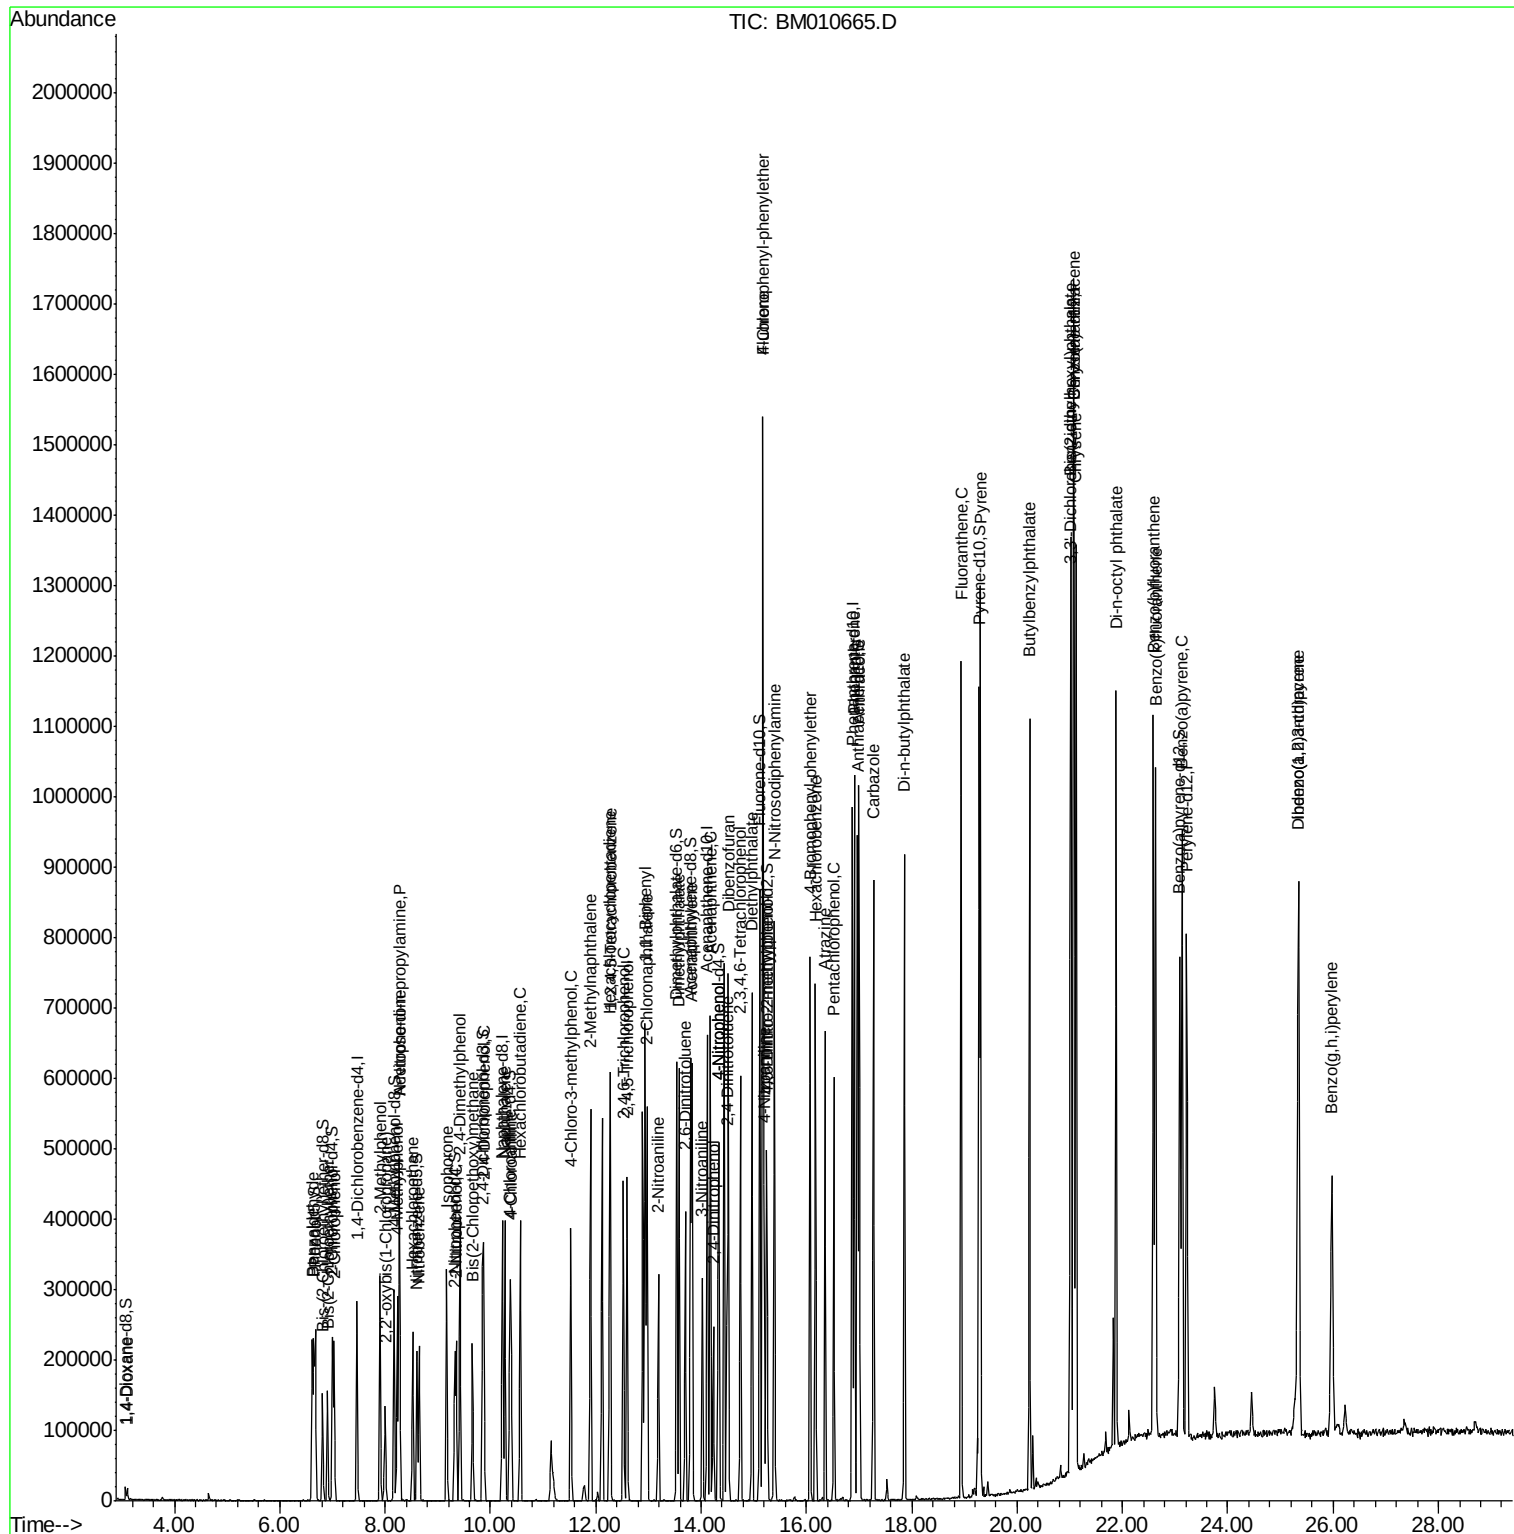

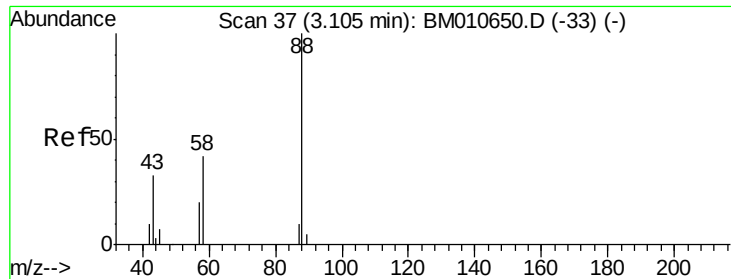

#2

1,4-Dioxane

Concen: 8.09 ng/uL

RT: 3.10 min Scan# 37

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044


Tgt Ion: 88 Resp: 9951

Ion Ratio Lower Upper

88 100

43 24.7 1.1 1.7#




58 48.1 0.0 0.0#

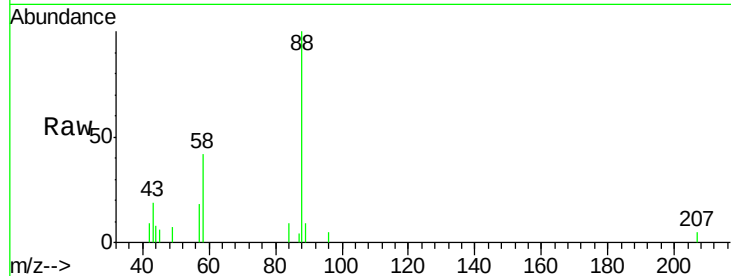

Abundance Ion 88.00 (87.70 to 88.70): BM010665.D (-3)

Ion 43.00 (42.70 to 43.70): BM010665.D (-3)

Ion 58.00 (57.70 to 58.70): BM010665.D (-3)

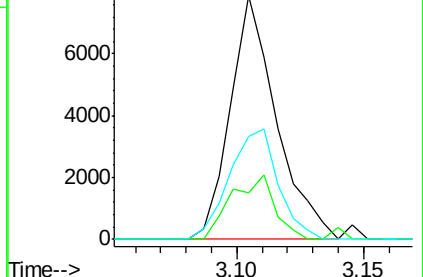

#4

Benzaldehyde

Concen: 21.23 ng/uL

RT: 6.62 min Scan# 635

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21


Tgt Ion: 77 Resp: 75127

Ion Ratio Lower Upper

77 100

105 90.3 66.1 99.1



106 91.8 67.8 101.6




Abundance Ion 77.00 (76.70 to 77.70): BM010665.D (-6)

Ion 105.00 (104.70 to 105.70): BM010665.D (-6)

Ion 106.00 (105.70 to 106.70): BM010665.D (-6)

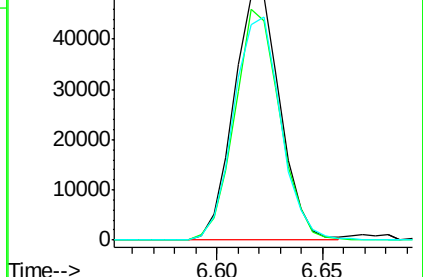



#6

Phenol

Concen: 17.63 ng/ul

RT: 6.67 min Scan# 644

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044


Tgt Ion: 94 Resp: 109211

Ion Ratio Lower Upper

94 100

65 34.9 28.2 42.4




66 54.6 47.2 70.8

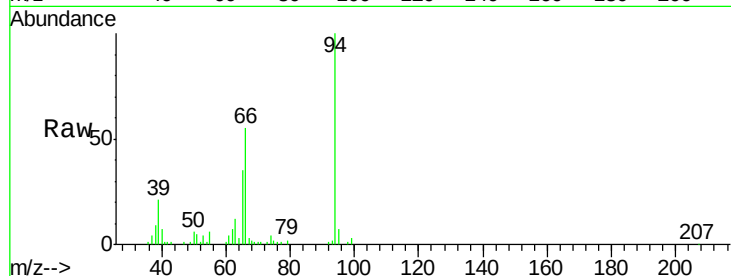

Abundance Ion 94.00 (93.70 to 94.70): BM010665.D (-610) (-)

Ion 65.00 (64.70 to 65.70): BM010665.D (-610) (-)

Ion 66.00 (65.70 to 66.70): BM010665.D (-610) (-)

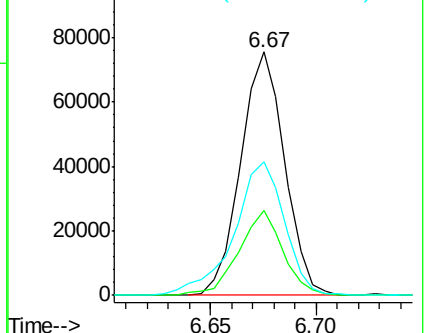

#8

Bis(2-Chloroethyl)ether

Concen: 17.95 ng/ul

RT: 6.90 min Scan# 683

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21


Tgt Ion: 93 Resp: 80925

Ion Ratio Lower Upper

93 100

63 61.6 57.3 85.9



95 31.2 26.6 39.8




Abundance Ion 93.00 (92.70 to 93.70): BM010665.D (-649) (-)

Ion 63.00 (62.70 to 63.70): BM010665.D (-649) (-)

Ion 95.00 (94.70 to 95.70): BM010665.D (-649) (-)

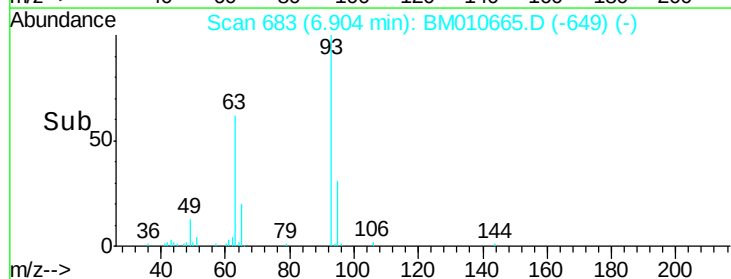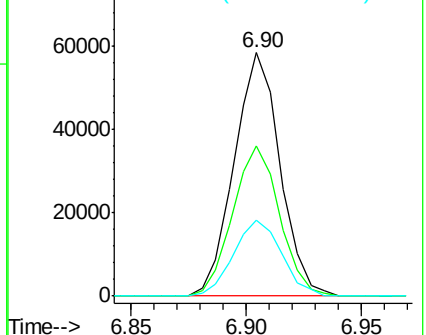

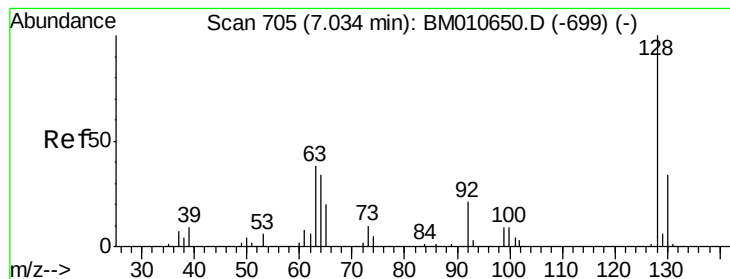

#10

2-Chlorophenol

Concen: 18.77 ng/ul

RT: 7.03 min Scan# 705

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044


Tgt Ion:128 Resp: 79131

Ion Ratio Lower Upper

128 100

64 46.4 38.0 57.0




130 31.3 24.4 36.6

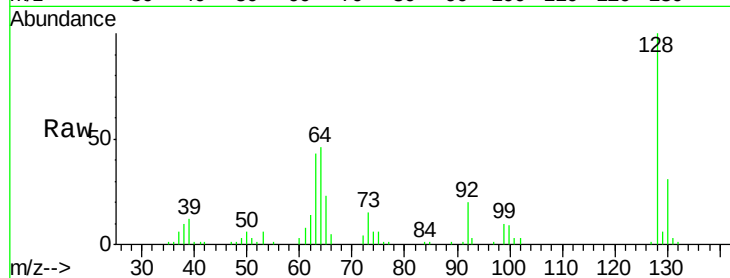

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 130.00 (129.70 to 130.70): E

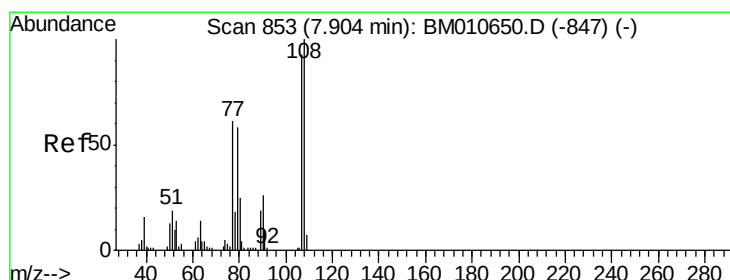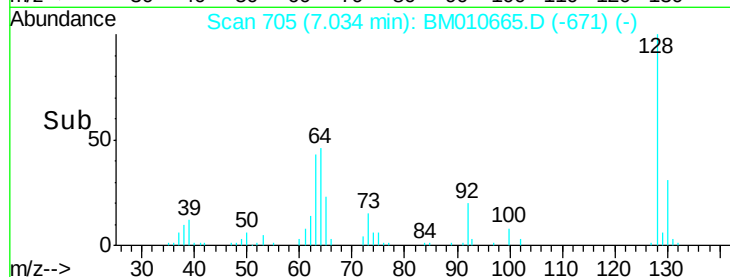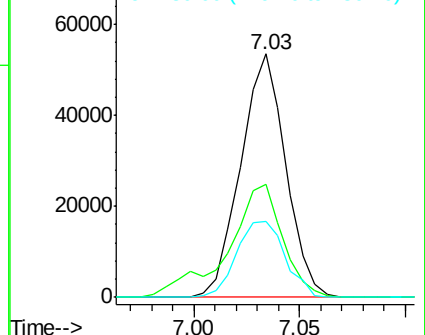

#11

2-Methylphenol

Concen: 18.39 ng/ul

RT: 7.90 min Scan# 853

Delta R.T. -0.00 min

Lab File: BM010665.D


Acq: 22 Jun 2017 18:21

Tgt Ion:108 Resp: 86816

Ion Ratio Lower Upper



108 100


107 87.9 72.6 108.8

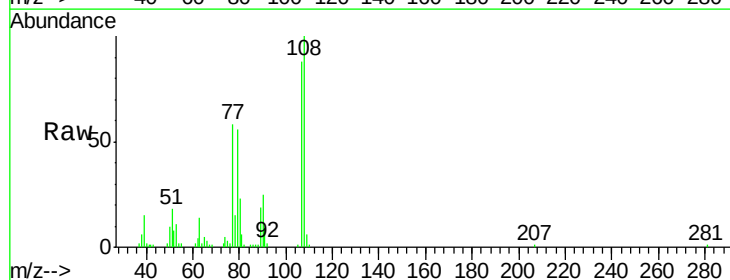

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E



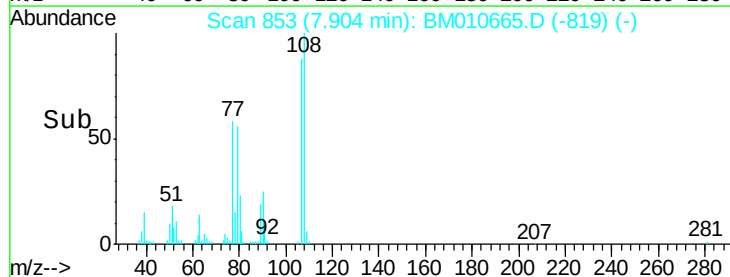
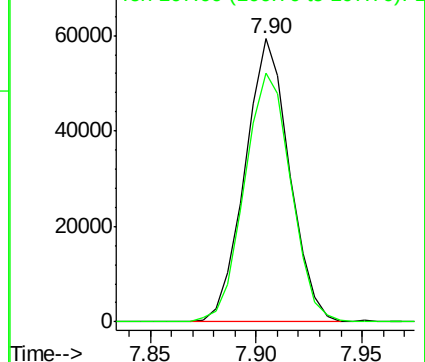




#12
 2,2'-oxybis(1-chloropropane)
 Concen: 15.95 ng/ul
 RT: 8.00 min Scan# 870
 Delta R.T. -0.00 min
 Lab File: BM010665.D
 Acq: 22 Jun 2017 18:21




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02044


Tgt Ion: 45 Resp: 50195
 Ion Ratio Lower Upper
 45 100
 77 28.6 21.8 32.6
 79 27.3 17.6 26.4#

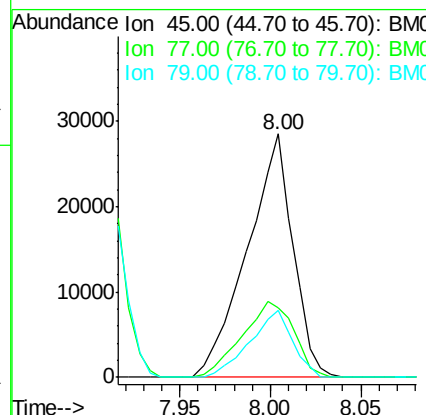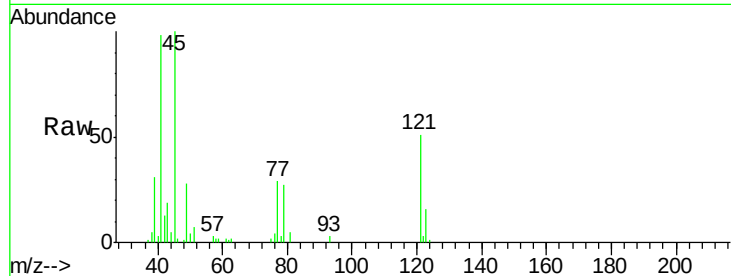

#14
 Acetophenone
 Concen: 18.55 ng/ul
 RT: 8.27 min Scan# 916
 Delta R.T. -0.00 min
 Lab File: BM010665.D
 Acq: 22 Jun 2017 18:21

Tgt Ion: 105 Resp: 151024
 Ion Ratio Lower Upper
 105 100
 77 86.1 74.2 111.4
 51 24.7 23.4 35.2

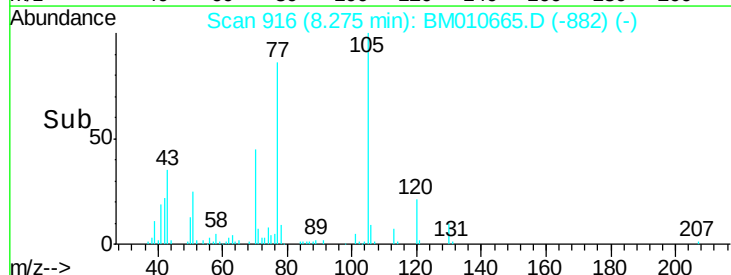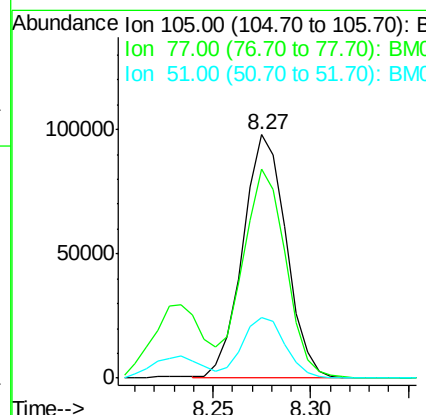

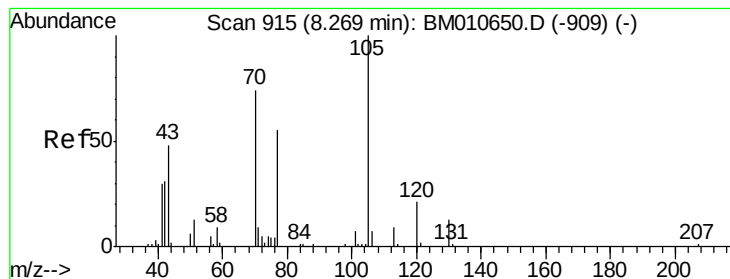

#15

N-Nitroso-di-n-propylamine

Concen: 18.07 ng/ul

RT: 8.27 min Scan# 915

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044

Tgt Ion: 70 Resp: 79277


Ion Ratio Lower Upper

70 100

42 46.0 41.1 61.7

101 9.4 6.7 10.1

130 18.3 14.6 22.0



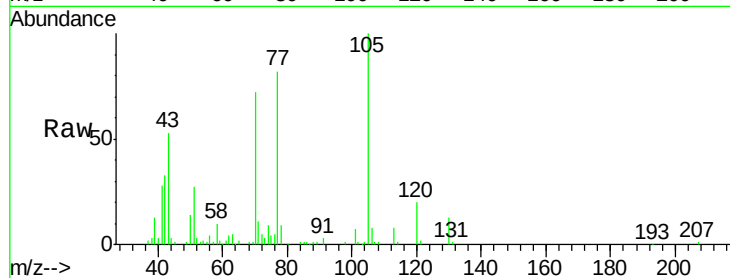


Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

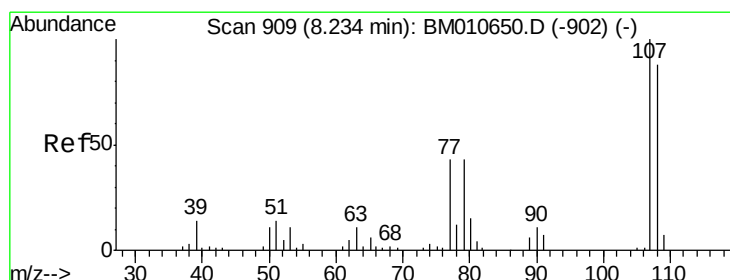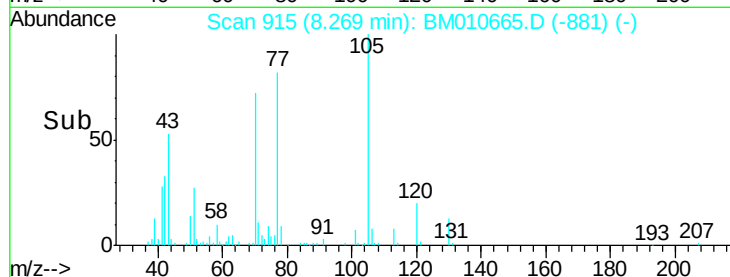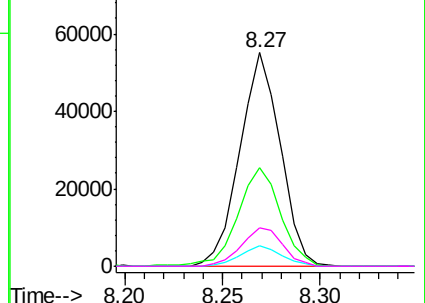

#16

4-Methylphenol

Concen: 18.97 ng/ul

RT: 8.23 min Scan# 909

Delta R.T. -0.00 min

Lab File: BM010665.D


Acq: 22 Jun 2017 18:21

Tgt Ion: 108 Resp: 98498

Ion Ratio Lower Upper



108 100


107 110.6 84.9 127.3

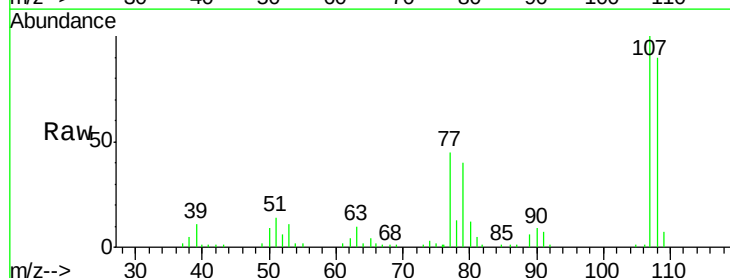

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

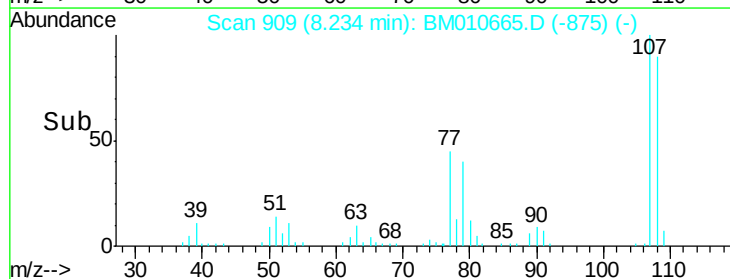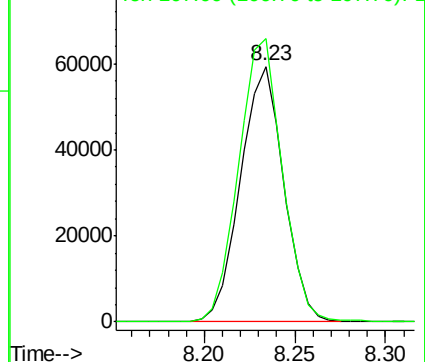


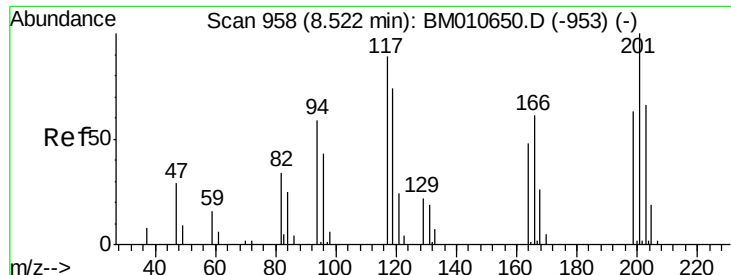




#17
Hexachloroethane
Concen: 20.45 ng/ul
RT: 8.52 min Scan# 958
Delta R.T. -0.00 min
Lab File: BM010665.D
Acq: 22 Jun 2017 18:21

Instrument :
BNA_M
ClientSampleId :
SSTD02044

Tgt Ion:117 Resp: 38335
Ion Ratio Lower Upper
117 100
201 106.5 111.6 167.4#
199 73.8 67.8 101.6

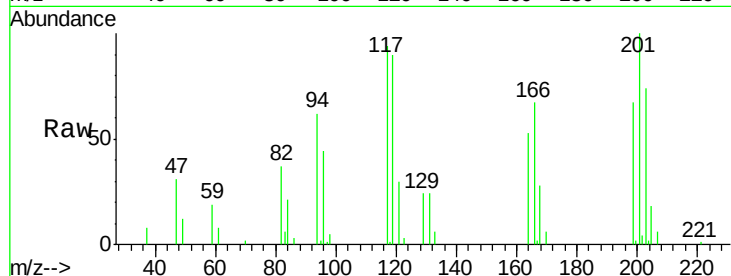


Abundance Ion 117.00 (116.70 to 117.70): E
Ion 201.00 (200.70 to 201.70): E
Ion 199.00 (198.70 to 199.70): E


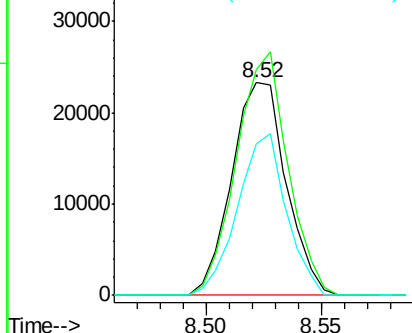



#20
Nitrobenzene
Concen: 19.66 ng/ul
RT: 8.65 min Scan# 980
Delta R.T. 0.01 min
Lab File: BM010665.D
Acq: 22 Jun 2017 18:21

Tgt Ion: 77 Resp: 119174
Ion Ratio Lower Upper
77 100
123 37.5 31.0 46.6
65 13.3 12.2 18.2

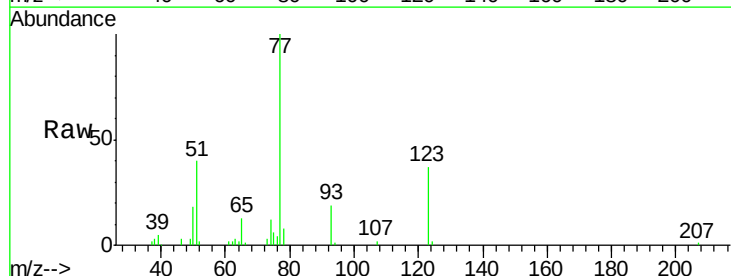

Abundance Ion 77.00 (76.70 to 77.70): BM0
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BM0

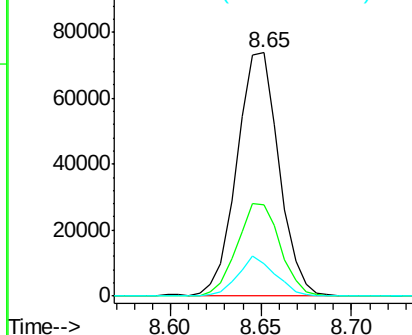

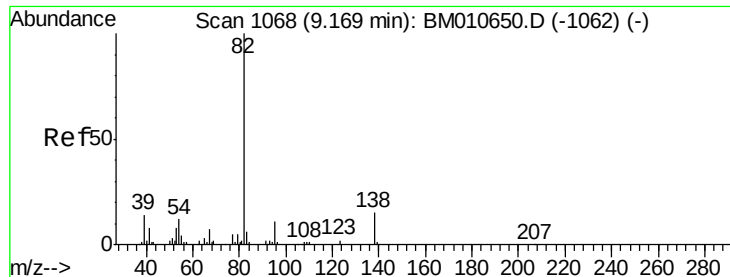

#21

Isophorone

Concen: 18.02 ng/ul

RT: 9.17 min Scan# 1068

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044


Tgt Ion: 82 Resp: 217147

Ion Ratio Lower Upper

82 100

95 10.6 7.8 11.8

138 17.0 11.9 17.9



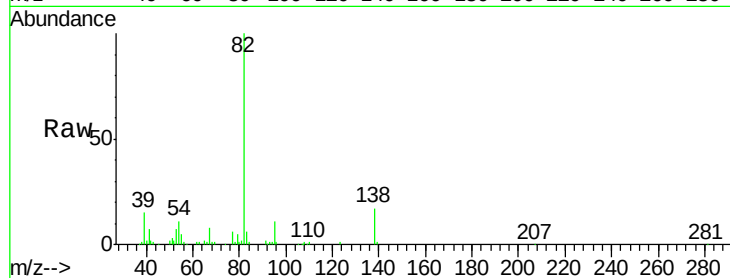


Abundance Ion 82.00 (81.70 to 82.70): BM010665.D (-1062) (-)

Ion 95.00 (94.70 to 95.70): BM010665.D (-1062) (-)

Ion 138.00 (137.70 to 138.70): BM010665.D (-1062) (-)

Time-->

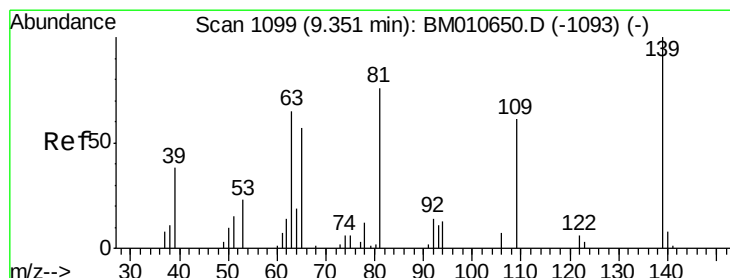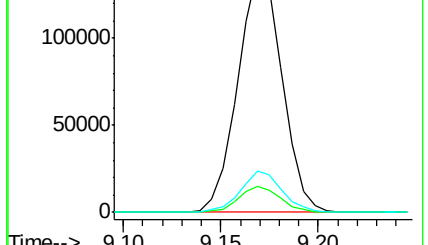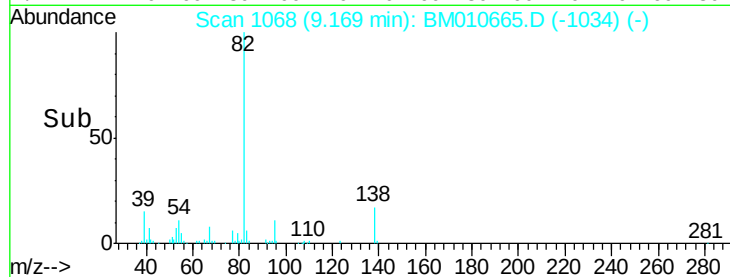

#23

2-Nitrophenol

Concen: 20.08 ng/ul

RT: 9.35 min Scan# 1099

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21


Tgt Ion: 139 Resp: 50993

Ion Ratio Lower Upper

139 100

65 62.7 55.4 83.0

109 60.3 42.2 63.2


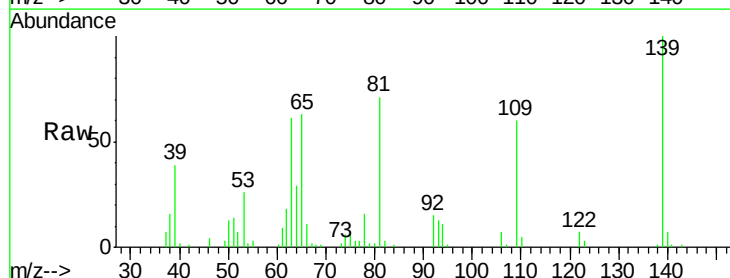



Abundance Ion 139.00 (138.70 to 139.70): BM010665.D (-1093) (-)

Ion 65.00 (64.70 to 65.70): BM010665.D (-1093) (-)

Ion 109.00 (108.70 to 109.70): BM010665.D (-1093) (-)

Time-->

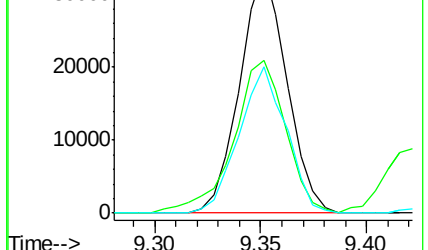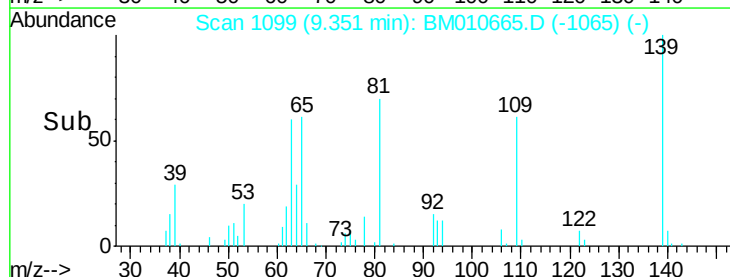

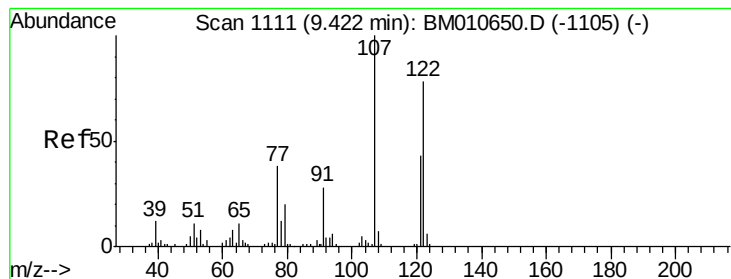

#24

2,4-Dimethylphenol

Concen: 19.50 ng/ul

RT: 9.42 min Scan# 1111

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044





Tgt Ion: 107 Resp: 125916

Ion Ratio Lower Upper

107 100

121 41.4 31.9 47.9

122 73.5 57.8 86.6

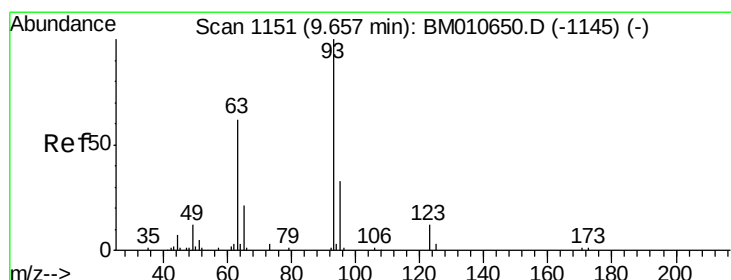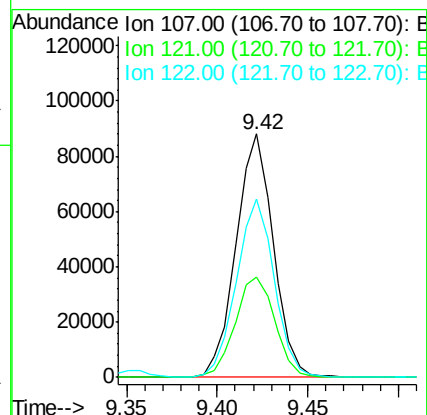

#25

Bis(2-Chloroethoxy)methane

Concen: 18.10 ng/ul

RT: 9.66 min Scan# 1151

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21




Tgt Ion: 93 Resp: 120987


Ion Ratio Lower Upper

93 100

95 32.3 28.5 42.7

123 9.7 8.9 13.3

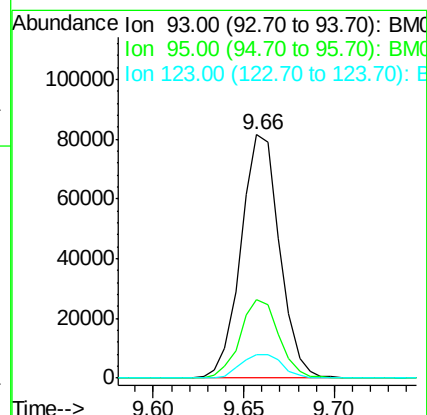


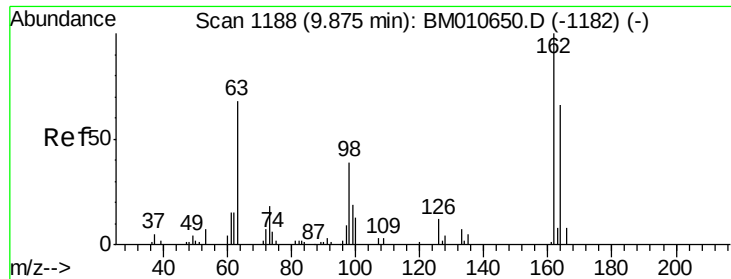




#27
2,4-Dichlorophenol
Concen: 20.08 ng/ul
RT: 9.87 min Scan# 1188
Delta R.T. -0.00 min
Lab File: BM010665.D
Acq: 22 Jun 2017 18:21

Instrument :
BNA_M
ClientSampleId :
SSTD02044

Tgt Ion:162 Resp: 98522
Ion Ratio Lower Upper
162 100
164 68.2 47.8 71.6
98 36.8 23.0 34.4#




Abundance Ion 162.00 (161.70 to 162.70): E
Ion 164.00 (163.70 to 164.70): E
Ion 98.00 (97.70 to 98.70): BM


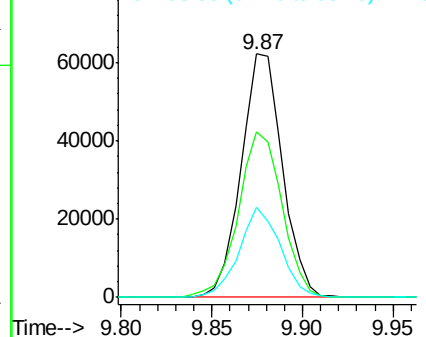



#28
Naphthalene
Concen: 19.43 ng/ul
RT: 10.27 min Scan# 1256
Delta R.T. -0.00 min
Lab File: BM010665.D
Acq: 22 Jun 2017 18:21

Tgt Ion:128 Resp: 281609
Ion Ratio Lower Upper
128 100
129 9.6 8.8 13.2
127 14.2 10.6 16.0



Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E




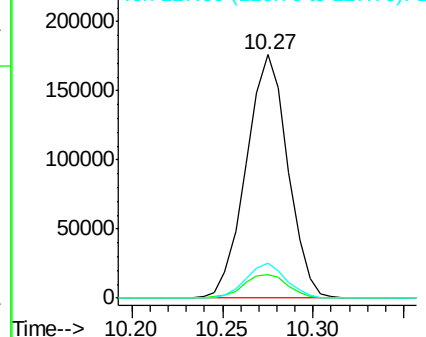




#30
4-Chloroaniline
Concen: 21.41 ng/ul
RT: 10.39 min Scan# 1276
Delta R.T. -0.00 min
Lab File: BM010665.D
Acq: 22 Jun 2017 18:21




Instrument :
BNA_M
ClientSampleId :
SSTD02044


Tgt Ion:127 Resp: 114366
Ion Ratio Lower Upper
127 100
129 34.3 28.4 42.6

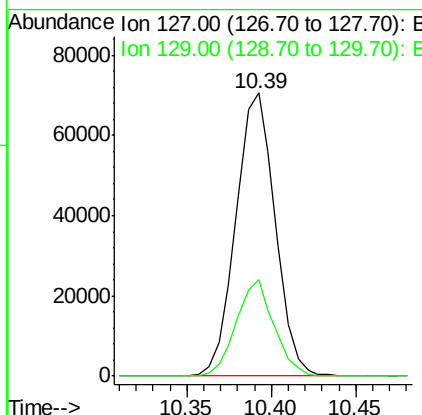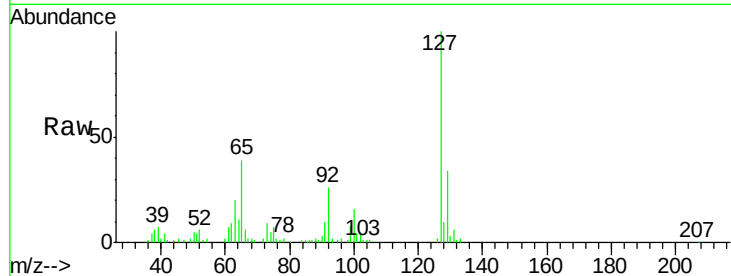

#31
Hexachlorobutadiene
Concen: 21.27 ng/ul
RT: 10.57 min Scan# 1306
Delta R.T. 0.01 min
Lab File: BM010665.D
Acq: 22 Jun 2017 18:21

Tgt Ion:225 Resp: 78697
Ion Ratio Lower Upper
225 100
223 67.2 49.4 74.2
227 62.6 45.4 68.2



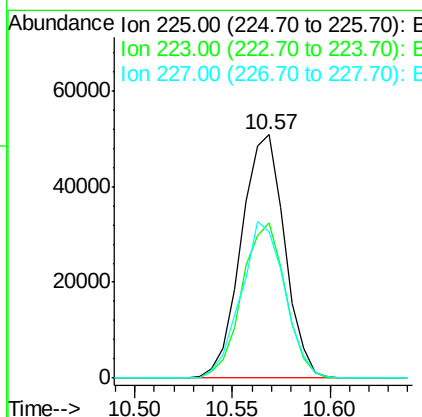
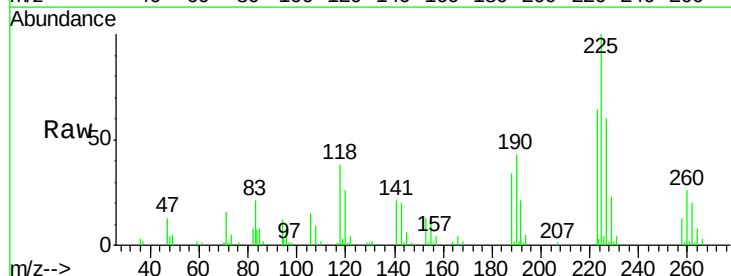




#33
 4-Chloro-3-methylphenol
 Concen: 19.70 ng/ul
 RT: 11.52 min Scan# 1468
 Delta R.T. -0.00 min
 Lab File: BM010665.D
 Acq: 22 Jun 2017 18:21




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02044


Tgt Ion	Ratio	Lower	Upper
107	100		
144	24.1	20.4	30.6
142	69.1	60.5	90.7

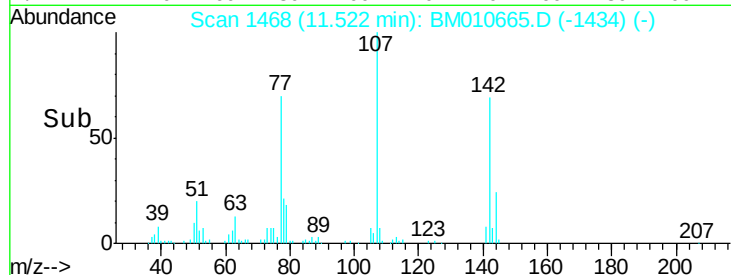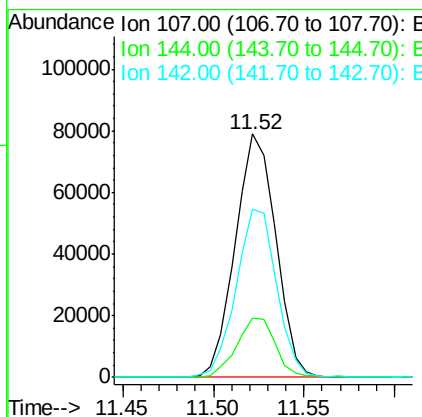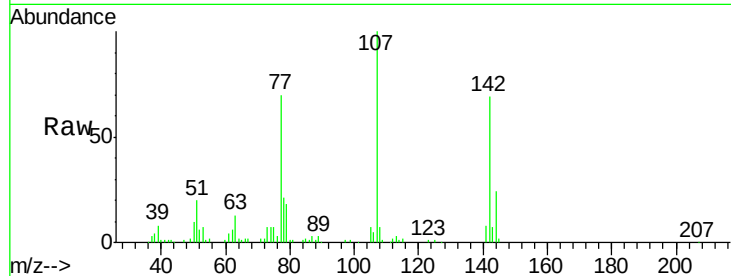

#34
 2-Methylnaphthalene
 Concen: 19.72 ng/ul
 RT: 11.90 min Scan# 1532
 Delta R.T. -0.00 min
 Lab File: BM010665.D
 Acq: 22 Jun 2017 18:21

Tgt Ion	Ratio	Lower	Upper
142	100		
141	90.2	74.1	111.1

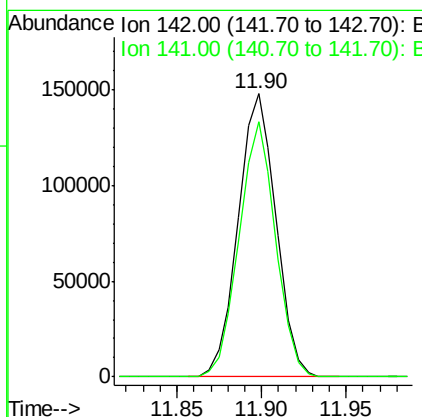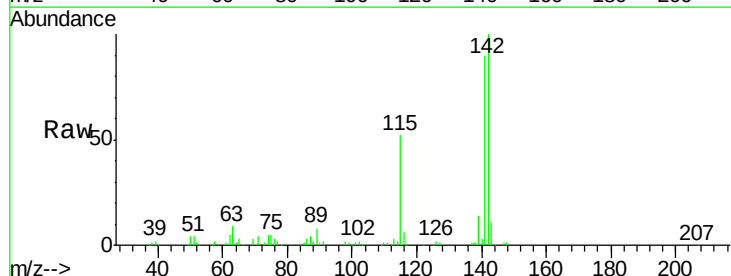

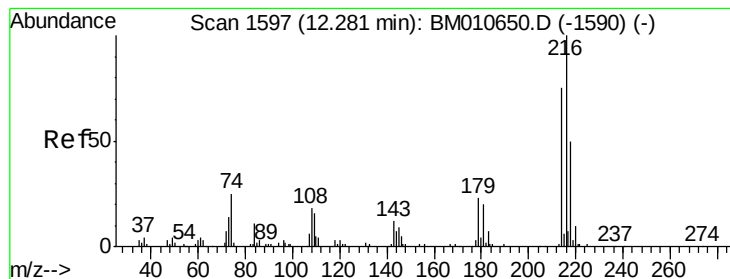

#36

1,2,4,5-Tetrachlorobenzene

Concen: 20.69 ng/ul

RT: 12.27 min Scan# 1596

Delta R.T. -0.01 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21

Instrument :

BNA_M

ClientSampleId :

SSTD02044

Tgt Ion:216 Resp: 149558


Ion Ratio Lower Upper

216 100

214 77.5 60.6 90.8

179 20.4 17.5 26.3

108 20.3 11.3 16.9#



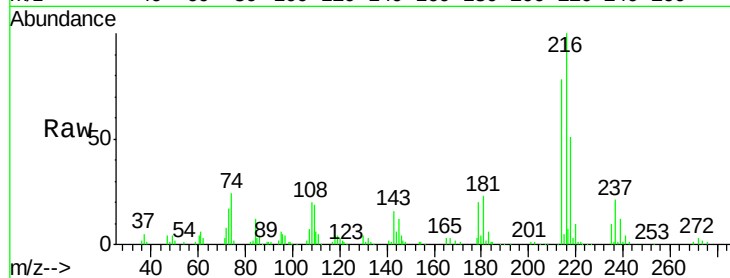


Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

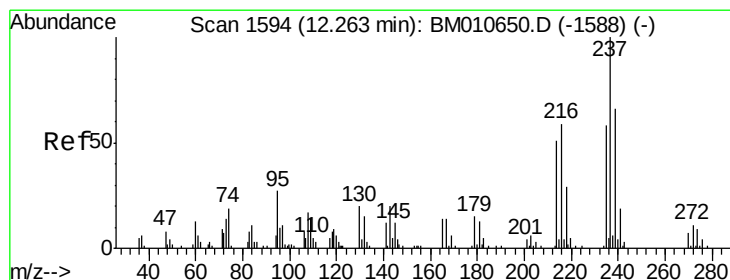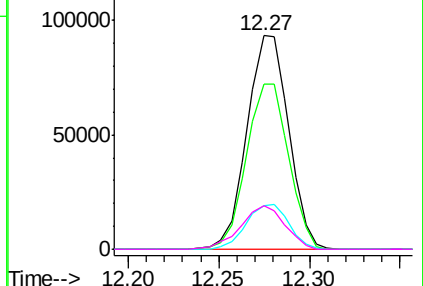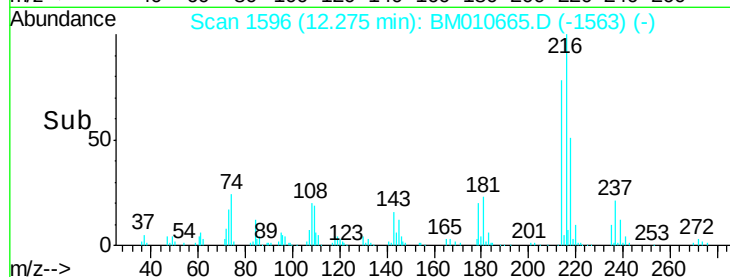

#37

Hexachlorocyclopentadiene

Concen: 20.11 ng/ul

RT: 12.26 min Scan# 1594

Delta R.T. -0.00 min

Lab File: BM010665.D

Acq: 22 Jun 2017 18:21


Tgt Ion:237 Resp: 83574

Ion Ratio Lower Upper

237 100

235 59.5 50.2 75.4


272 15.1 11.0 16.6

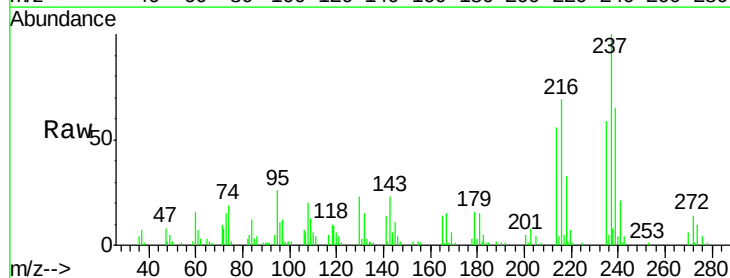

Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E

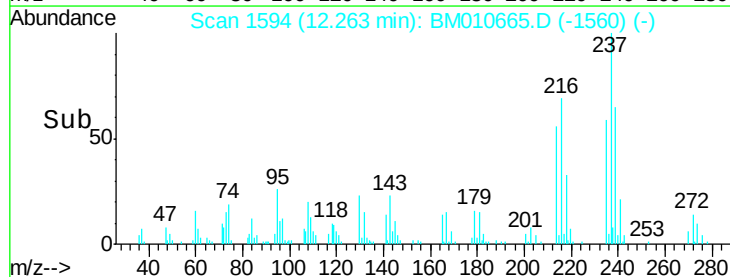

Time-->

