

Data File : BM010679.D
Acq On : 23 Jun 2017 02:44
Operator : SJ/JU
Sample : I3653-07 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C50

Quant Time: Jun 23 05:10:51 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 23 05:06:10 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	89068	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	398372	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.12	164	265523	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	89526	20.00	ng/ul	0.11
75) Chrysene-d12	21.09	240	730097	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	566274	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	293	0.19	ng/uL	0.00
5) Phenol-d5	6.65	99	17926	2.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	10786	2.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	14162	2.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	15817	2.25	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	7480	2.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	8978	2.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	17897	2.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	23673	3.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	66040	2.83	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	73687	2.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	8877	2.16	ng/ul	0.00
57) Fluorene-d10	15.12	176	56052	2.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.25	200	6793	12.35	ng/ul	0.01
70) Anthracene-d10	16.97	188	89526	20.71	ng/ul	0.00
76) Pyrene-d10	19.28	212	102774	3.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.09	264	74386	2.72	ng/ul	0.00

Target Compounds

						Qvalue
28) Naphthalene	10.27	128	1695653	85.53	ng/ul	100
30) 4-Chloroaniline	10.27	127	224670	30.76	ng/ul#	24
34) 2-Methylnaphthalene	11.90	142	340616	21.37	ng/ul	100
40) 1,1'-Biphenyl	12.93	154	298976	14.40	ng/ul#	98
47) Acenaphthylene	13.83	152	127296	4.93	ng/ul#	94
49) Acenaphthene	14.18	153	1591922	91.39	ng/ul	99
53) Dibenzofuran	14.52	168	2217437	84.06	ng/ul	92
58) Fluorene	15.18	166	2477233	112.16	ng/ul	100
60) 4-Nitroaniline	15.18	138	35367	7.50	ng/ul#	1
64) N-Nitrosodiphenylamine	15.49	169	10523	4.24	ng/ul#	52
69) Phenanthrene	17.02	178	5725419	1202.94	ng/ul	99
71) Anthracene	17.02	178	5721846	1166.90	ng/ul	98
72) Carbazole	17.28	167	1659050	387.81	ng/ul	98
74) Fluoranthene	19.09	202	68018	11.09	ng/ul#	97
77) Pyrene	19.32	202	4068121	96.47	ng/ul#	97
80) Benzo(a)anthracene	21.07	228	1468468	34.54	ng/ul	96
82) Chrysene	21.12	228	1303258	34.38	ng/ul	97
85) Benzo(b)fluoranthene	22.59	252	1030491	28.03	ng/ul#	99
86) Benzo(k)fluoranthene	22.59	252	1030491	29.57	ng/ul#	98
88) Benzo(a)pyrene	23.13	252	608973	18.00	ng/ul	100
89) Indeno(1,2,3-cd)pyrene	25.33	276	225171	6.42	ng/ul	98
91) Benzo(g,h,i)perylene	25.98	276	154898	5.54	ng/ul	98

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
Quantitation Report (Not Reviewed)

Data File : BM010679.D
Acq On : 23 Jun 2017 02:44
Operator : SJ/JU
Sample : I3653-07 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C50

Quant Time: Jun 23 05:10:51 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 23 05:06:10 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM010679.D

Acq On : 23 Jun 2017 02:44

Operator : SJ/JU

Sample : I3653-07 5X

Misc :

ALS Vial : 30 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

F5C50


Quant Time: Jun 23 05:10:51 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jun 23 05:06:10 2017

Response via : Initial Calibration

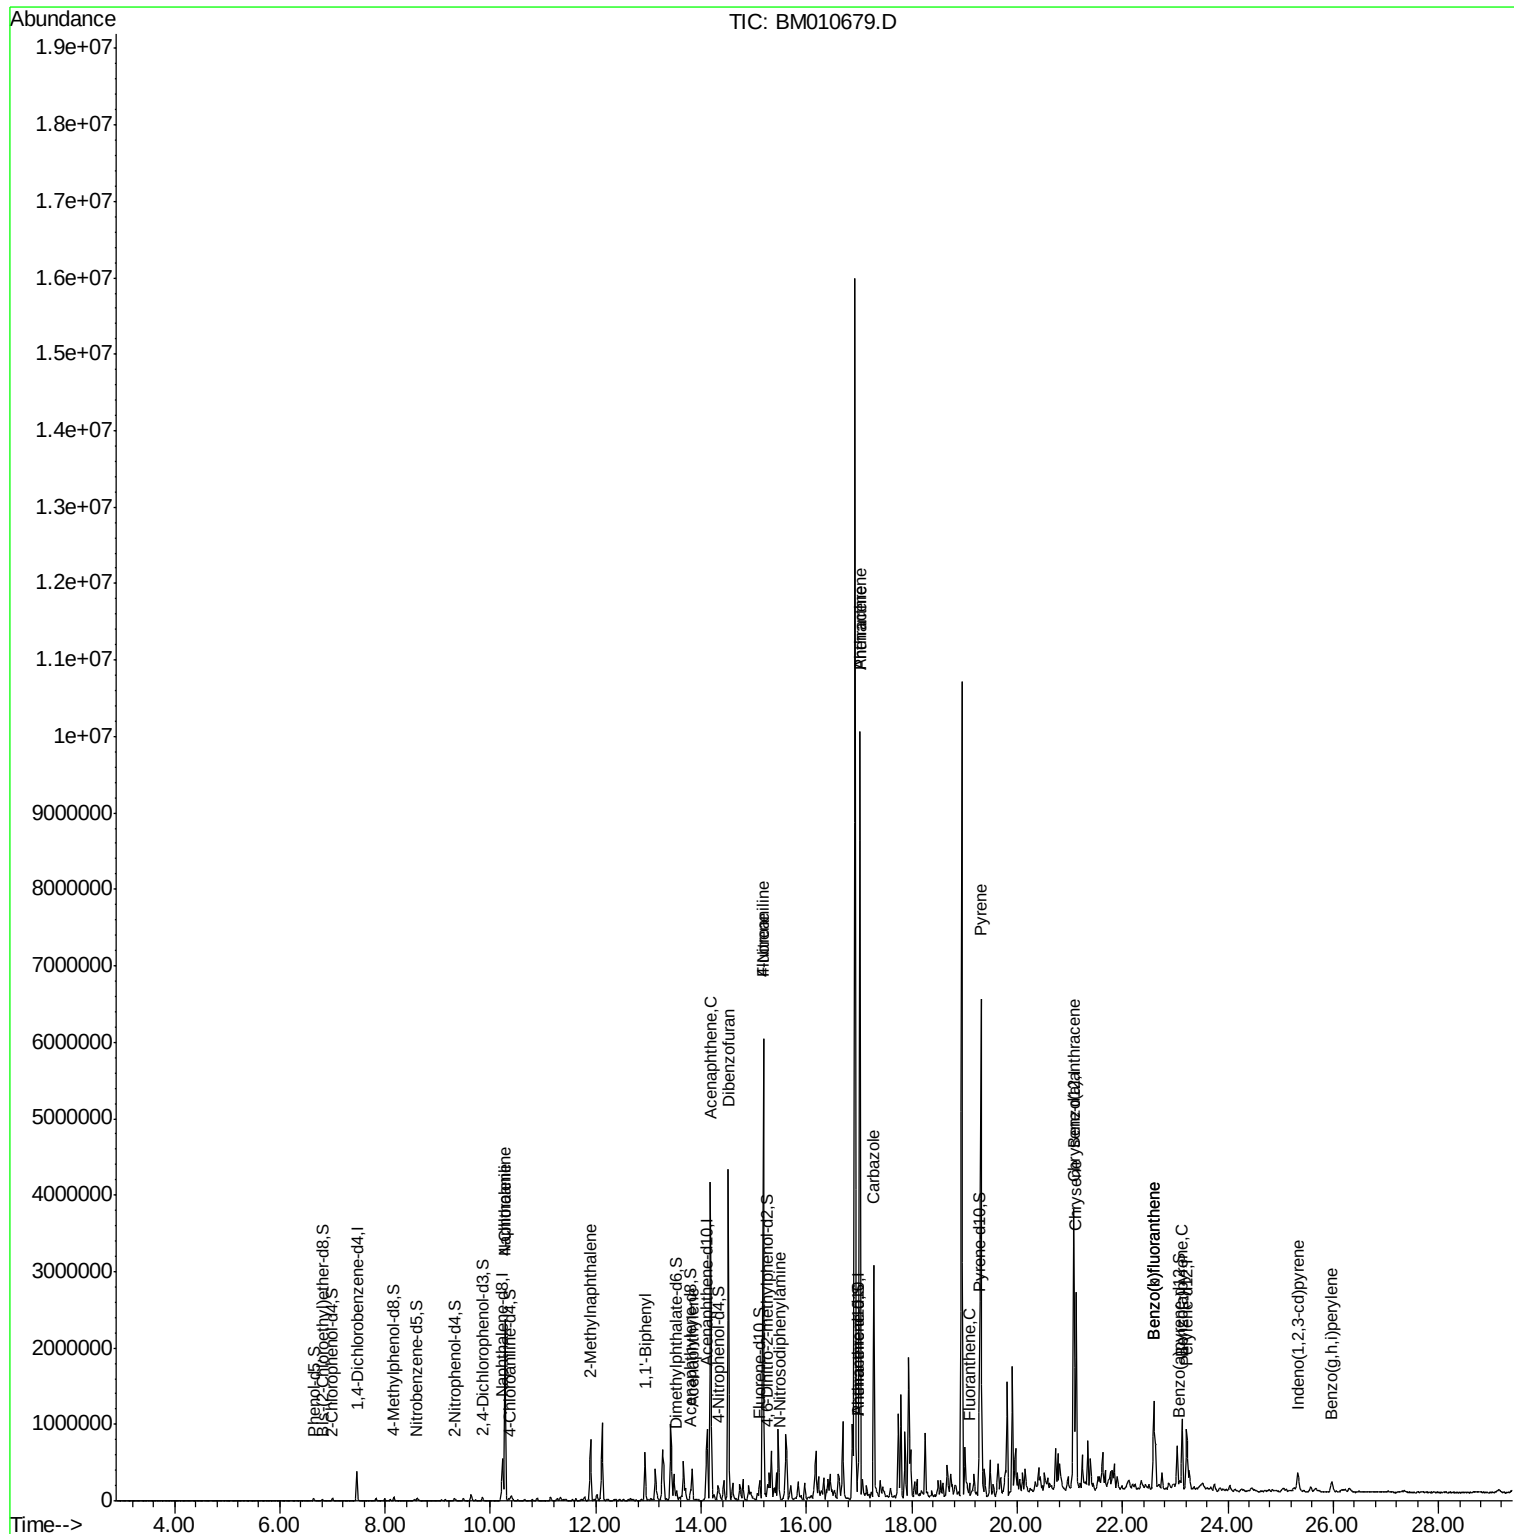



#28

Naphthalene

Concen: 85.53 ng/ul

RT: 10.27 min Scan# 1256

Delta R.T. -0.00 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44

Instrument :

BNA_M

ClientSampleId :

F5C50


Tgt Ion:128 Resp: 1695653

Ion Ratio Lower Upper

128 100

129 10.8 8.8 13.2




127 13.5 10.6 16.0

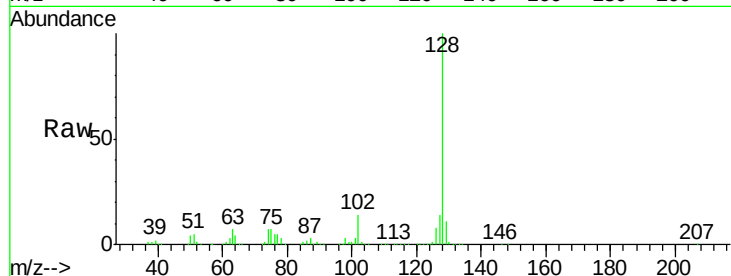

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

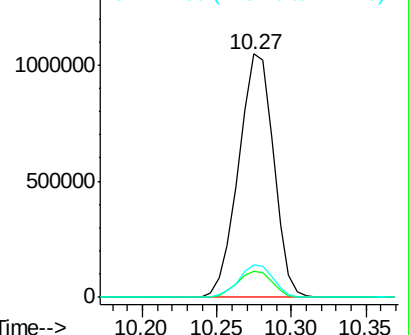

#30

4-Chloroaniline

Concen: 30.76 ng/ul

RT: 10.27 min Scan# 1256

Delta R.T. -0.12 min

Lab File: BM010679.D


Acq: 23 Jun 2017 02:44

Tgt Ion:127 Resp: 224670

Ion Ratio Lower Upper



127 100


129 80.2 28.4 42.6#



Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

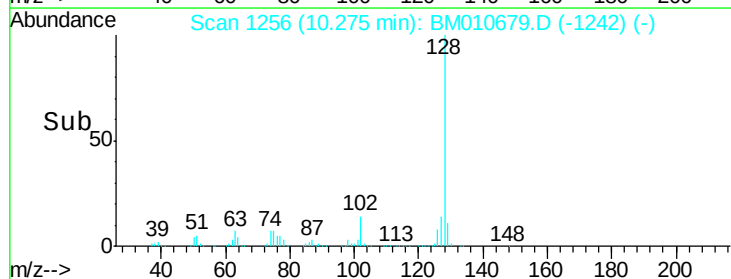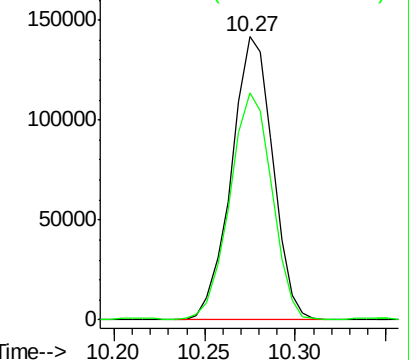

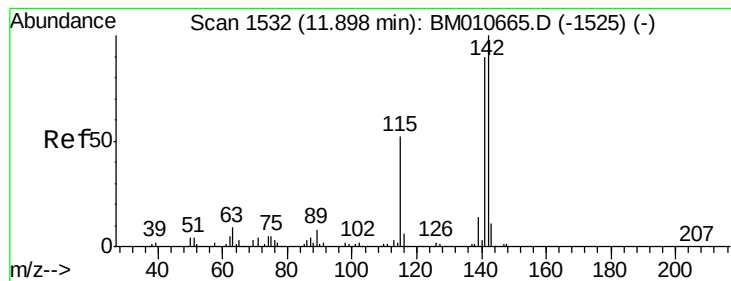

#34

2-Methylnaphthalene

Concen: 21.37 ng/ul

RT: 11.90 min Scan# 1532

Delta R.T. -0.00 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44

Instrument :

BNA_M

ClientSampleId :


F5C50

Tgt Ion:142 Resp: 340616

Ion Ratio Lower Upper

142 100

141 92.3 74.1 111.1



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

250000

200000

150000

100000

50000



0

11.85

11.90

11.95

Time-->

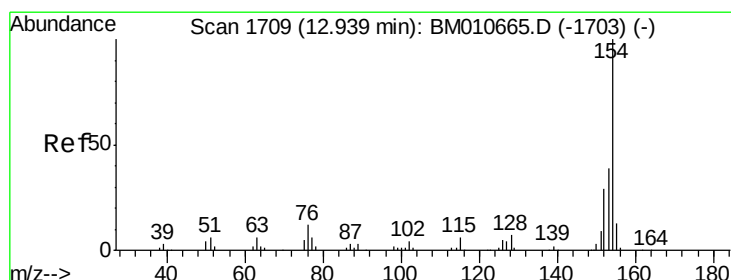

#40

1,1'-Biphenyl

Concen: 14.40 ng/ul

RT: 12.93 min Scan# 1708

Delta R.T. -0.01 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44


Tgt Ion:154 Resp: 298976

Ion Ratio Lower Upper

154 100

153 41.0 32.6 48.8

76 12.8 8.5 12.7#

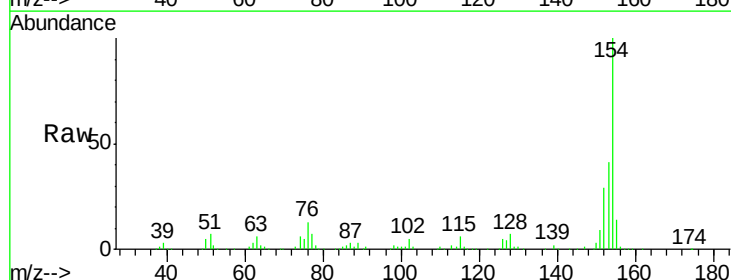

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

250000

200000

150000

100000

50000


0


12.90

12.95

13.00

Time-->




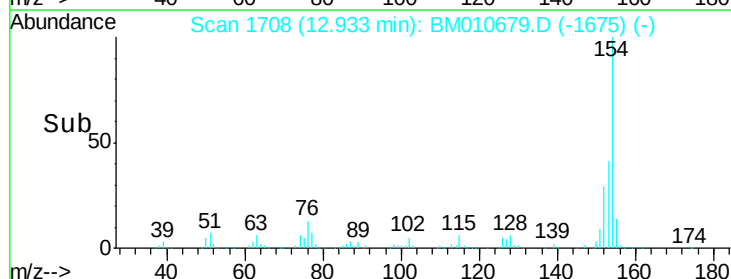




#47
Acenaphthylene
Concen: 4.93 ng/ul
RT: 13.83 min Scan# 1860
Delta R.T. -0.01 min
Lab File: BM010679.D
Acq: 23 Jun 2017 02:44




Instrument :
BNA_M
ClientSampleId :
F5C50


Tgt Ion:152 Resp: 127296
Ion Ratio Lower Upper
152 100
151 20.4 16.3 24.5
153 19.4 10.2 15.4#

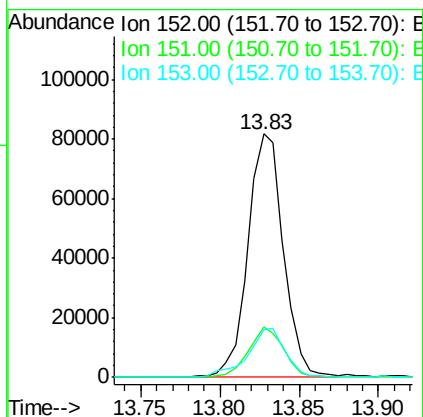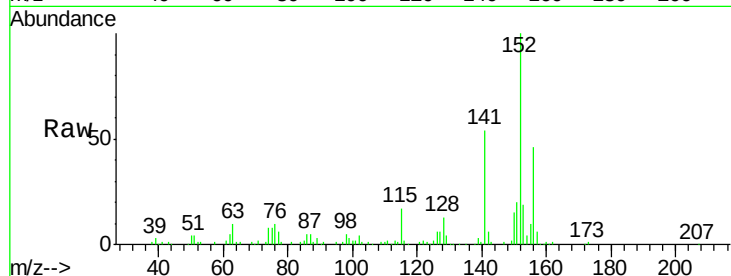

#49
Acenaphthene
Concen: 91.39 ng/ul
RT: 14.18 min Scan# 1920
Delta R.T. -0.00 min
Lab File: BM010679.D
Acq: 23 Jun 2017 02:44

Tgt Ion:153 Resp: 1591922
Ion Ratio Lower Upper
153 100
152 48.2 37.6 56.4
154 87.5 70.4 105.6



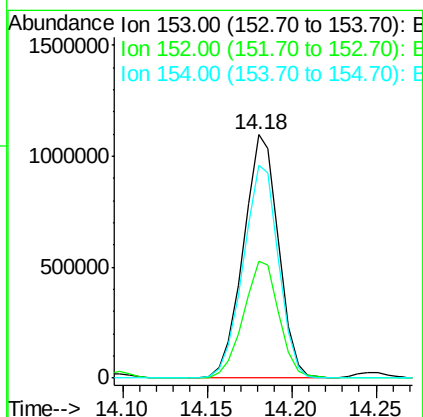



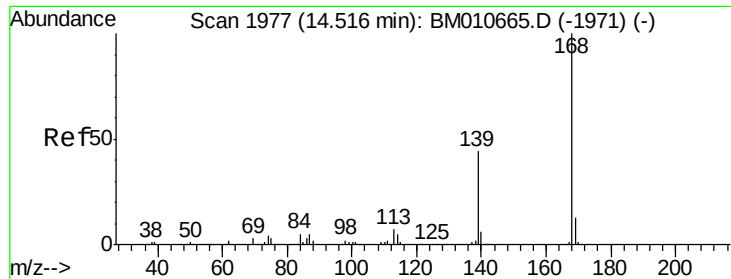

#53
Dibenzenofuran
Concen: 84.06 ng/ul
RT: 14.52 min Scan# 1978
Delta R.T. 0.01 min
Lab File: BM010679.D
Acq: 23 Jun 2017 02:44




Instrument :
BNA_M
ClientSampleId :
F5C50


Tgt Ion:168 Resp: 2217437
Ion Ratio Lower Upper
168 100
139 43.5 30.8 46.2

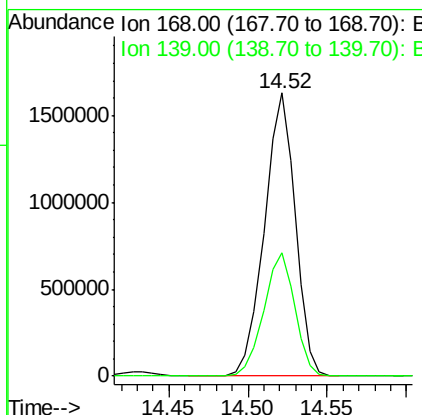

#58
Fluorene
Concen: 112.16 ng/ul
RT: 15.18 min Scan# 2090
Delta R.T. 0.01 min
Lab File: BM010679.D
Acq: 23 Jun 2017 02:44

Tgt Ion:166 Resp: 2477233
Ion Ratio Lower Upper
166 100
165 97.8 77.9 116.9
167 13.5 10.6 16.0


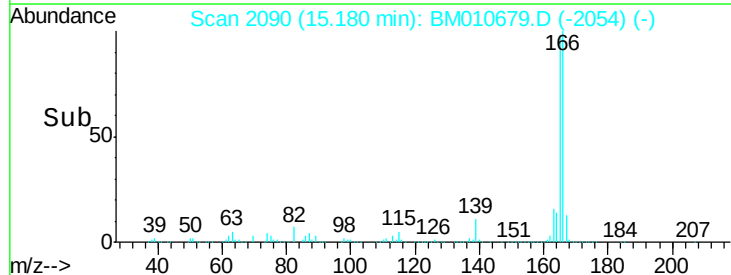
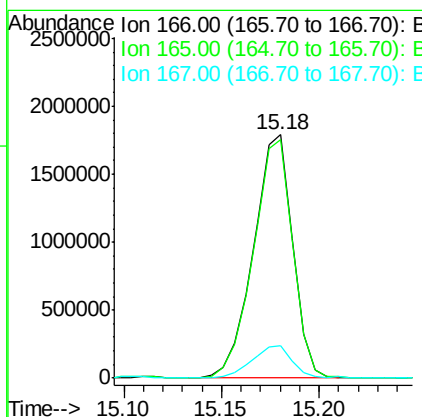





#60
4-Nitroaniline
Concen: 7.50 ng/ul
RT: 15.18 min Scan# 2090
Delta R.T. -0.02 min
Lab File: BM010679.D
Acq: 23 Jun 2017 02:44




Instrument :
BNA_M
ClientSampleId :
F5C50


Tgt Ion:138 Resp: 35367
Ion Ratio Lower Upper
138 100
92 1.9 52.7 79.1#
108 3.7 140.4 210.6#

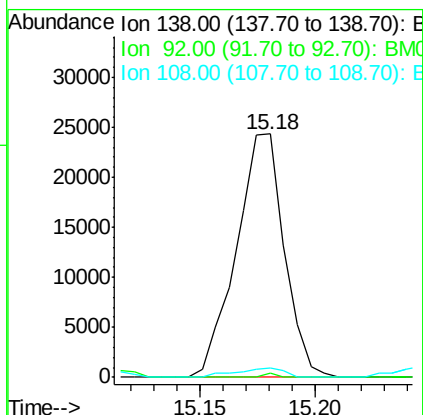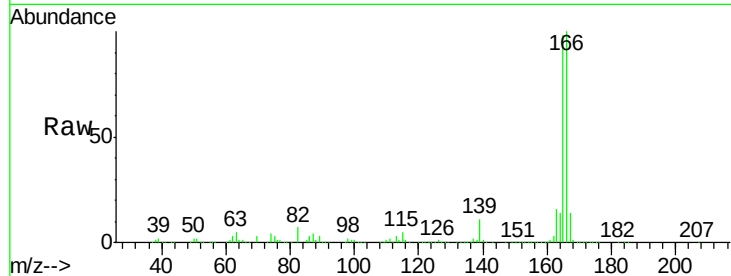

#64
N-Nitrosodiphenylamine
Concen: 4.24 ng/ul
RT: 15.49 min Scan# 2143
Delta R.T. 0.10 min
Lab File: BM010679.D
Acq: 23 Jun 2017 02:44

Tgt Ion:169 Resp: 10523
Ion Ratio Lower Upper
169 100
168 8.8 54.0 81.0#
167 38.0 29.1 43.7

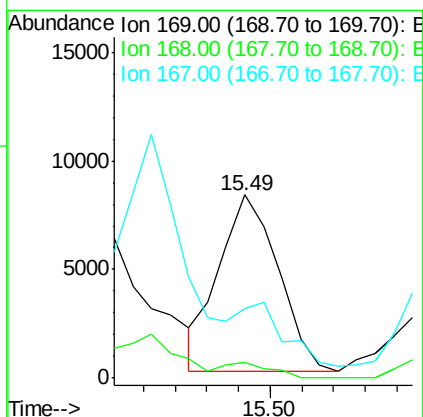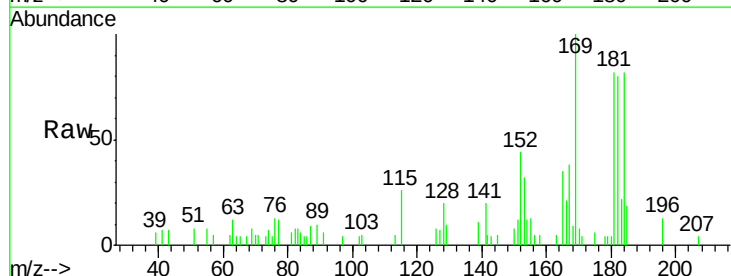

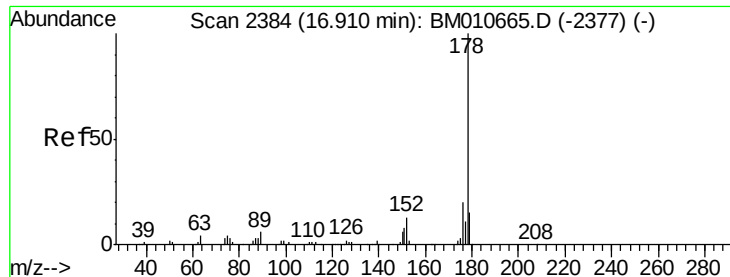

#69

Phenanthrene

Concen: 1202.94 ng/ul

RT: 17.02 min Scan# 2402

Delta R.T. 0.11 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44

Instrument :

BNA_M

ClientSampleId :

F5C50


Tgt Ion:178 Resp: 5725419

Ion Ratio Lower Upper

178 100

179 15.5 12.6 19.0




176 19.2 14.9 22.3

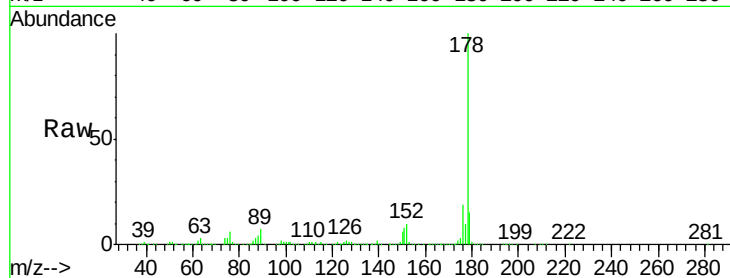

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

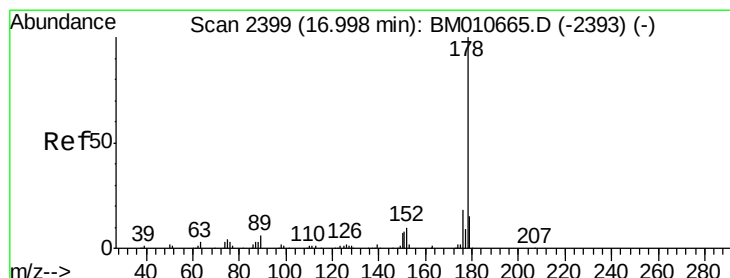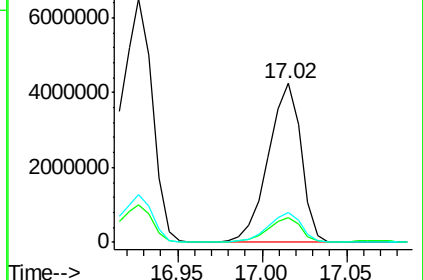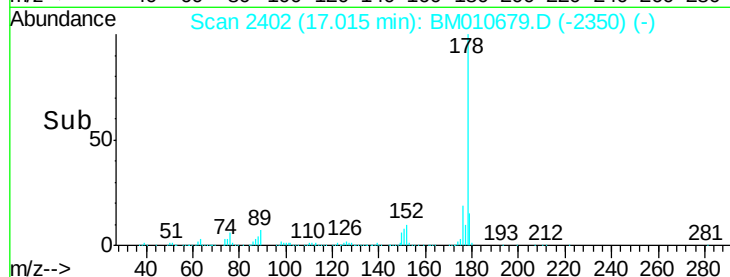

#71

Anthracene

Concen: 1166.90 ng/ul

RT: 17.02 min Scan# 2402

Delta R.T. 0.02 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44


Tgt Ion:178 Resp: 5721846

Ion Ratio Lower Upper

178 100

179 15.5 11.7 17.5



176 19.2 14.6 21.8

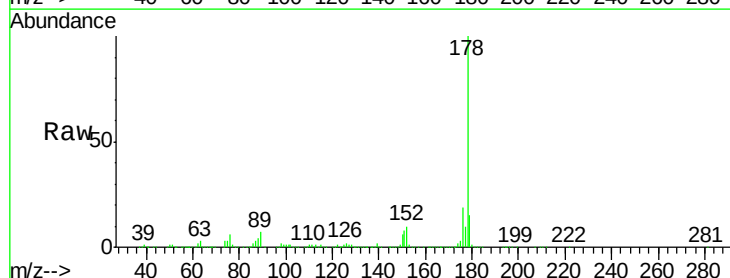


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



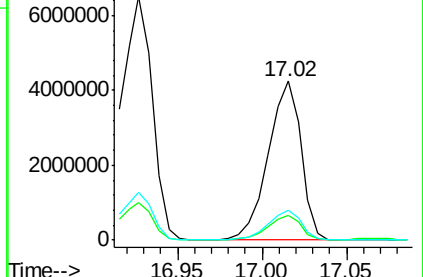
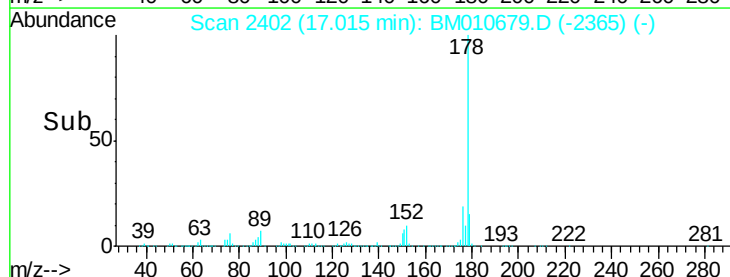


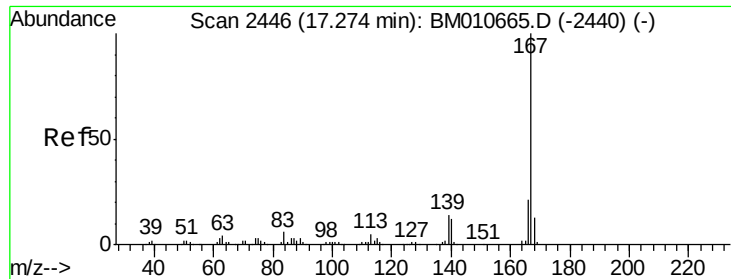

#72
 Carbazole
 Concen: 387.81 ng/ul
 RT: 17.28 min Scan# 2447
 Delta R.T. 0.01 min
 Lab File: BM010679.D
 Acq: 23 Jun 2017 02:44




Instrument :
 BNA_M
 ClientSampleId :
 F5C50


Tgt Ion:167 Resp: 1659050
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.1 25.7
 139 14.0 10.0 15.0

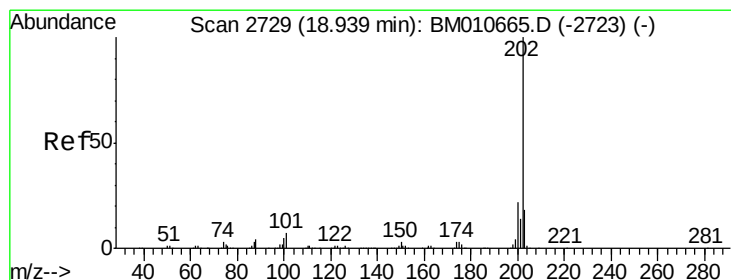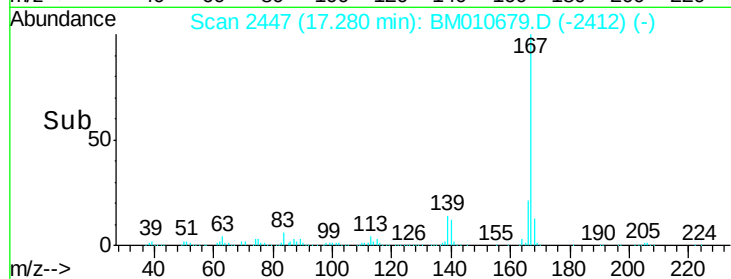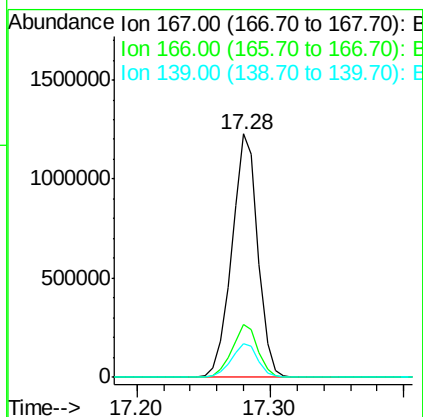

#74
 Fluoranthene
 Concen: 11.09 ng/ul
 RT: 19.09 min Scan# 2755
 Delta R.T. 0.15 min
 Lab File: BM010679.D
 Acq: 23 Jun 2017 02:44

Tgt Ion:202 Resp: 68018
 Ion Ratio Lower Upper
 202 100
 101 6.3 4.6 7.0
 100 5.6 3.4 5.2#

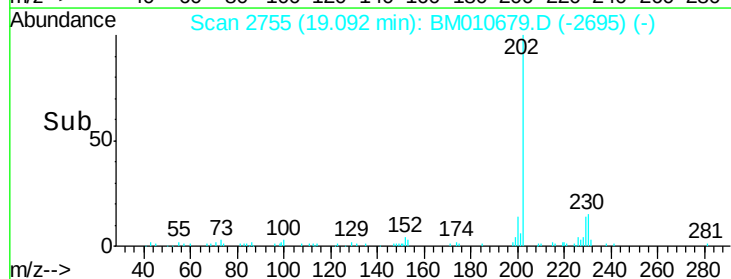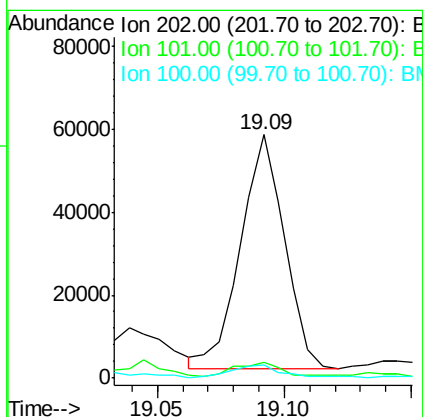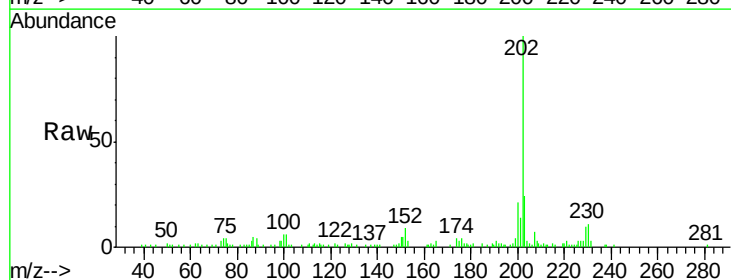



#77

Pyrene

Concen: 96.47 ng/ul

RT: 19.32 min Scan# 2793

Delta R.T. 0.01 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44

Instrument :

BNA_M

ClientSampleId :

F5C50


Tgt Ion:202 Resp: 4068121

Ion Ratio Lower Upper

202 100

101 8.1 5.1 7.7#




100 6.3 4.9 7.3



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

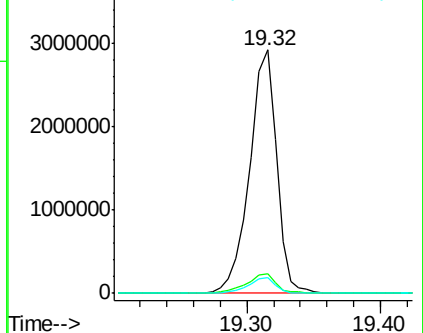

#80

Benzo(a)anthracene

Concen: 34.54 ng/ul

RT: 21.07 min Scan# 3091

Delta R.T. -0.00 min

Lab File: BM010679.D

Acq: 23 Jun 2017 02:44


Tgt Ion:228 Resp: 1468468

Ion Ratio Lower Upper

228 100

229 20.8 15.4 23.0



226 28.5 21.4 32.0




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

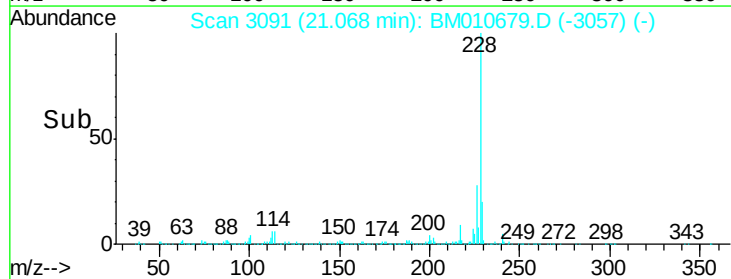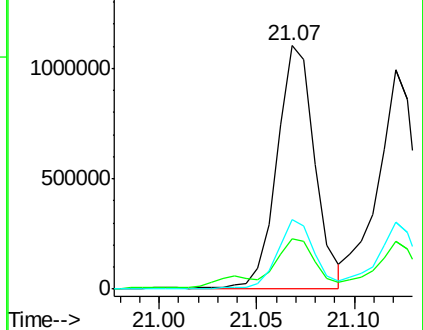




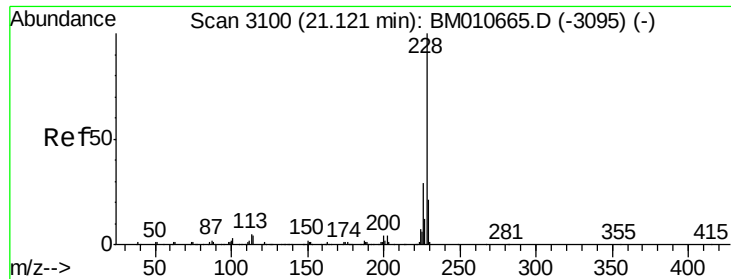


#82
Chrysene
 Concen: 34.38 ng/ul
 RT: 21.12 min Scan# 3100
 Delta R.T. -0.00 min
 Lab File: BM010679.D
 Acq: 23 Jun 2017 02:44

Instrument :
 BNA_M
 ClientSampleId :
 F5C50

Tgt Ion: 228 Resp: 1303258

Ion	Ratio	Lower	Upper
228	100		
226	30.4	23.4	35.2
229	21.5	15.5	23.3

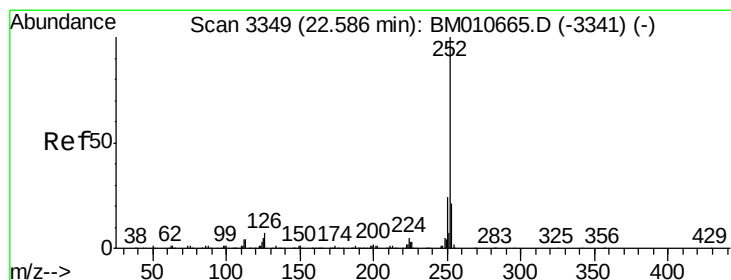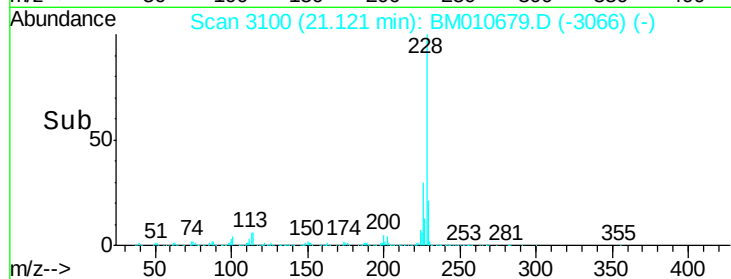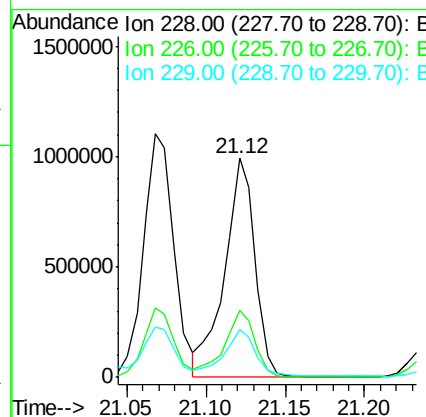

#85
Benzo(b)fluoranthene
 Concen: 28.03 ng/ul
 RT: 22.59 min Scan# 3350
 Delta R.T. 0.01 min
 Lab File: BM010679.D
 Acq: 23 Jun 2017 02:44

Tgt Ion: 252 Resp: 1030491

Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.9	26.9
125	5.7	3.6	5.4

