

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
 Data File : BM010655.D
 Acq On : 22 Jun 2017 12:21
 Operator : SJ/JU
 Sample : I3767-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC63

Manual Integrations
 APPROVED

mohammad
 6/26/2017 8:23:43 AM

Quant Time: Jun 23 04:19:48 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 23 01:03:57 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	54294	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	239497	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.12	164	168418	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.87	188	431373	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	525581	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	436202	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	1727	1.82	ng/uL	0.00
5) Phenol-d5	6.65	99	38763	7.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	82770	28.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	93716	25.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	74732	17.43	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	58447	34.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	71069	36.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	129109	31.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	6284	1.44	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	514439	34.80	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	585057	34.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	19765	7.60	ng/ul	-0.01
57) Fluorene-d10	15.12	176	439940	34.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	89044	33.61	ng/ul	0.00
70) Anthracene-d10	16.96	188	727108m	34.90	ng/ul	0.00
76) Pyrene-d10	19.27	212	864129	35.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.09	264	726328	34.45	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.10	88	44070	41.634	ng/uL#	43

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
Data File : BM010655.D
Acq On : 22 Jun 2017 12:21
Operator : SJ/JU
Sample : I3767-01
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDC63

Manual Integrations
APPROVED

mohammad
6/26/2017 8:23:43 AM

Quant Time: Jun 23 04:19:48 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 23 01:03:57 2017
Response via : Initial Calibration

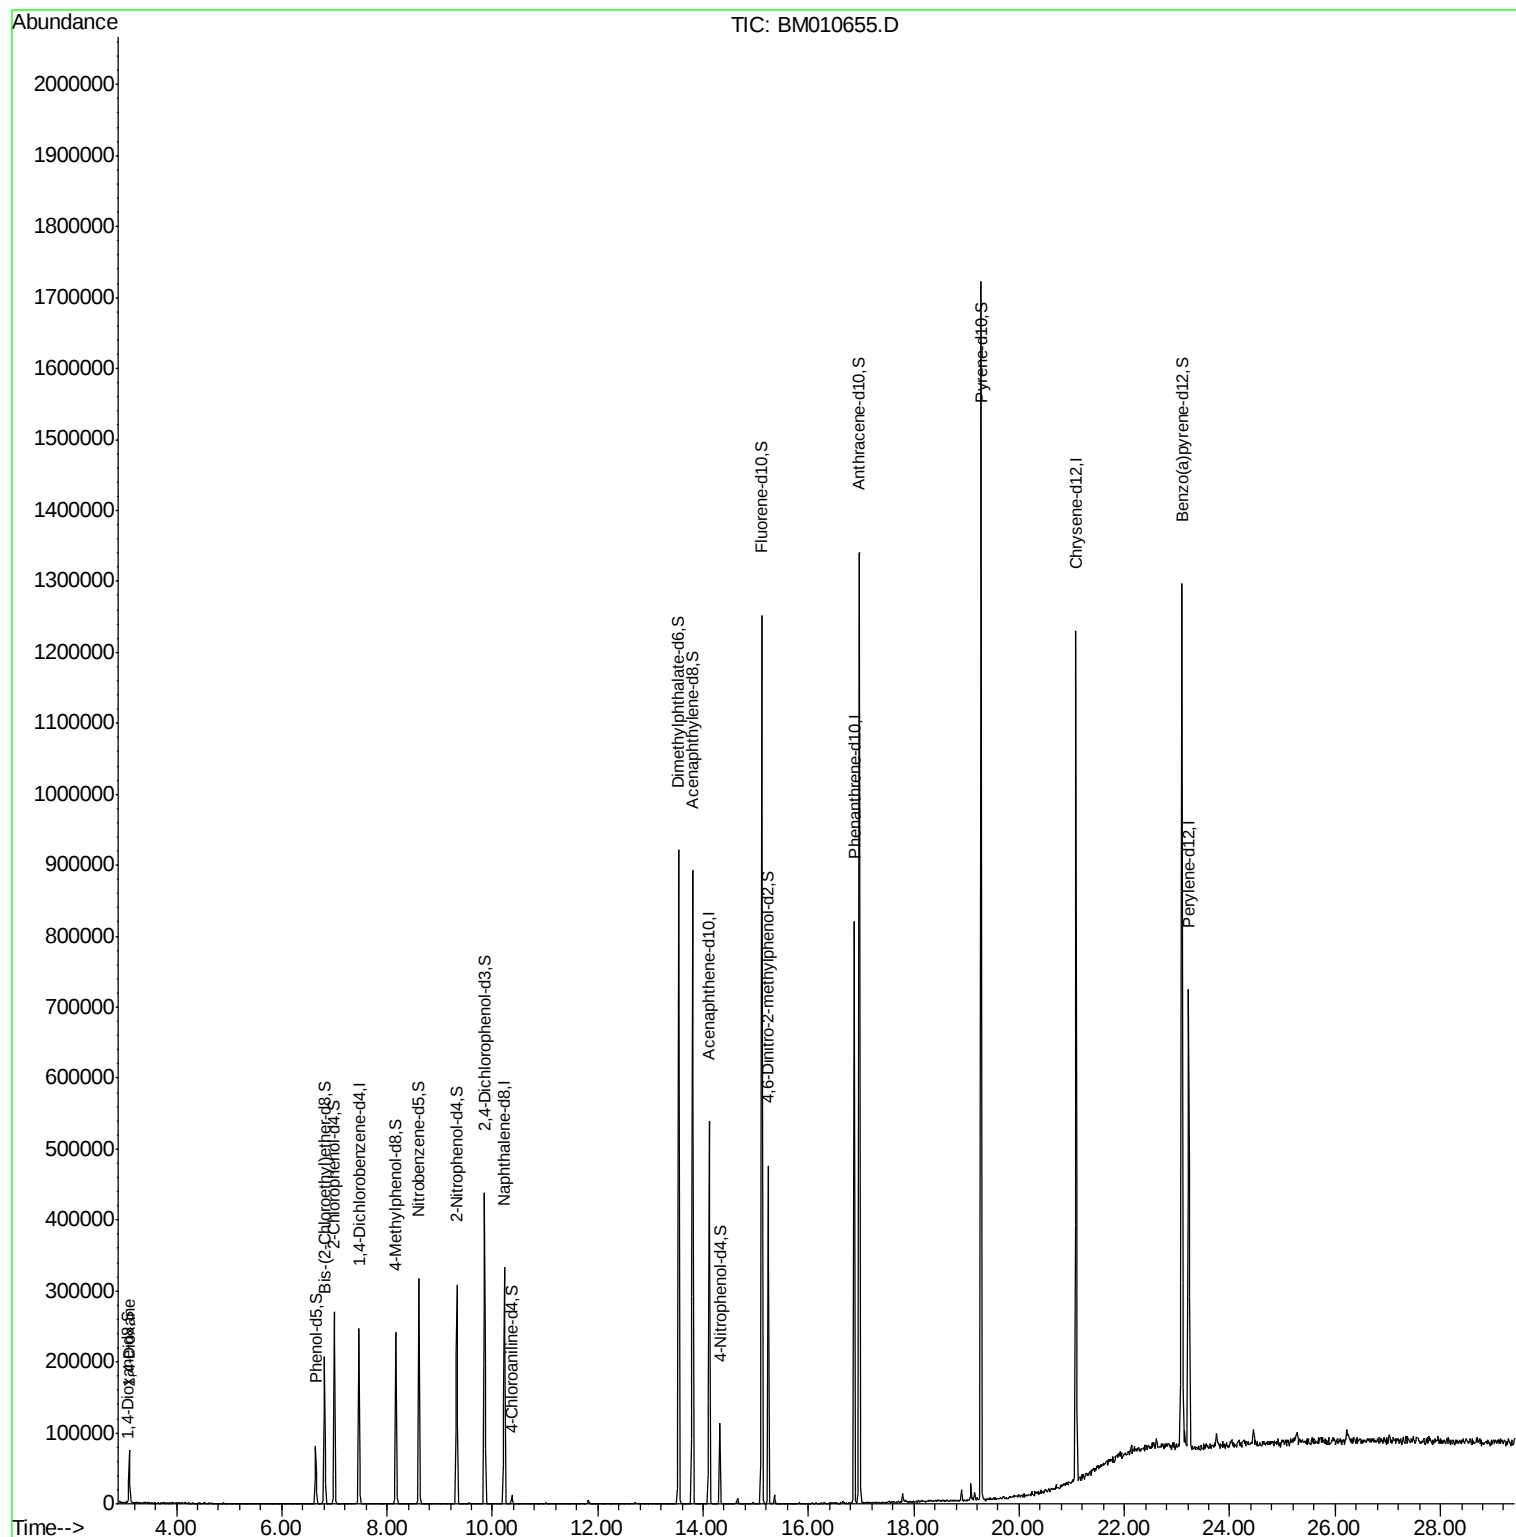

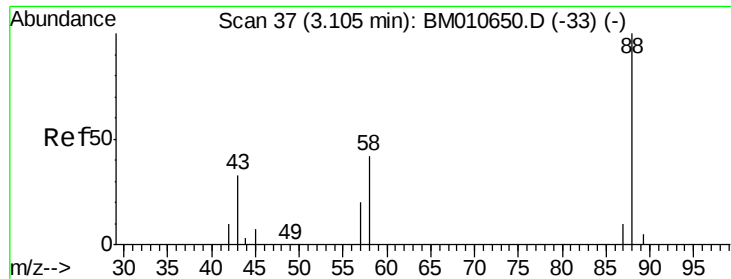

#2

1,4-Dioxane

Concen: 41.634 ng/uL

RT: 3.10 min Scan# 37

Delta R.T. -0.00 min

Lab File: BM010655.D

Acq: 22 Jun 2017 12:21

Instrument :

BNA_M

ClientSampleId :

BDC63

Tgt Ion: 88 Resp: 44070

Ion Ratio Lower Upper

88 100

43 23.6 1.1 1.7#

58 49.5 0.0 0.0#

Manual Integrations
APPROVED

mohammad

6/26/2017 8:23:43 AM

