

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
 Data File : BM010663.D
 Acq On : 22 Jun 2017 17:09
 Operator : SJ/JU
 Sample : I3522-15DL 30X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5D31DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.463	771	778	785	rBB	228454	343126	17.80%	2.460%
2	10.222	1240	1247	1253	rBV	316676	524183	27.19%	3.757%
3	13.533	1805	1810	1814	rBV2	18414	22420	1.16%	0.161%
4	13.798	1849	1855	1858	rBV	15065	24931	1.29%	0.179%
5	13.827	1858	1860	1866	rVB2	18401	22397	1.16%	0.161%
6	14.116	1902	1909	1916	rBV2	512491	781146	40.53%	5.599%
7	14.516	1972	1977	1982	rBB	22283	28274	1.47%	0.203%
8	15.116	2074	2079	2083	rBV	27260	33788	1.75%	0.242%
9	15.169	2083	2088	2095	rVB2	64785	86558	4.49%	0.620%
10	16.868	2368	2377	2381	rBV	741043	1054843	54.73%	7.561%
11	16.910	2381	2384	2389	rVB	206352	257881	13.38%	1.848%
12	16.998	2394	2399	2406	rVV	1356534	1876333	97.34%	13.449%
13	17.274	2440	2446	2457	rBV	471974	628470	32.61%	4.505%
14	17.745	2520	2526	2529	rBV	12943	20268	1.05%	0.145%
15	17.792	2529	2534	2540	rVB2	26576	37118	1.93%	0.266%
16	17.868	2543	2547	2552	rBV	45574	59544	3.09%	0.427%
17	17.939	2552	2559	2563	rBV2	31094	54931	2.85%	0.394%
18	18.098	2581	2586	2590	rVB2	17593	23850	1.24%	0.171%
19	18.292	2615	2619	2623	rVB3	19244	26434	1.37%	0.189%
20	18.674	2680	2684	2688	rBV3	14491	22142	1.15%	0.159%
21	18.815	2703	2708	2717	rVB2	24935	38067	1.97%	0.273%
22	18.939	2724	2729	2735	rVB	454970	582461	30.22%	4.175%
23	19.274	2782	2786	2787	rVV	103869	112741	5.85%	0.808%
24	19.304	2787	2791	2800	rVB	385490	525118	27.24%	3.764%
25	19.380	2800	2804	2811	rVB4	19141	33117	1.72%	0.237%
26	19.486	2811	2822	2828	rBV	30893	55035	2.86%	0.394%
27	19.545	2828	2832	2838	rVB3	31824	52685	2.73%	0.378%
28	19.645	2840	2849	2853	rBV4	39081	89406	4.64%	0.641%
29	19.774	2866	2871	2872	rBV4	36004	46583	2.42%	0.334%
30	19.809	2874	2877	2882	rVB	52282	66759	3.46%	0.479%
31	19.909	2890	2894	2897	rBV	46197	49350	2.56%	0.354%
32	19.962	2897	2903	2908	rBV2	61229	103115	5.35%	0.739%
33	20.103	2922	2927	2931	rBV	32149	44540	2.31%	0.319%
34	20.151	2931	2935	2941	rBV2	26673	52837	2.74%	0.379%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
 Data File : BM010663.D
 Acq On : 22 Jun 2017 17:09
 Operator : SJ/JU
 Sample : I3522-15DL 30X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5D31DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Title : SVOA CALIBRATION

35	20.298	2957	2960	2965	rVB6	18014	22655	1.18%	0.162%
36	20.527	2994	2999	3000	rBV5	14445	19295	1.00%	0.138%
37	20.556	3000	3004	3012	rVB2	70402	99633	5.17%	0.714%
38	20.727	3026	3033	3036	rBV2	72748	122666	6.36%	0.879%
39	20.762	3036	3039	3042	rVV2	47013	63515	3.30%	0.455%
40	20.803	3042	3046	3051	rVV2	64381	126130	6.54%	0.904%
41	20.851	3051	3054	3064	rVB3	48744	84042	4.36%	0.602%
42	20.968	3071	3074	3078	rVB3	23385	30718	1.59%	0.220%
43	21.080	3081	3093	3097	rBV2	1175119	1927519	100.00%	13.816%
44	21.115	3097	3099	3106	rVB	255764	349062	18.11%	2.502%
45	21.239	3116	3120	3121	rBV3	21459	24225	1.26%	0.174%
46	21.345	3134	3138	3141	rVB	110105	129771	6.73%	0.930%
47	21.386	3141	3145	3149	rBV3	40264	58028	3.01%	0.416%
48	21.439	3151	3154	3159	rVB6	27566	31380	1.63%	0.225%
49	21.574	3173	3177	3178	rBV4	23613	29315	1.52%	0.210%
50	21.621	3178	3185	3190	rVV2	68731	133228	6.91%	0.955%
51	21.668	3190	3193	3198	rVV4	51052	75610	3.92%	0.542%
52	21.803	3214	3216	3220	rBV5	21375	29128	1.51%	0.209%
53	22.333	3303	3306	3307	rBV3	22365	26838	1.39%	0.192%
54	22.586	3343	3349	3354	rBV2	325460	738972	38.34%	5.297%
55	22.750	3374	3377	3383	rVB	52114	71448	3.71%	0.512%
56	22.874	3395	3398	3401	rBV5	22467	38384	1.99%	0.275%
57	23.039	3421	3426	3431	rBV2	158930	268746	13.94%	1.926%
58	23.127	3436	3441	3448	rVB	166607	312339	16.20%	2.239%
59	23.221	3451	3457	3463	rBV	703736	1217518	63.17%	8.727%
60	25.327	3810	3815	3821	rBV2	70666	140341	7.28%	1.006%


Sum of corrected areas: 13950957

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
Data File : BM010663.D
Acq On : 22 Jun 2017 17:09
Operator : SJ/JU
Sample : I3522-15DL 30X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D31DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

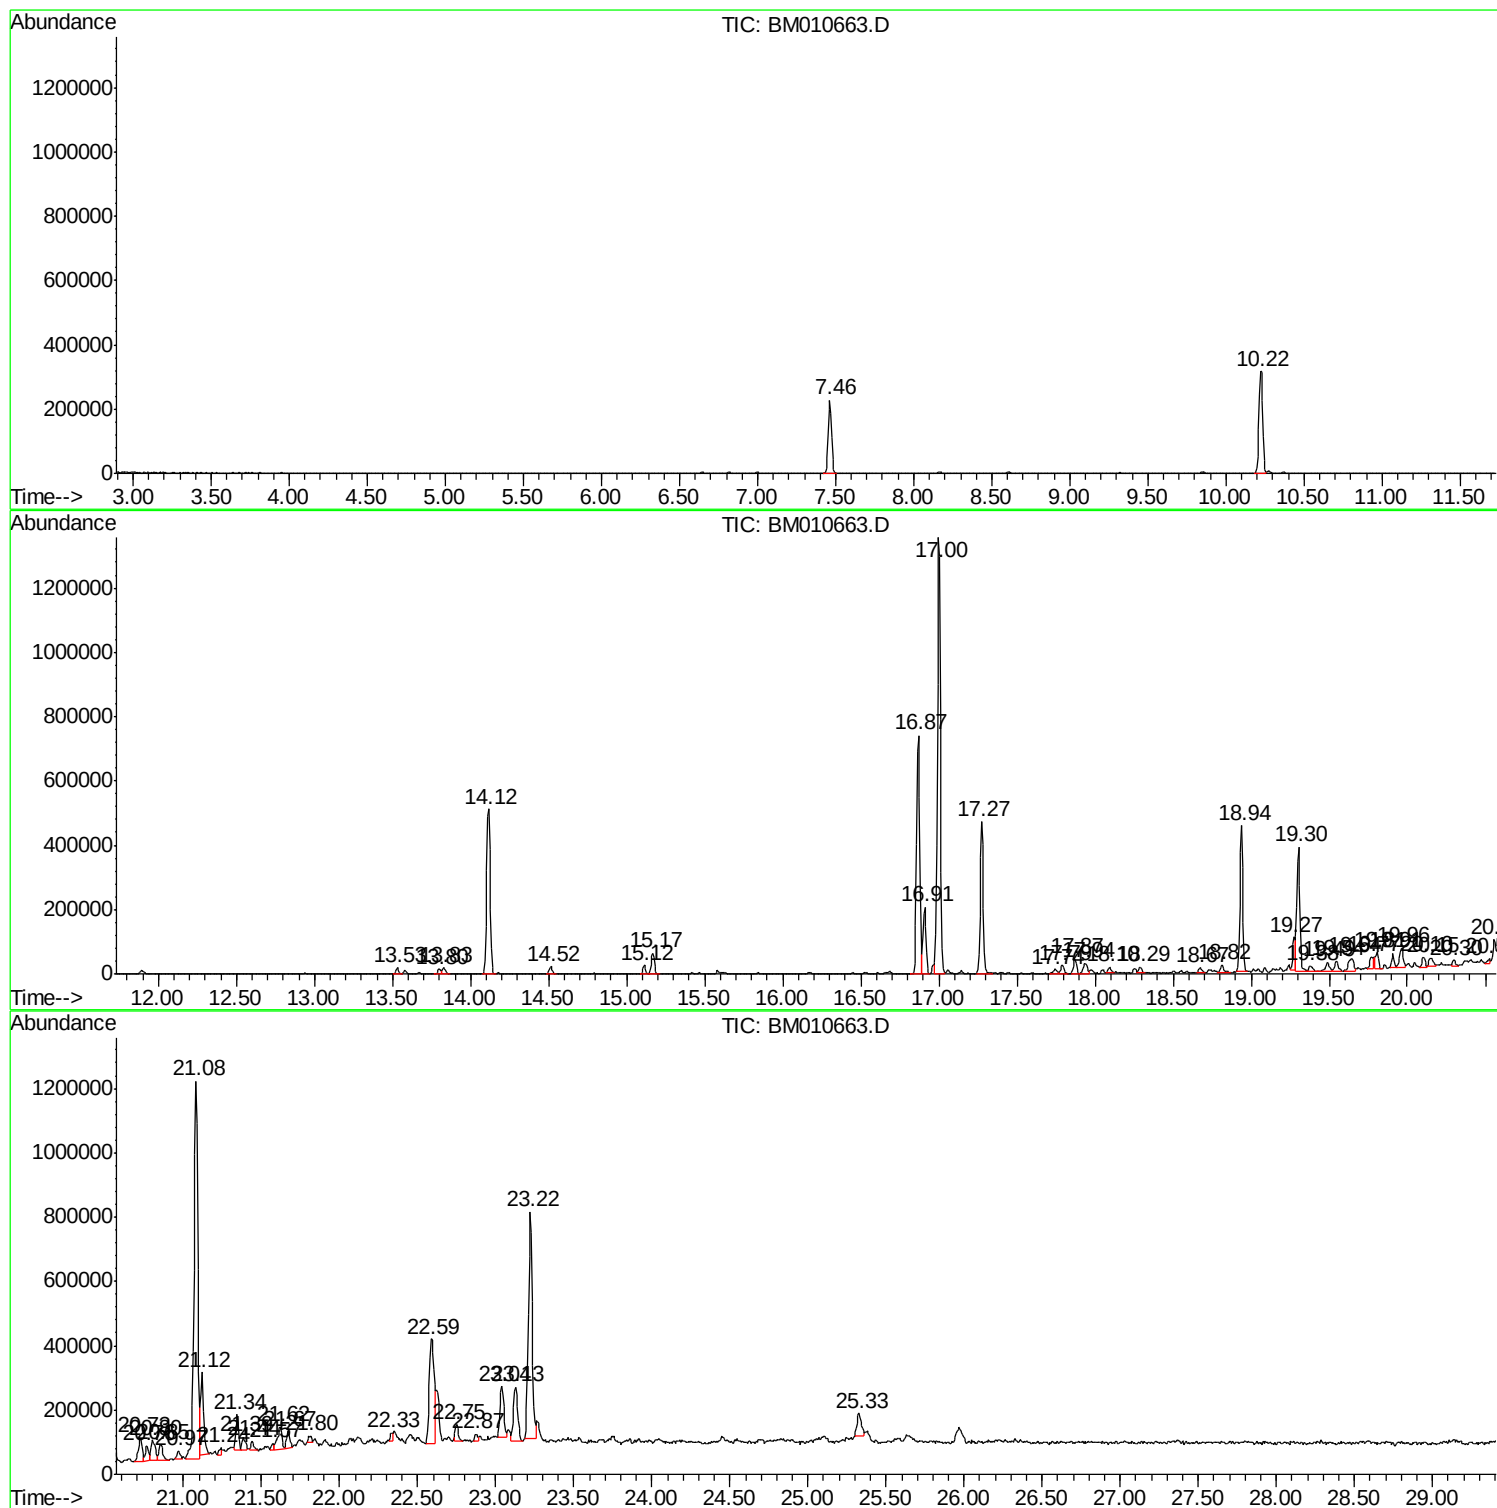

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
Data File : BM010663.D
Acq On : 22 Jun 2017 17:09
Operator : SJ/JU
Sample : I3522-15DL 30X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D31DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062217\
Data File : BM010663.D
Acq On : 22 Jun 2017 17:09
Operator : SJ/JU
Sample : I3522-15DL 30X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5D31DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc