


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062220\
 Data File : BM026483.D
 Acq On : 22 Jun 2020 09:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 10:20:20 2020

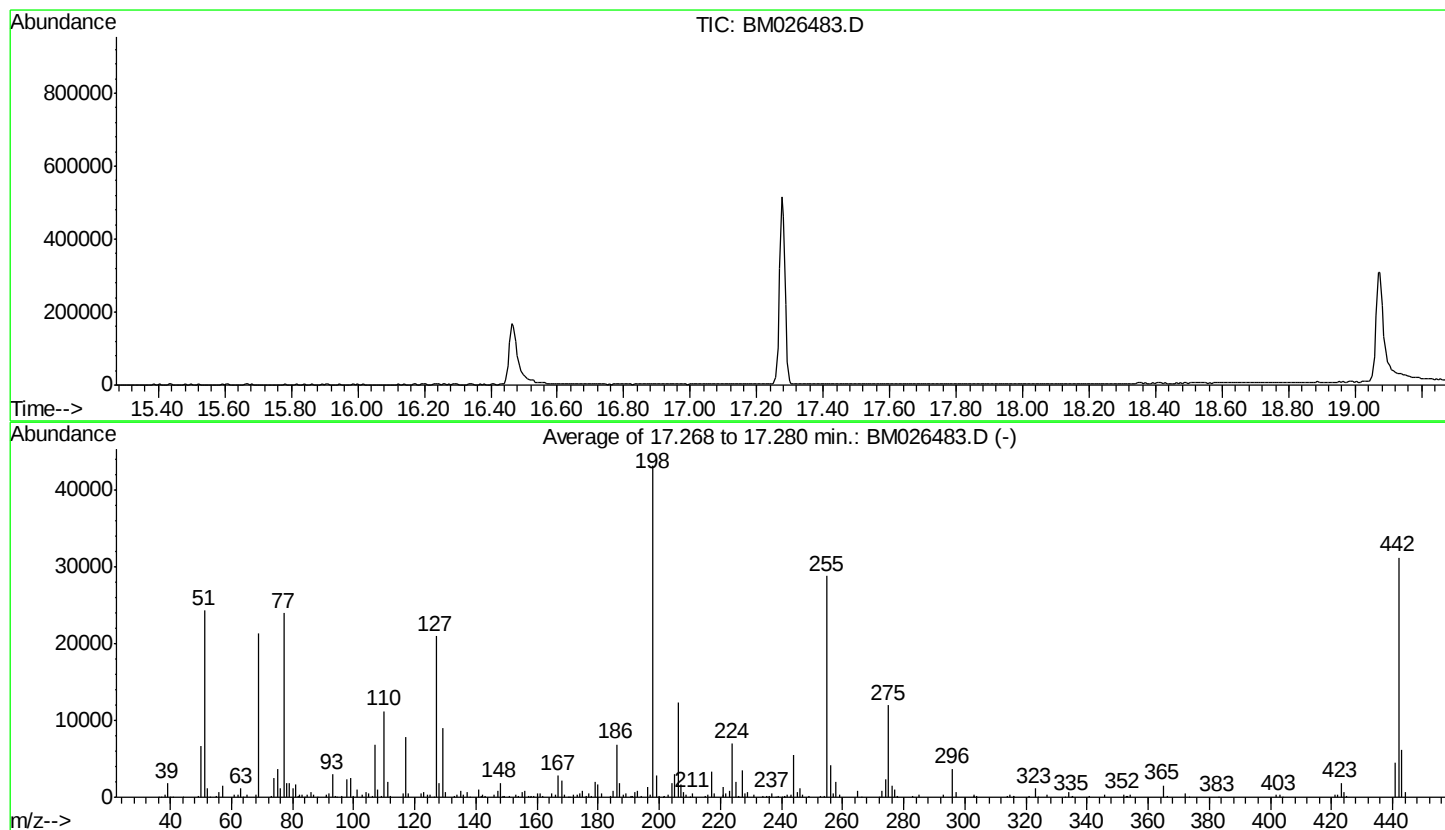

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	24282	PASS
68	69	0.00	2	1.8	383	PASS
69	198	0.00	100	49.4	21346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	20997	PASS
197	198	0.00	2	0.6	257	PASS
198	198	100	100	100.0	43176	PASS
199	198	5	9	6.6	2843	PASS
275	198	10	60	27.6	11932	PASS
365	198	1	100	3.6	1560	PASS
441	198	0.01	100	10.4	4497	PASS
442	198	50	100	72.3	31234	PASS
443	442	15	24	19.8	6185	PASS