


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
Data File : BM030535.D
Acq On : 23 Jun 2021 03:48
Operator : CG/JU
Sample : M2662-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDF4

Manual Integrations
APPROVED

mohammad
6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:50:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 01:33:40 2021
Response via : Initial Calibration

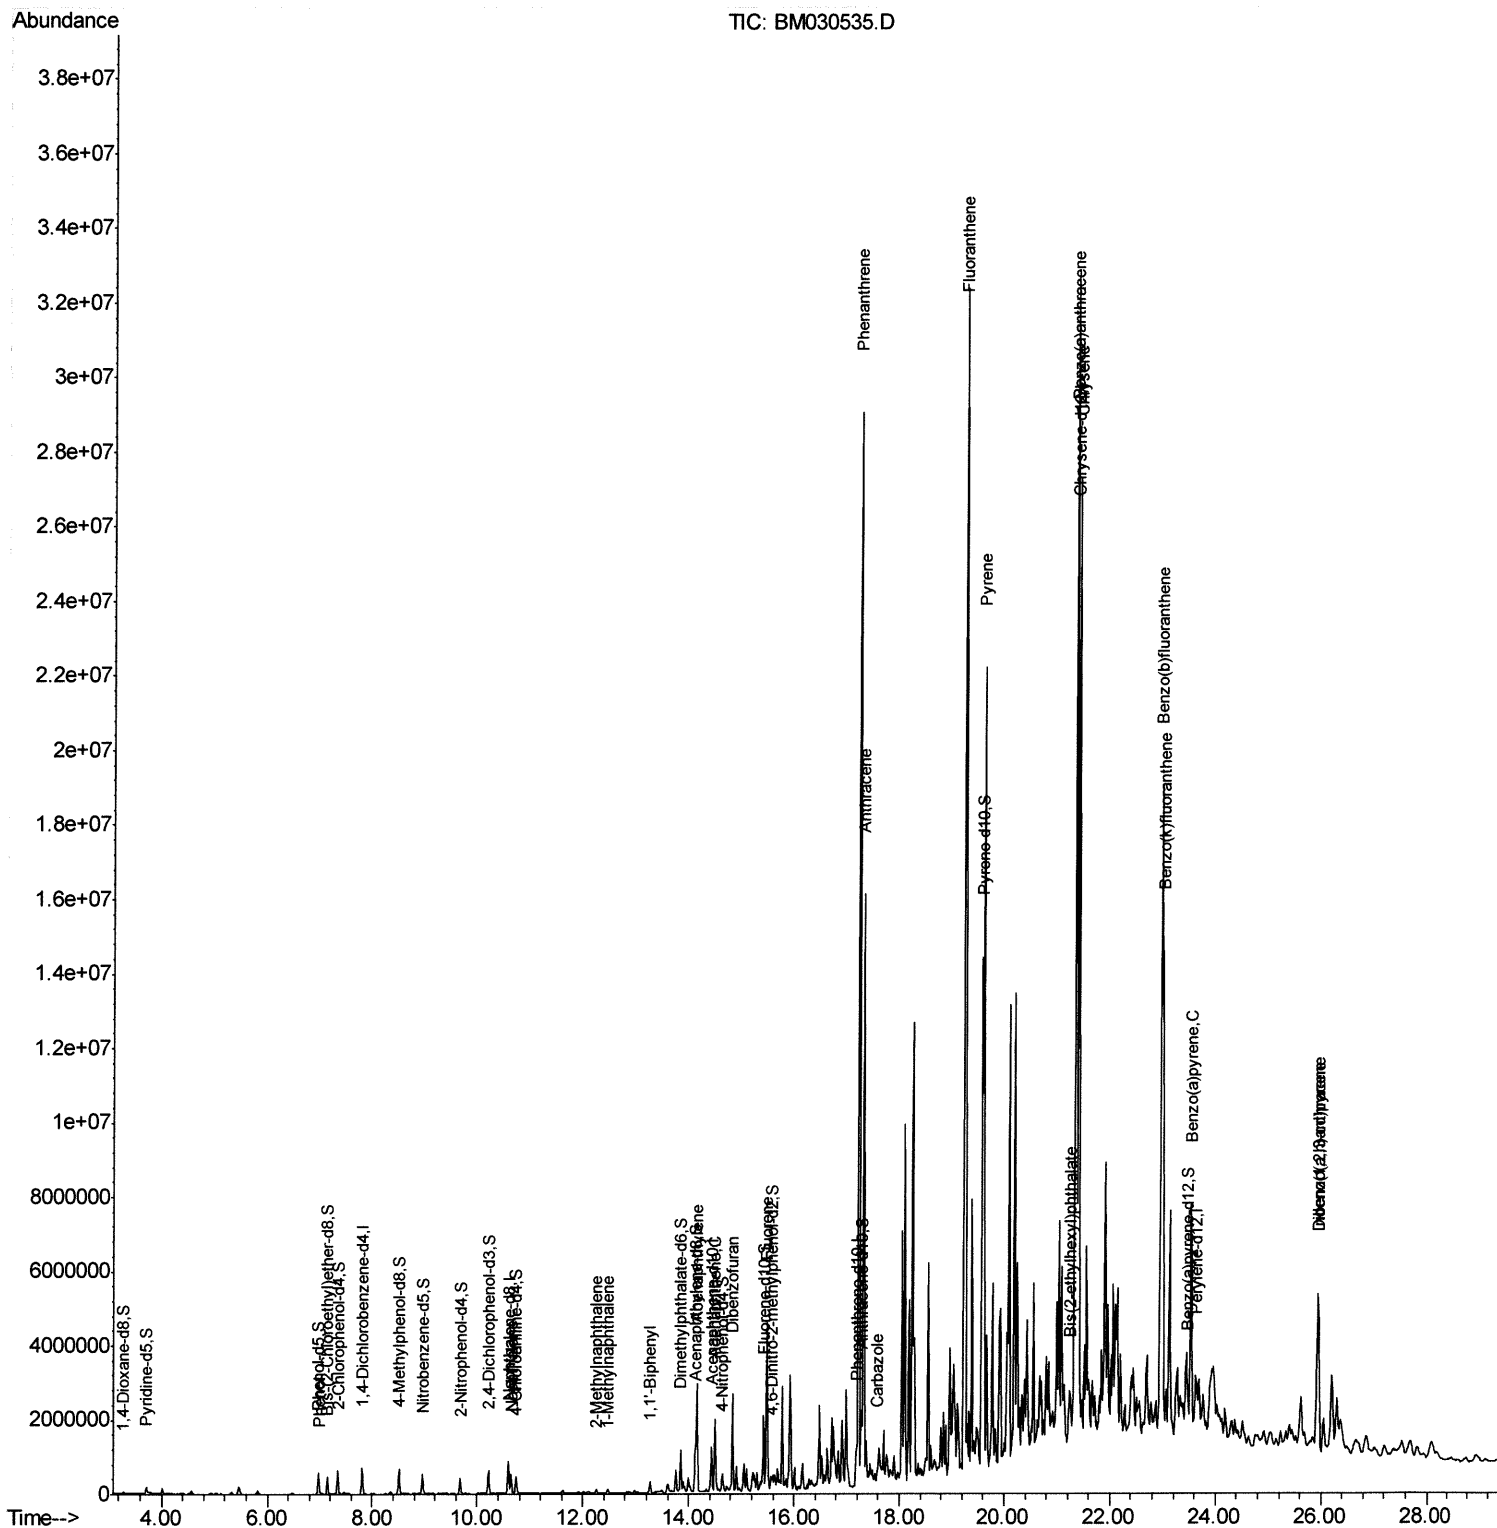




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:36:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

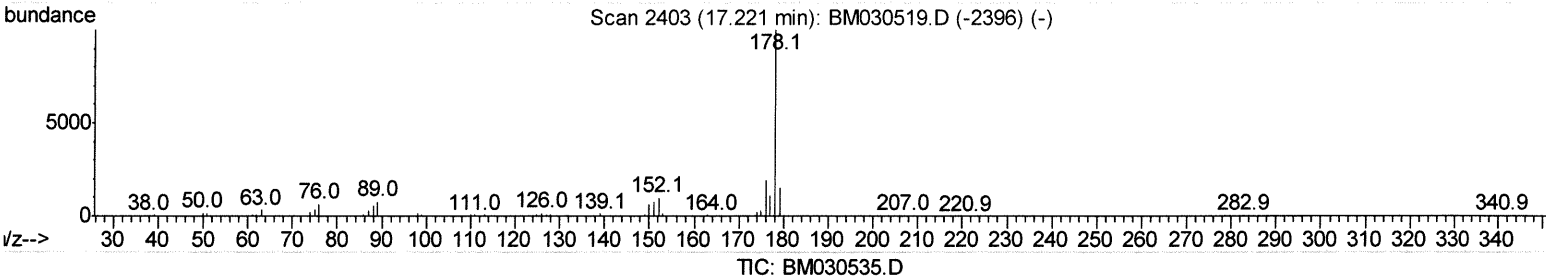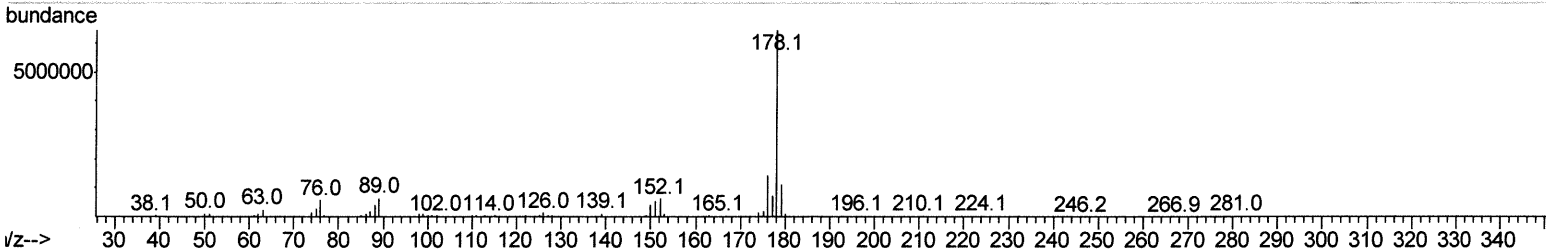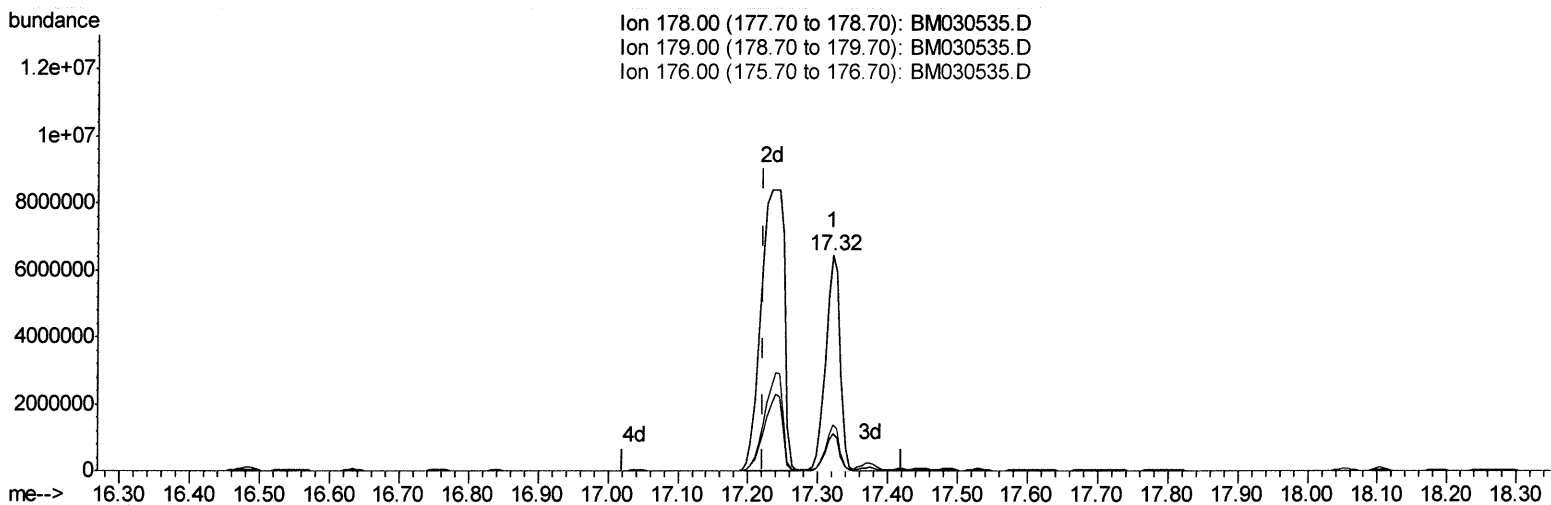

(72) Phenanthrene

17.321min (+0.100) 205.86ng/ul

response 9337177

Ion	Exp%	Act%
178.00	100	100
179.00	15.10	17.48
176.00	19.00	21.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:36:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

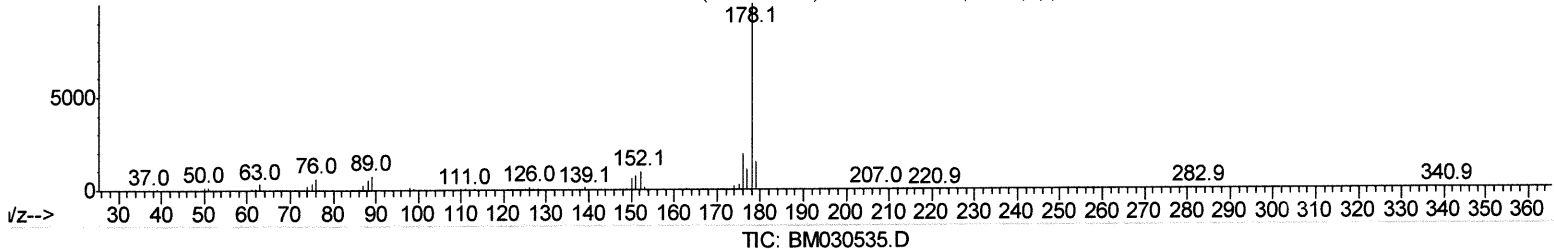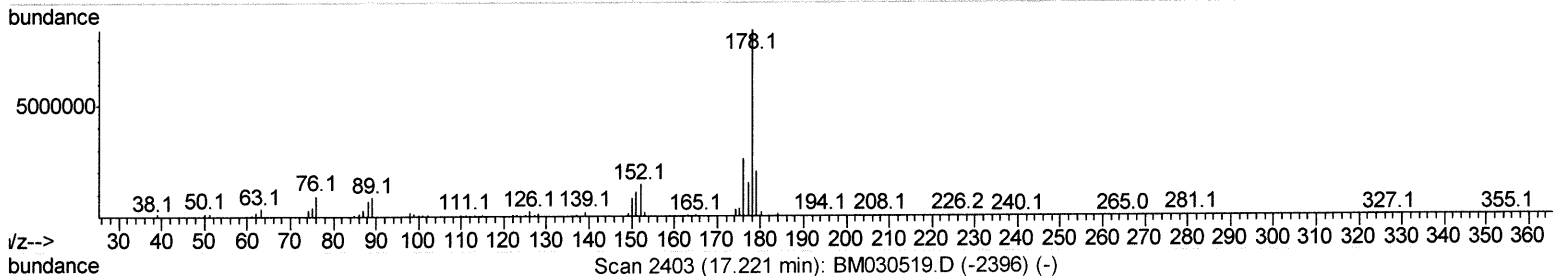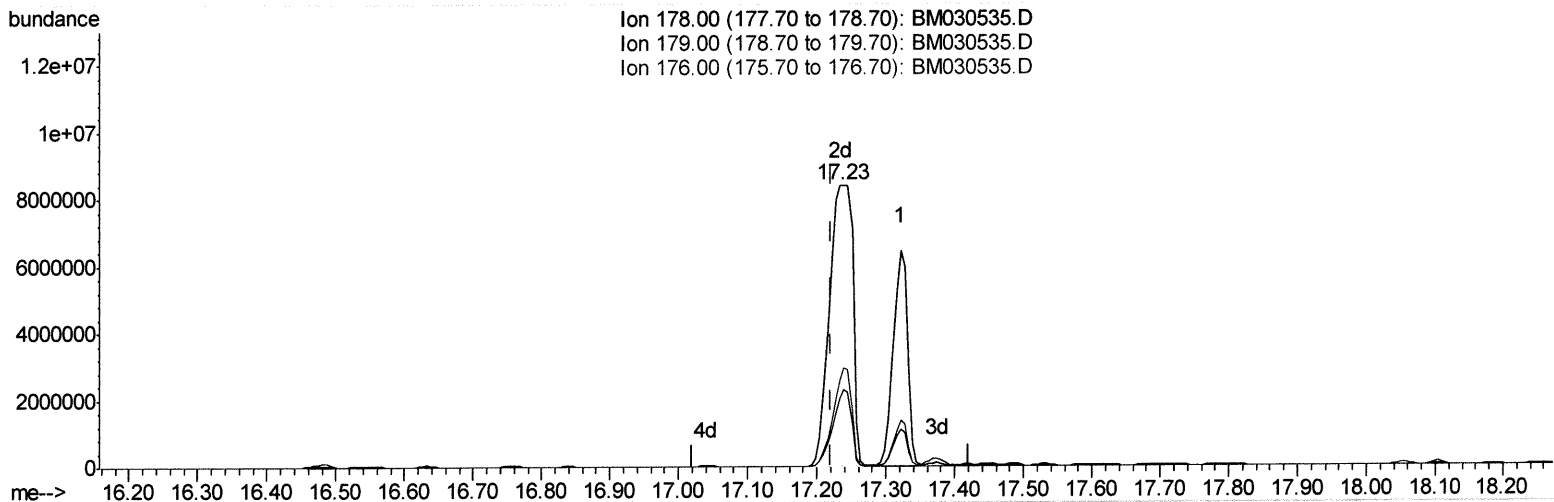

(72) Phenanthrene

17.233min (+0.012) 431.36ng/ul m

JU 6/23/21

response 19565796

Ion	Exp%	Act%
178.00	100	100
179.00	15.10	24.09#
176.00	19.00	30.64#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
Data File : BM030535.D
Acq On : 23 Jun 2021 03:48
Operator : CG/JU
Sample : M2662-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDF4

Manual Integrations
APPROVED

mohammad
6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:40:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 01:33:40 2021
Response via : Initial Calibration

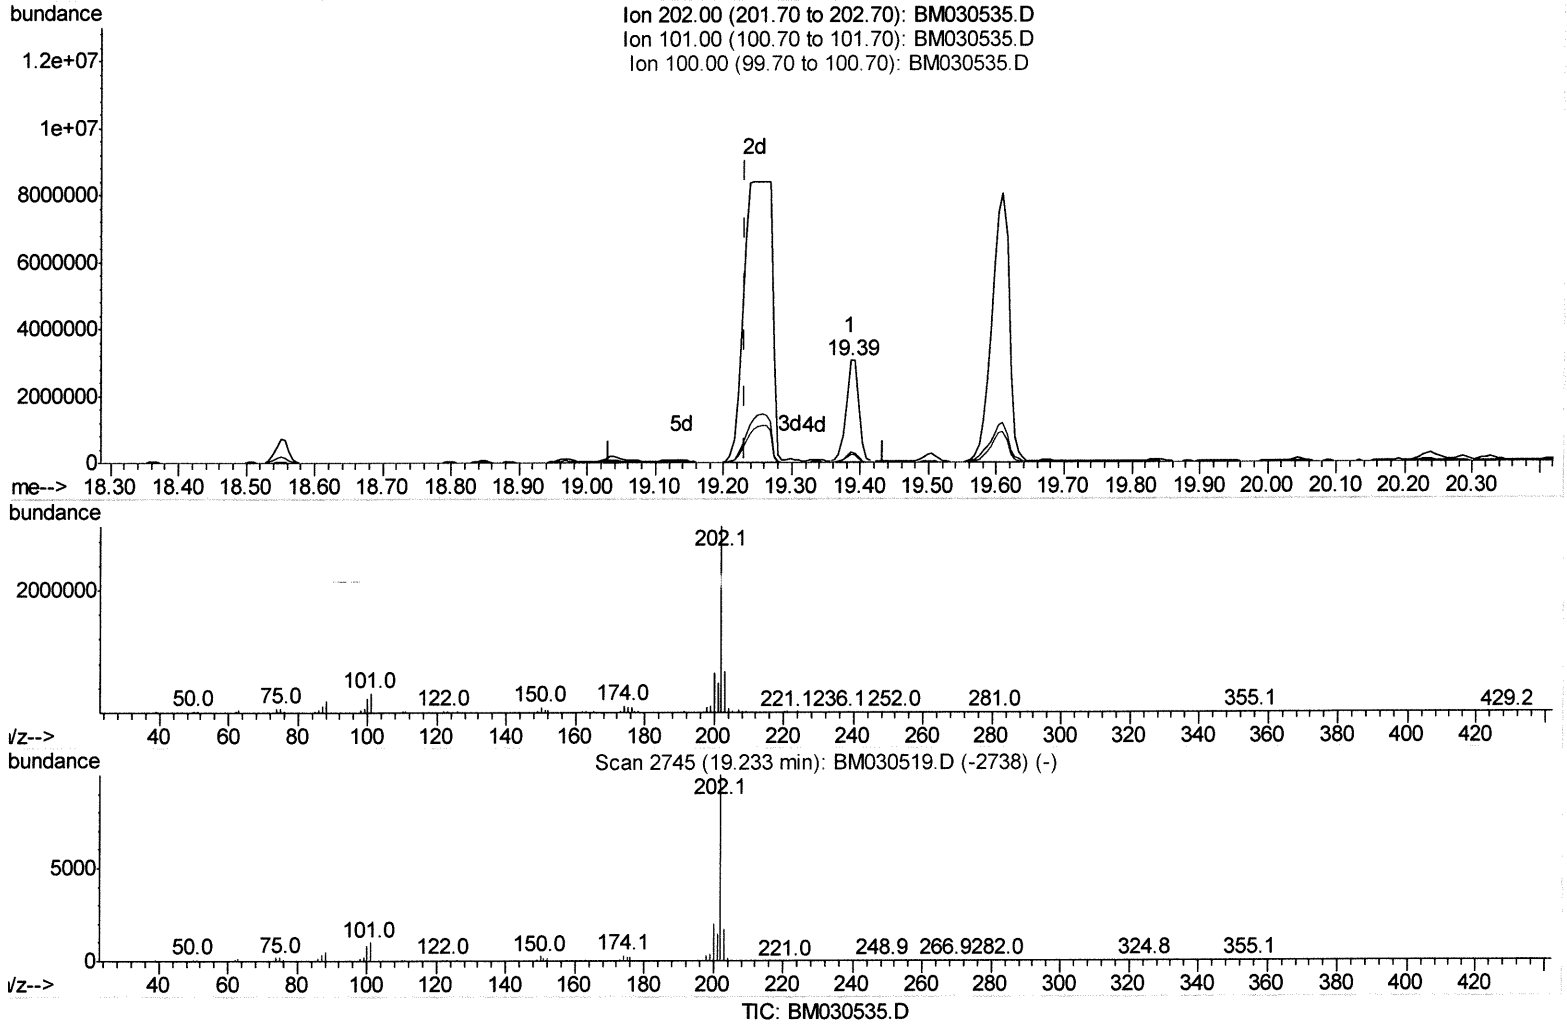

(80) Fluoranthene

19.386min (+0.153) 58.11ng/ul

response 3978451

Ion	Exp%	Act%
202.00	100	100
101.00	11.00	10.33
100.00	8.50	7.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:40:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

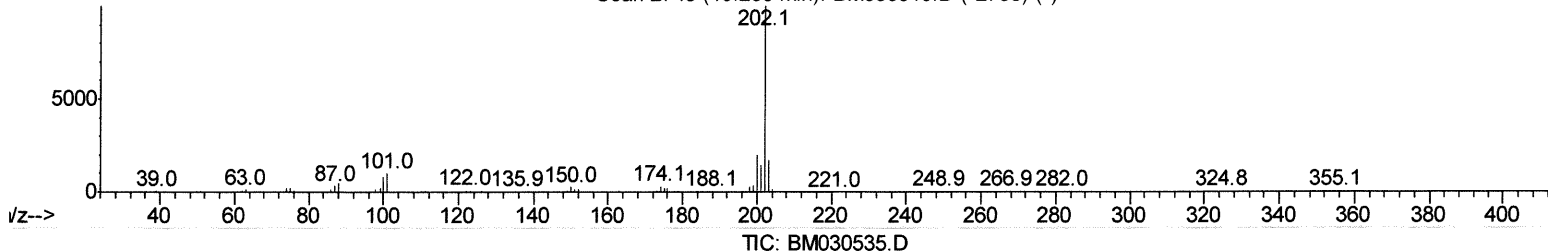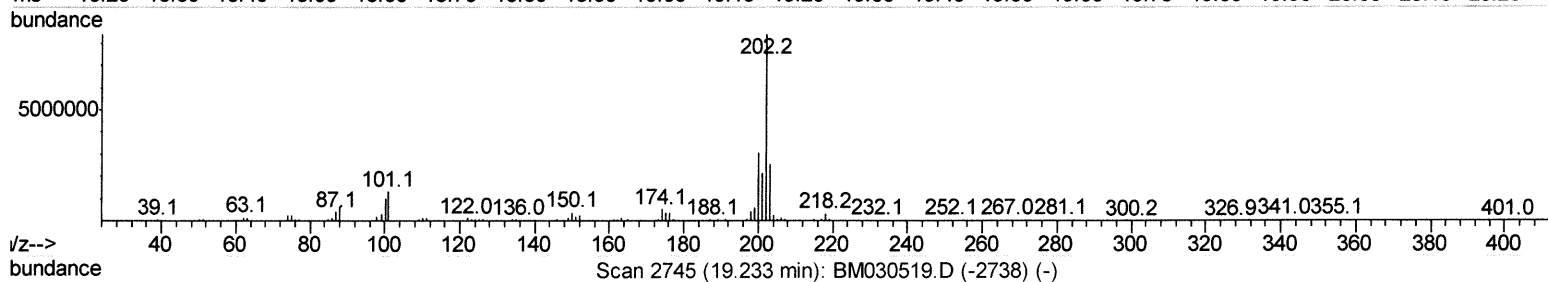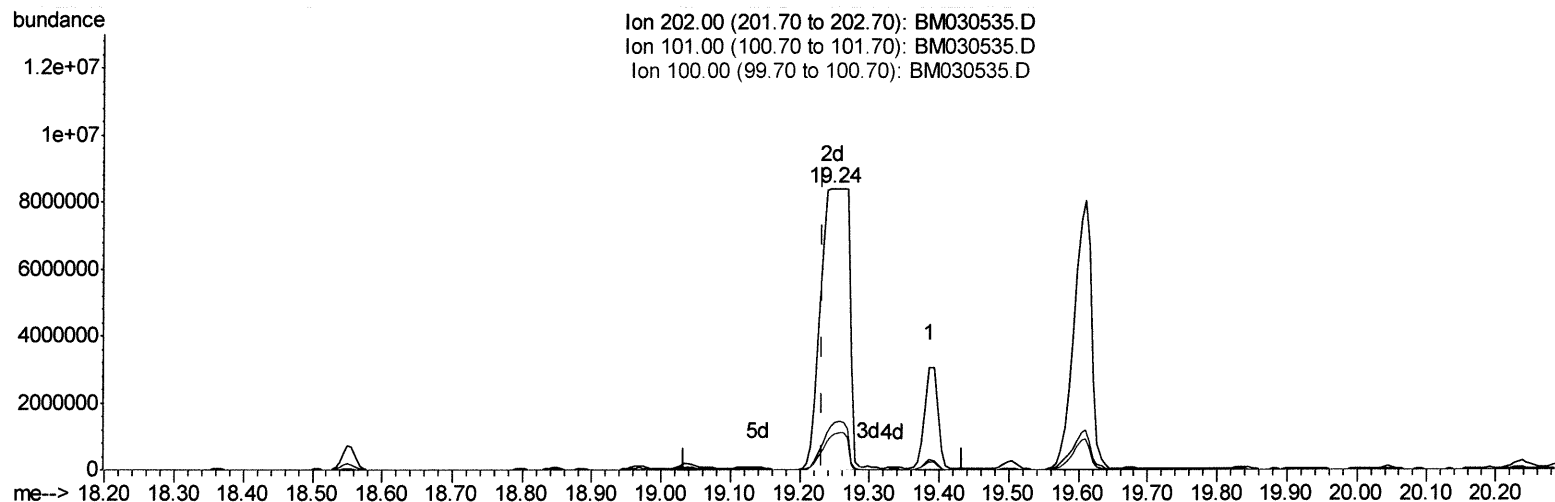

(80) Fluoranthene

19.245min (+0.012) 347.37ng/ul m *JU 6/23/21*

response 23783342

Ion	Exp%	Act%
202.00	100	100
101.00	11.00	15.52#
100.00	8.50	11.96#
0.00	0.00	0.00



Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:41:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

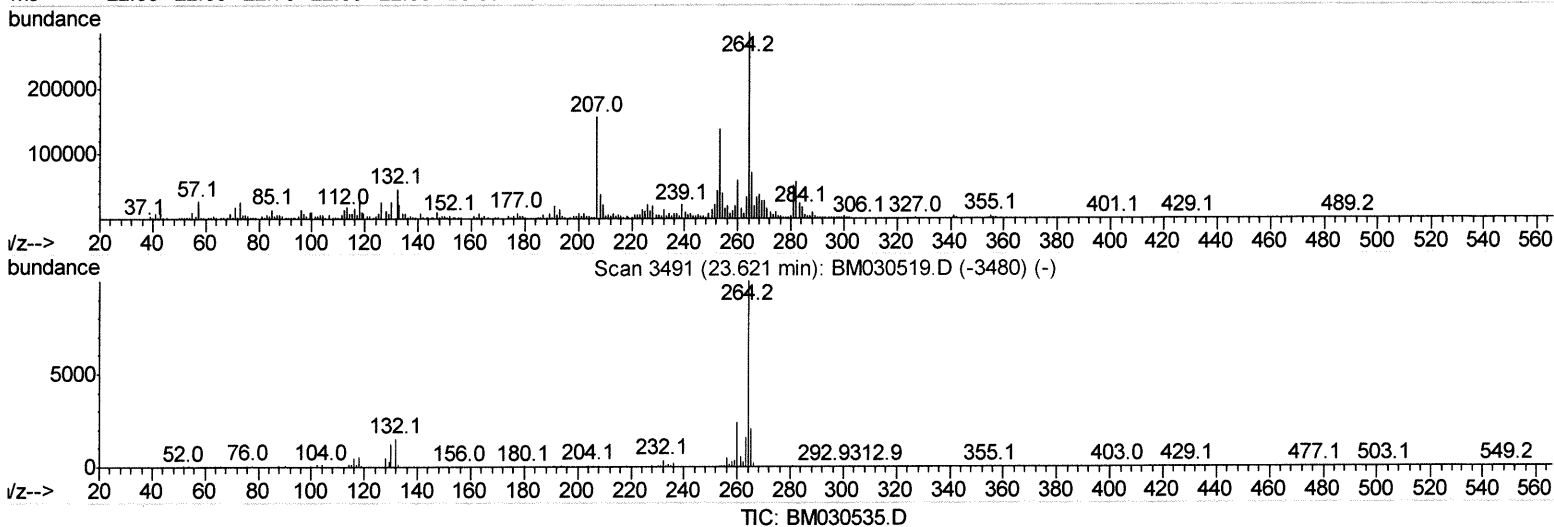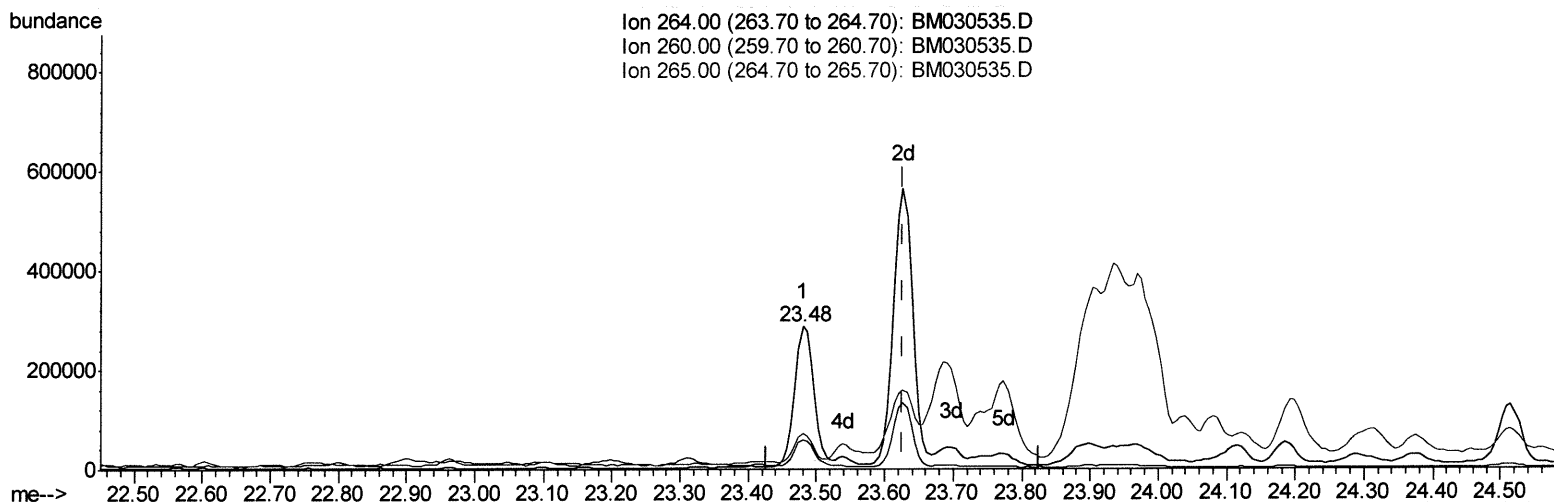

(88) Perylene-d12 (I)

23.480min (-0.147) 20.00ng/ul

response 501198

Ion	Exp%	Act%
264.00	100	100
260.00	23.80	20.80
265.00	21.70	24.70
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:41:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

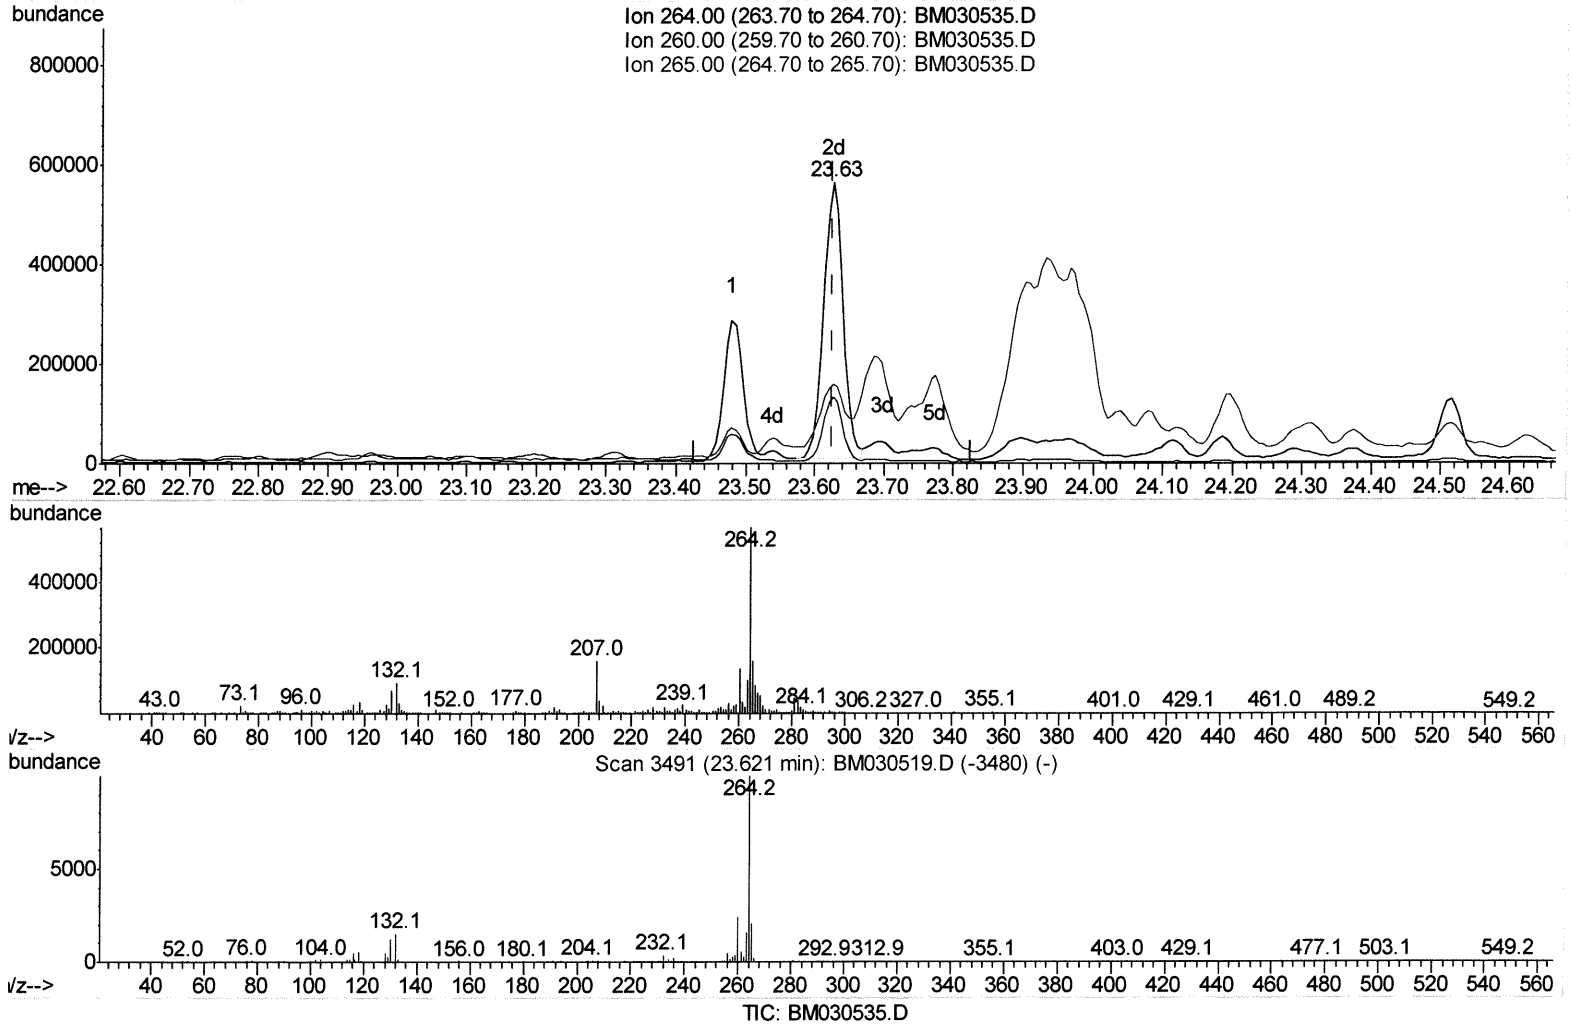

(88) Perylene-d12 (I)

23.627min (-0.000) 20.00ng/ul *mf 6/23/21*

response 1085064

Ion	Exp%	Act%
264.00	100	100
260.00	23.80	23.76
265.00	21.70	28.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:42:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

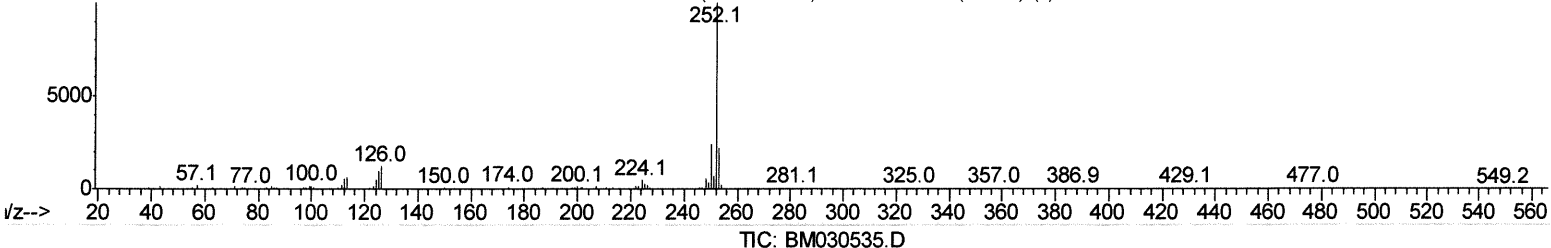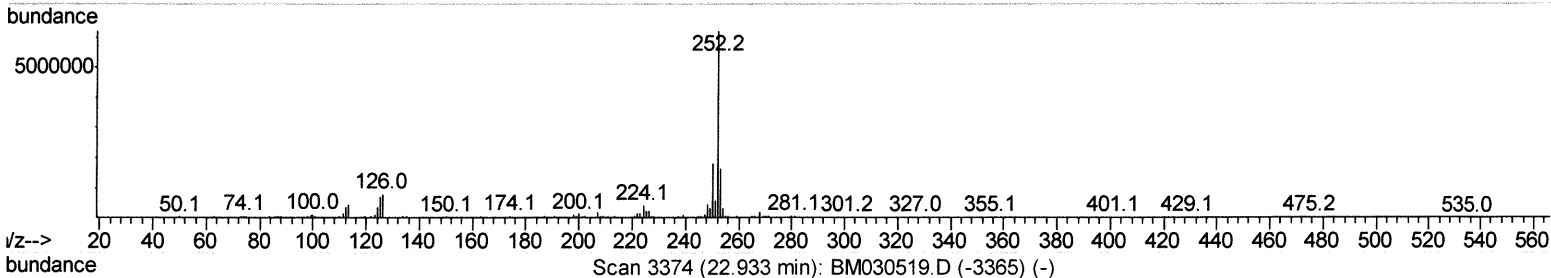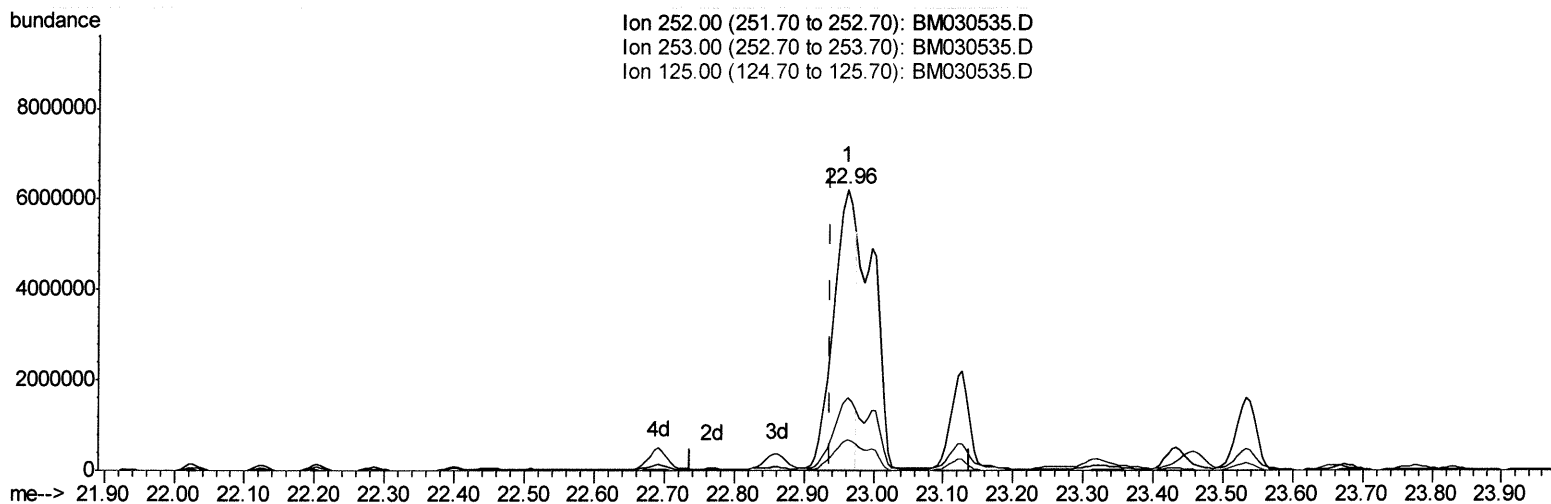

(90) Benzo(b)fluoranthene

22.962min (+0.023) 199.10ng/ul

response 13716026

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	25.76
125.00	9.60	10.82
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
Data File : BM030535.D
Acq On : 23 Jun 2021 03:48
Operator : CG/JU
Sample : M2662-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDF4

Manual Integrations
APPROVED

mohammad
6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:42:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 01:33:40 2021
Response via : Initial Calibration

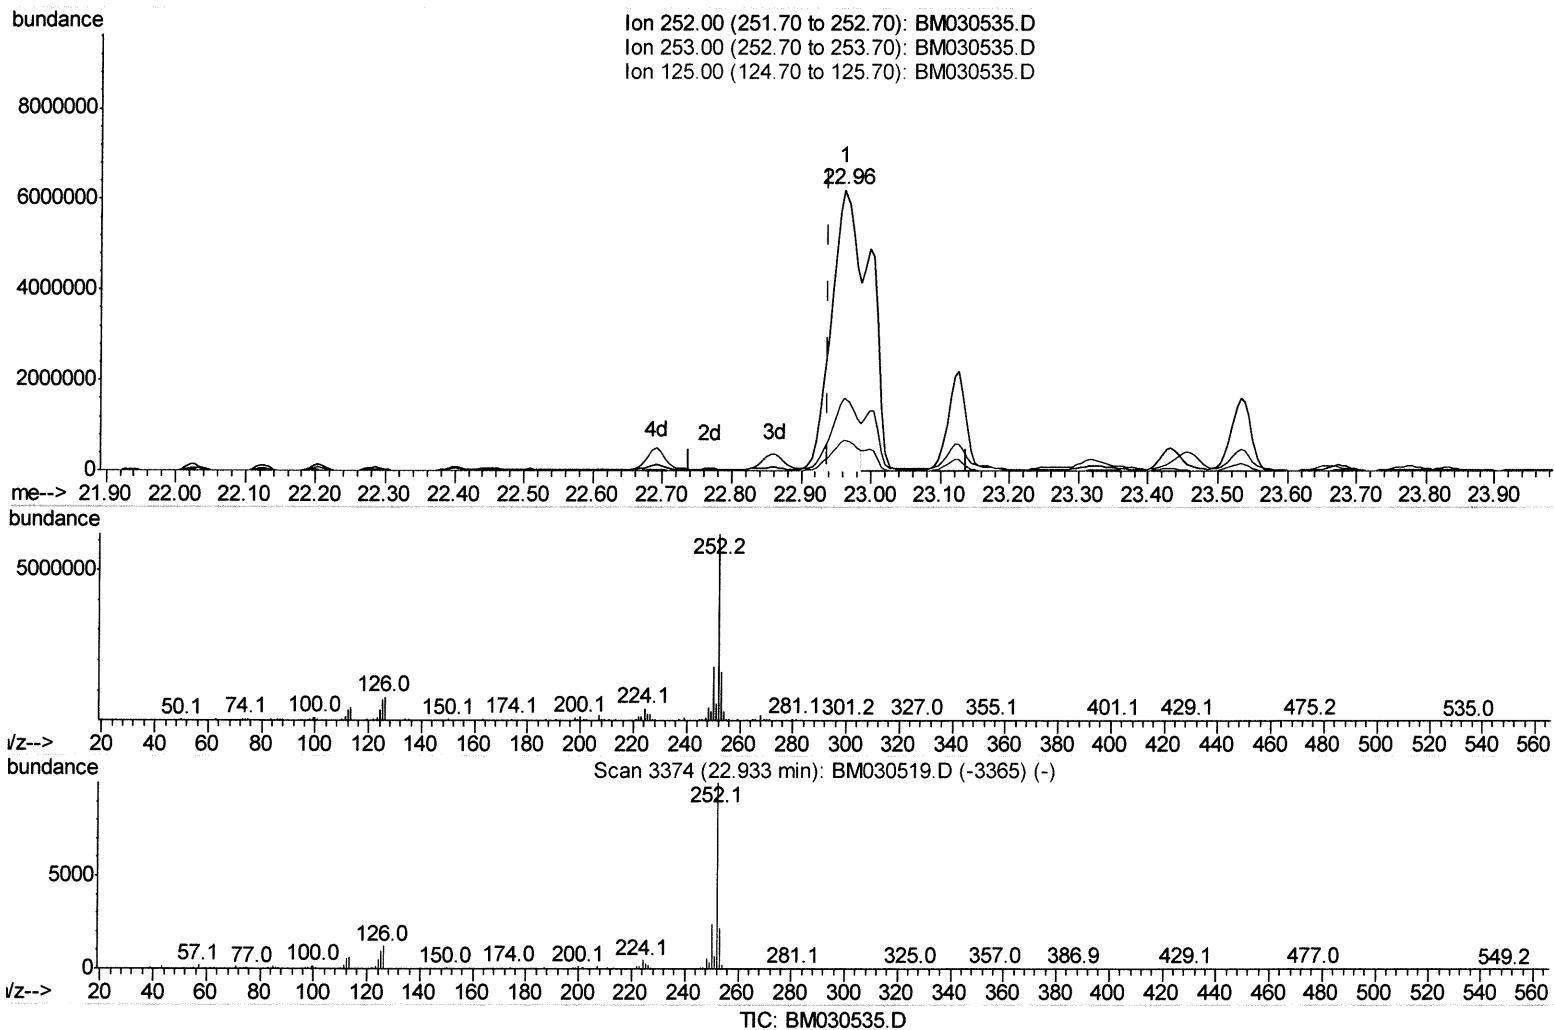

(90) Benzo(b)fluoranthene

22.962min (+0.023) 244.22ng/ul m

JP 6/28/24

response 16824199

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	25.76
125.00	9.60	10.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:44:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

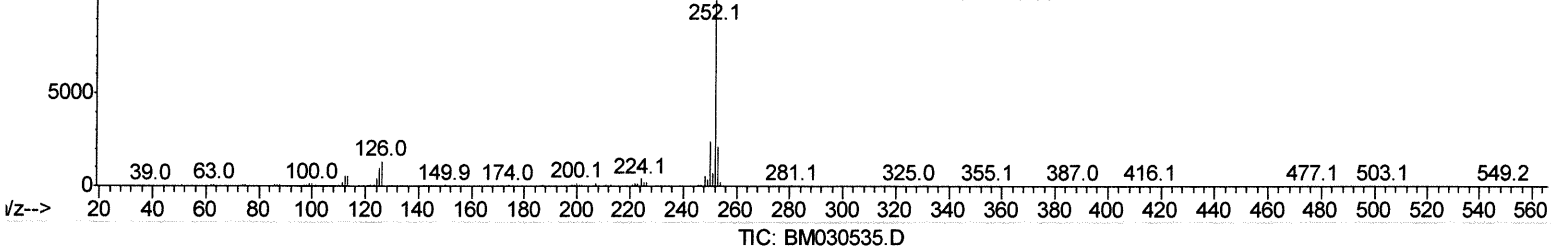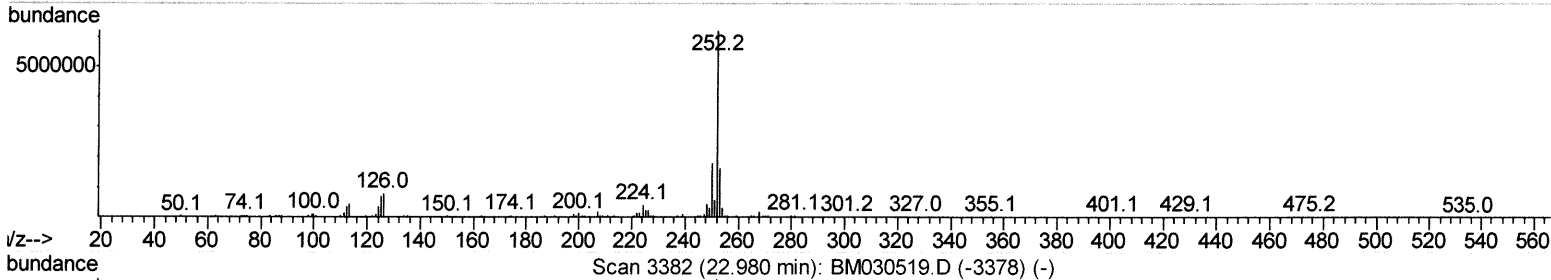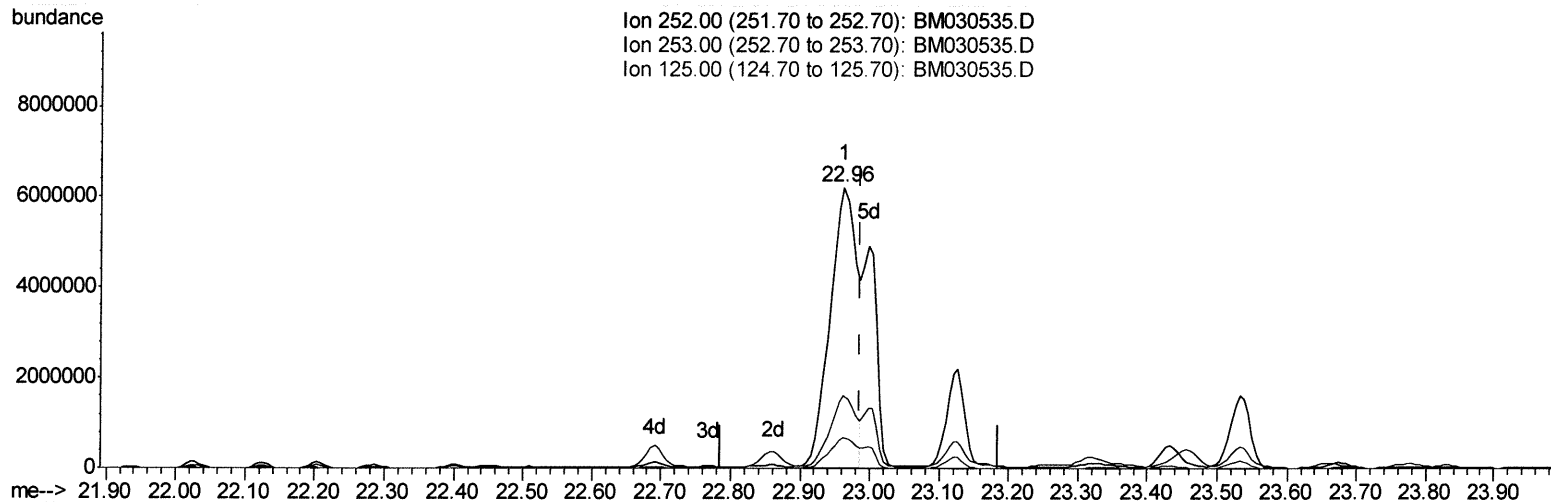

(91) Benzo(k)fluoranthene

22.962min (-0.024) 253.19ng/ul

response 16762138

Ion	Exp%	Act%
252.00	100	100
253.00	21.80	25.76
125.00	9.90	10.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:44:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

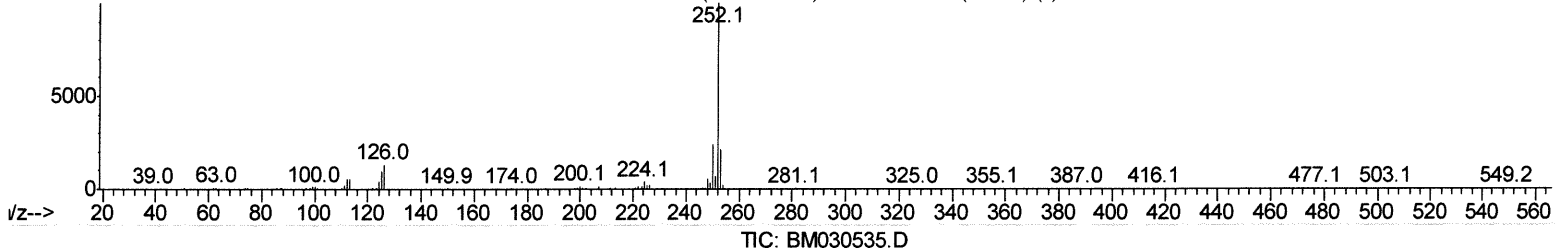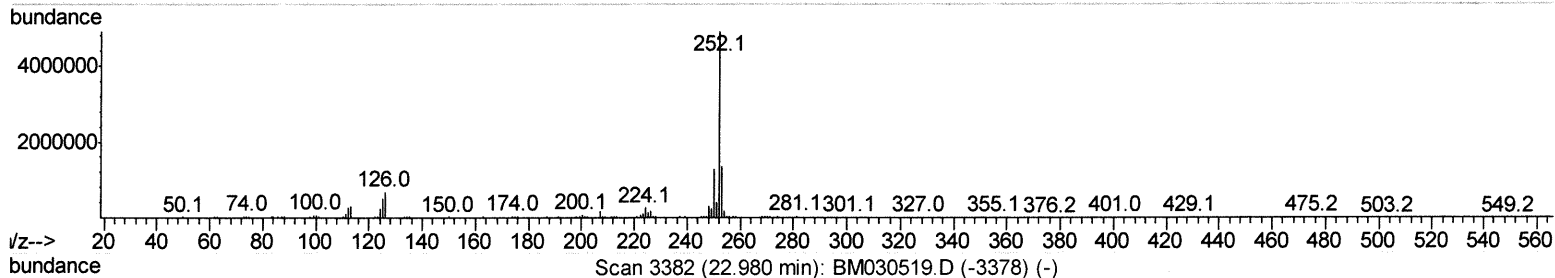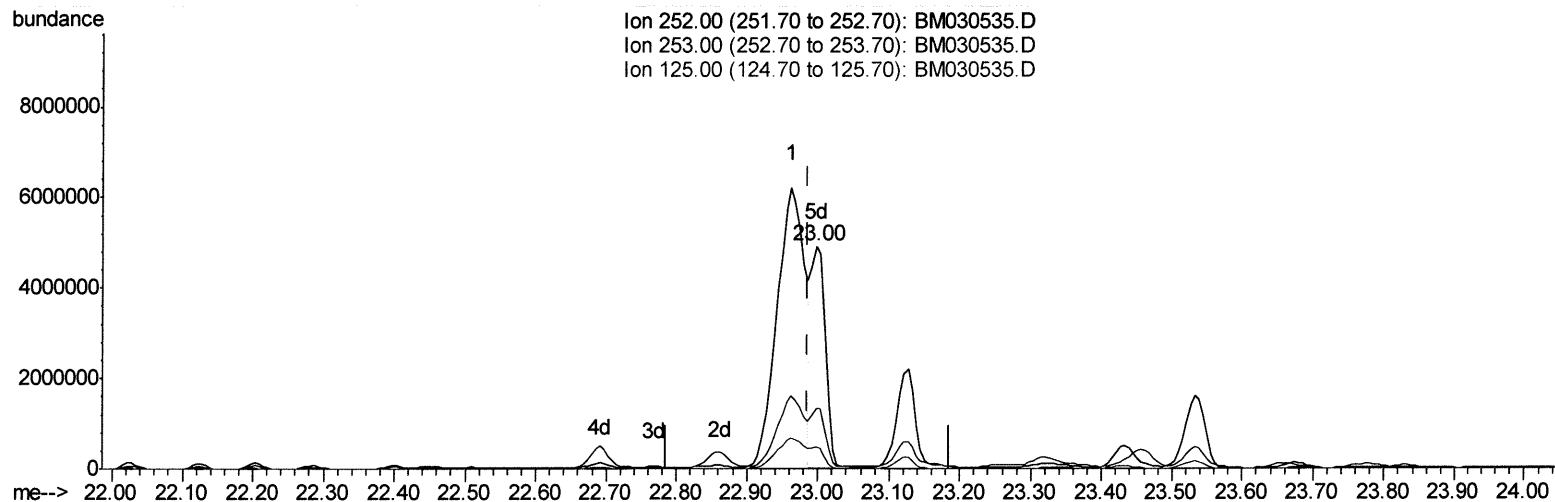

(91) Benzo(k)fluoranthene

22.997min (+0.012) 101.76ng/ul m *JU 6/23/21*

response 6737078

Ion	Exp%	Act%
252.00	100	100
253.00	21.80	27.12#
125.00	9.90	10.04
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:45:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

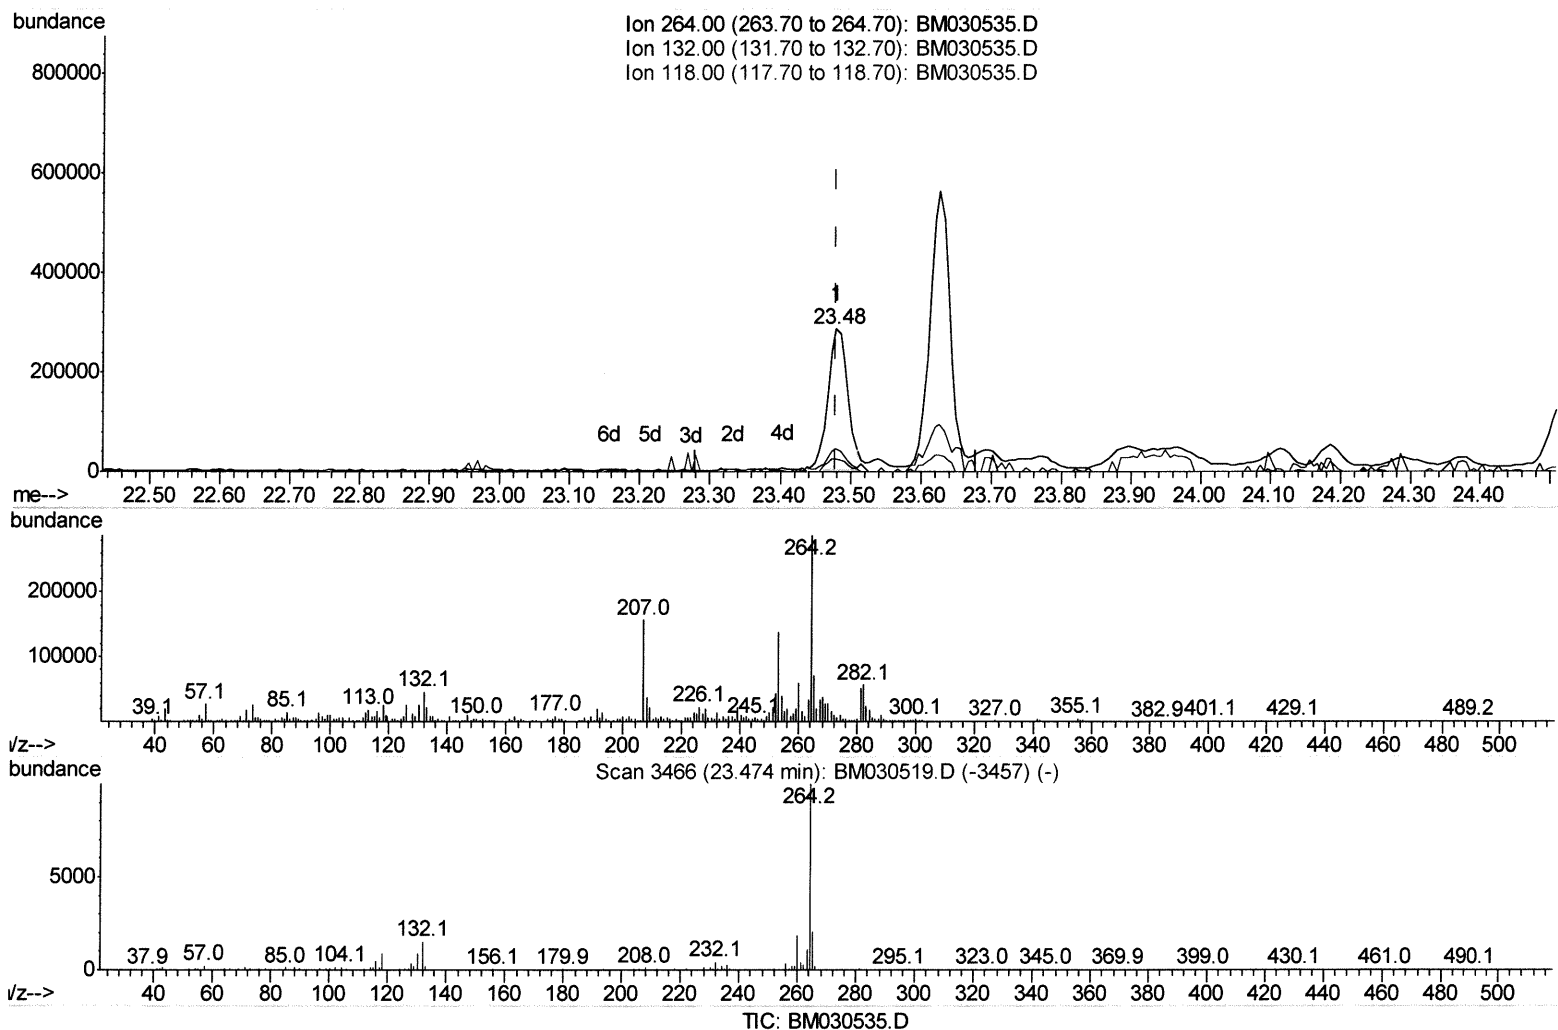

(92) Benzo(a)pyrene-d12 (S)

23.480min (-0.000) 9.61ng/ul

response 542037

Ion	Exp%	Act%
264.00	100	100
132.00	16.00	15.85
118.00	9.10	8.98
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:45:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

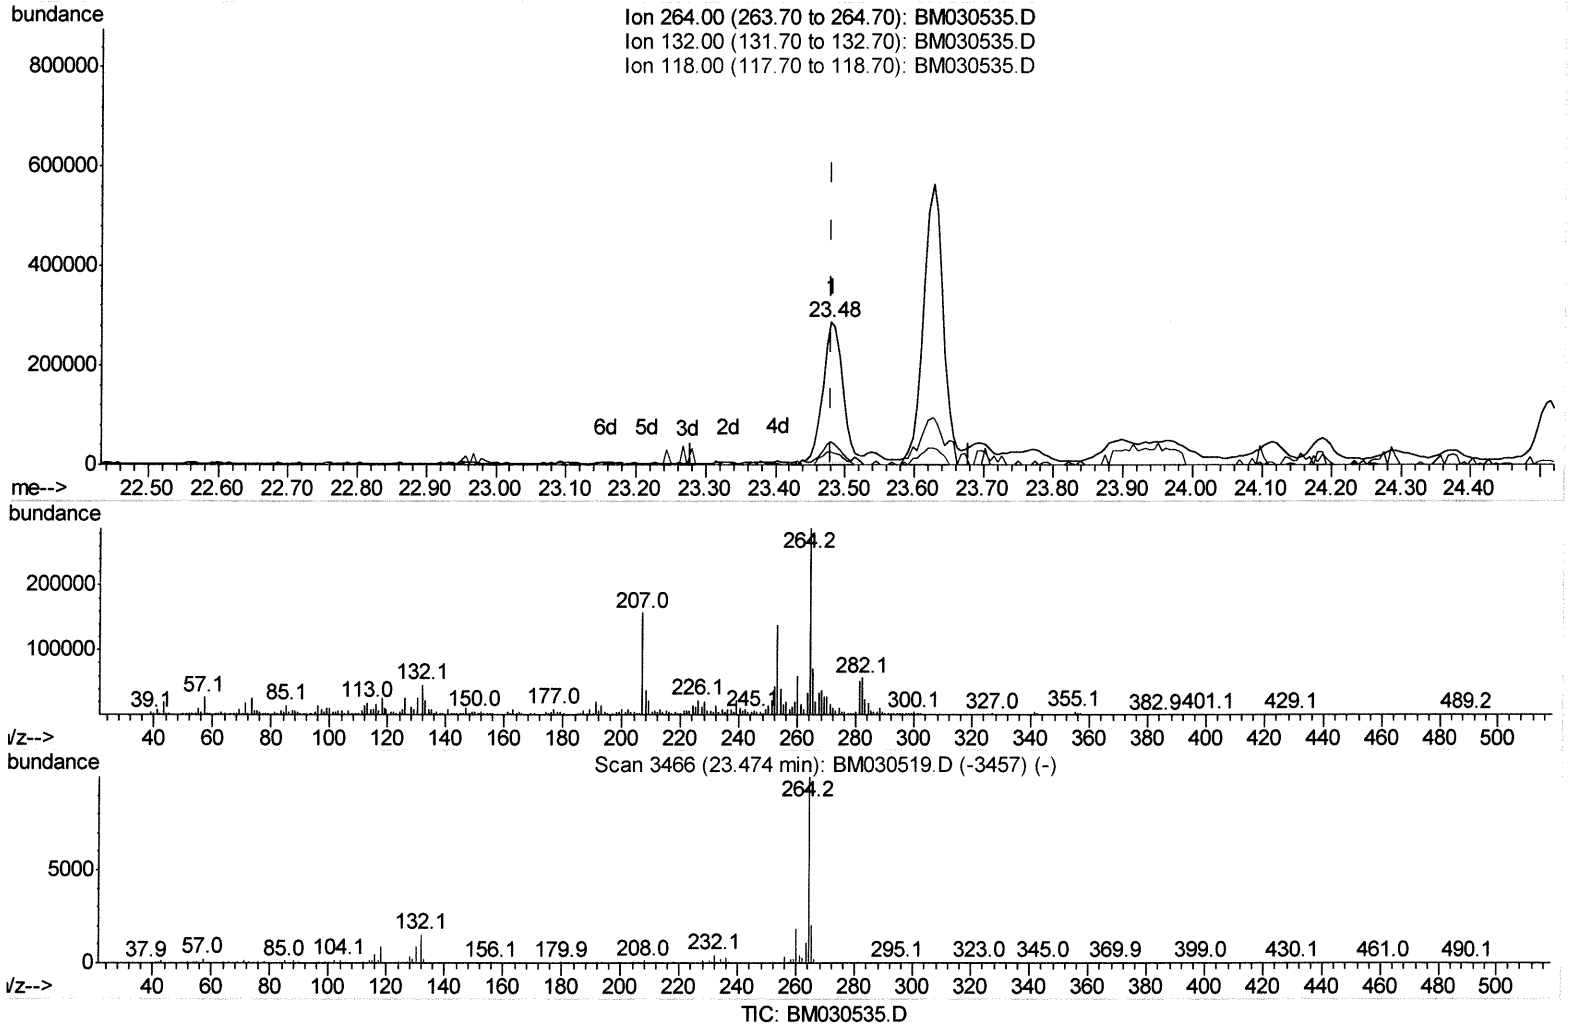

(92) Benzo(a)pyrene-d12 (S)

23.480min (-0.000) 9.87ng/ul m *Ju 6/23/21*

response 556647

Ion	Exp%	Act%
264.00	100	100
132.00	16.00	15.85
118.00	9.10	8.98
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:46:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

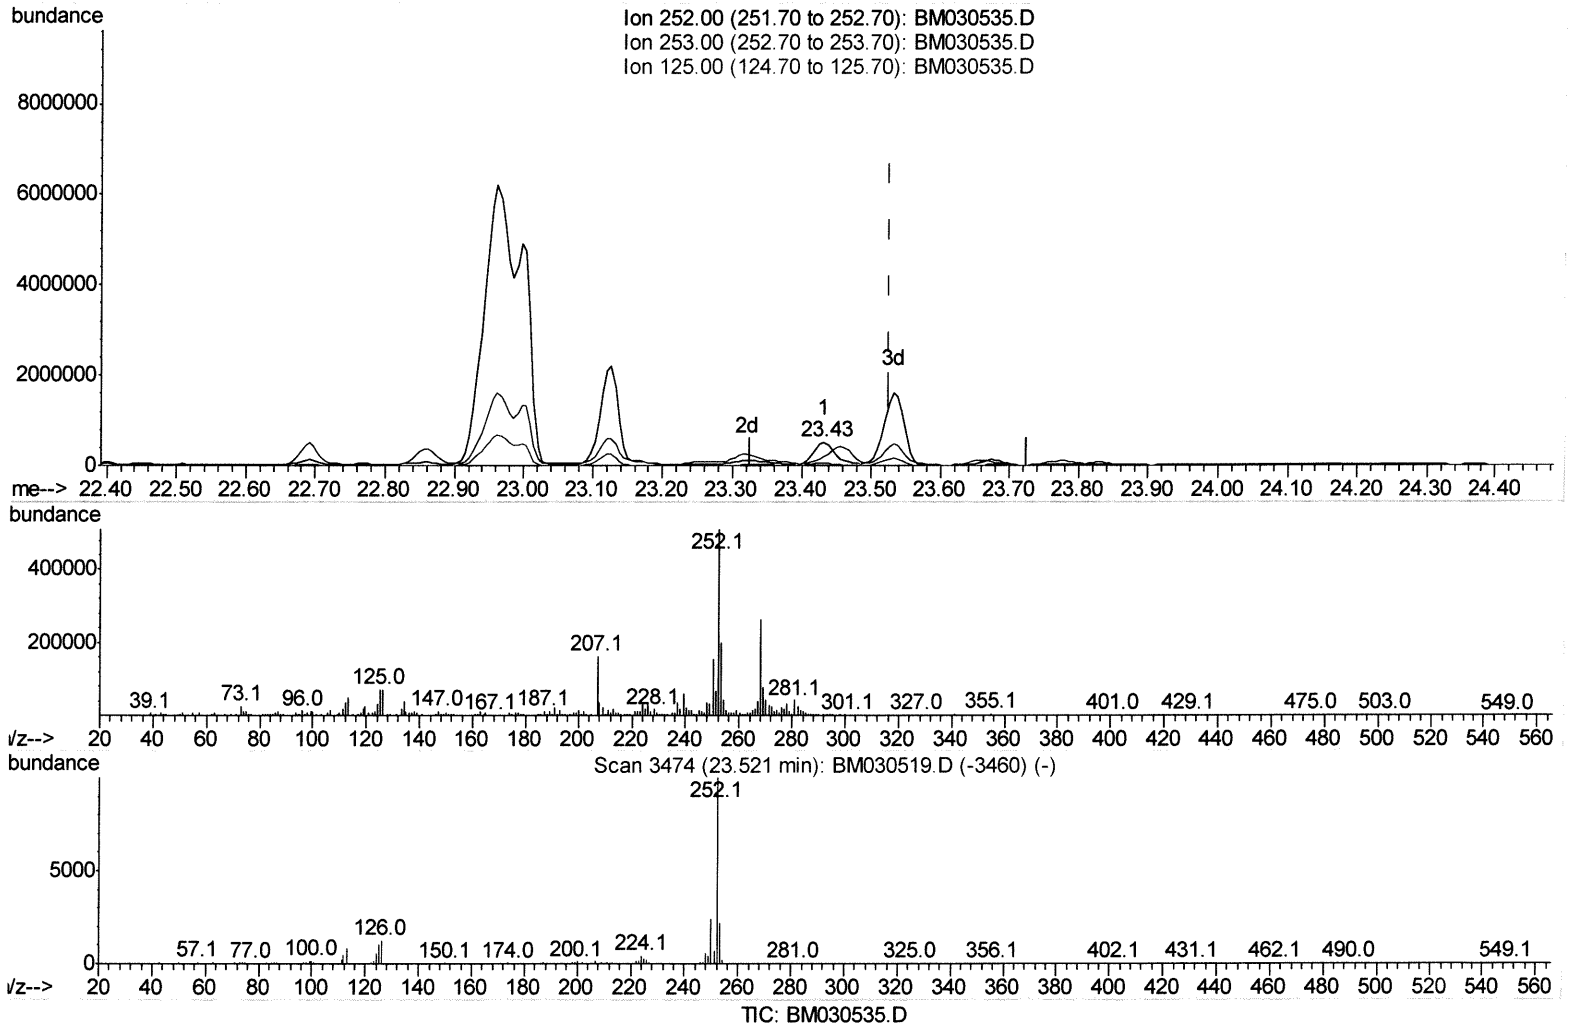

(93) Benzo(a)pyrene (C)

23.433min (-0.094) 16.60ng/ul

response 1027987

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	39.25#
125.00	10.80	13.74#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:46:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

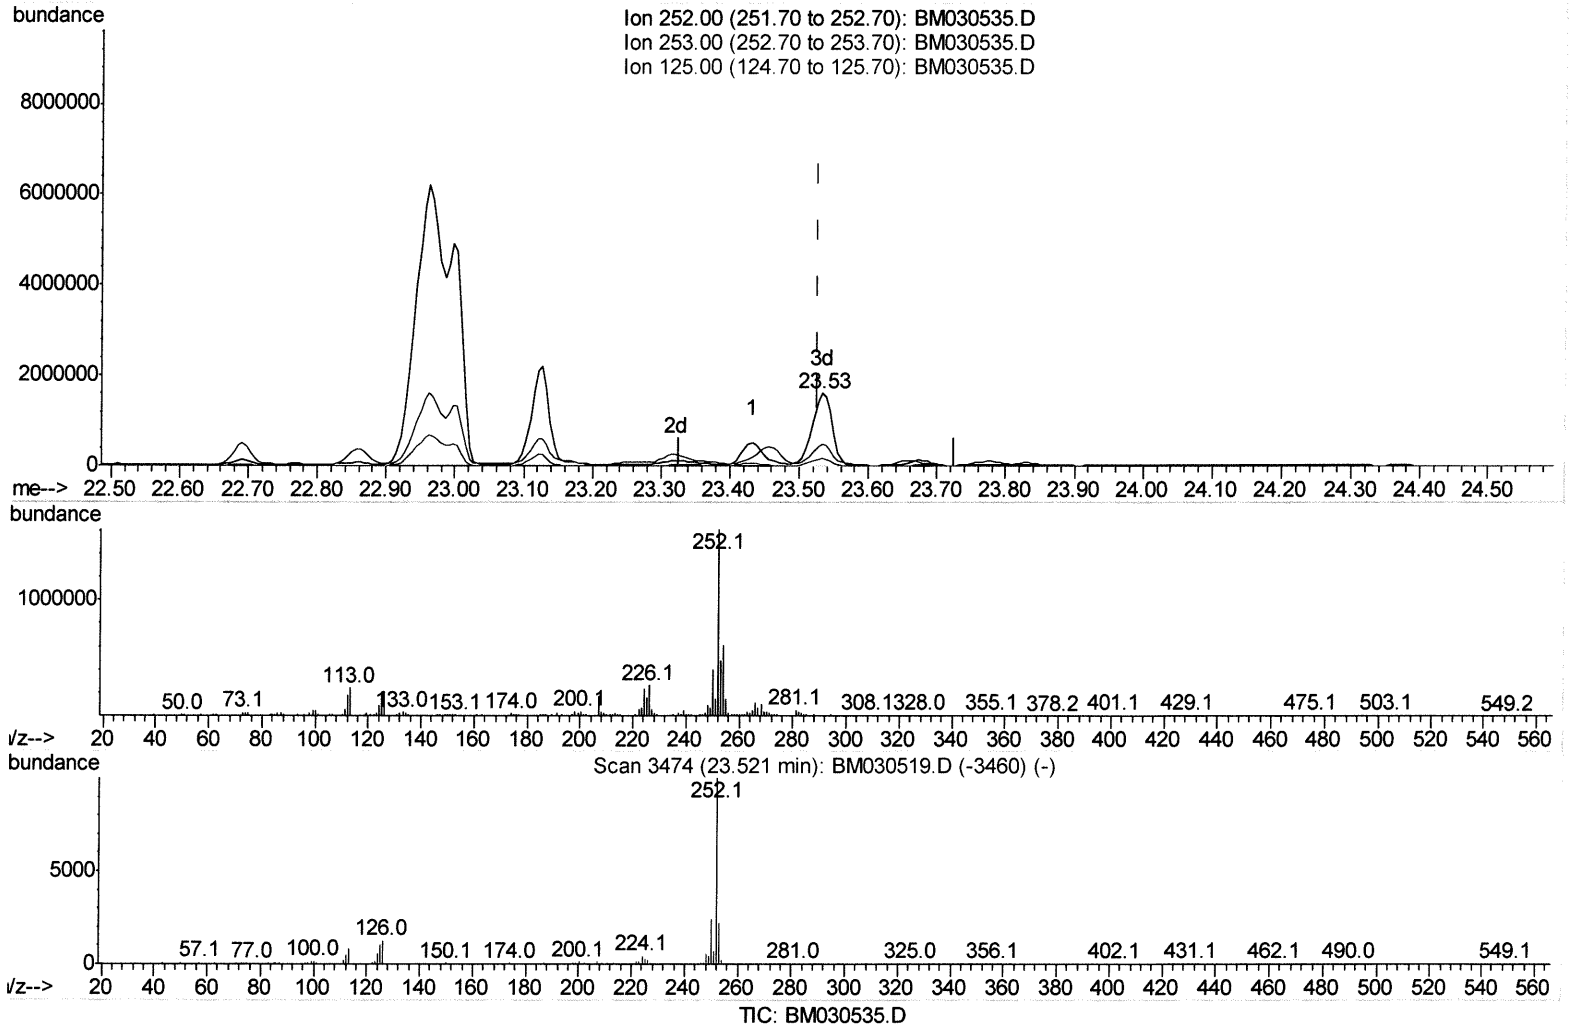

(93) Benzo(a)pyrene (C)

23.533min (+0.006) 51.11ng/ul m

JU 6/20/21

response 3166019

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	29.29#
125.00	10.80	10.38
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:47:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

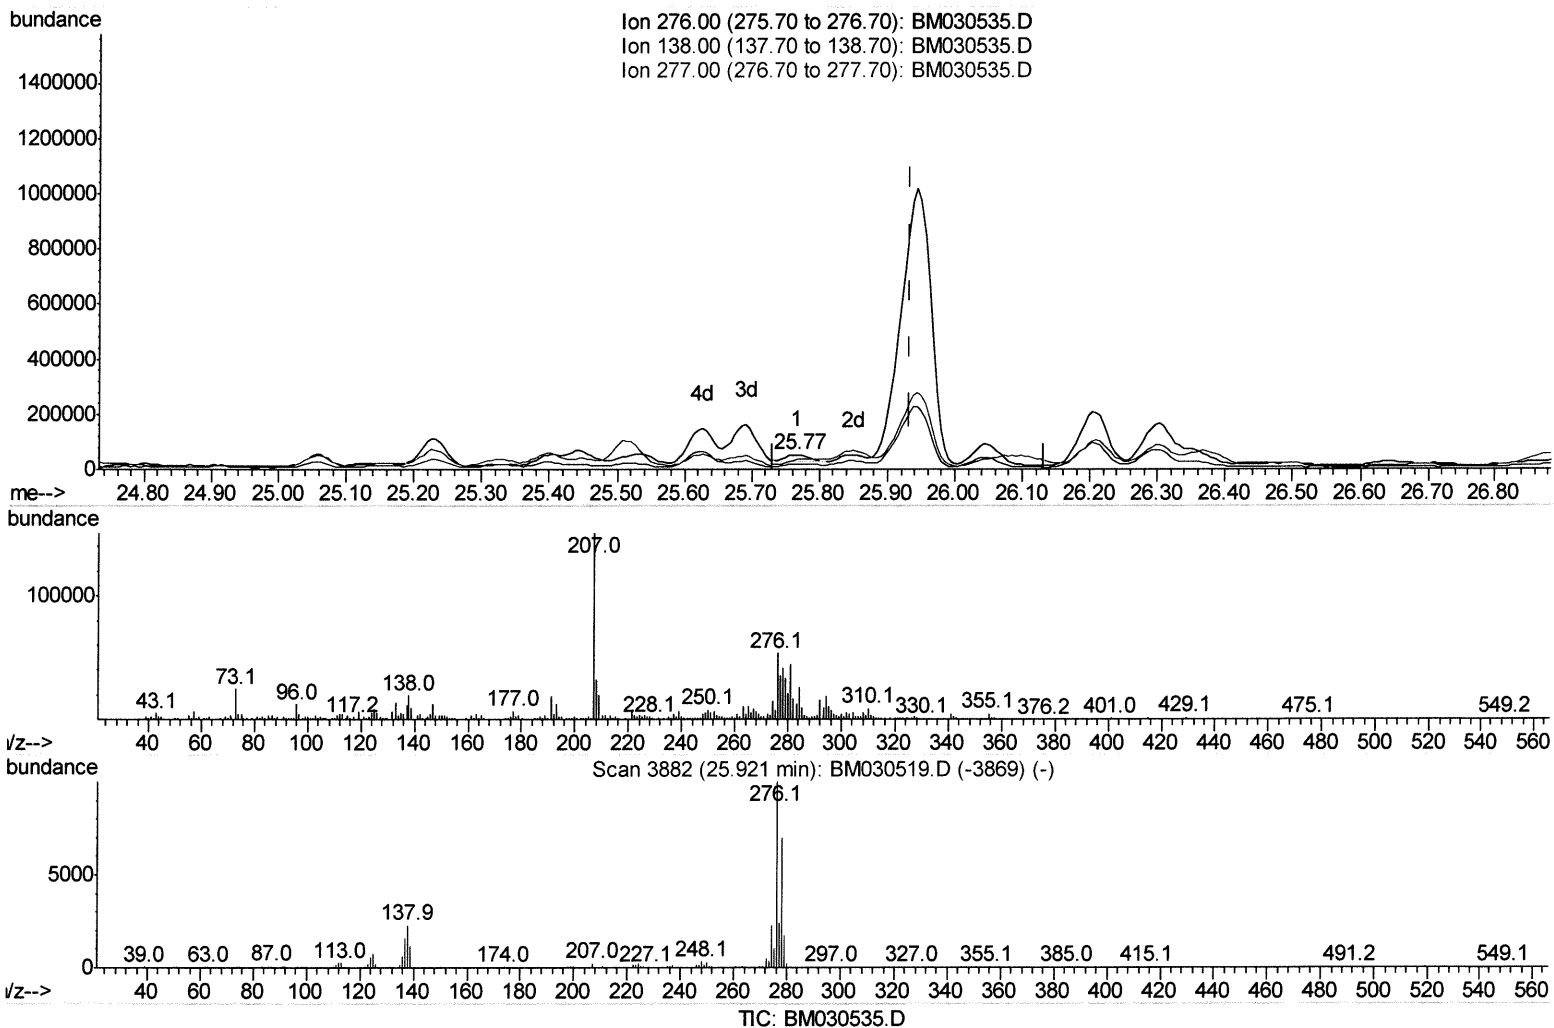

(94) Indeno(1,2,3-cd)pyrene

25.768min (-0.165) 0.84ng/ul

response 65423

Ion	Exp%	Act%
276.00	100	100
138.00	24.40	36.57#
277.00	24.50	66.70#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:47:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

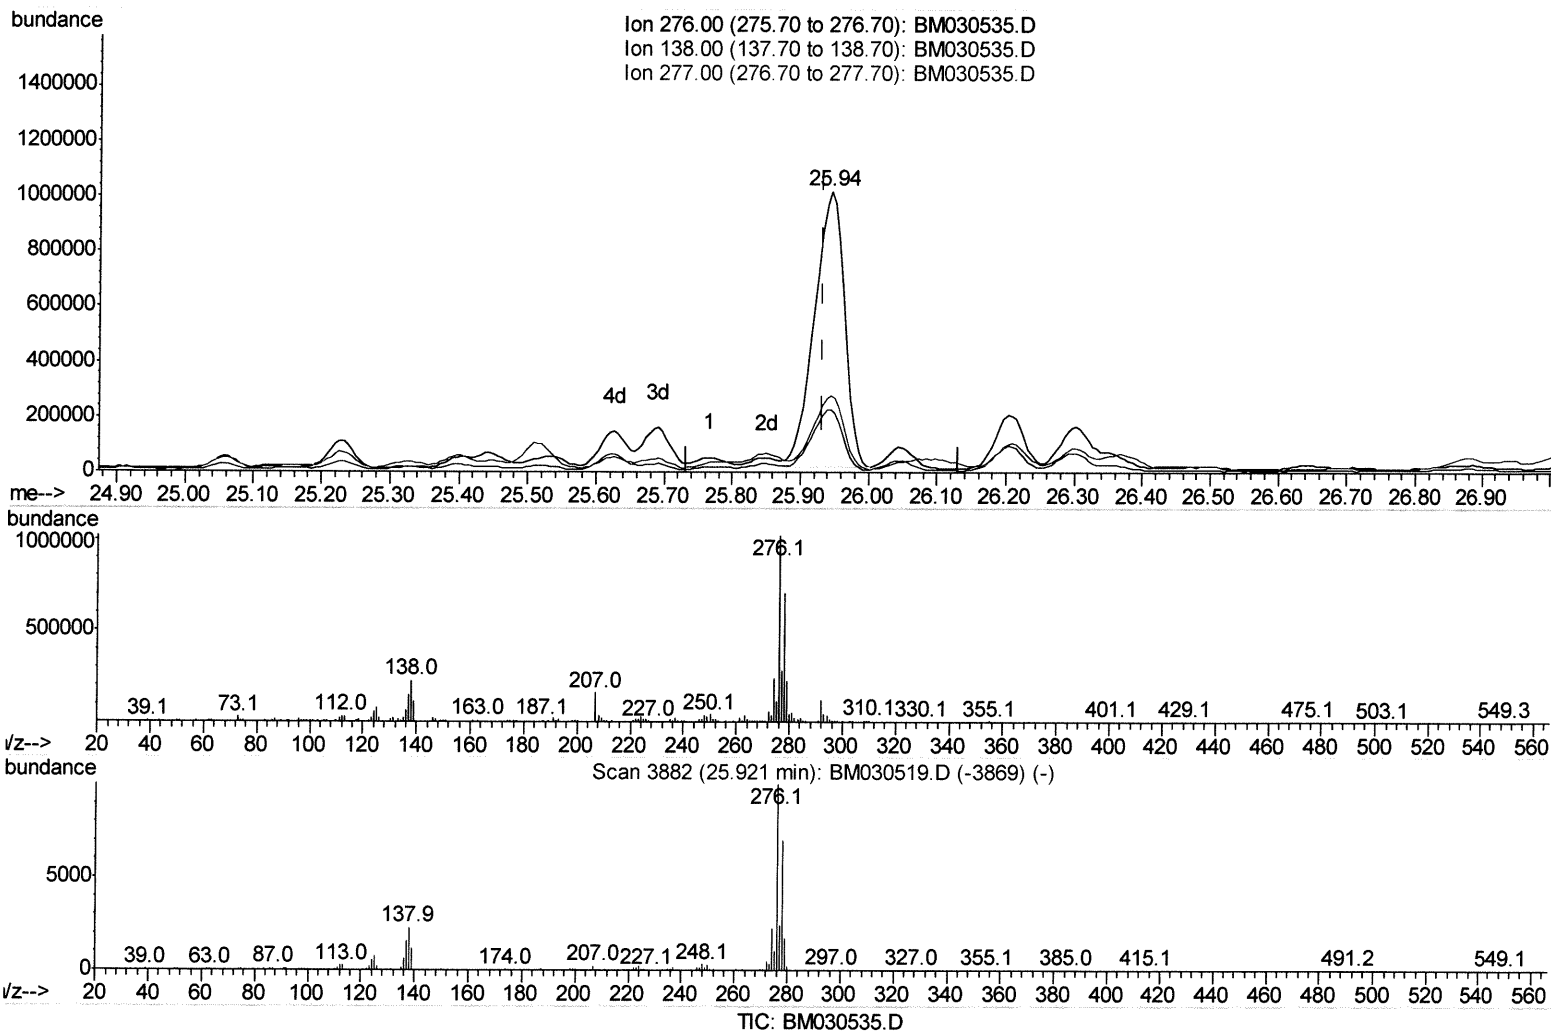

(94) Indeno(1,2,3-cd)pyrene

25.944min (+0.012) 39.66ng/ul m

response 3092562

Ion	Exp%	Act%
276.00	100	100
138.00	24.40	22.15
277.00	24.50	27.37
0.00	0.00	0.00

Ju 6/23/21


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:48:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

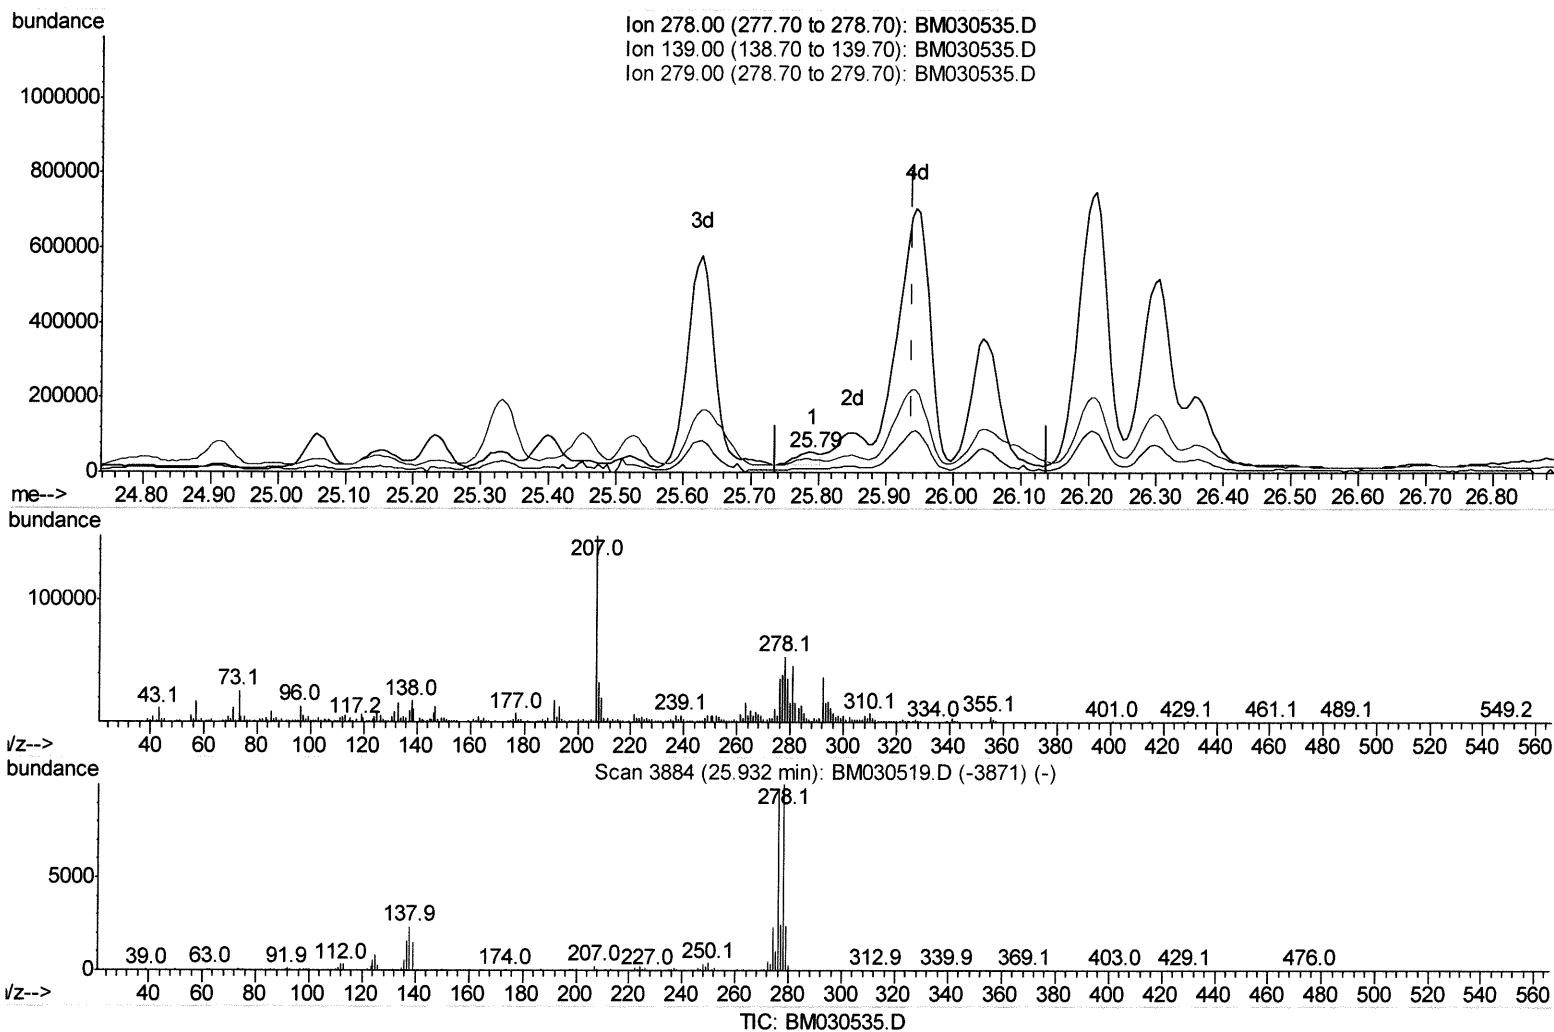

(95) Dibenzo(a,h)anthracene

25.791min (-0.147) 1.27ng/ul

response 81903

Ion	Exp%	Act%
278.00	100	100
139.00	16.00	20.50#
279.00	23.90	66.62#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BGDF4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:48:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

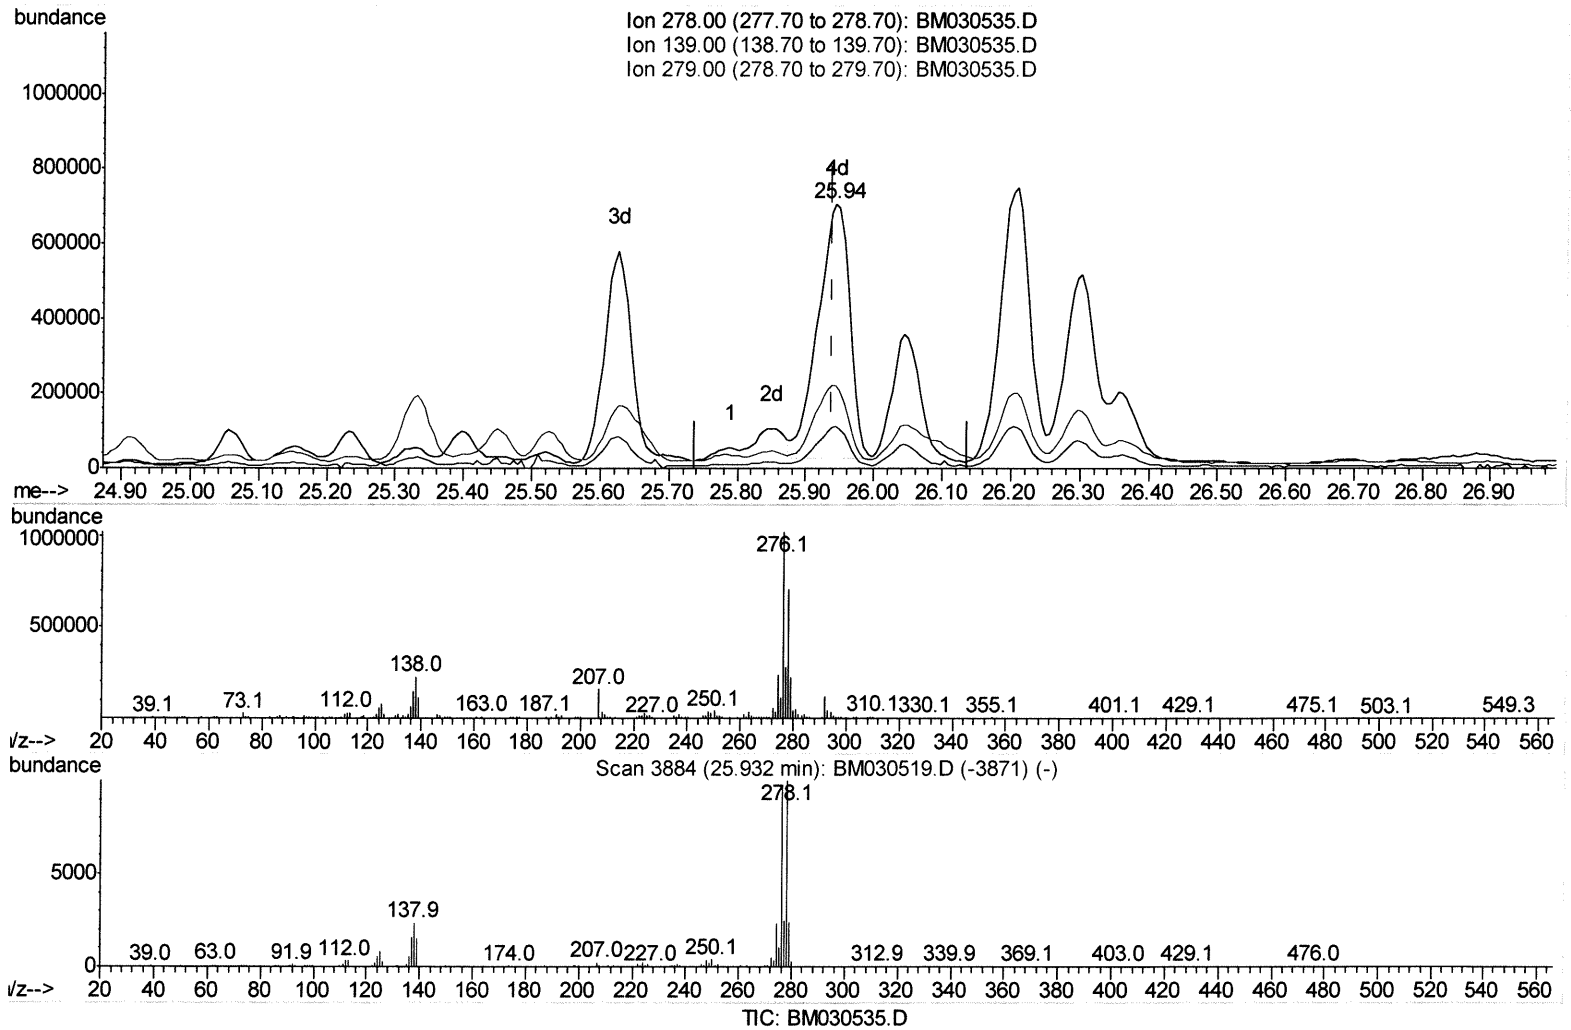

(95) Dibenzo(a,h)anthracene

25.944min (+0.006) 34.08ng/ul m

response 2202826

Ion	Exp%	Act%
278.00	100	100
139.00	16.00	15.91
279.00	23.90	31.18#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
 Data File : BM030535.D
 Acq On : 23 Jun 2021 03:48
 Operator : CG/JU
 Sample : M2662-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDF4

Quant Time: Jun 23 04:50:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:54 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	189005	20.00	ng/ul	0.00
20) Naphthalene-d8	10.60	136	710437	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.44	164	417152	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.18	188	844627	20.00	ng/ul	0.00
79) Chrysene-d12	21.36	240	1069891	20.00	ng/ul	0.01
88) Perylene-d12	23.63	264	1085064m	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	15933	3.42	ng/uL	0.00
4) Pyridine-d5	3.70	84	114534	9.14	ng/ul	0.00
7) Phenol-d5	6.97	99	313834	19.25	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.14	67	208266	20.33	ng/ul	0.00
11) 2-Chlorophenol-d4	7.34	132	267030	21.22	ng/ul	0.00
15) 4-Methylphenol-d8	8.51	113	251304	19.81	ng/ul	0.00
21) Nitrobenzene-d5	8.96	128	119376	22.52	ng/ul	0.00
24) 2-Nitrophenol-d4	9.68	143	127088	21.57	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.22	165	245141	21.72	ng/ul	0.00
31) 4-Chloroaniline-d4	10.74	131	265286	16.86	ng/ul	0.00
46) Dimethylphthalate-d6	13.85	166	731123	25.38	ng/ul	0.00
49) Acenaphthylene-d8	14.13	160	918412	24.56	ng/ul	0.00
54) 4-Nitrophenol-d4	14.64	143	77119	14.13	ng/ul	0.00
60) Fluorene-d10	15.43	176	676466	26.48	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.57	200	50528	9.14	ng/ul	0.02
73) Anthracene-d10	17.28	188	1047153	26.56	ng/ul	0.00
81) Pyrene-d10	19.57	212	793390	14.15	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.48	264	556647m	9.87	ng/ul	0.00

Target Compounds

				Ovalue	
8) Phenol	7.00	94	22932	1.391	ng/ul 95
30) Naphthalene	10.65	128	421215	11.710	ng/ul 100
36) 2-Methylnaphthalene	12.26	142	54428	2.168	ng/ul 99
37) 1-Methylnaphthalene	12.47	142	49496	1.948	ng/ul# 98
43) 1,1'-Biphenyl	13.27	154	121481	3.946	ng/ul 100
50) Acenaphthylene	14.16	152	1950465	56.240	ng/ul 99
52) Acenaphthene	14.50	153	773709	30.741	ng/ul 97
56) Dibenzofuran	14.83	168	1233986	35.169	ng/ul 98
61) Fluorene	15.49	166	1905371	65.892	ng/ul 100
72) Phenanthrene	17.23	178	19565796m	431.364	ng/ul
74) Anthracene	17.32	178	9325787	201.088	ng/ul 94
77) Carbazole	17.58	167	133668	3.214	ng/ul# 88
80) Fluoranthene	19.24	202	23783342m	347.369	ng/ul
82) Pyrene	19.61	202	14230653	197.808	ng/ul 96
85) Benzo(a)anthracene	21.34	228	16771814	252.602	ng/ul# 69
86) Bis(2-ethylhexyl)phthalate	21.26	149	120283	3.531	ng/ul# 97
87) Chrysene	21.40	228	12869005	198.820	ng/ul# 81
90) Benzo(b)fluoranthene	22.96	252	16824199m	244.223	ng/ul
91) Benzo(k)fluoranthene	23.00	252	6737078m	101.762	ng/ul
93) Benzo(a)pyrene	23.53	252	3166019m	51.112	ng/ul
94) Indeno(1,2,3-cd)pyrene	25.94	276	3092562m	39.658	ng/ul
95) Dibenzo(a,h)anthracene	25.94	278	2202826m	34.076	ng/ul

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062221\
Data File : BM030535.D
Acq On : 23 Jun 2021 03:48
Operator : CG/JU
Sample : M2662-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDF4

Manual Integrations
APPROVED

mohammad
6/23/2021 4:48:54 PM

Quant Time: Jun 23 04:50:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 01:33:40 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
--------------------	------	------	----------	------	-------	-----------

-----	-----	-----	-----	-----	-----	-----
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed