

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030528.D
 Acq On : 22 Jun 2021 22:58
 Operator : CG/JU
 Sample : M2662-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDH5

Quant Time: Jun 23 01:32:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 22 15:07:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	156494	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	656076	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	425005	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	872493	20.000	ng/ul	0.00
79) Chrysene-d12	21.345	240	709391	20.000	ng/ul	0.00
88) Perylene-d12	23.609	264	644221	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	9627	2.494	ng/uL	0.00
4) Pyridine-d5	3.722	84	45821	4.418	ng/ul	0.02
7) Phenol-d5	6.975	99	174921	12.960	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	119704	14.111	ng/ul	0.00
11) 2-Chlorophenol-d4	7.346	132	147807	14.188	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	141216	13.445	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	68366	13.964	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	71430	13.129	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	138797	13.317	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	147110	10.122	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	454758	15.497	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	547336	14.369	ng/ul	0.00
54) 4-Nitrophenol-d4	14.645	143	38331	6.895	ng/ul	0.00
60) Fluorene-d10	15.427	176	405676	15.586	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	37337	6.541	ng/ul	0.00
73) Anthracene-d10	17.274	188	620783	15.245	ng/ul	0.00
81) Pyrene-d10	19.562	212	539087	14.503	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.462	264	297395	8.879	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.256	149	90215	3.995	ng/ul#	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030528.D
Acq On : 22 Jun 2021 22:58
Operator : CG/JU
Sample : M2662-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDH5


Quant Time: Jun 23 01:32:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 22 15:07:37 2021
Response via : Initial Calibration

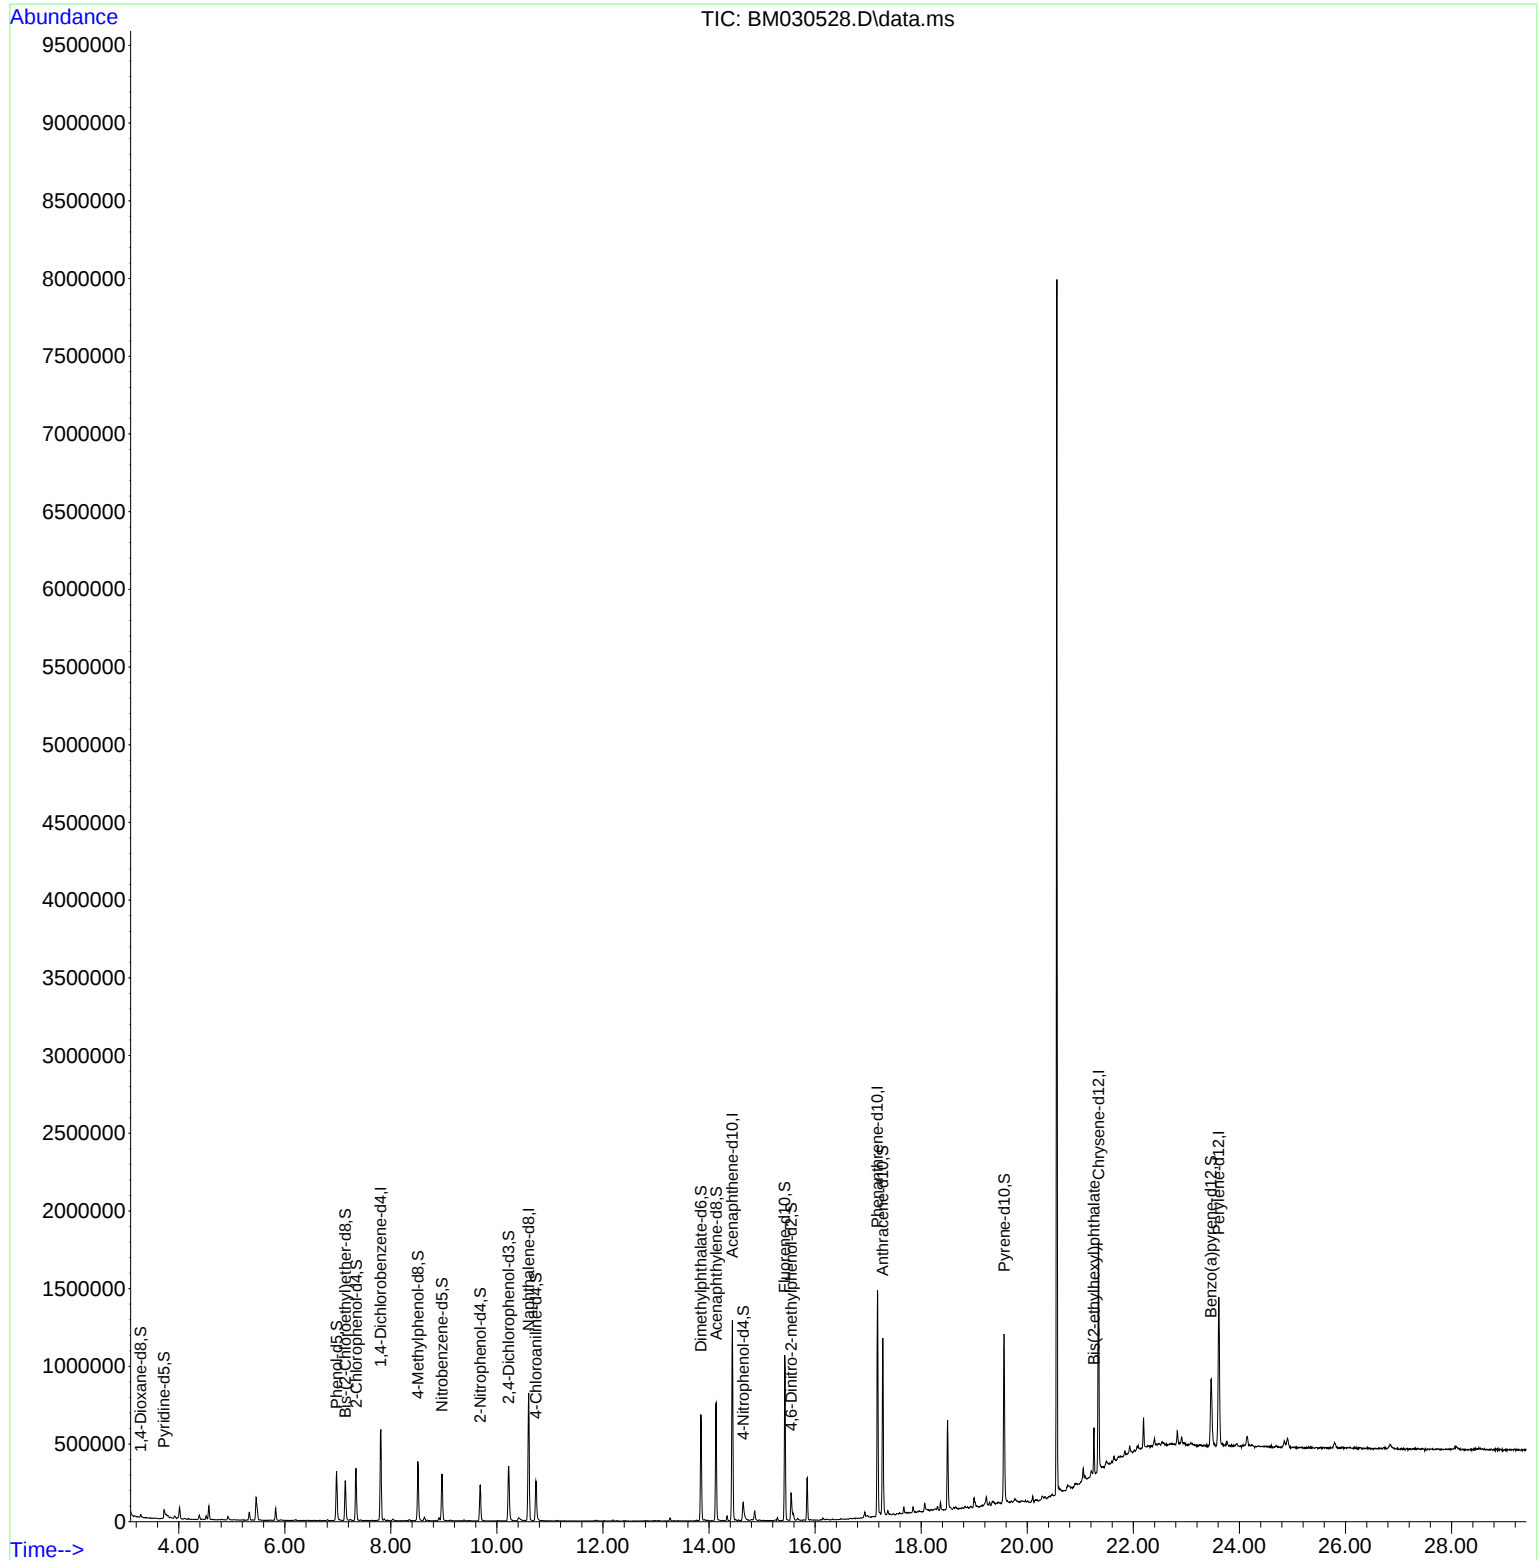

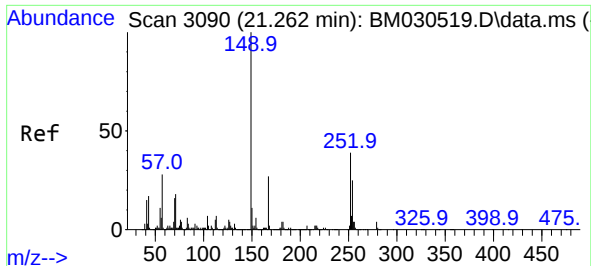

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.995 ng/ul
 RT: 21.256 min Scan# 3089
 Delta R.T. -0.006 min
 Lab File: BM030528.D
 Acq: 22 Jun 2021 22:58

Instrument :
 BNA_M
 ClientSampleId :
 BGDH5

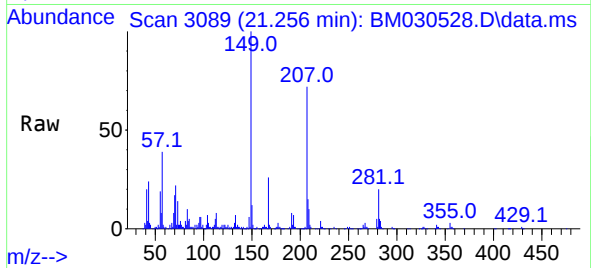

Tgt Ion:149 Resp: 90215
 Ion Ratio Lower Upper
 149 100
 167 26.4 20.7 31.1
 279 4.6 3.0 4.4#

