

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030529.D
 Acq On : 22 Jun 2021 23:35
 Operator : CG/JU
 Sample : M2662-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDB4

Quant Time: Jun 23 01:32:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 22 15:07:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	151279	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	620542	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	385700	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	734579	20.000	ng/ul	0.00
79) Chrysene-d12	21.344	240	626823	20.000	ng/ul	0.00
88) Perylene-d12	23.609	264	660163	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	12940	3.468	ng/uL	0.00
4) Pyridine-d5	3.716	84	68914	6.874	ng/ul	0.02
7) Phenol-d5	6.975	99	206242	15.808	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.139	67	140807	17.170	ng/ul	0.00
11) 2-Chlorophenol-d4	7.339	132	172906	17.169	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	141069	13.894	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	80134	17.305	ng/ul	0.00
24) 2-Nitrophenol-d4	9.680	143	85410	16.597	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	154329	15.655	ng/ul	0.00
31) 4-Chloroaniline-d4	10.733	131	176951	12.872	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	498329	18.712	ng/ul	0.00
49) Acenaphthylene-d8	14.133	160	624172	18.056	ng/ul	0.00
54) 4-Nitrophenol-d4	14.645	143	34528	6.844	ng/ul	0.00
60) Fluorene-d10	15.427	176	443040	18.756	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	36039	7.499	ng/ul	0.00
73) Anthracene-d10	17.274	188	656804	19.158	ng/ul	0.00
81) Pyrene-d10	19.562	212	725069	22.076	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.468	264	696504	20.293	ng/ul	-0.01
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.957	77	7787	1.228	ng/ul	93
86) Bis(2-ethylhexyl)phtha...	21.256	149	89429	4.481	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030529.D
Acq On : 22 Jun 2021 23:35
Operator : CG/JU
Sample : M2662-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDB4

Quant Time: Jun 23 01:32:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 22 15:07:37 2021
Response via : Initial Calibration

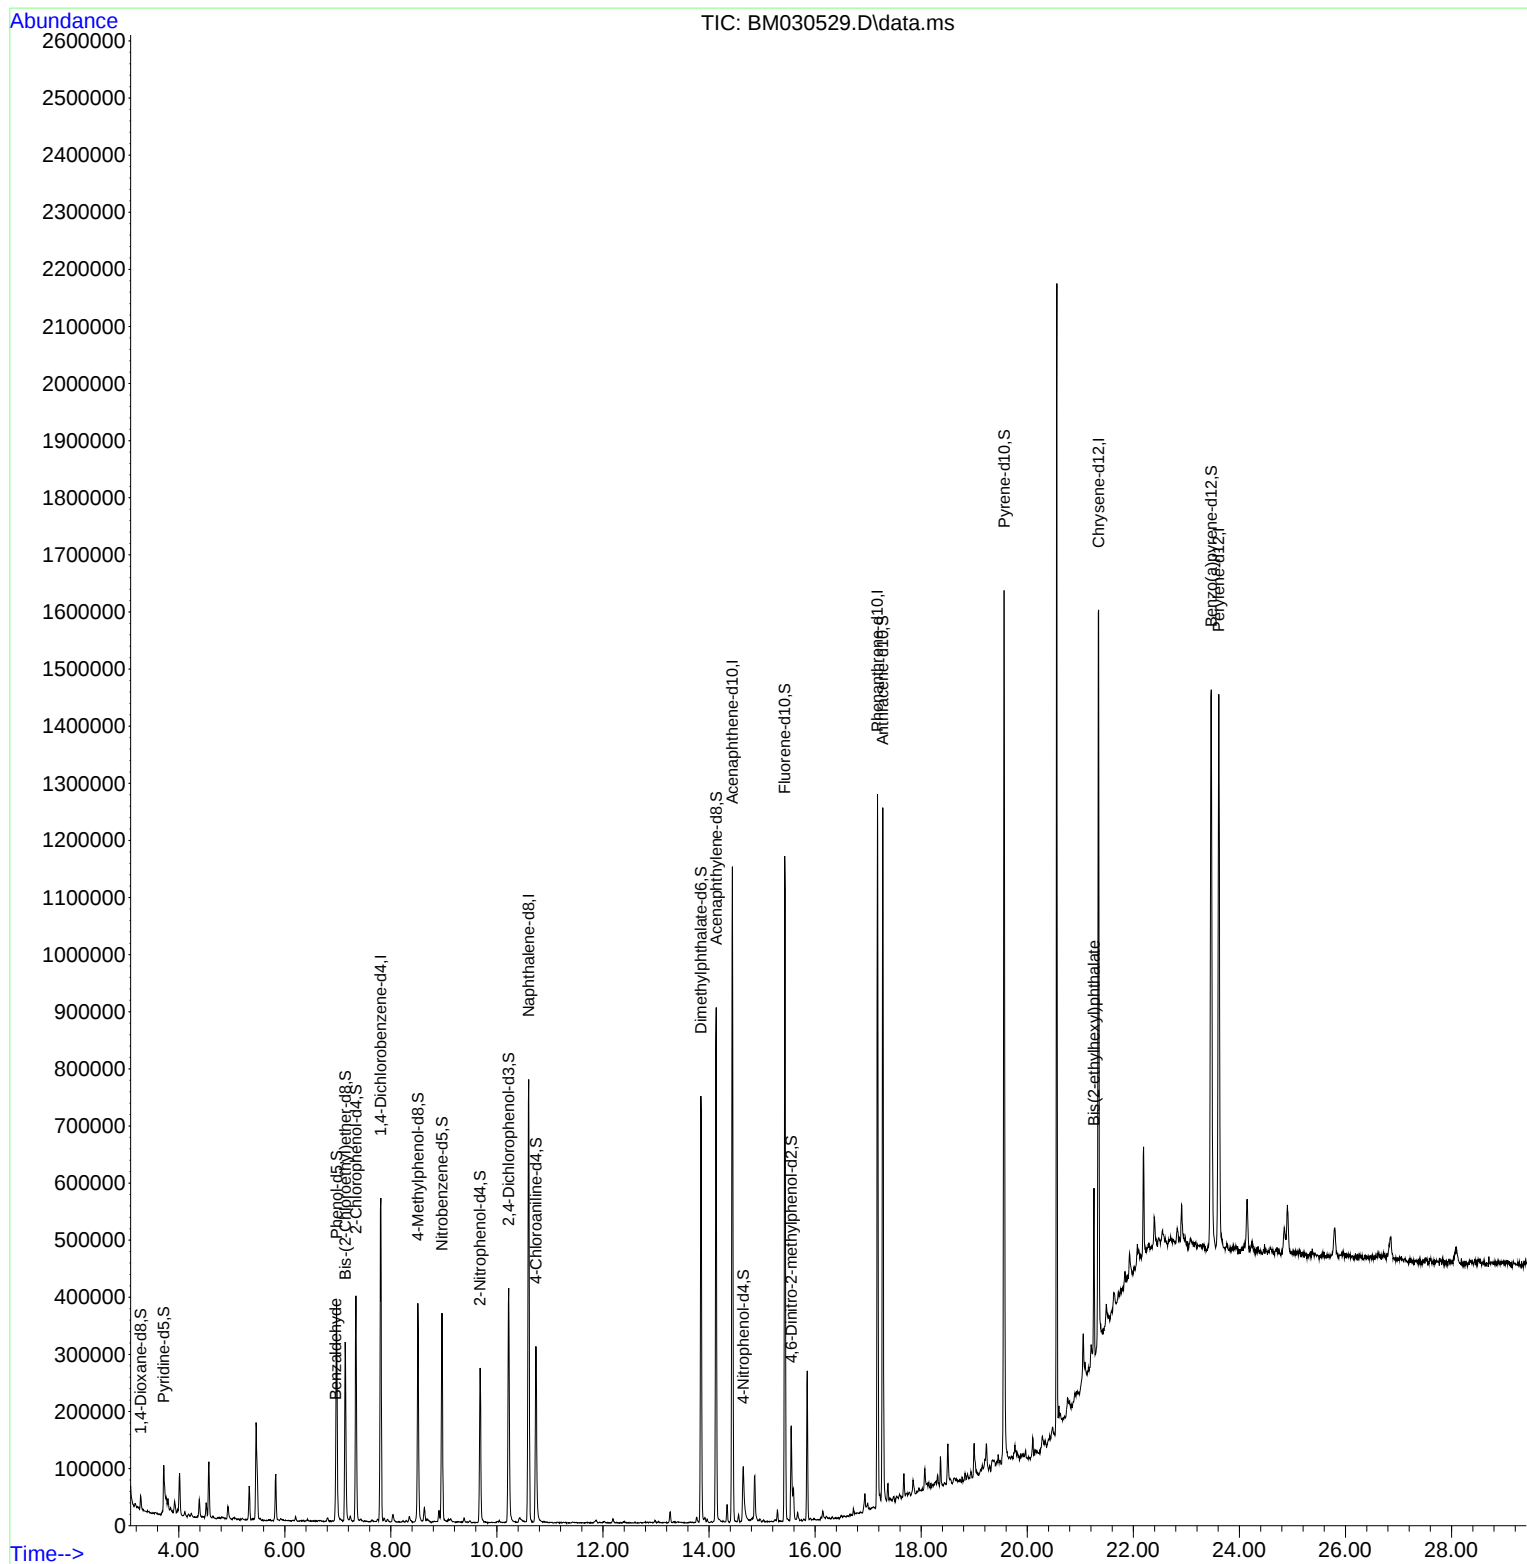




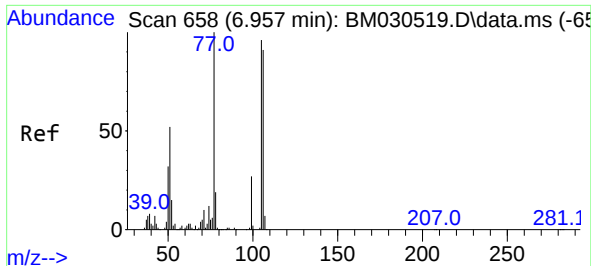


#6
Benzaldehyde
Concen: 1.228 ng/ul
RT: 6.957 min Scan# 658
Delta R.T. -0.000 min
Lab File: BM030529.D
Acq: 22 Jun 2021 23:35

Instrument :
BNA_M
ClientSampleId :
BGDB4

Tgt Ion: 77 Resp: 7787

Ion	Ratio	Lower	Upper
77	100		
105	99.7	82.2	123.4
106	83.5	75.0	112.4

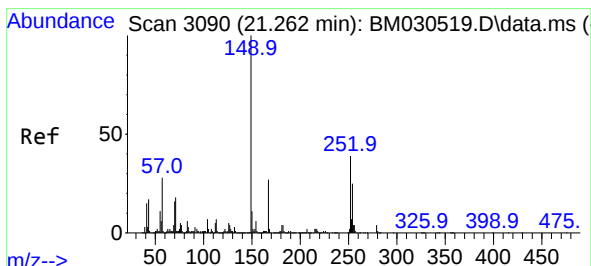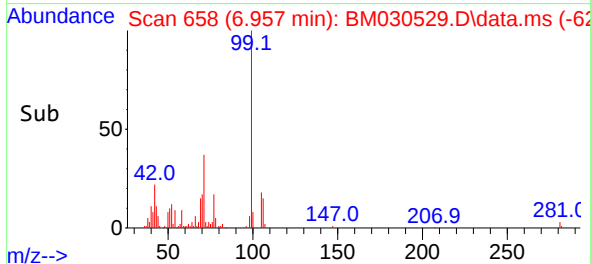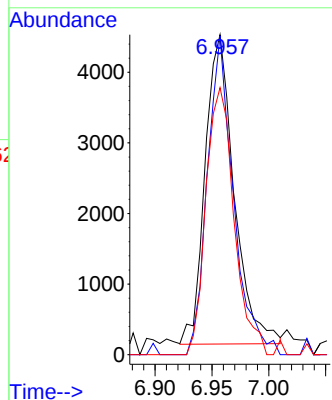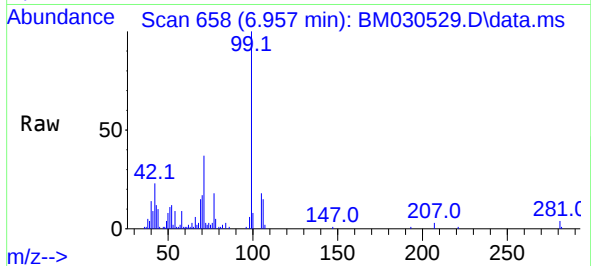

#86
Bis(2-ethylhexyl)phthalate
Concen: 4.481 ng/ul
RT: 21.256 min Scan# 3089
Delta R.T. -0.006 min
Lab File: BM030529.D
Acq: 22 Jun 2021 23:35

Tgt Ion: 149 Resp: 89429

Ion	Ratio	Lower	Upper
149	100		
167	25.6	20.7	31.1
279	4.5	3.0	4.4

