

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030532.D
 Acq On : 23 Jun 2021 01:24
 Operator : CG/JU
 Sample : M2662-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDE7

Quant Time: Jun 23 02:39:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	163575	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	697068	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	459075	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	902846	20.000	ng/ul	0.00
79) Chrysene-d12	21.339	240	711158	20.000	ng/ul	-0.01
88) Perylene-d12	23.609	264	689381	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	9602	2.380	ng/uL	0.00
4) Pyridine-d5	3.717	84	55074	5.080	ng/ul	0.02
7) Phenol-d5	6.975	99	188191	13.340	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	123745	13.955	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	151112	13.877	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	154251	14.050	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	70328	13.520	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	76660	13.262	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	150037	13.549	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	181409	11.747	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	518243	16.349	ng/ul	0.00
49) Acenaphthylene-d8	14.128	160	601277	14.613	ng/ul	0.00
54) 4-Nitrophenol-d4	14.639	143	39839	6.634	ng/ul	0.00
60) Fluorene-d10	15.428	176	451764	16.069	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	48211	8.162	ng/ul	0.00
73) Anthracene-d10	17.274	188	703552	16.697	ng/ul	0.00
81) Pyrene-d10	19.563	212	584270	15.679	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.462	264	349090	9.740	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.257	149	73863	3.262	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030532.D
Acq On : 23 Jun 2021 01:24
Operator : CG/JU
Sample : M2662-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDE7

Quant Time: Jun 23 02:39:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 01:33:40 2021
Response via : Initial Calibration

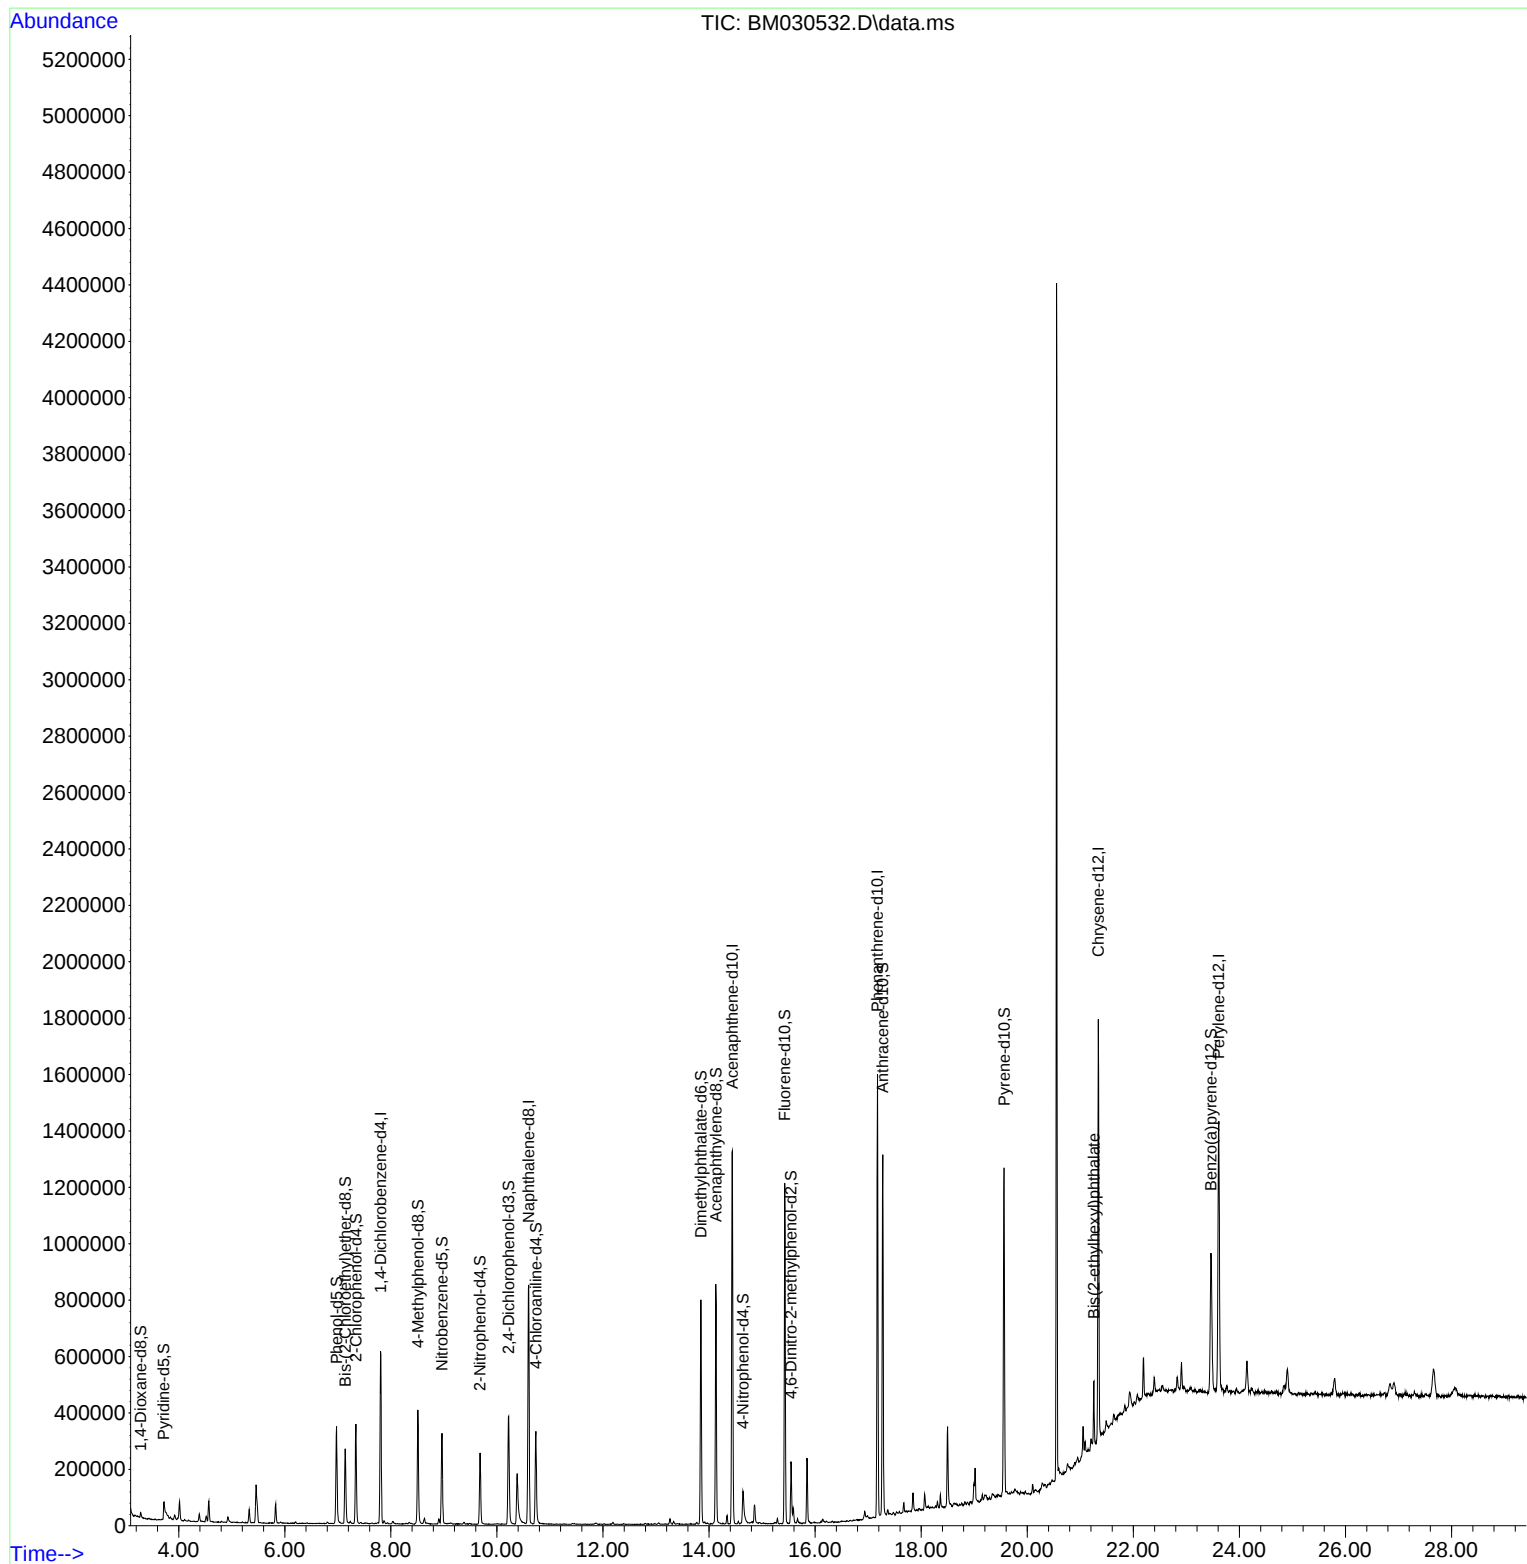

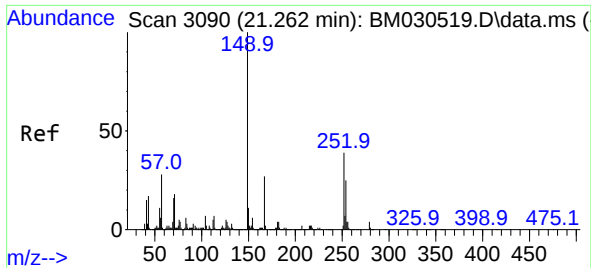

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.262 ng/ul
 RT: 21.257 min Scan# 3089
 Delta R.T. -0.006 min
 Lab File: BM030532.D
 Acq: 23 Jun 2021 01:24

Instrument :
 BNA_M
 ClientSampleId :
 BGDE7

Tgt Ion:	149	Resp:	73863
Ion	Ratio	Lower	Upper
149	100		
167	26.2	20.7	31.1
279	4.3	3.0	4.4

