

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030533.D
 Acq On : 23 Jun 2021 02:00
 Operator : CG/JU
 Sample : M2662-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD92

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:48 PM

Quant Time: Jun 23 02:39:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 01:33:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	154708	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	653575	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	428043	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.174	188	853995	20.000	ng/ul	0.00
79) Chrysene-d12	21.339	240	663920	20.000	ng/ul	-0.01
88) Perylene-d12	23.609	264	643398	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	8696	2.279	ng/uL	0.00
4) Pyridine-d5	3.722	84	47082	4.592	ng/ul	0.02
7) Phenol-d5	6.975	99	147027	11.019	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	101427	12.094	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	124397	12.078	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	121170	11.669	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	57700	11.831	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	59770	11.028	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	113944	10.974	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	108169	7.471	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	388479	13.144	ng/ul	0.00
49) Acenaphthylene-d8	14.128	160	468744	12.218	ng/ul	0.00
54) 4-Nitrophenol-d4	14.645	143	28800m	5.144	ng/ul	0.00
60) Fluorene-d10	15.428	176	347983	13.275	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	29042	5.198	ng/ul	0.00
73) Anthracene-d10	17.275	188	527698	13.240	ng/ul	0.00
81) Pyrene-d10	19.563	212	424303	12.197	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.462	264	220431	6.590	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.257	149	80981	3.831	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030533.D
Acq On : 23 Jun 2021 02:00
Operator : CG/JU
Sample : M2662-20
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BGD92

Manual Integrations
APPROVED

mohammad
6/23/2021 4:48:48 PM


Quant Time: Jun 23 02:39:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 01:33:40 2021
Response via : Initial Calibration

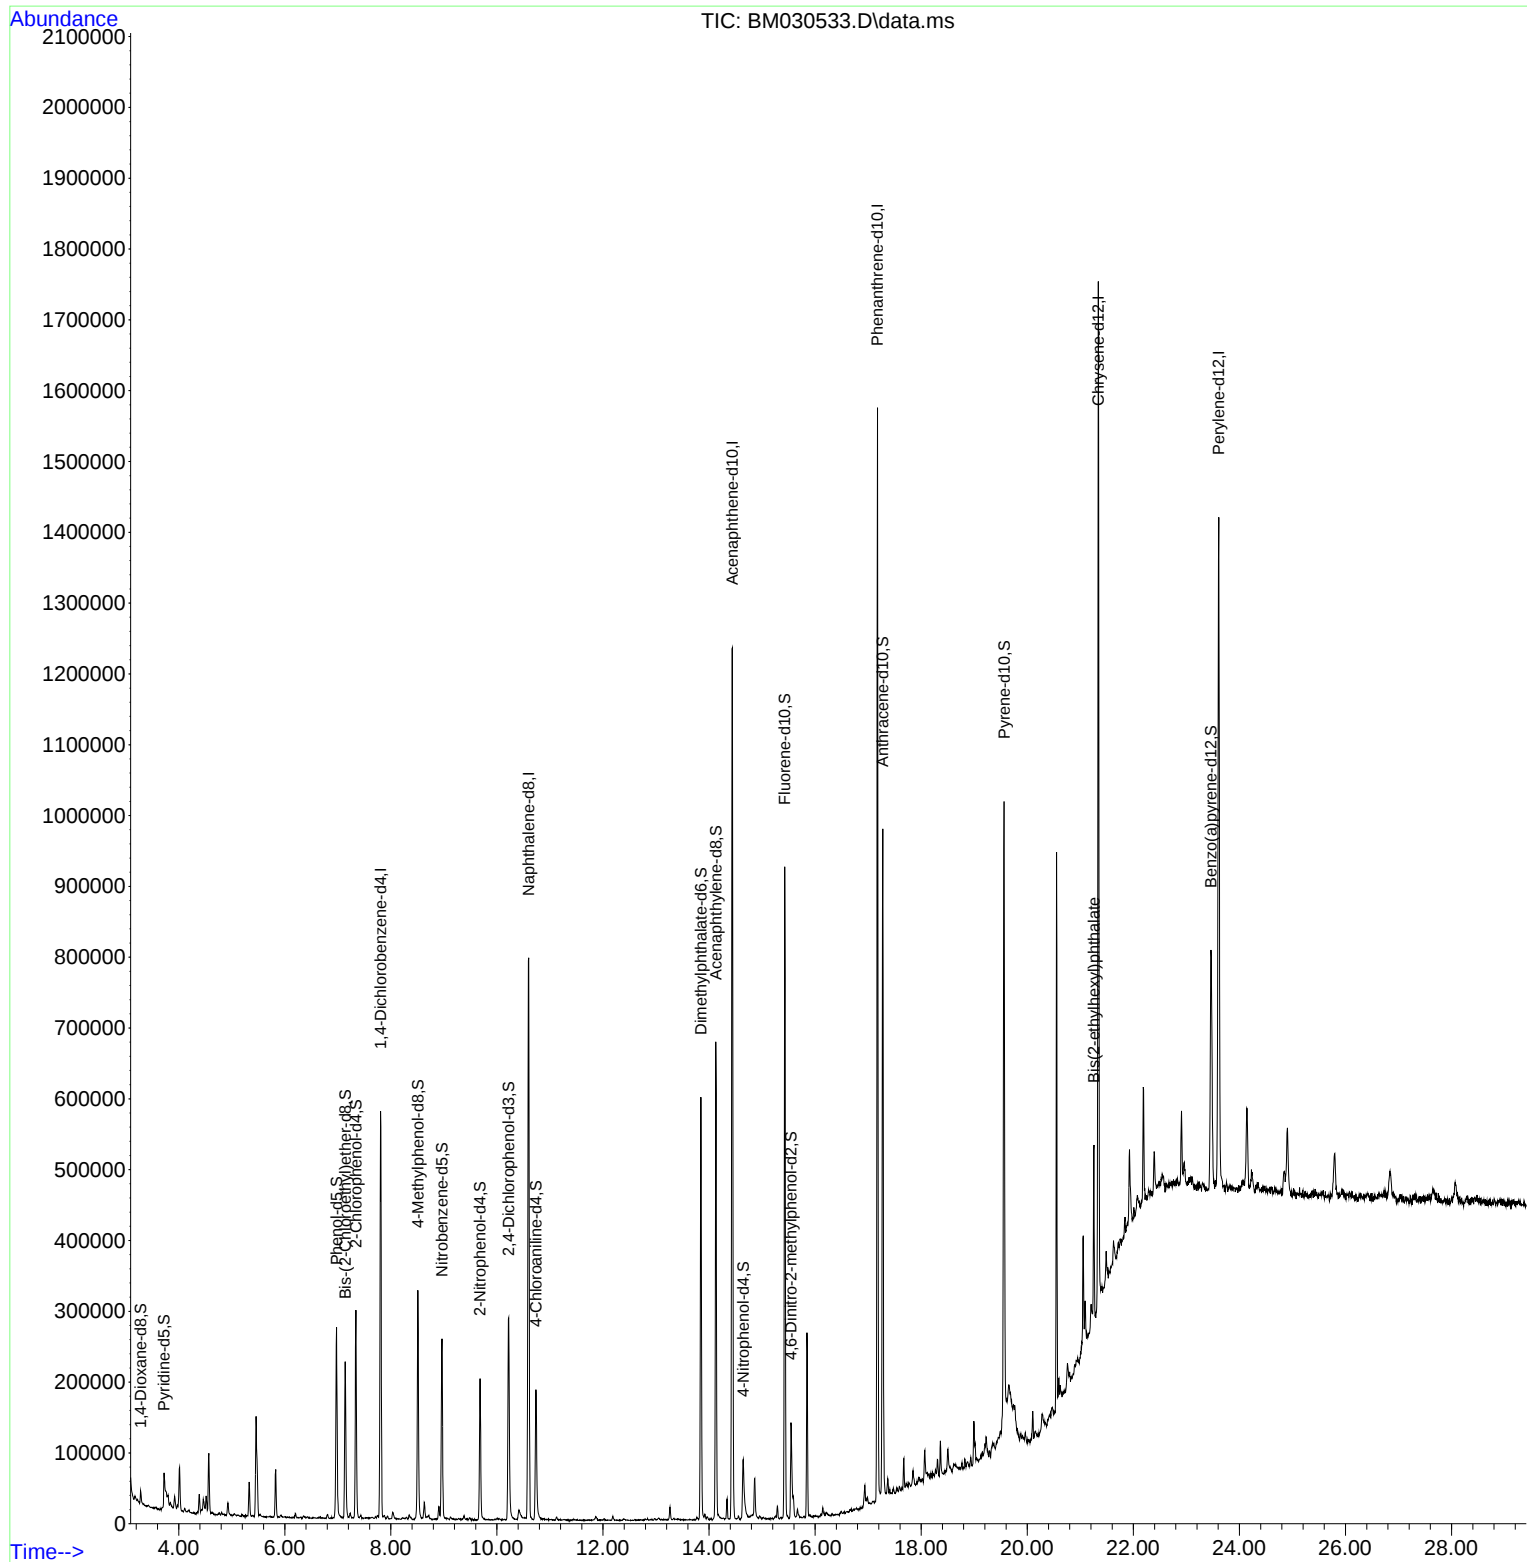

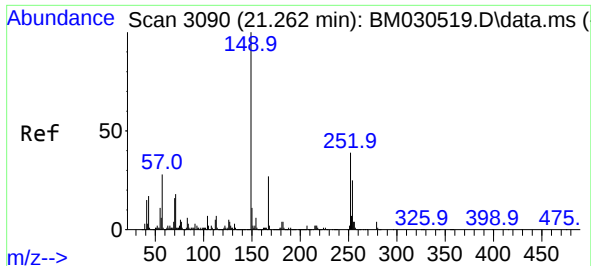

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.831 ng/ul
 RT: 21.257 min Scan# 3089
 Delta R.T. -0.006 min
 Lab File: BM030533.D
 Acq: 23 Jun 2021 02:00

Instrument :
 BNA_M
 ClientSampleId :
 BGD92

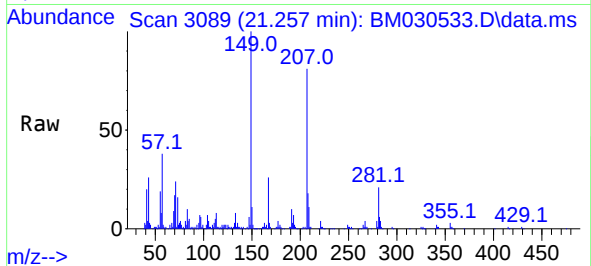

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.3	20.7	31.1
279	4.3	3.0	4.4

Manual Integrations
 APPROVED

mohammad
 6/23/2021 4:48:48 PM

