

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030540.D
 Acq On : 23 Jun 2021 06:48
 Operator : CG/JU
 Sample : M2662-21
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGD93

Quant Time: Jun 23 07:30:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 23 04:56:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	167992	20.000	ng/ul	0.00
20) Naphthalene-d8	10.592	136	663161	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.433	164	380286	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.174	188	694192	20.000	ng/ul	0.00
79) Chrysene-d12	21.345	240	673277	20.000	ng/ul	0.00
88) Perylene-d12	23.609	264	760869	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	12829	3.096	ng/uL	0.00
4) Pyridine-d5	3.710	84	88782	7.974	ng/ul	0.01
7) Phenol-d5	6.975	99	268728	18.548	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	172542	18.947	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	224801	20.101	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	220827	19.585	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	105433	21.306	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	115017	20.914	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	215780	20.482	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	211303	14.383	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	608758	23.184	ng/ul	0.00
49) Acenaphthylene-d8	14.127	160	772553	22.666	ng/ul	0.00
54) 4-Nitrophenol-d4	14.639	143	55170	11.090	ng/ul	0.00
60) Fluorene-d10	15.427	176	527715	22.659	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	37830	8.329	ng/ul	0.00
73) Anthracene-d10	17.274	188	761921	23.518	ng/ul	0.00
81) Pyrene-d10	19.562	212	870270	24.668	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.468	264	998919	25.252	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.256	149	102764	4.794	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030540.D
Acq On : 23 Jun 2021 06:48
Operator : CG/JU
Sample : M2662-21
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGD93

Quant Time: Jun 23 07:30:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 23 04:56:16 2021
Response via : Initial Calibration

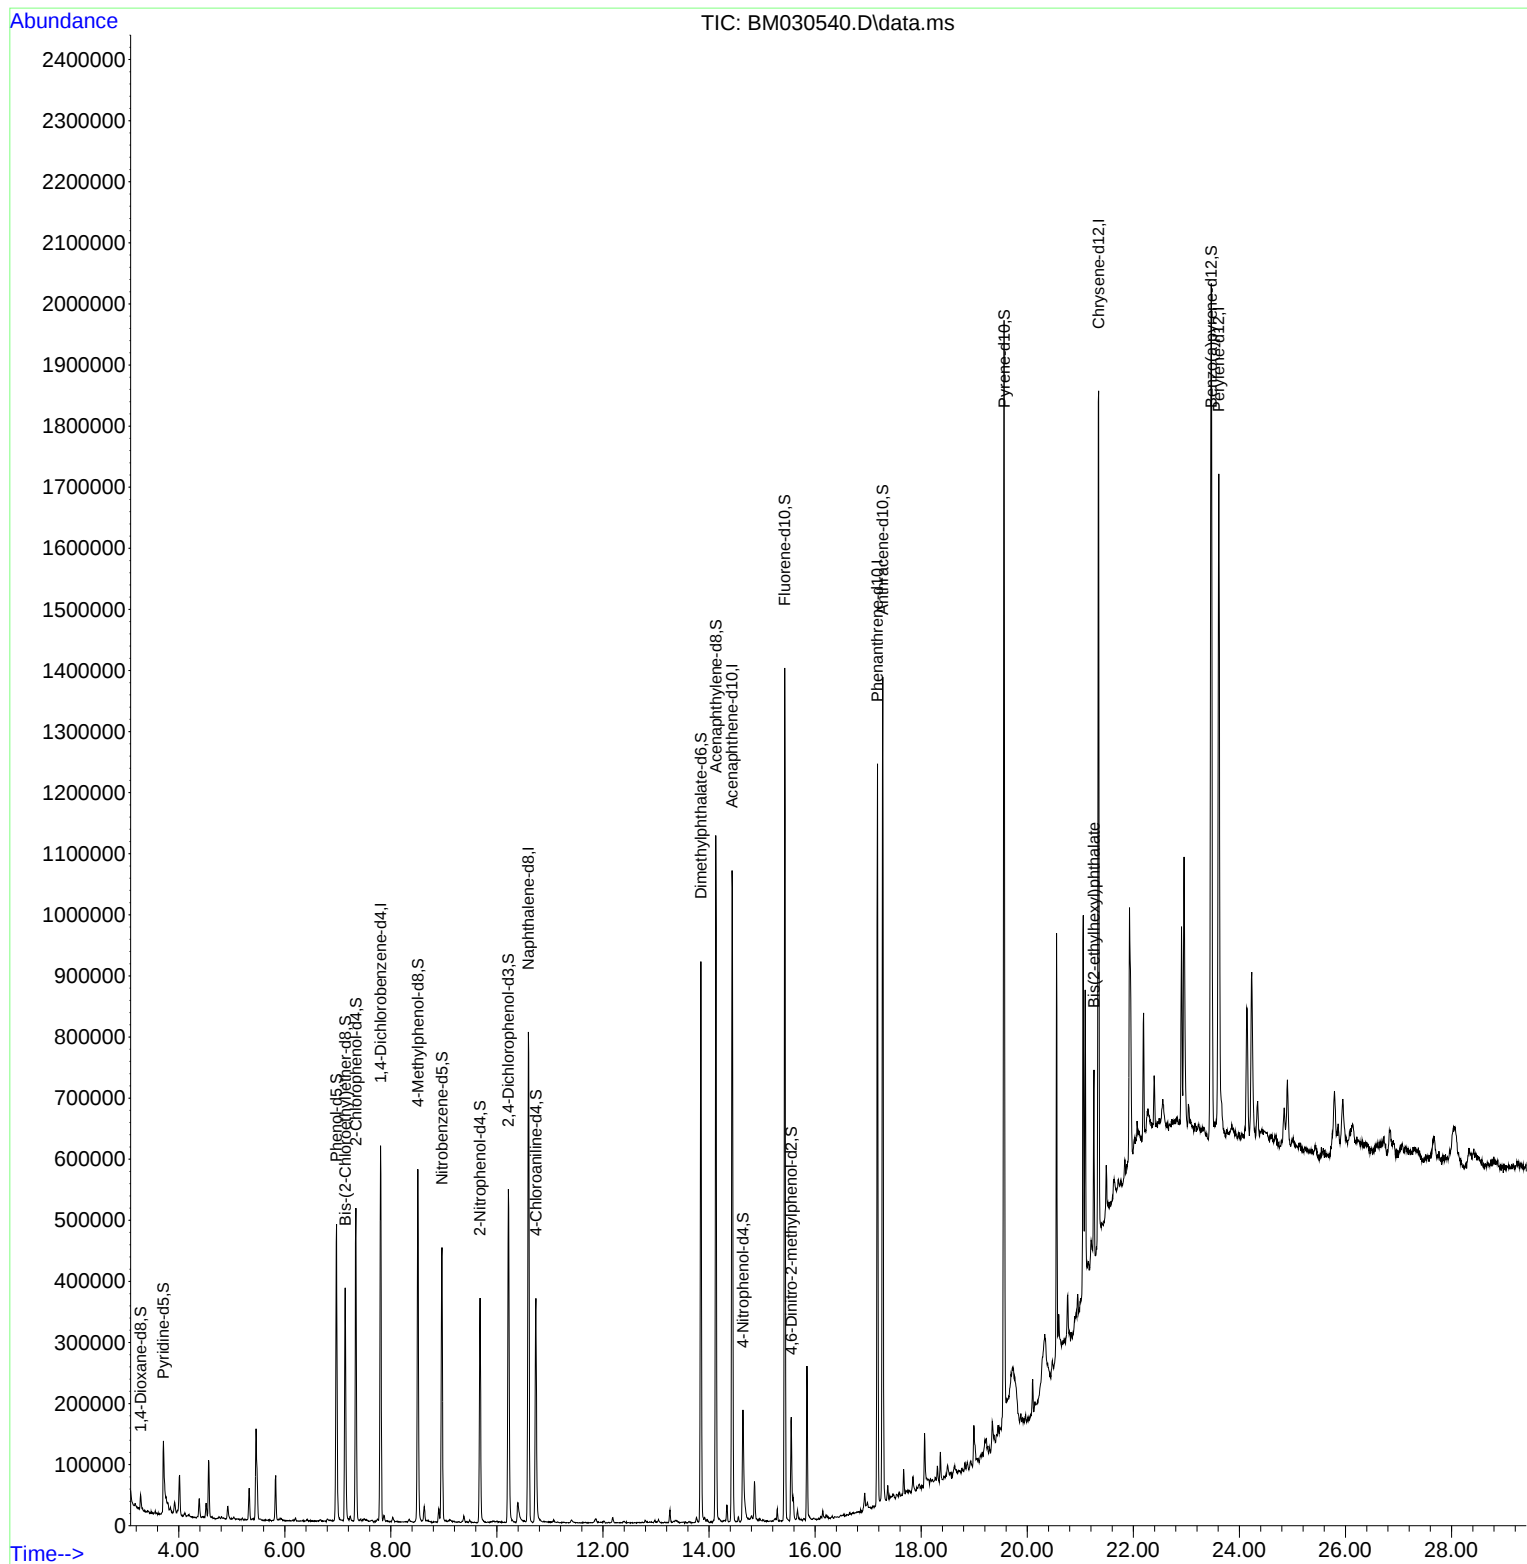

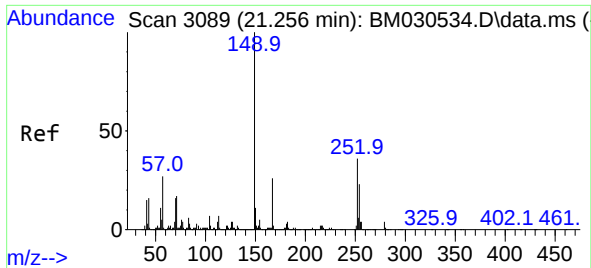

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.794 ng/ul
 RT: 21.256 min Scan# 3089
 Delta R.T. -0.006 min
 Lab File: BM030540.D
 Acq: 23 Jun 2021 06:48

Instrument :
 BNA_M
 ClientSampleId :
 BGD93

Tgt Ion:149 Resp: 102764
 Ion Ratio Lower Upper
 149 100
 167 25.4 20.7 31.1
 279 5.0 3.0 4.4#

