

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030517.D
 Acq On : 22 Jun 2021 16:12
 Operator : CG/JU
 Sample : M2780-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030517.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.016	155	158	164	rVB2	9501	12248	0.68%	0.137%
2	4.898	304	308	309	rBV4	2199	2464	0.14%	0.028%
3	5.122	345	346	350	rBV3	2522	2744	0.15%	0.031%
4	5.351	384	385	388	rBV3	2125	2362	0.13%	0.026%
5	5.692	440	443	446	rBV3	1769	1859	0.10%	0.021%
6	5.945	482	486	488	rBV4	1513	2243	0.12%	0.025%
7	6.334	549	552	555	rBV3	1810	2949	0.16%	0.033%
8	6.469	573	575	577	rBV2	1513	1844	0.10%	0.021%
9	6.969	654	660	661	rBV5	2340	3938	0.22%	0.044%
10	7.298	713	716	720	rVB5	1467	2322	0.13%	0.026%
11	7.463	740	744	746	rBV5	1307	1860	0.10%	0.021%
12	7.810	794	803	811	rBV	524647	842355	46.72%	9.439%
13	8.828	974	976	982	rVB5	1803	3138	0.17%	0.035%
14	9.333	1059	1062	1065	rBV4	1470	2298	0.13%	0.026%
15	9.404	1068	1074	1076	rBV5	2835	4919	0.27%	0.055%
16	10.251	1215	1218	1223	rVB5	1215	2287	0.13%	0.026%
17	10.475	1251	1256	1259	rBV5	1236	2425	0.13%	0.027%
18	10.598	1268	1277	1289	rBV	643142	1129272	62.63%	12.654%
19	11.792	1477	1480	1483	rBV5	1823	2789	0.15%	0.031%
20	11.886	1487	1496	1506	rBV	34791	104823	5.81%	1.175%
21	12.245	1555	1557	1562	rBV4	1931	3295	0.18%	0.037%
22	12.569	1607	1612	1615	rBV6	1685	2493	0.14%	0.028%
23	13.874	1827	1834	1845	rBV	51128	118660	6.58%	1.330%
24	14.439	1923	1930	1945	rBV	947023	1479232	82.04%	16.575%
25	14.621	1958	1961	1964	rVV4	2174	2589	0.14%	0.029%
26	15.298	2074	2076	2080	rBV4	1718	2812	0.16%	0.032%
27	15.427	2093	2098	2103	rBV4	11854	21535	1.19%	0.241%
28	15.557	2116	2120	2123	rVB4	1987	3280	0.18%	0.037%
29	16.086	2206	2210	2212	rBV4	1243	1871	0.10%	0.021%
30	16.592	2294	2296	2300	rVB4	1393	1844	0.10%	0.021%
31	16.668	2303	2309	2317	rBV9	4961	11421	0.63%	0.128%
32	16.733	2317	2320	2323	rBV5	1669	2058	0.11%	0.023%
33	16.980	2357	2362	2365	rVB3	3507	5742	0.32%	0.064%
34	17.074	2374	2378	2379	rVB3	2095	2284	0.13%	0.026%
35	17.180	2387	2396	2410	rBV	1087610	1620048	89.85%	18.153%
36	17.280	2411	2413	2417	rVB4	3197	4260	0.24%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030517.D
 Acq On : 22 Jun 2021 16:12
 Operator : CG/JU
 Sample : M2780-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	17.862	2510	2512	2514	rBV2	2337	1822	0.10%	0.020%
38	18.380	2598	2600	2602	rBV3	3402	2033	0.11%	0.023%
39	18.621	2639	2641	2644	rBV4	3104	3168	0.18%	0.035%
40	18.674	2647	2650	2651	rBV2	2921	3136	0.17%	0.035%
41	18.733	2658	2660	2663	rVB4	2609	2505	0.14%	0.028%
42	18.998	2703	2705	2707	rBV3	4113	3373	0.19%	0.038%
43	21.350	3100	3105	3113	rBV	1264503	1690621	93.77%	18.944%
44	23.621	3485	3491	3501	rVB2	937575	1803026	100.00%	20.204%




Sum of corrected areas: 8924247

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030517.D
Acq On : 22 Jun 2021 16:12
Operator : CG/JU
Sample : M2780-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

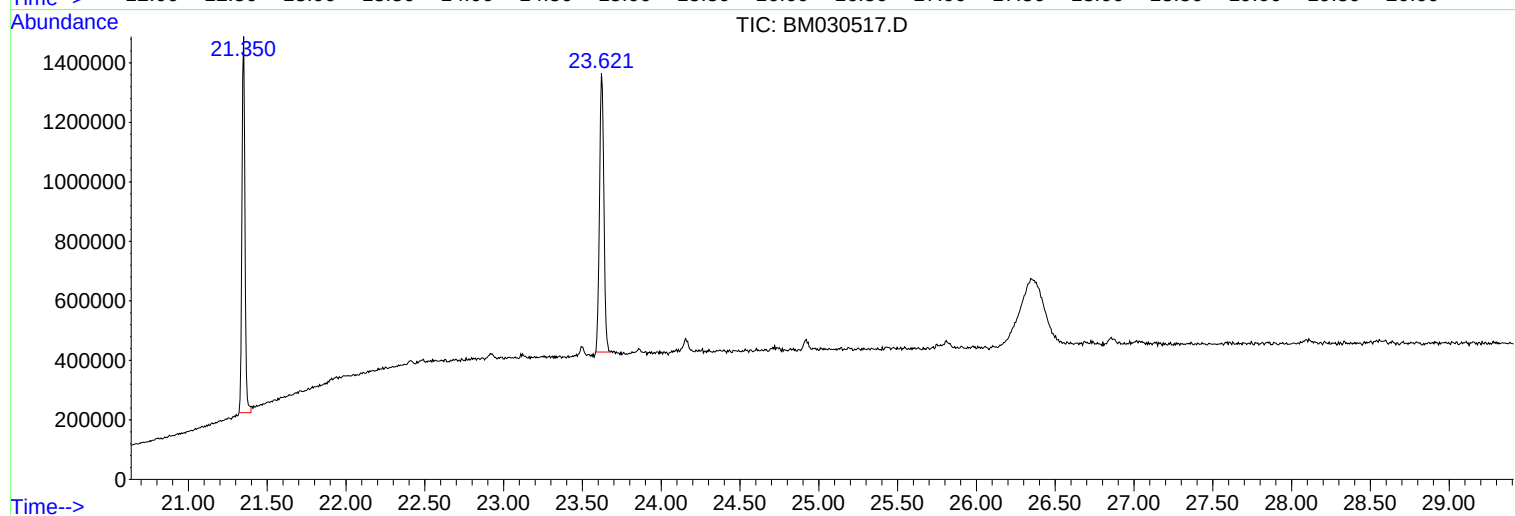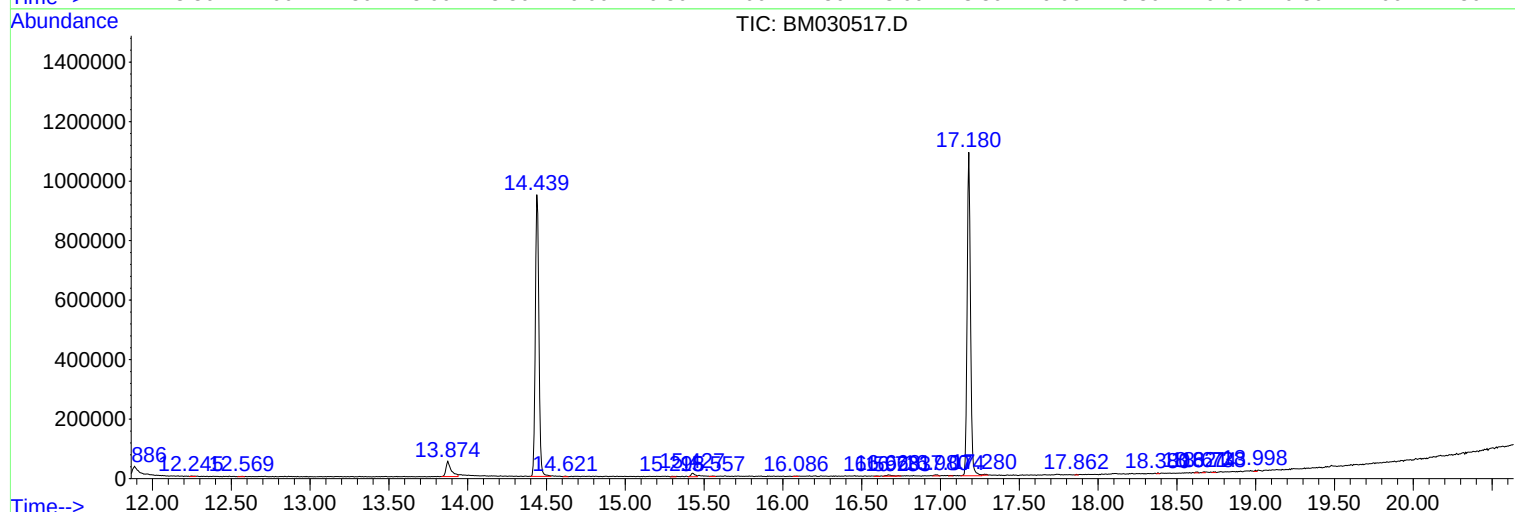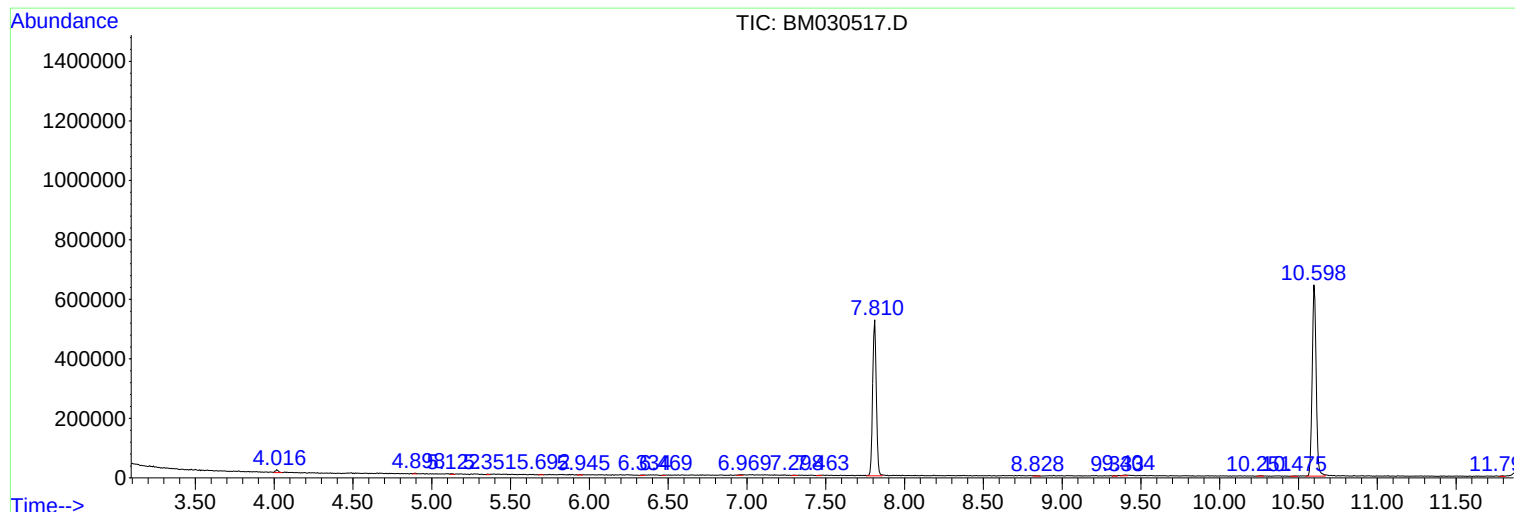

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030517.D
Acq On : 22 Jun 2021 16:12
Operator : CG/JU
Sample : M2780-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030517.D
Acq On : 22 Jun 2021 16:12
Operator : CG/JU
Sample : M2780-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
