

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030520.D
 Acq On : 22 Jun 2021 18:05
 Operator : CG/JU
 Sample : PB137201BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030520.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	44	rVB	52341	79540	1.85%	0.174%
2	3.698	101	104	128	rBV	526290	978761	22.81%	2.145%
3	4.016	155	158	164	rVB2	11208	14564	0.34%	0.032%
4	6.975	654	661	672	rBV	761726	1260888	29.39%	2.763%
5	7.145	683	690	701	rBV	612891	1012620	23.60%	2.219%
6	7.345	717	724	735	rBV	812022	1316329	30.68%	2.885%
7	7.810	796	803	811	rBV	603661	949109	22.12%	2.080%
8	8.516	915	923	934	rBV	925576	1554684	36.24%	3.407%
9	8.963	991	999	1010	rBV	737637	1258625	29.34%	2.759%
10	9.686	1114	1122	1135	rBV	616475	1032610	24.07%	2.263%
11	10.222	1204	1213	1229	rBV	924707	1592216	37.11%	3.490%
12	10.598	1270	1277	1288	rVB	821046	1400045	32.63%	3.068%
13	10.739	1293	1301	1317	rBV	877968	1653623	38.54%	3.624%
14	11.857	1472	1491	1506	rBV3	63451	231066	5.39%	0.506%
15	12.192	1543	1548	1554	rBV2	15291	28129	0.66%	0.062%
16	13.410	1749	1755	1761	rVB8	2448	5712	0.13%	0.013%
17	13.851	1821	1830	1847	rBV	1745013	2616283	60.98%	5.734%
18	14.133	1871	1878	1893	rBV	2005407	2905146	67.71%	6.367%
19	14.439	1923	1930	1940	rBV	1272549	1915611	44.65%	4.198%
20	14.639	1957	1964	1980	rBV	651226	1100086	25.64%	2.411%
21	15.433	2089	2099	2109	rBV	2604650	3671625	85.58%	8.047%
22	15.551	2113	2119	2135	rVV	683082	1016747	23.70%	2.228%
23	15.674	2135	2140	2146	rVB	31212	50087	1.17%	0.110%
24	16.109	2210	2214	2218	rBV5	2739	4653	0.11%	0.010%
25	16.215	2228	2232	2236	rBV5	8341	10961	0.26%	0.024%
26	16.674	2304	2310	2314	rBV5	5825	9282	0.22%	0.020%
27	16.968	2357	2360	2364	rVB2	5208	6601	0.15%	0.014%
28	17.180	2389	2396	2405	rBV	1552461	2193728	51.13%	4.808%
29	17.280	2406	2413	2424	rBV	2696793	3854644	89.84%	8.448%
30	17.733	2486	2490	2494	rBV6	4333	6017	0.14%	0.013%
31	18.680	2648	2651	2658	rBV6	3473	7256	0.17%	0.016%
32	19.127	2726	2727	2731	rBV4	4413	4918	0.11%	0.011%
33	19.203	2736	2740	2746	rVV	26243	39845	0.93%	0.087%
34	19.456	2779	2783	2786	rBV	24617	34588	0.81%	0.076%
35	19.568	2796	2802	2809	rBV	3107222	4290507	100.00%	9.403%
36	21.350	3100	3105	3112	rBV	1556585	2076469	48.40%	4.551%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030520.D
Acq On : 22 Jun 2021 18:05
Operator : CG/JU
Sample : PB137201BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK201

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Title : SVOA CALIBRATION

37	23.480	3460	3467	3479	rVB	1796630	3520579	82.06%	7.716%
38	23.621	3485	3491	3502	rVB2	980762	1922731	44.81%	4.214%




Sum of corrected areas: 45626885

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030520.D
Acq On : 22 Jun 2021 18:05
Operator : CG/JU
Sample : PB137201BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK201

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

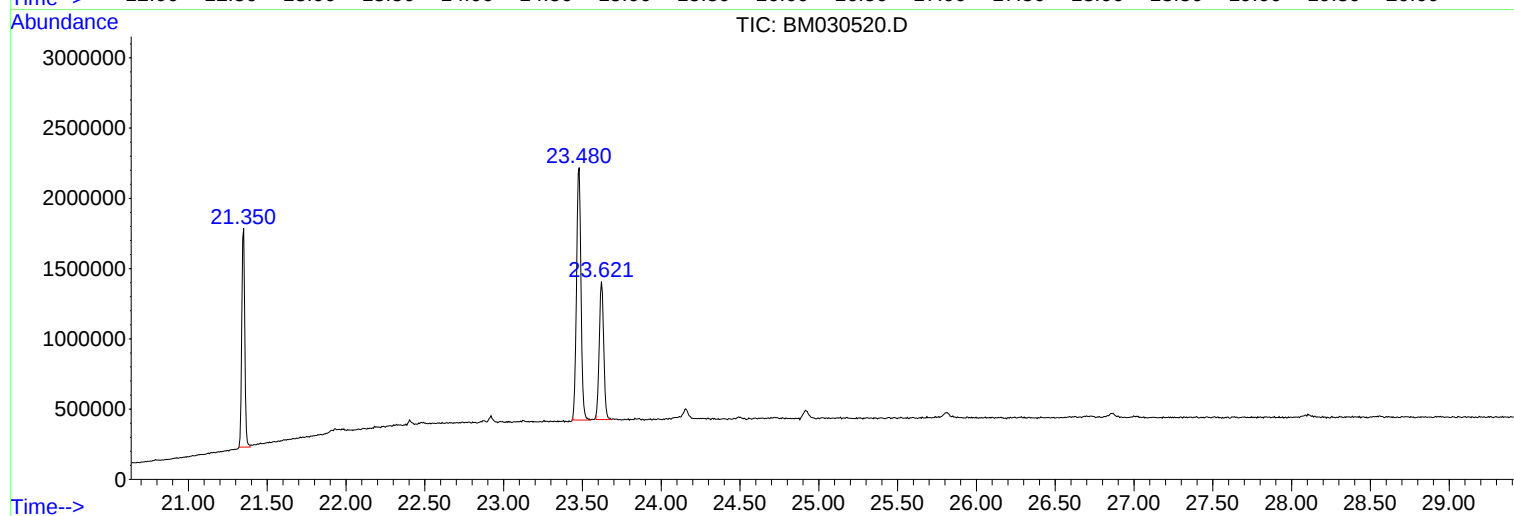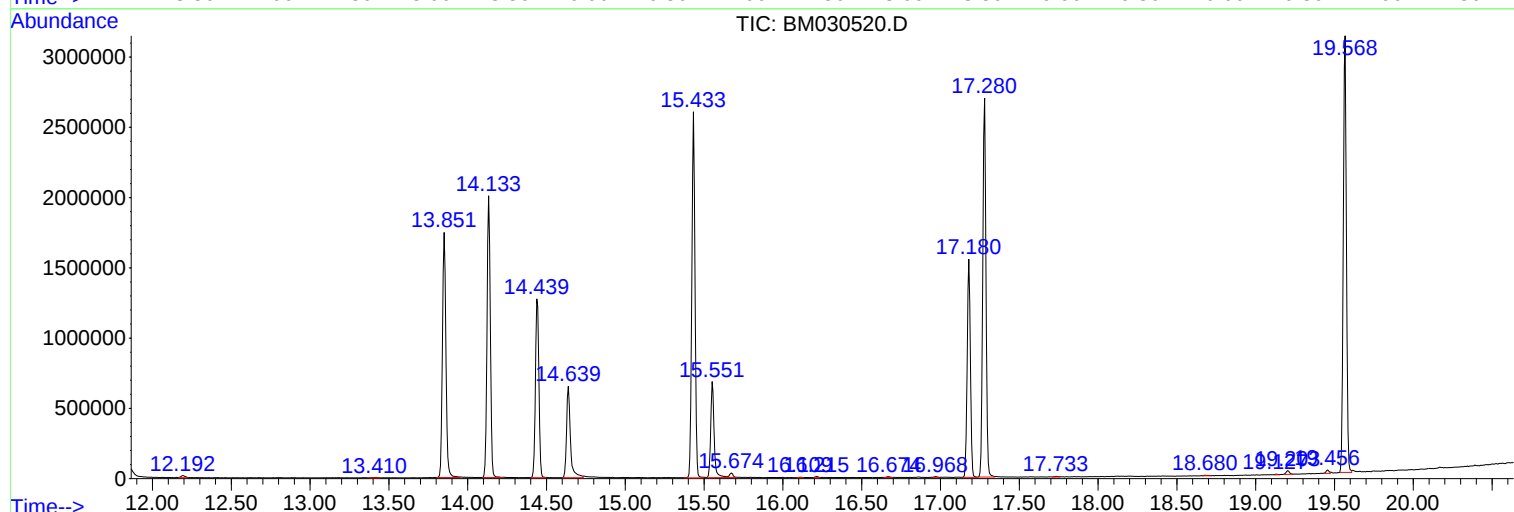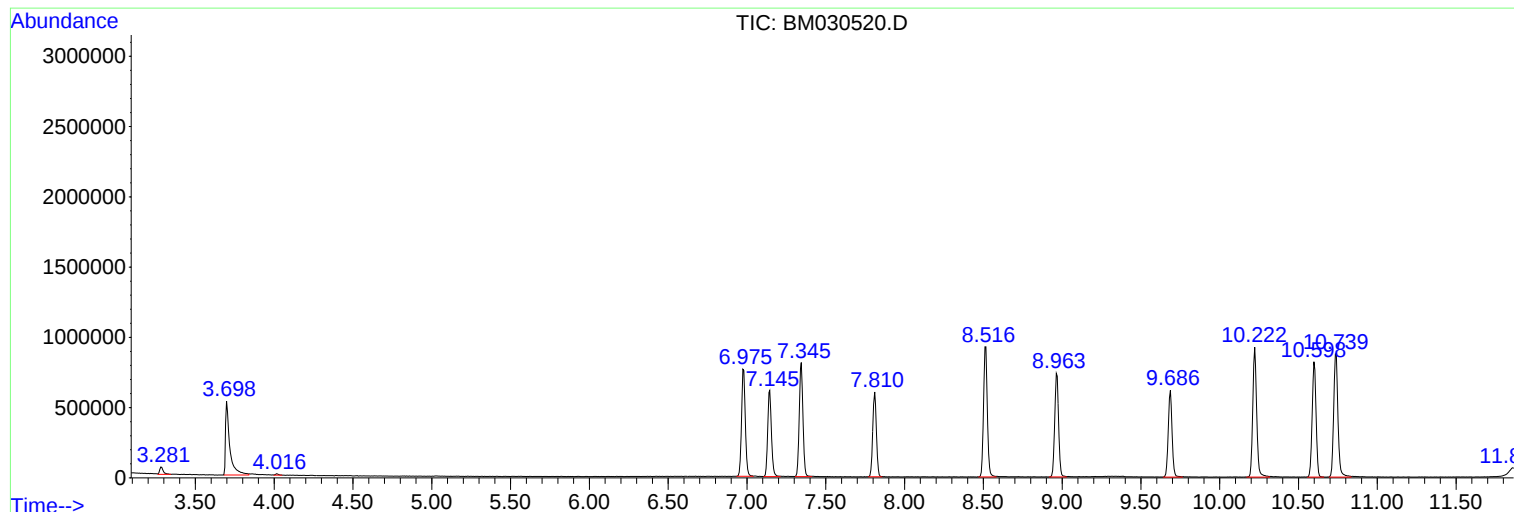

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030520.D
Acq On : 22 Jun 2021 18:05
Operator : CG/JU
Sample : PB137201BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK201










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclohexasiloxane, dodecane... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.860	3.30 ng/ul	231066	Naphthalene-d8	10.598

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexasiloxane, dodecamethyl-	444	C12H36O6Si6	000540-97-6	91
2			Cyclohexasiloxane, dodecamethyl-	444	C12H36O6Si6	000540-97-6	90
3			Cyclohexasiloxane, dodecamethyl-	444	C12H36O6Si6	000540-97-6	74
4			3-Trimethylsilyloxystearic acid,...	444	C24H52O3Si2	1000079-42-6	25
5			1,1,1,5,7,7,7-Heptamethyl-3,3-bi...	444	C13H40O5Si6	038147-00-1	16

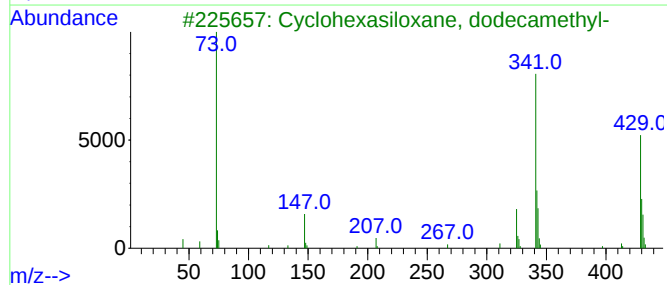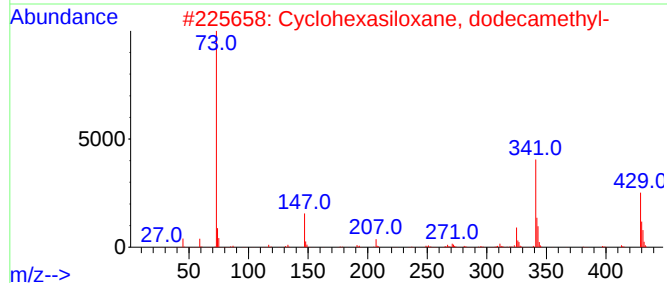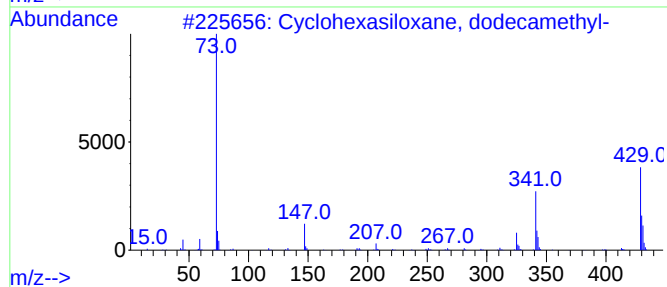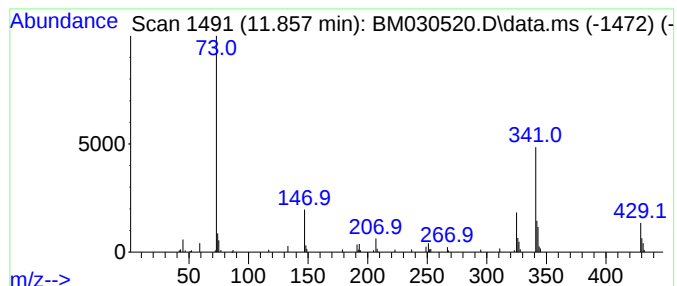

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030520.D
Acq On : 22 Jun 2021 18:05
Operator : CG/JU
Sample : PB137201BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK201

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclohexasiloxa...	11.860	3.3	ng/ul	231066	2	10.598	1400050	20.0