

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
 Data File : BM030543.D
 Acq On : 23 Jun 2021 08:36
 Operator : CG/JU
 Sample : PB137214BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030543.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	41	rVB	59474	77985	2.04%	0.161%
2	3.693	100	103	127	rBV	626346	1140625	29.90%	2.360%
3	4.010	154	157	163	rVB	12003	18199	0.48%	0.038%
4	5.028	326	330	335	rVB6	2735	3861	0.10%	0.008%
5	6.975	653	661	675	rBV	921875	1515030	39.71%	3.135%
6	7.140	682	689	699	rBV	730400	1153795	30.24%	2.388%
7	7.340	715	723	734	rBV	974913	1563790	40.99%	3.236%
8	7.804	793	802	812	rBV	763811	1200840	31.47%	2.485%
9	8.128	852	857	860	rVB5	3071	4516	0.12%	0.009%
10	8.510	913	922	937	rBV	1141616	1867834	48.96%	3.865%
11	8.963	991	999	1012	rBV	877252	1490794	39.07%	3.085%
12	9.681	1113	1121	1132	rBV	735914	1229628	32.23%	2.545%
13	10.216	1204	1212	1225	rBV	1126225	1920538	50.34%	3.974%
14	10.592	1269	1276	1288	rVB	1074930	1774366	46.51%	3.672%
15	10.728	1291	1299	1319	rBV	1067186	1933103	50.67%	4.000%
16	11.863	1485	1492	1496	rBV5	3408	7946	0.21%	0.016%
17	12.186	1541	1547	1555	rBV	19236	33959	0.89%	0.070%
18	13.057	1691	1695	1702	rVB3	2427	4479	0.12%	0.009%
19	13.845	1822	1829	1840	rBV	1823121	2520631	66.07%	5.216%
20	14.127	1869	1877	1888	rBV	2269756	3254552	85.30%	6.735%
21	14.433	1922	1929	1938	rBV	1524547	2269219	59.48%	4.696%
22	14.633	1956	1963	1981	rBV	566012	1008661	26.44%	2.087%
23	15.427	2091	2098	2106	rBV	2645999	3815366	100.00%	7.896%
24	15.545	2112	2118	2134	rBV	455518	672805	17.63%	1.392%
25	15.669	2134	2139	2148	rVB2	30620	50021	1.31%	0.104%
26	16.110	2208	2214	2220	rVB7	2669	6068	0.16%	0.013%
27	16.216	2225	2232	2238	rVB4	28290	44845	1.18%	0.093%
28	16.857	2337	2341	2345	rBV5	4410	5595	0.15%	0.012%
29	16.957	2355	2358	2364	rVB2	5506	7599	0.20%	0.016%
30	17.174	2387	2395	2405	rBV	1599632	2264801	59.36%	4.687%
31	17.274	2405	2412	2423	rVV	2483345	3586094	93.99%	7.421%
32	17.457	2440	2443	2447	rBV6	3104	5166	0.14%	0.011%
33	17.557	2457	2460	2463	rBV4	2973	3904	0.10%	0.008%
34	19.198	2735	2739	2742	rBV	23191	32192	0.84%	0.067%
35	19.451	2778	2782	2786	rBV	20120	28209	0.74%	0.058%
36	19.562	2794	2801	2816	rBV	2691710	3691544	96.75%	7.639%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030543.D
Acq On : 23 Jun 2021 08:36
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK214

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Title : SVOA CALIBRATION

37	21.339	3098	3103	3109	rBV	1560729	2068159	54.21%	4.280%
38	23.468	3458	3465	3478	rVB	1990635	3812398	99.92%	7.890%
39	23.609	3483	3489	3498	rVB2	1158159	2233082	58.53%	4.621%


Sum of corrected areas: 48322199

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030543.D
Acq On : 23 Jun 2021 08:36
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

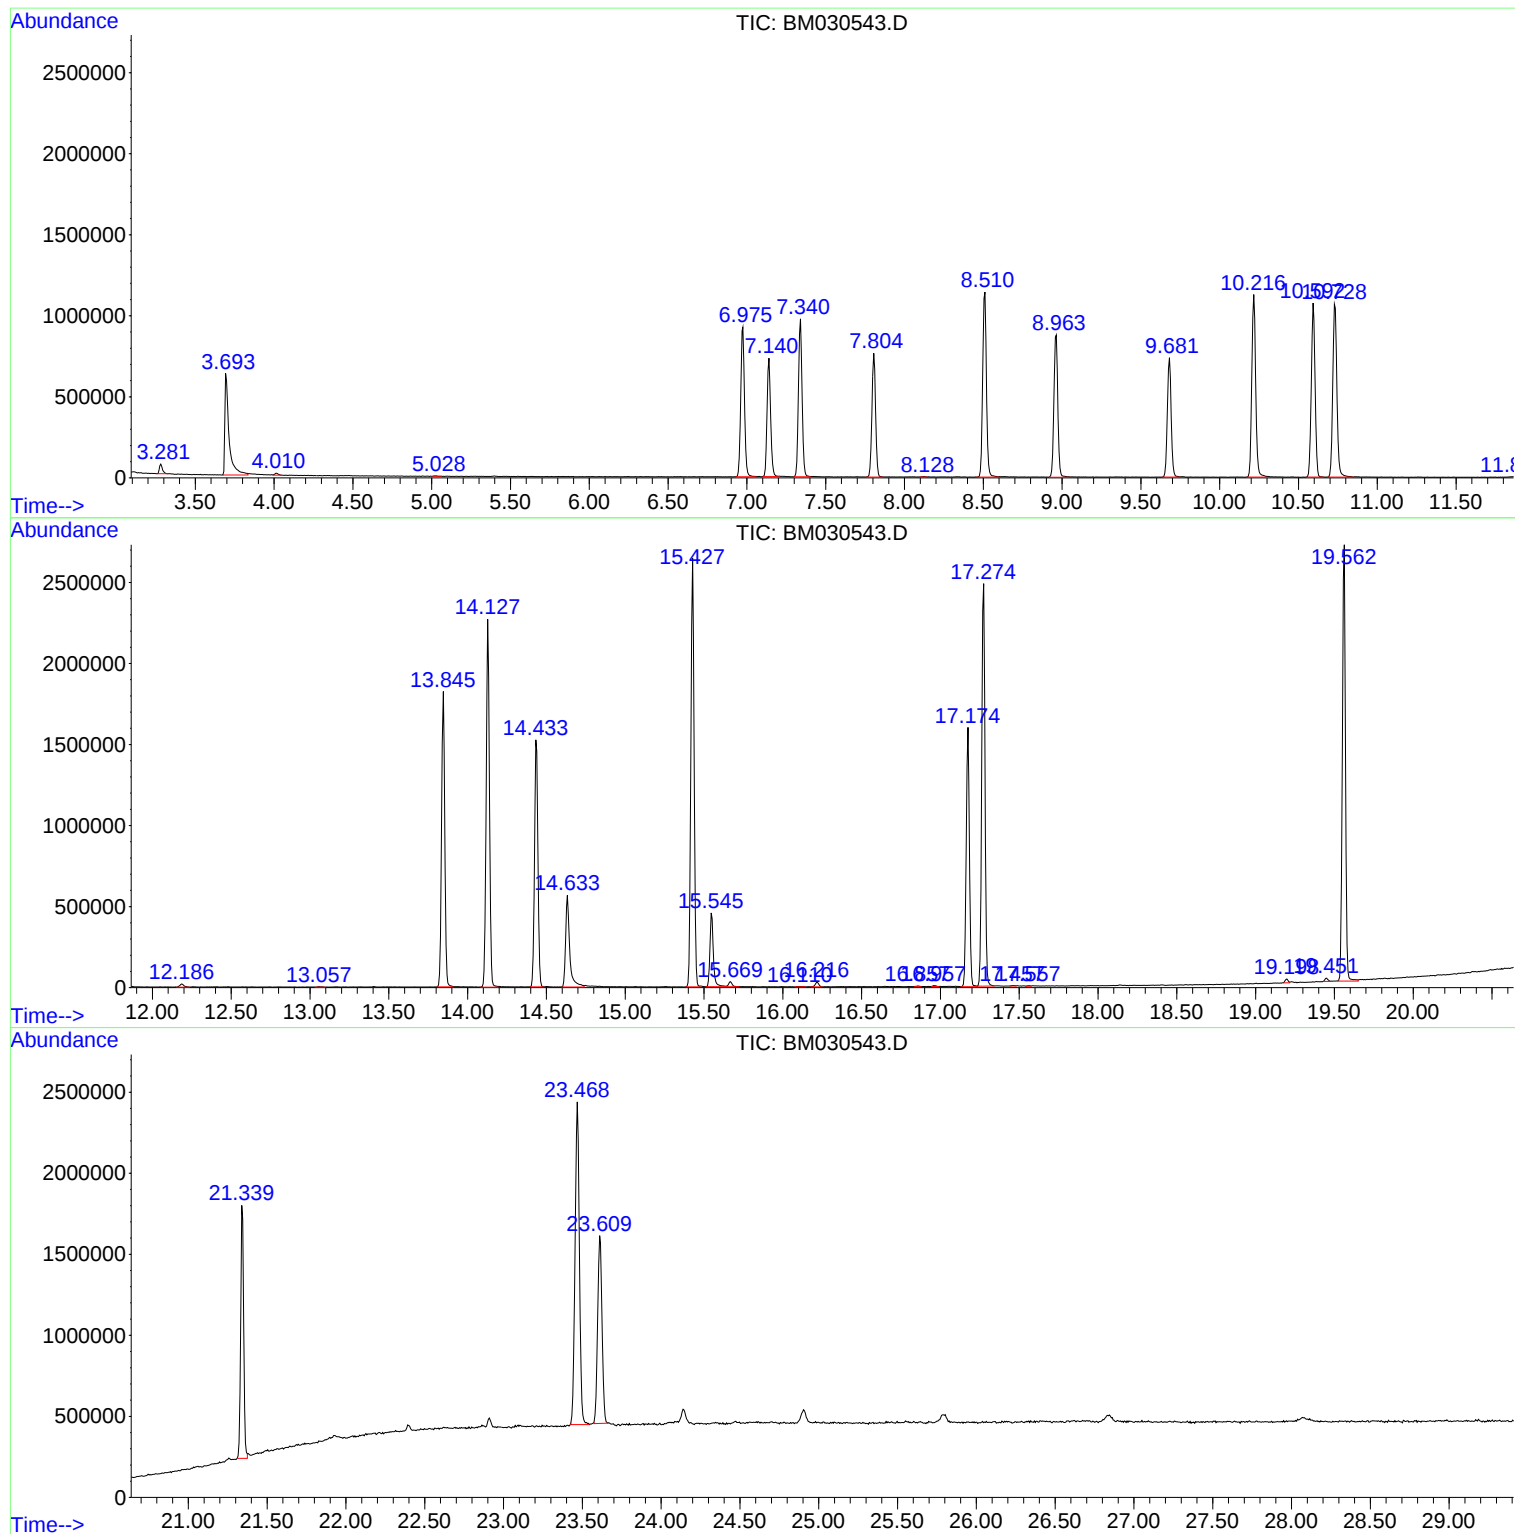

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030543.D
Acq On : 23 Jun 2021 08:36
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062221\
Data File : BM030543.D
Acq On : 23 Jun 2021 08:36
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
