
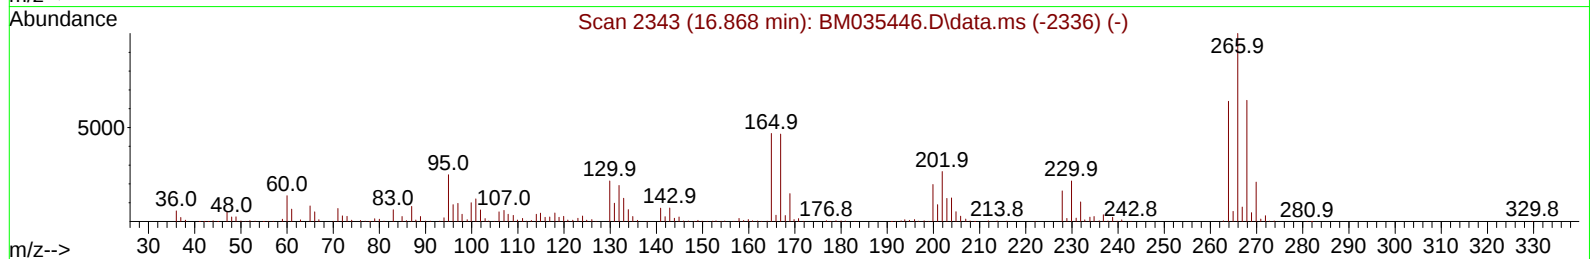
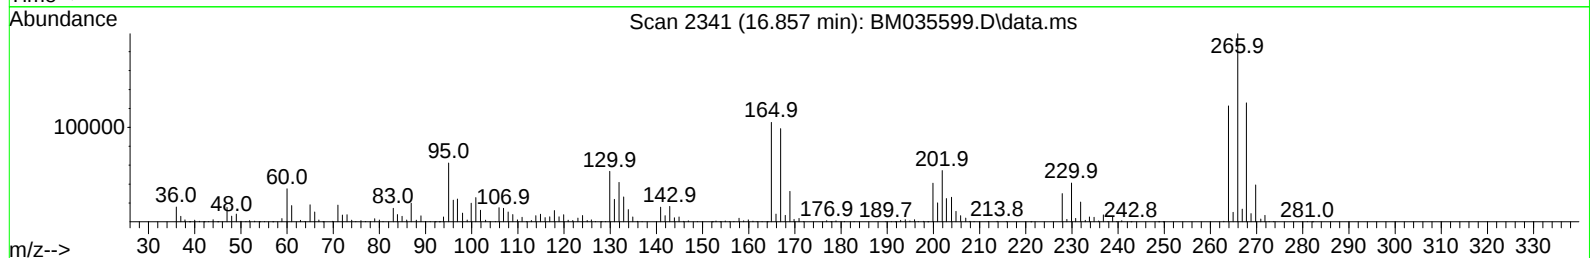


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035599.D
Acq On : 22 Jun 2022 13:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:52:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 07:33:33 2022
Response via : Initial Calibration

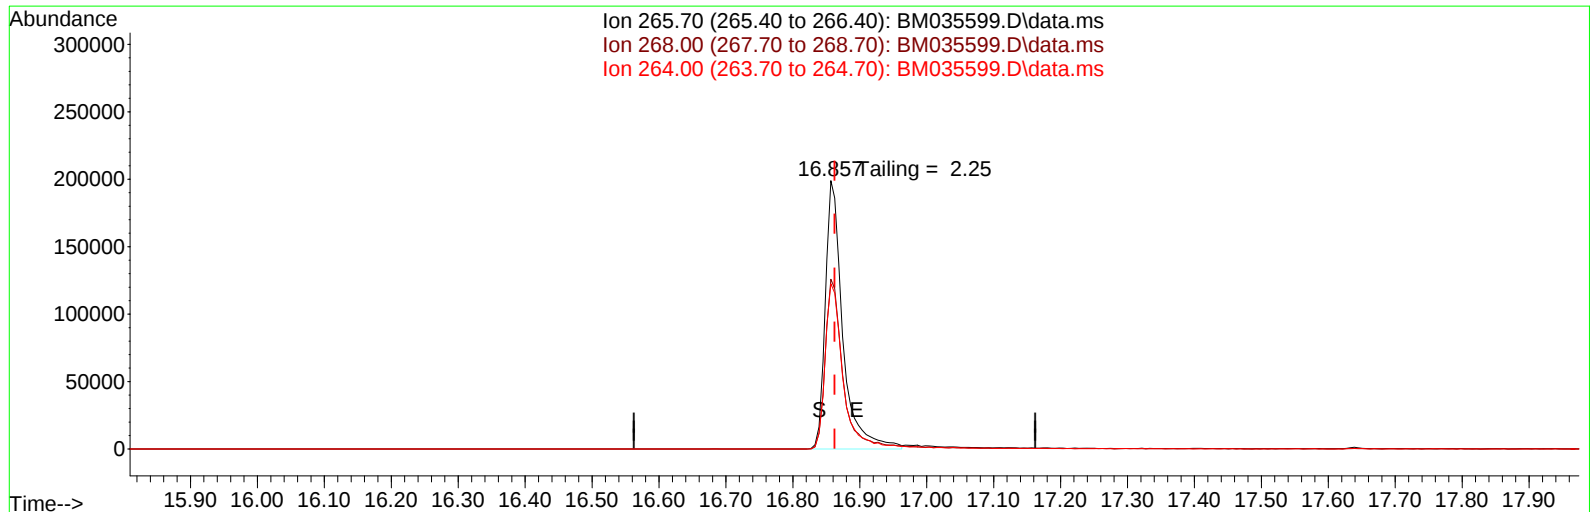

TIC: BM035599.D\data.ms

(70) Pentachlorophenol (C)




16.857min (-0.006) 286189.83 ng

response 365487

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.25
264.00	63.30	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035599.D
Acq On : 22 Jun 2022 13:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:52:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 07:33:33 2022
Response via : Initial Calibration

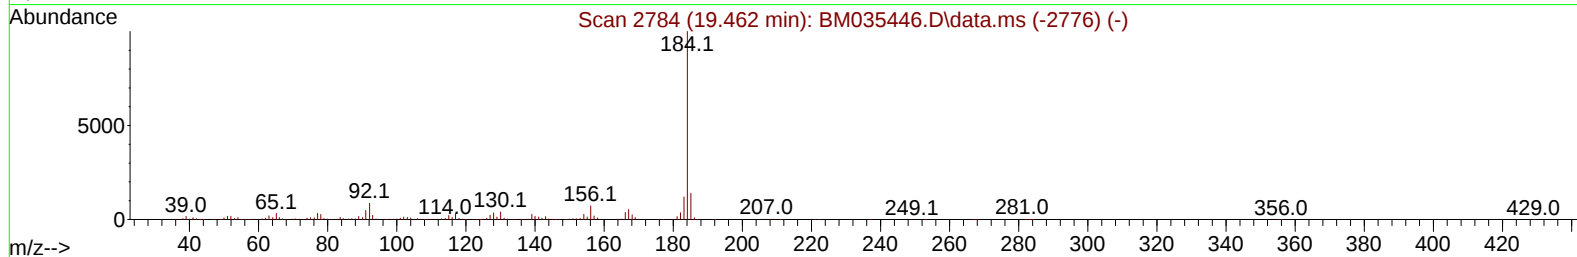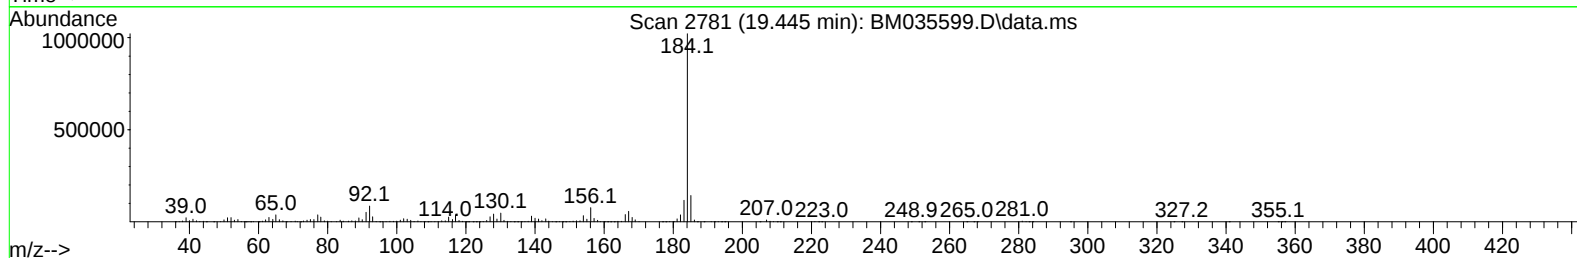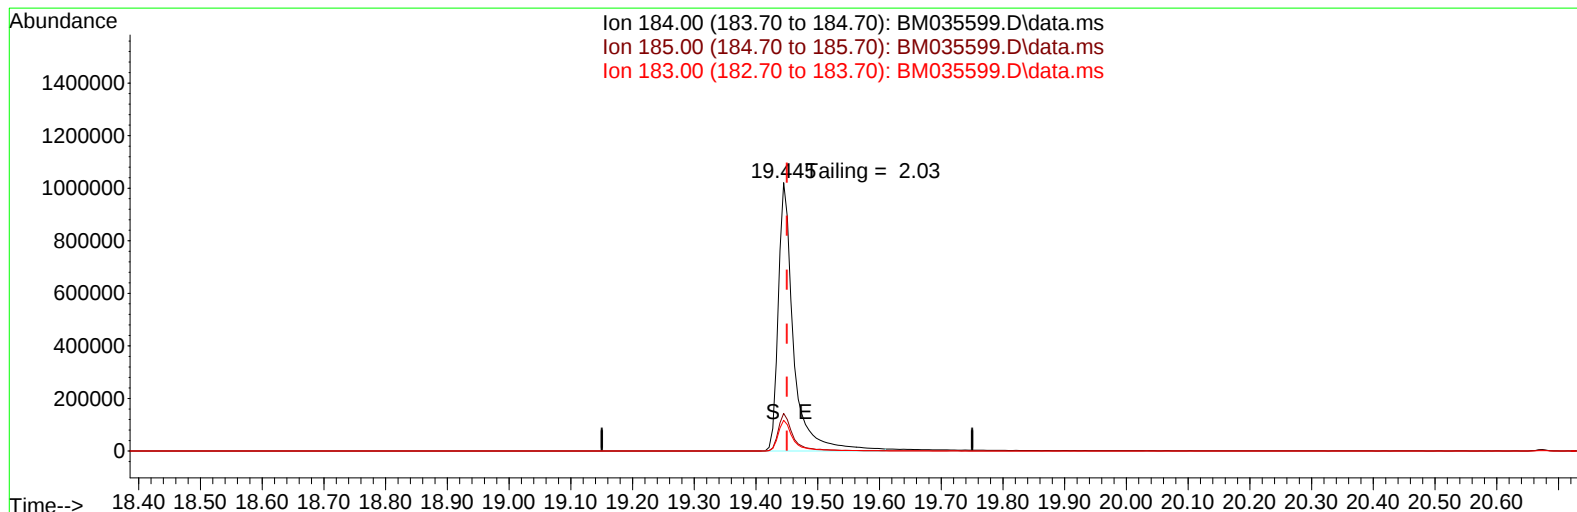

TIC: BM035599.D\data.ms

(77) Benzidine**19.445min (-0.006) 132462.73 ng****response 1801929**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.01
183.00	11.90	11.45
0.00	0.00	0.00