

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
 Data File : BM035601.D
 Acq On : 22 Jun 2022 15:39
 Operator : CG/JU
 Sample : PB145755BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145755BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	388	394	419	rBV	3345998	5450652	60.55%	11.573%
2	7.004	660	666	692	rBV	2792045	5313327	59.02%	11.281%
3	7.804	794	802	818	rBV	633841	1097118	12.19%	2.329%
4	8.963	992	999	1028	rBV	1745320	3459860	38.43%	7.346%
5	10.598	1270	1277	1302	rBV	702499	1513505	16.81%	3.213%
6	13.069	1690	1697	1726	rBV	5047994	8151545	90.55%	17.307%
7	14.445	1924	1931	1949	rBV	1063387	1889606	20.99%	4.012%
8	15.939	2179	2185	2216	rBV	2662862	4798832	53.31%	10.189%
9	17.198	2392	2399	2419	rBV	1017794	1914265	21.27%	4.064%
10	19.815	2839	2844	2859	rBV	6820977	9001864	100.00%	19.112%
11	21.386	3106	3111	3123	rBV	1283592	2146742	23.85%	4.558%
12	23.715	3501	3507	3525	rBV2	1007591	2362486	26.24%	5.016%




Sum of corrected areas: 47099802

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035601.D
Acq On : 22 Jun 2022 15:39
Operator : CG/JU
Sample : PB145755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145755BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

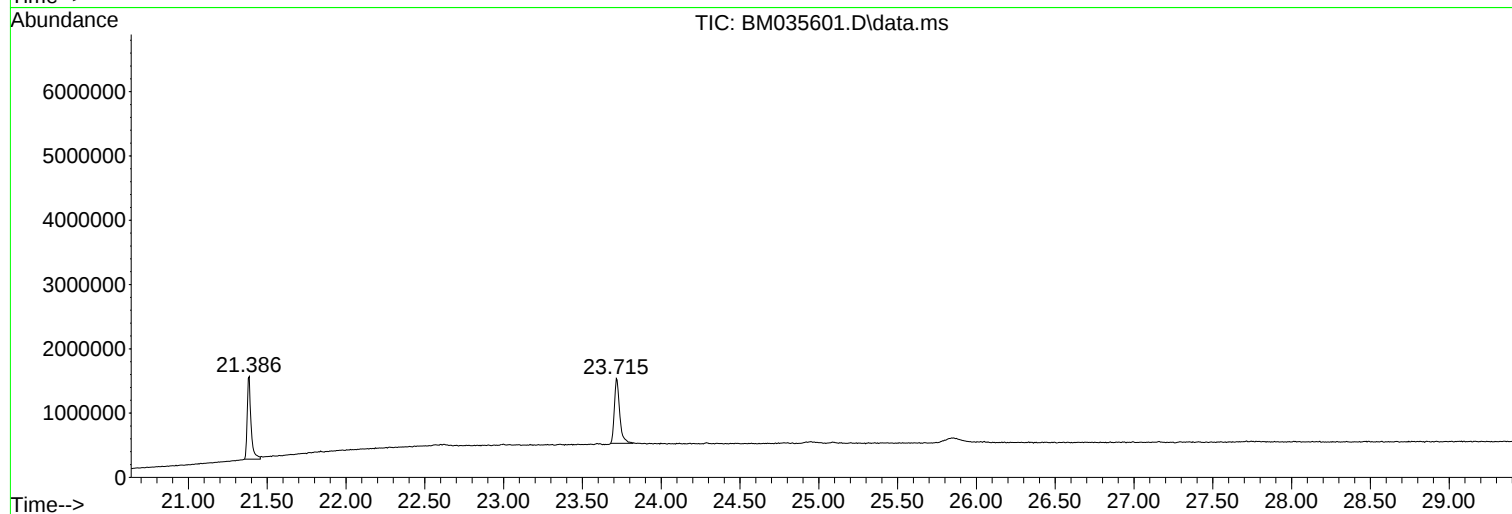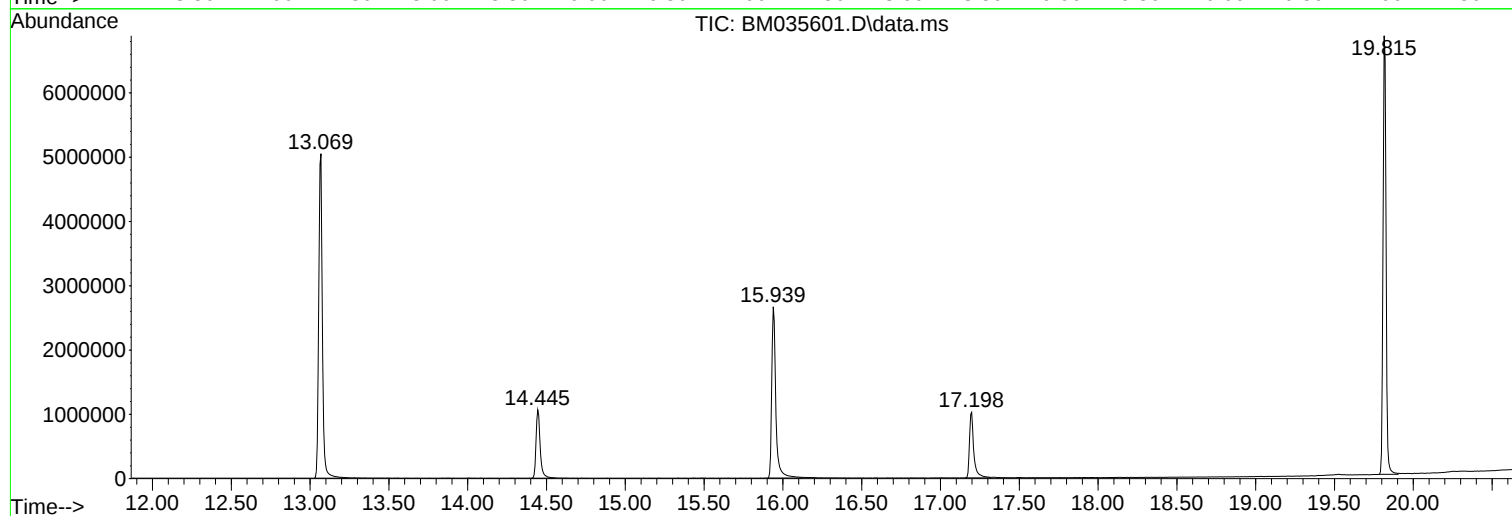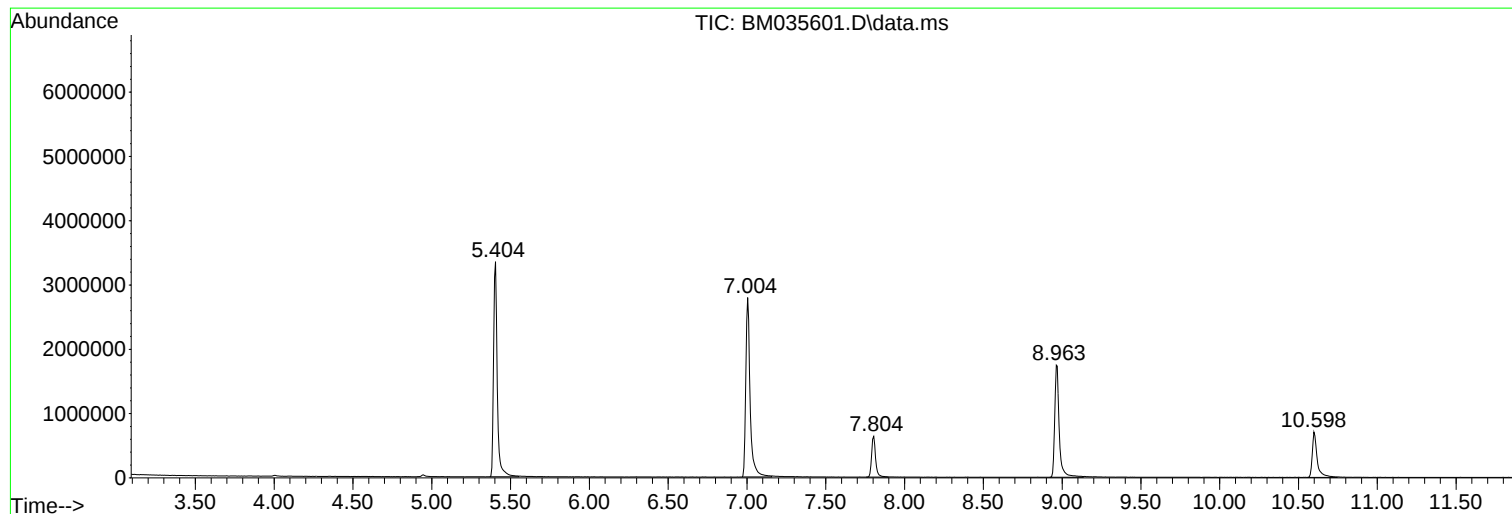

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035601.D
Acq On : 22 Jun 2022 15:39
Operator : CG/JU
Sample : PB145755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145755BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035601.D
Acq On : 22 Jun 2022 15:39
Operator : CG/JU
Sample : PB145755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145755BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------