


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
 Data File : BM035599.D
 Acq On : 22 Jun 2022 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 23 07:33:33 2022

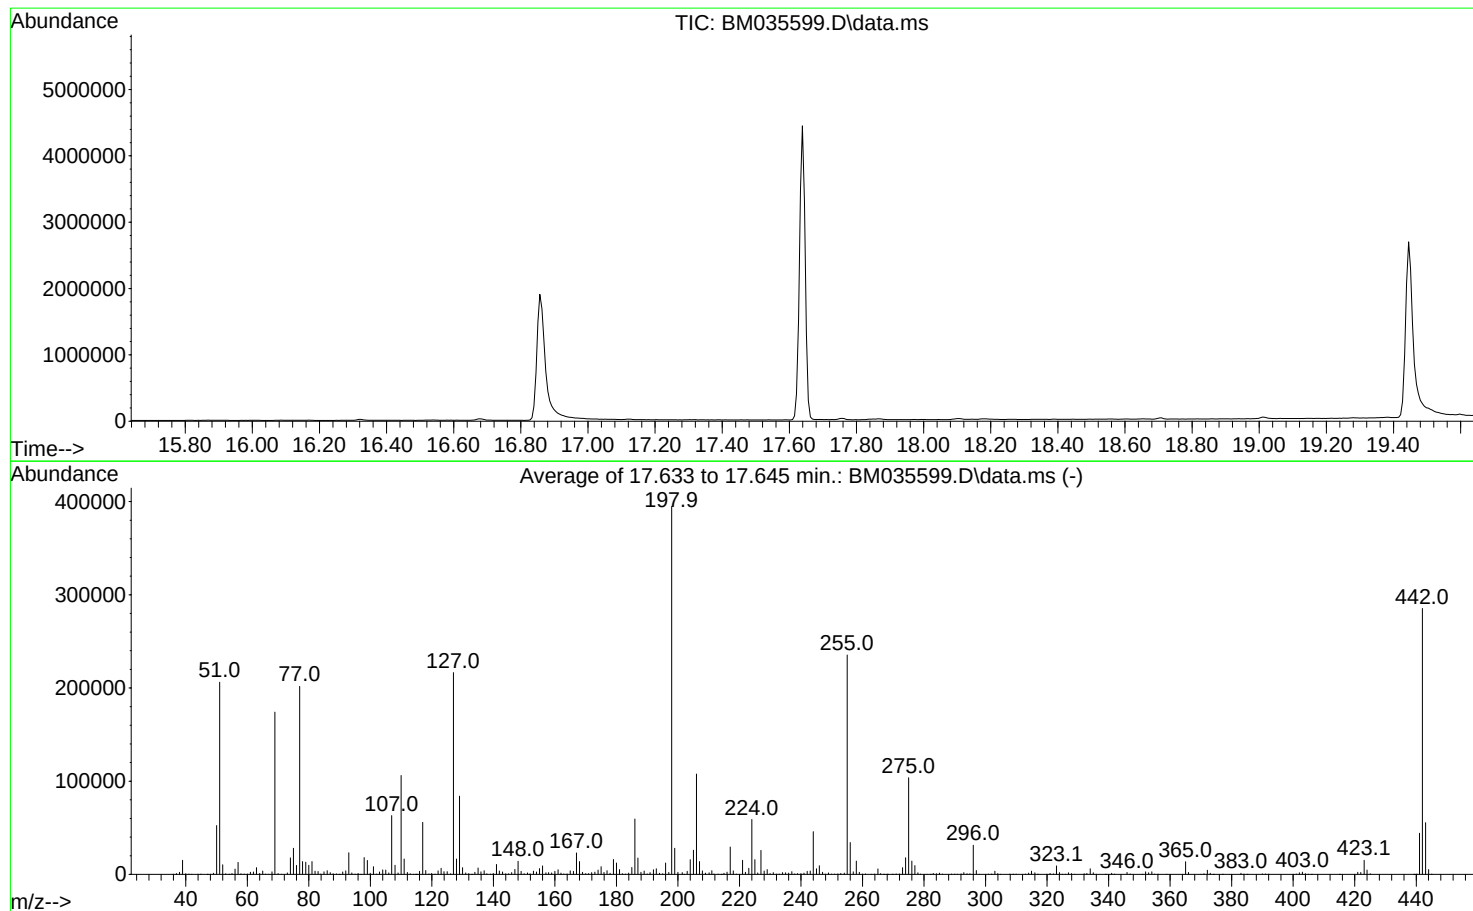




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	206258	PASS
68	69	0.00	2	1.6	2795	PASS
69	198	0.00	100	44.1	174128	PASS
70	69	0.00	2	0.5	886	PASS
127	198	10	80	54.9	216512	PASS
197	198	0.00	2	0.5	2083	PASS
198	198	100	100	100.0	394709	PASS
199	198	5	9	7.1	27936	PASS
275	198	10	60	26.3	103789	PASS
365	198	1	100	3.4	13491	PASS
441	198	0.01	100	11.2	44131	PASS
442	442	50	100	100.0	285312	PASS
443	442	15	24	19.4	55448	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035599.D
Acq On : 22 Jun 2022 13:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 23 08:52:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 07:33:33 2022
Response via : Initial Calibration

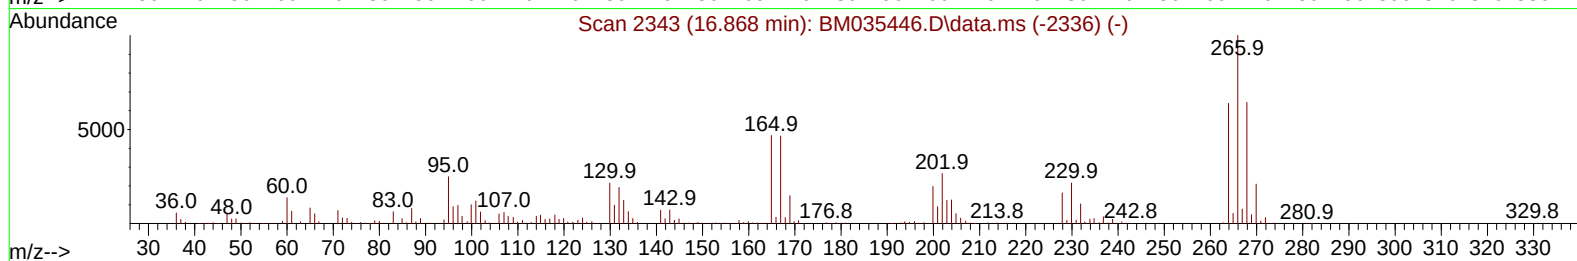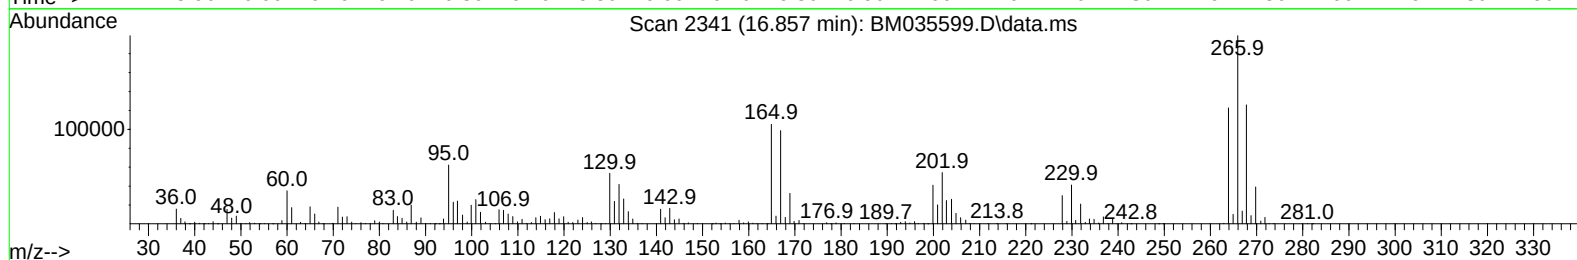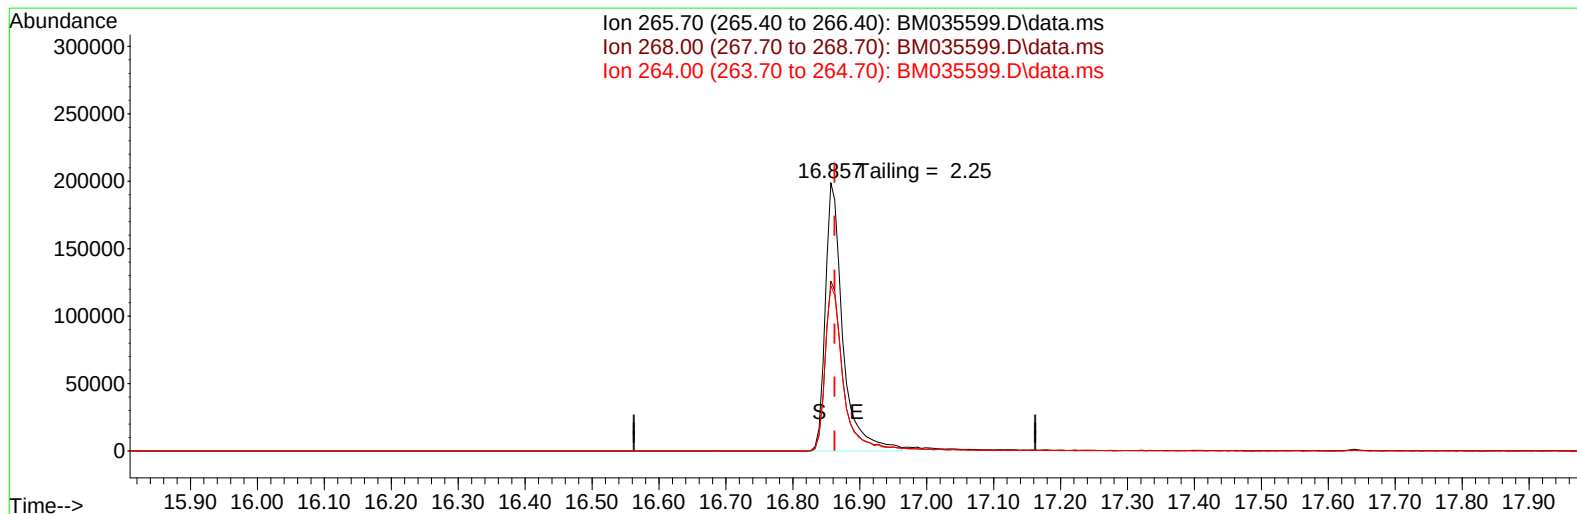

TIC: BM035599.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.006) 286189.83 ng




response 365487

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.25
264.00	63.30	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062222\
Data File : BM035599.D
Acq On : 22 Jun 2022 13:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 23 08:52:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 07:33:33 2022
Response via : Initial Calibration

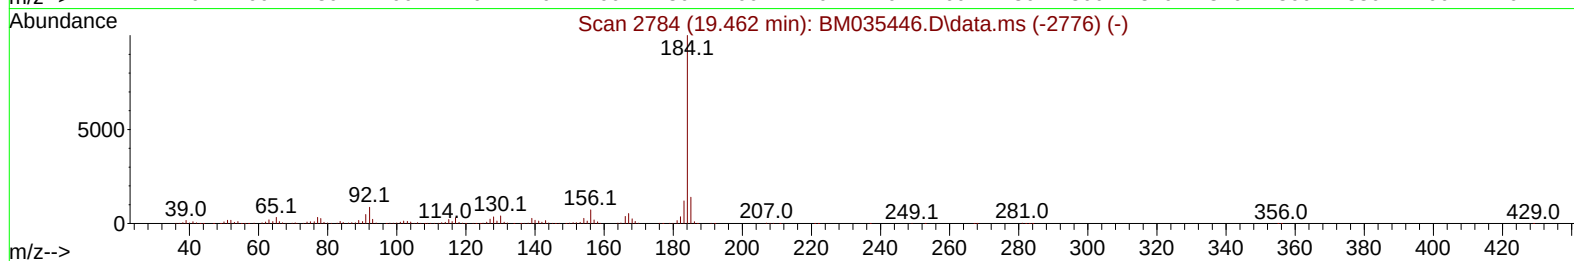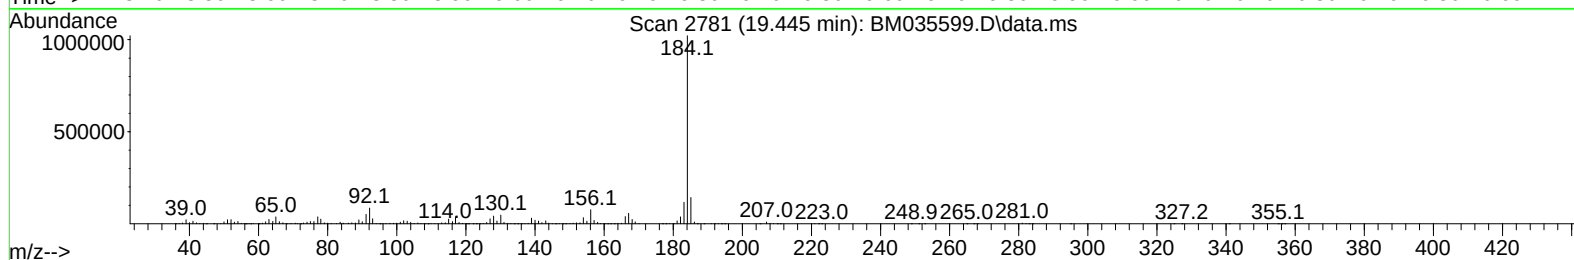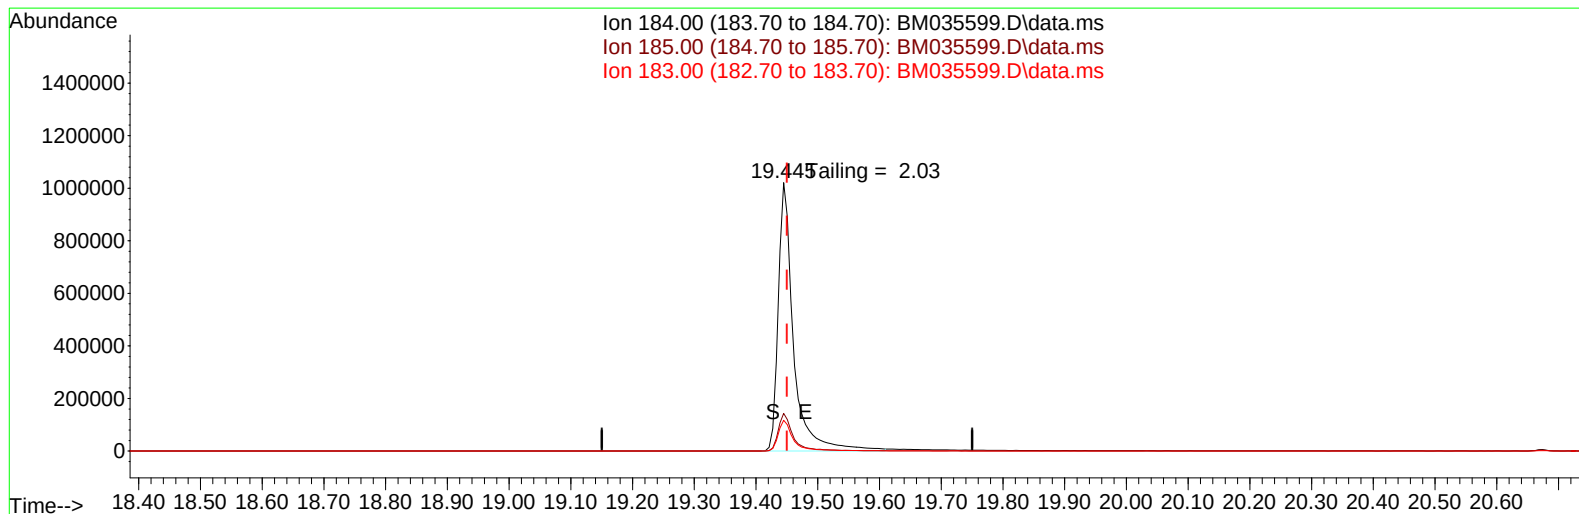

TIC: BM035599.D\data.ms

(77) Benzidine

19.445min (-0.006) 132462.73 ng

response 1801929

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.01
183.00	11.90	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/22/2022	BNA_M	<u>BM035599.D</u>
Compound Name	Response	Retention Time
DDT	1200689	20.674
DDD	14769	20.239
DDE	1640	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16409	1217098	1.35

Instrument :
BNA_M
ClientSampleId :
DFTPP