

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 188.00 (187.70 to 188.70): BM046226.D\data.ms
Ion 94.00 (93.70 to 94.70): BM046226.D\data.ms
Ion 80.00 (79.70 to 80.70): BM046226.D\data.ms

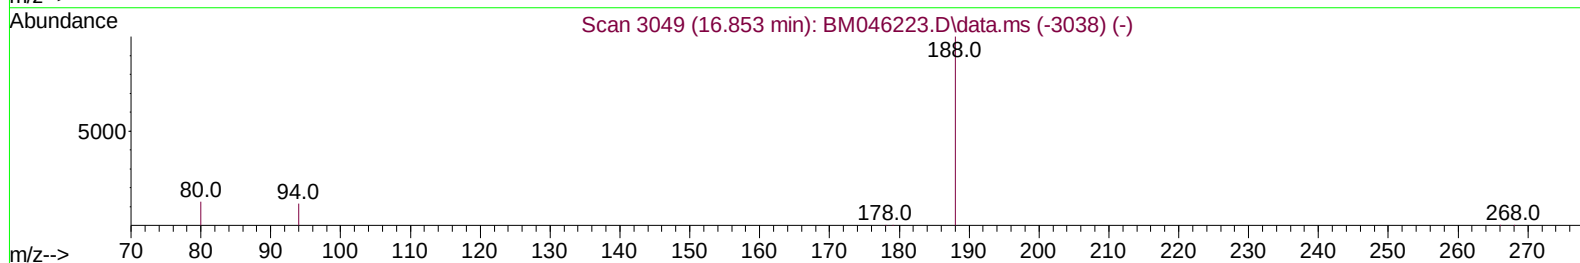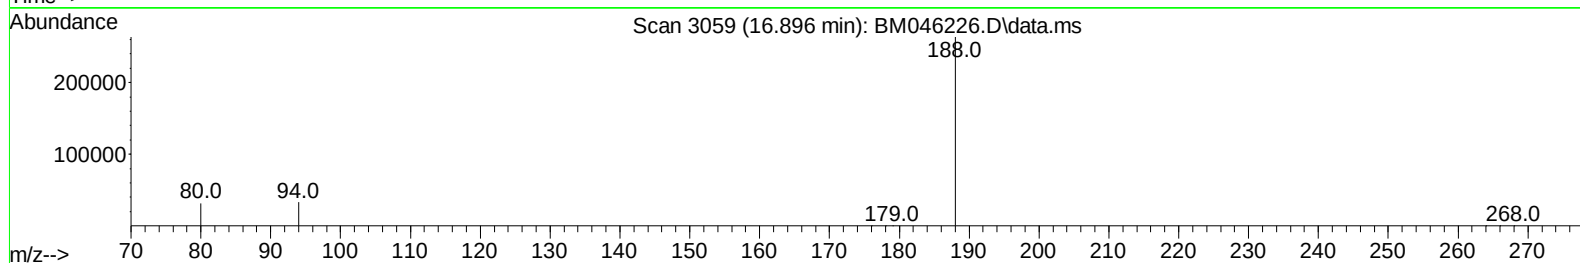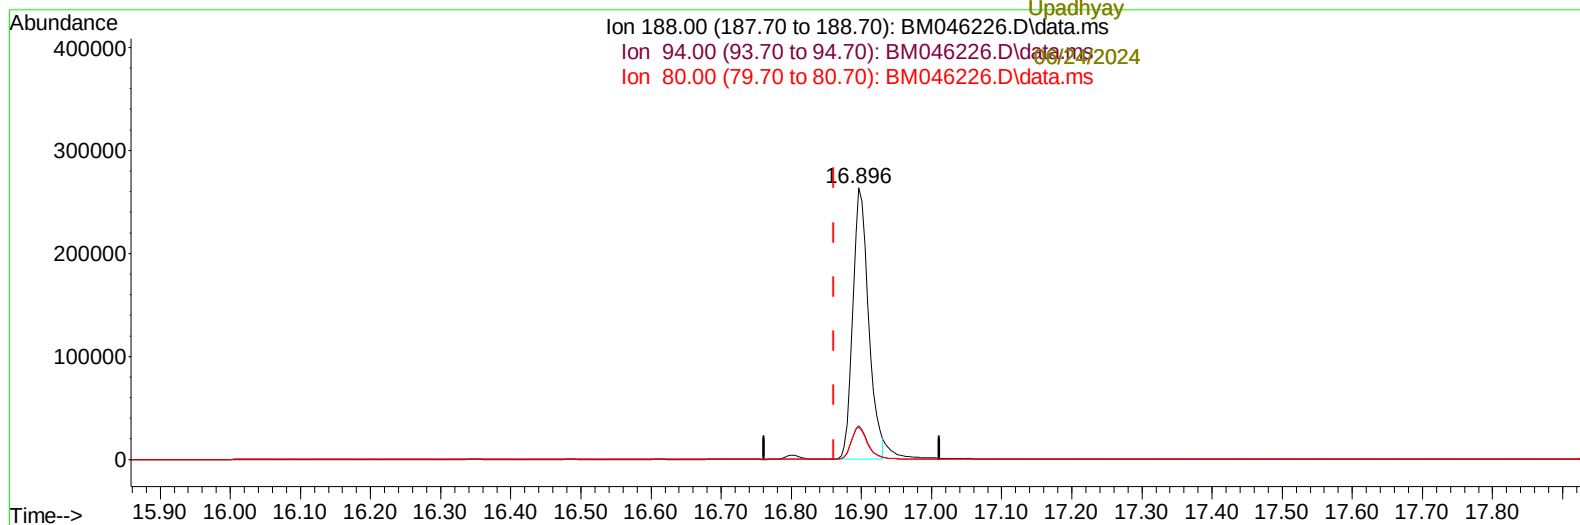

TIC: BM046226.D\data.ms

(13) Phenanthrene-d10 (I)**16.896min (+ 0.035) 0.40 ng/u1****response 411598**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	12.43
80.00	15.20	11.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 188.00 (187.70 to 188.70): BM046226.D\data.ms
Ion 94.00 (93.70 to 94.70): BM046226.D\data.ms
Ion 80.00 (79.70 to 80.70): BM046226.D\data.ms

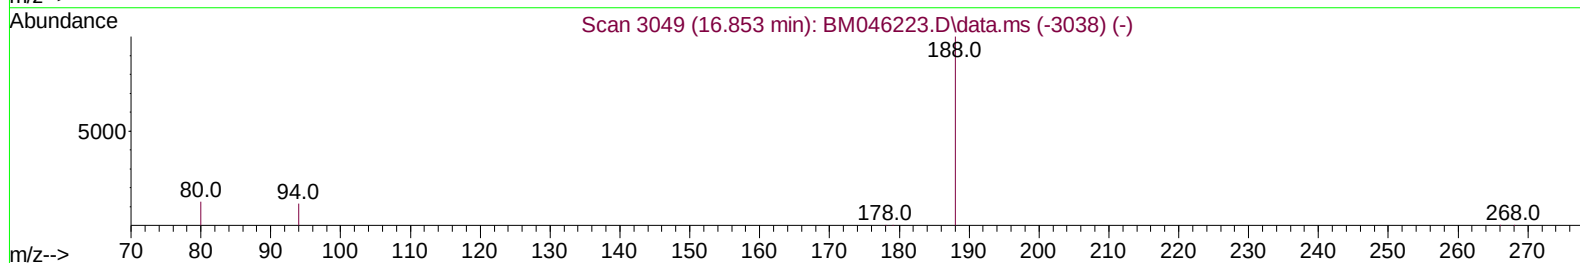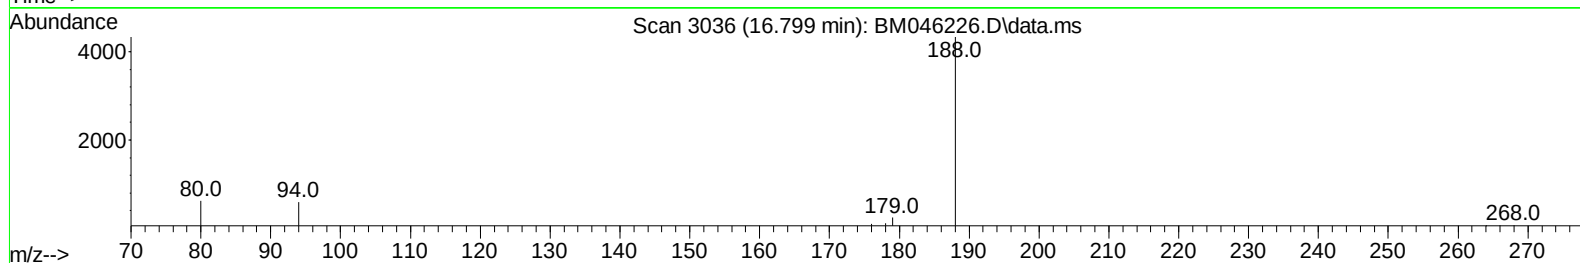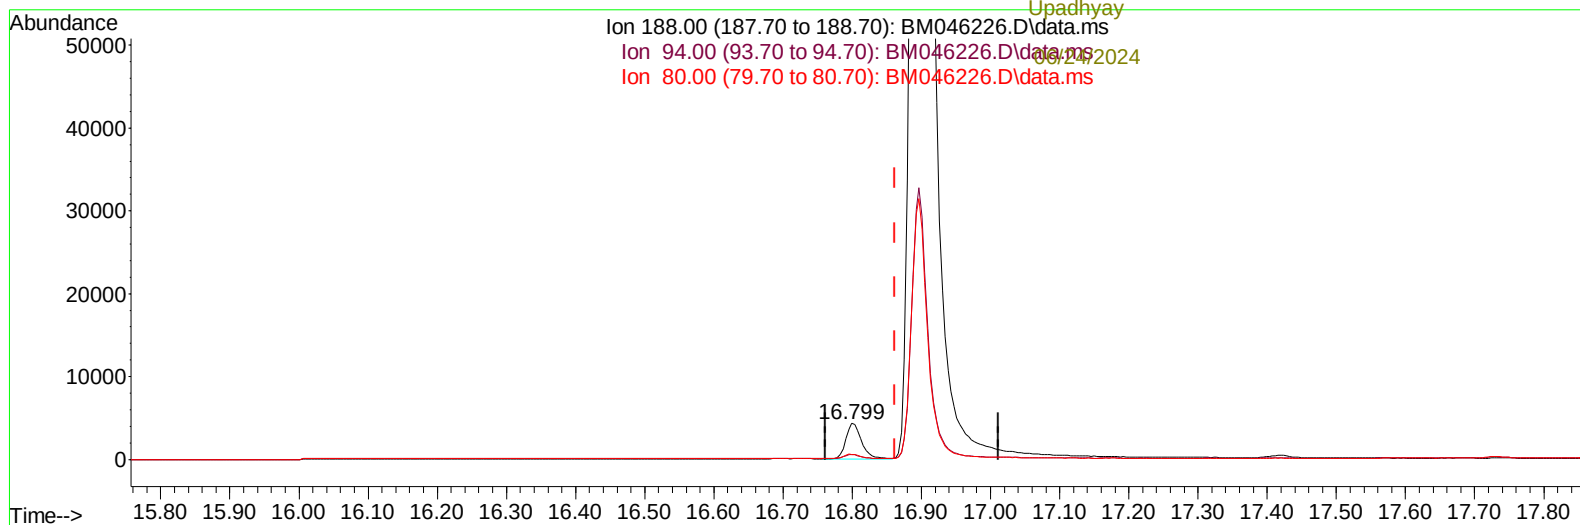

TIC: BM046226.D\data.ms

(13) Phenanthrene-d10 (I)

16.799min (-0.062) 0.40 ng/ul m

response 6820

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	13.76
80.00	15.20	14.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4C72

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay

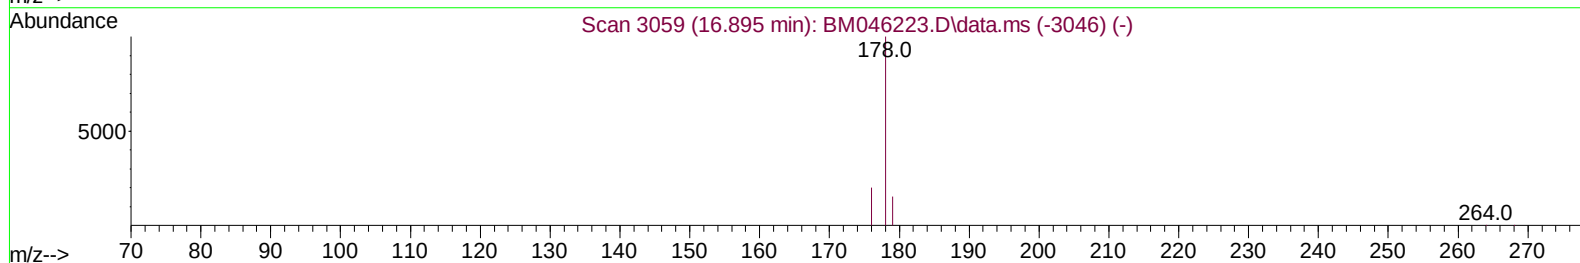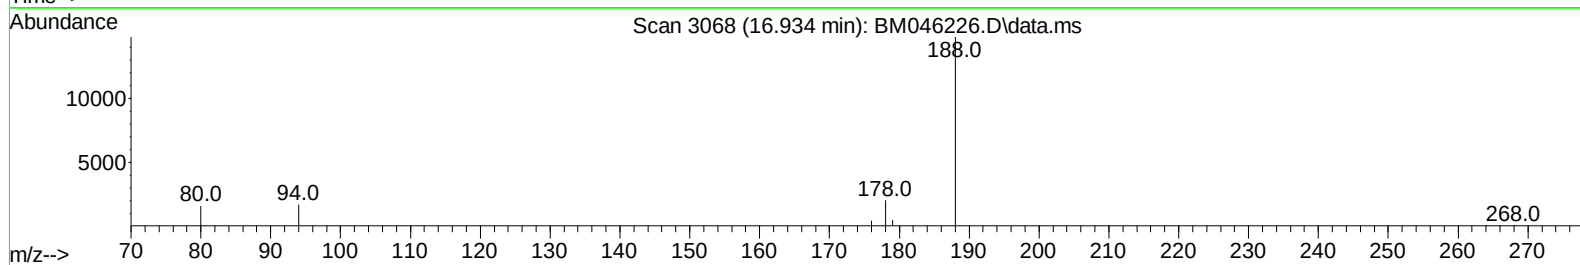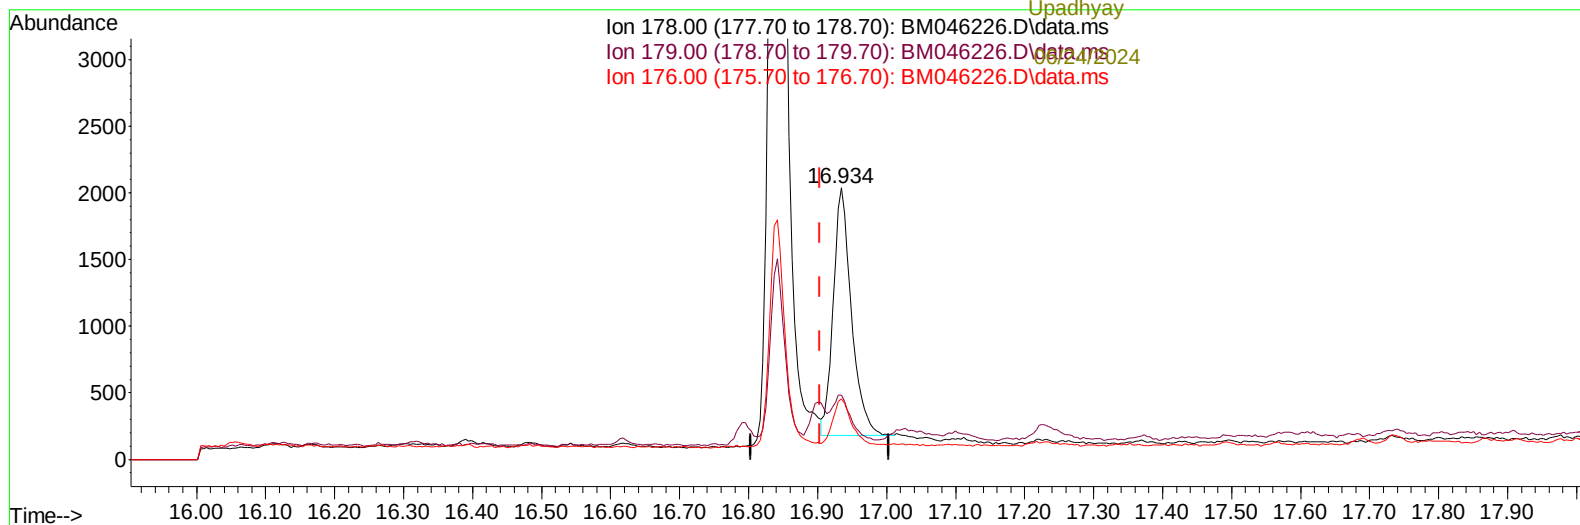

TIC: BM046226.D\data.ms

(15) Phenanthrene

16.934min (+ 0.031) 0.18 ng/u1

response 3371

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	23.76#
176.00	21.40	22.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 178.00 (177.70 to 178.70): BM046226.D\data.ms
Ion 179.00 (178.70 to 179.70): BM046226.D\data.ms
Ion 176.00 (175.70 to 176.70): BM046226.D\data.ms

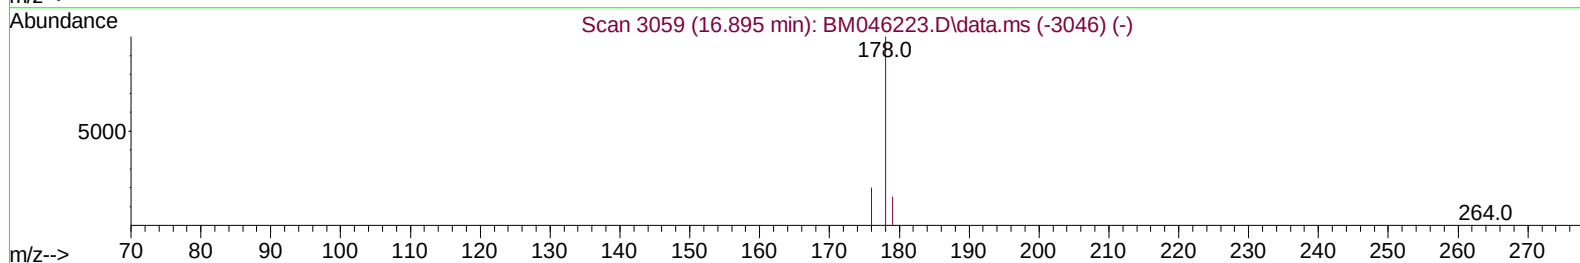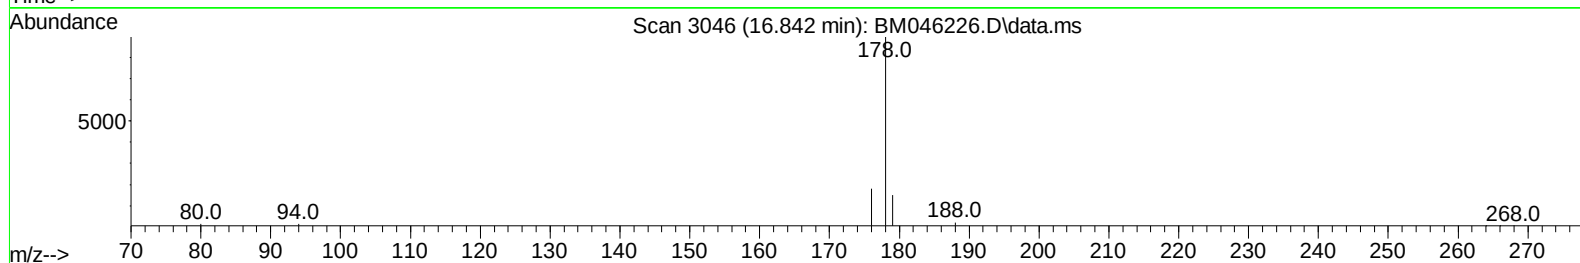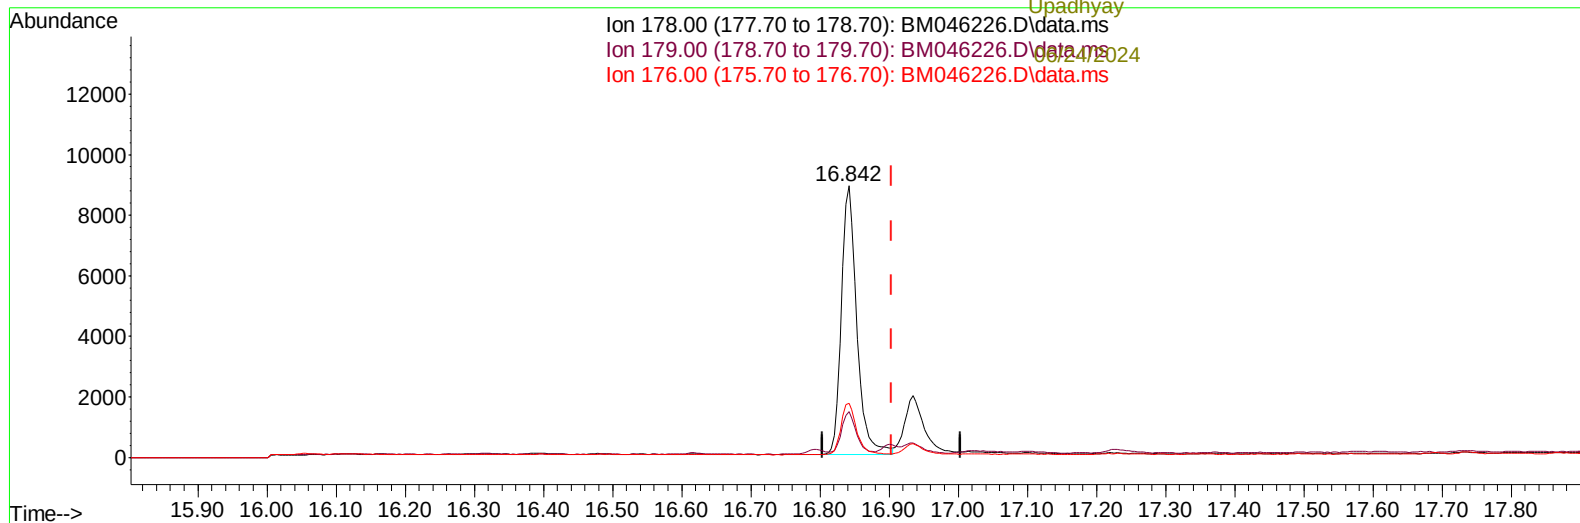

TIC: BM046226.D\data.ms

(15) Phenanthrene

16.842min (-0.062) 0.72 ng/ul m

response 13716

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	16.79
176.00	21.40	20.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
 Data File : BM046226.D
 Acq On : 23 Jun 2024 09:35
 Operator : MA/JU
 Sample : P2776-19
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 02:25:34 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
 Supervised By :Jagrut
 Upadhyay

Ion 178.00 (177.70 to 178.70): BM046226.D\data.ms
 Ion 179.00 (178.70 to 179.70): BM046226.D\data.ms
 Ion 176.00 (175.70 to 176.70): BM046226.D\data.ms

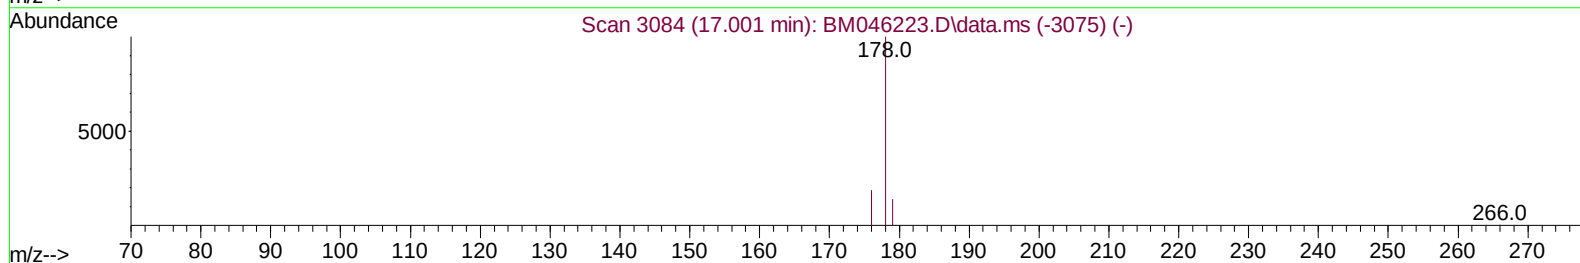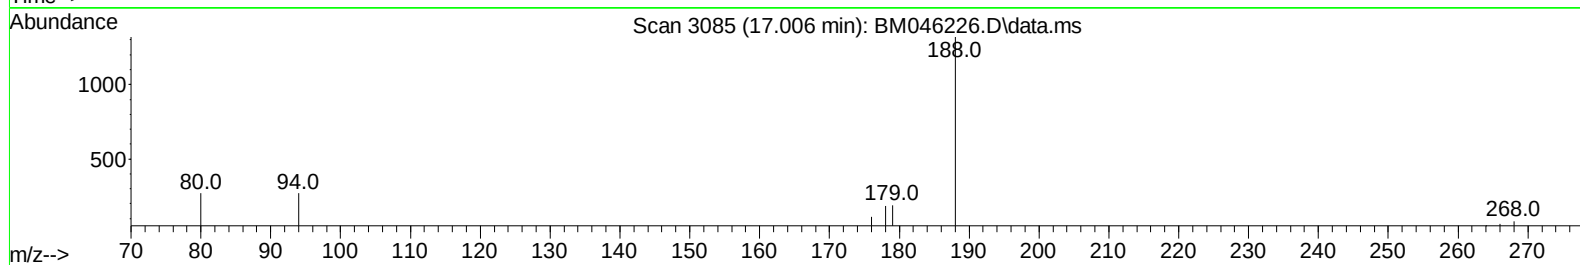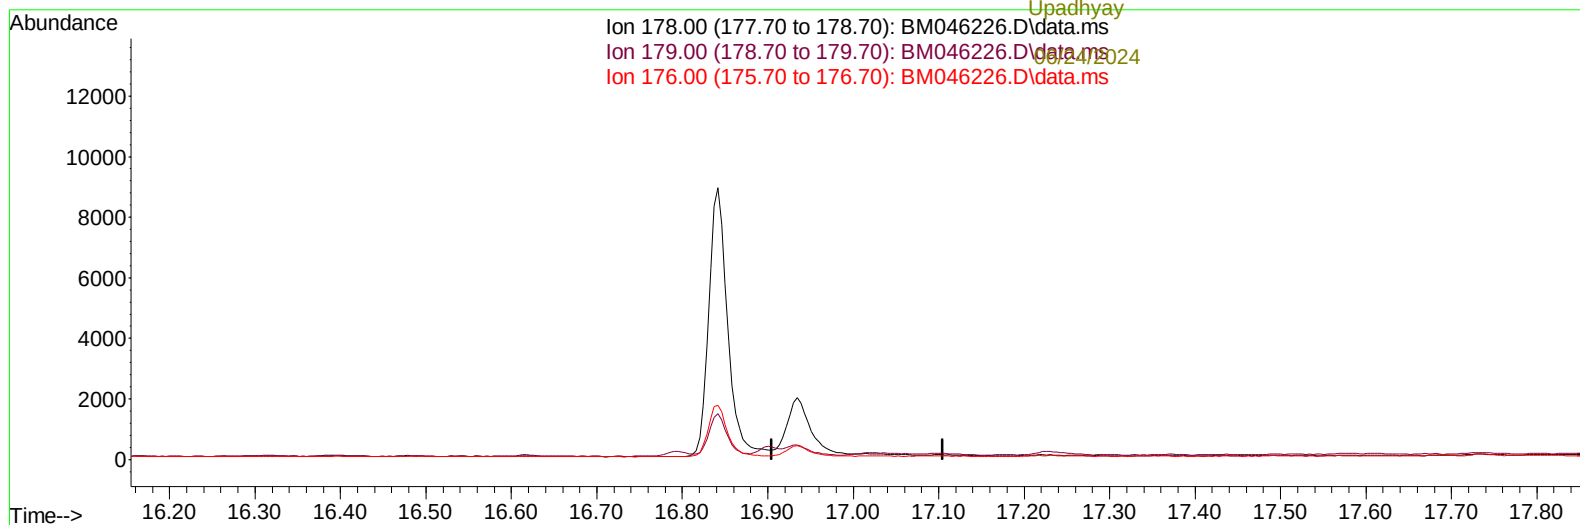

TIC: BM046226.D\data.ms

(16) Anthracene

17.005min (-17.005) 0.00 ng/ul

response 0

Ion	Exp%	Act%
178.00	100.00	0.00
179.00	18.60	0.00#
176.00	21.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72


Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024


Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay


Ion 178.00 (177.70 to 178.70): BM046226.D\data.ms
Ion 179.00 (178.70 to 179.70): BM046226.D\data.ms
Ion 176.00 (175.70 to 176.70): BM046226.D\data.ms

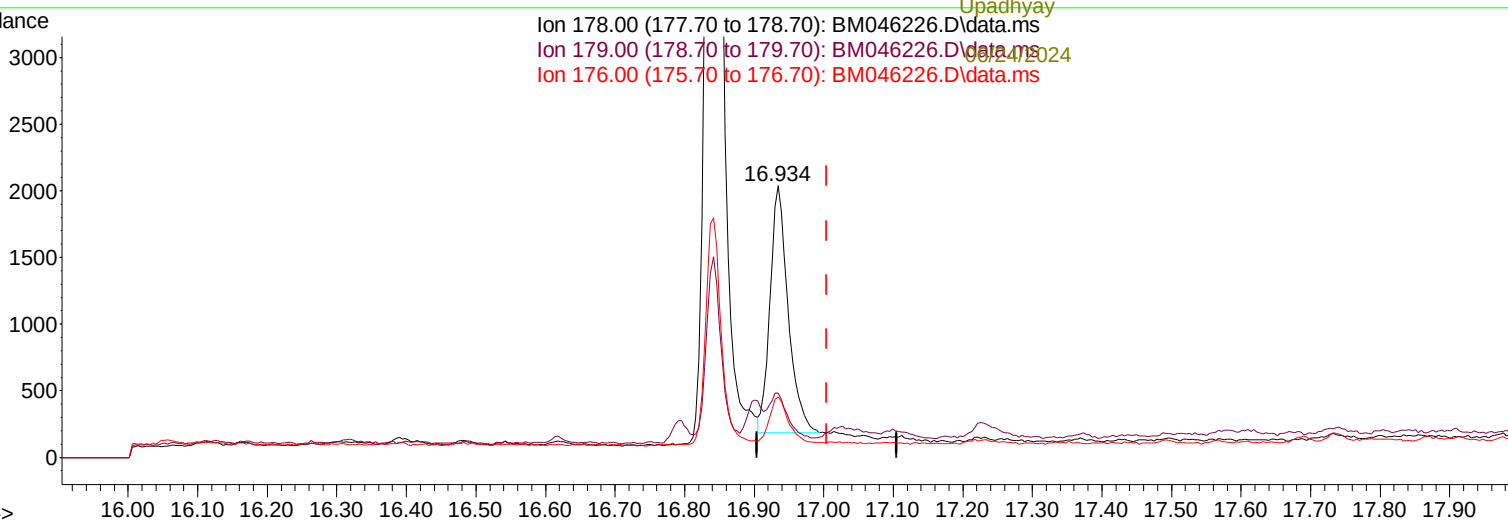

Scan 3068 (16.934 min): BM046226.D\data.ms

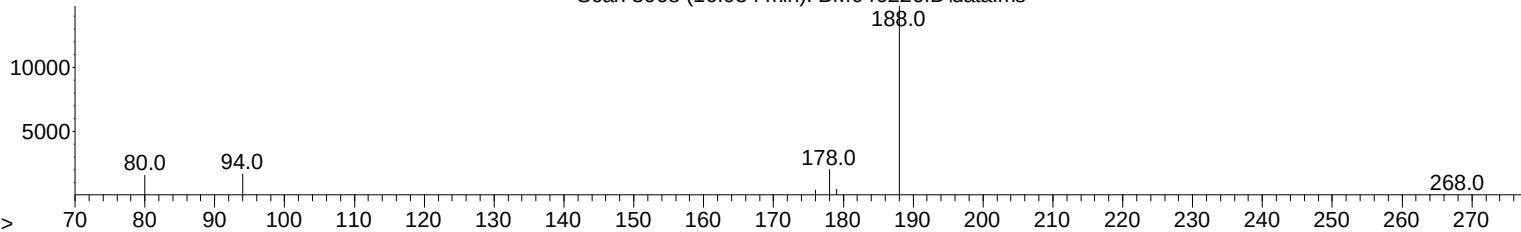

Scan 3084 (17.001 min): BM046223.D\data.ms (-3075) (-)

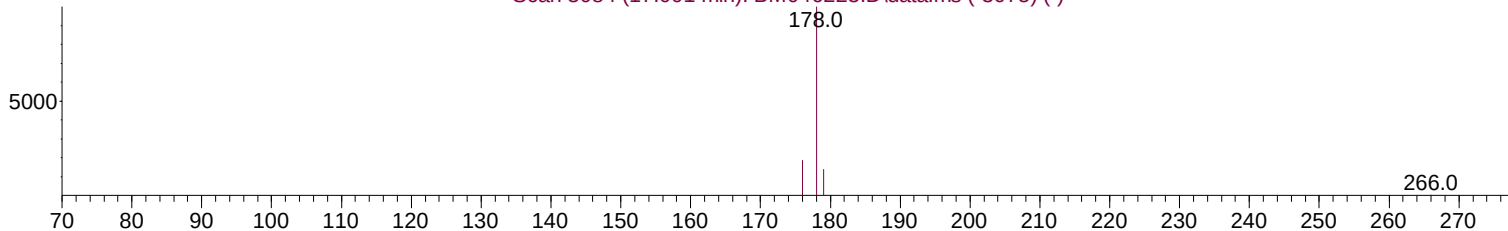

TIC: BM046226.D\data.ms

(16) Anthracene

16.934min (-0.070) 0.23 ng/ul m

response 3345

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.60	23.76#
176.00	21.20	22.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 240.00 (239.70 to 240.70): BM046226.D\data.ms
Ion 120.00 (119.70 to 120.70): BM046226.D\data.ms
Ion 236.00 (235.70 to 236.70): BM046226.D\data.ms

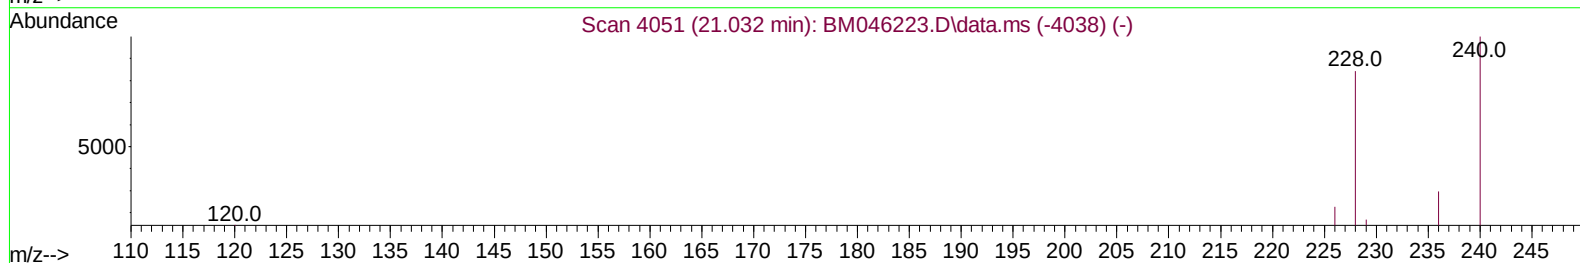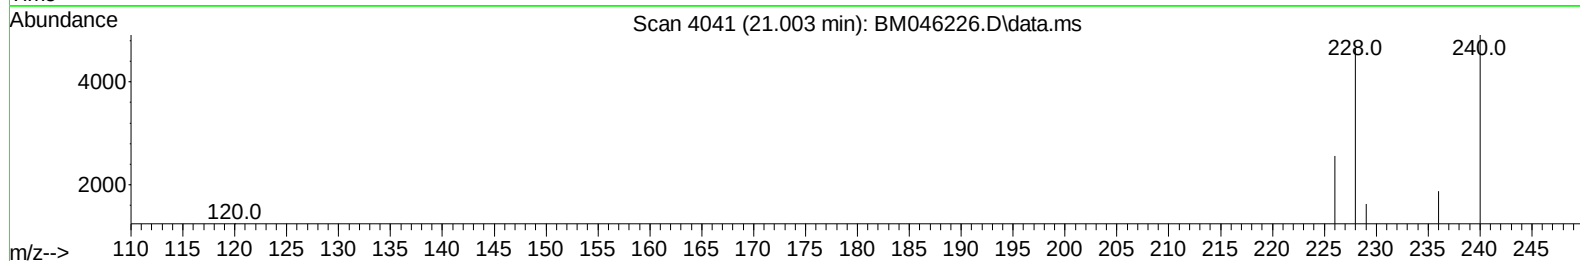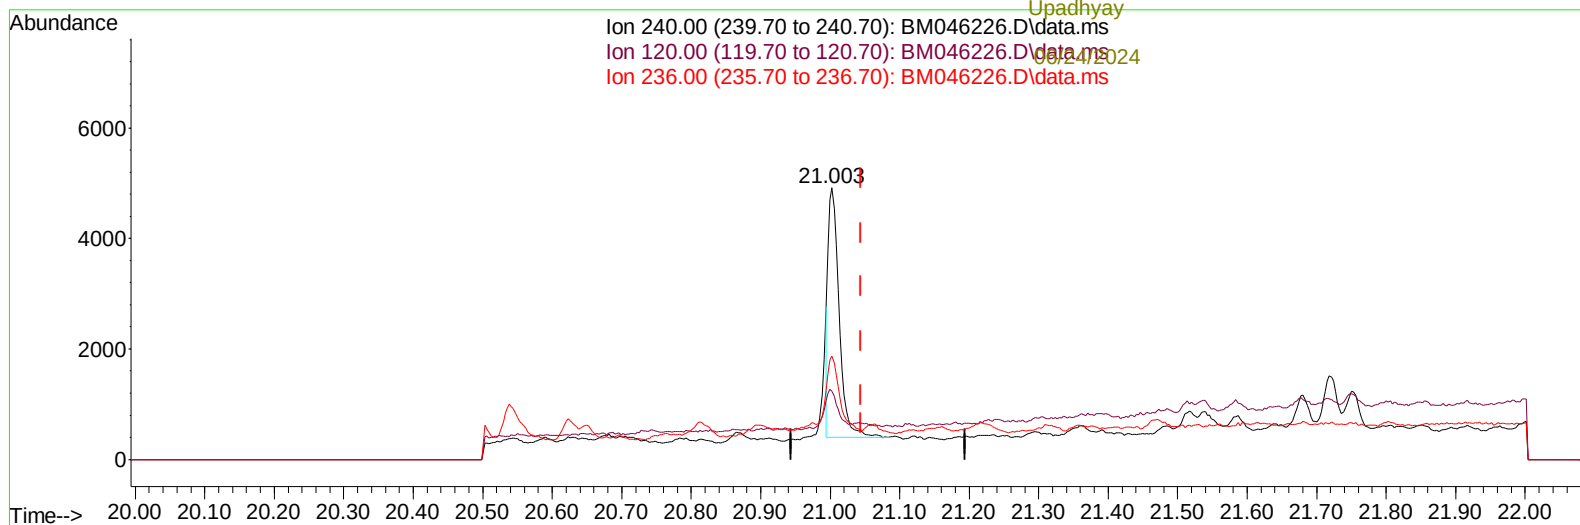

TIC: BM046226.D\data.ms

(17) Chrysene-d12

21.003min (-0.041) 0.40 ng/u1

response 4985

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	23.50	25.13
236.00	33.60	38.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 240.00 (239.70 to 240.70): BM046226.D\data.ms
Ion 120.00 (119.70 to 120.70): BM046226.D\data.ms
Ion 236.00 (235.70 to 236.70): BM046226.D\data.ms

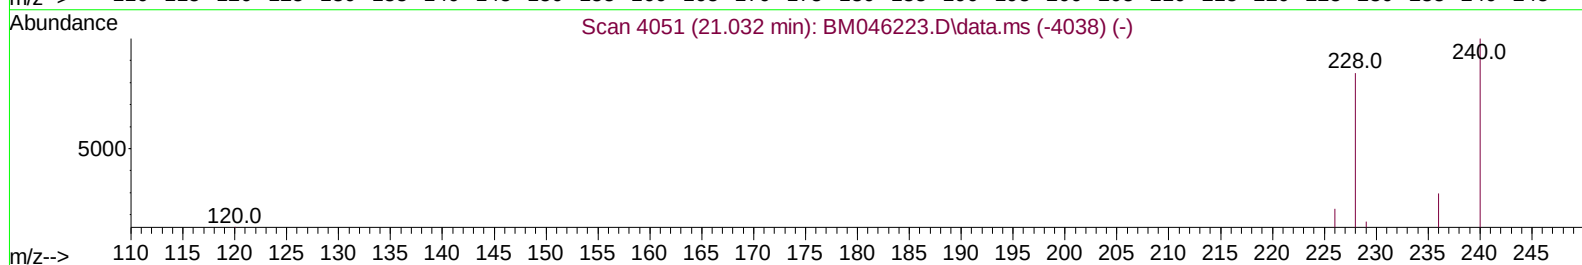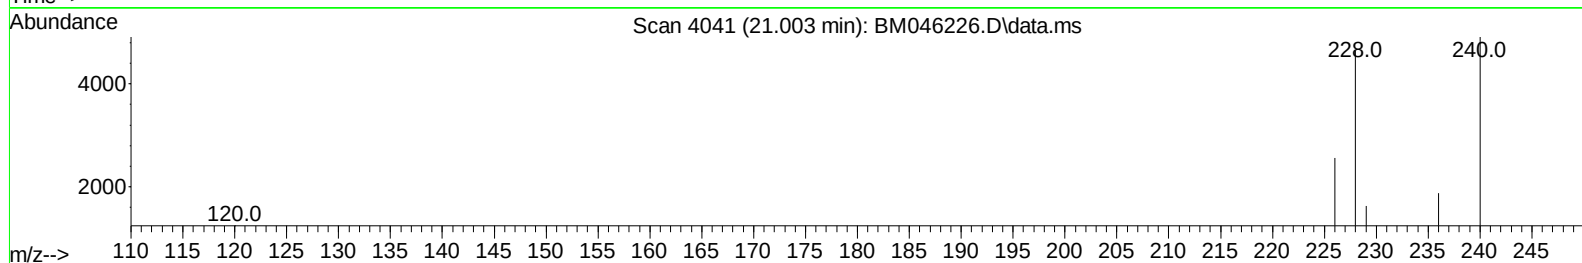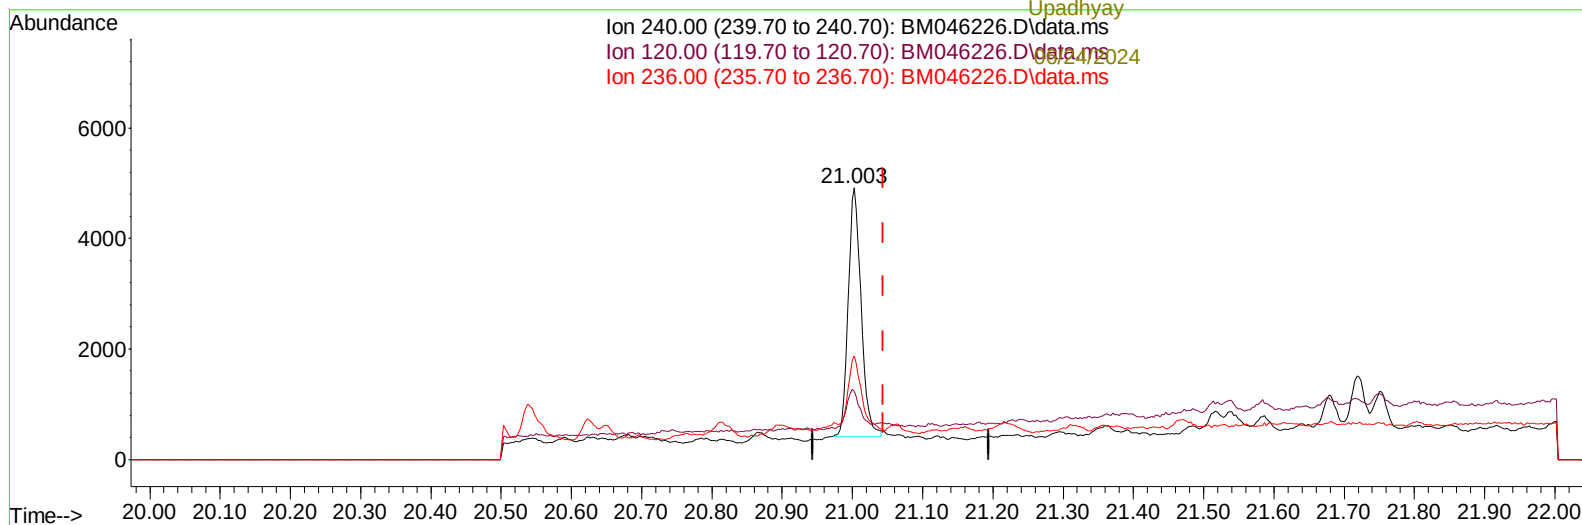

TIC: BM046226.D\data.ms

(17) Chrysene-d12

21.003min (-0.041) 0.40 ng/ul m

response 5741

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	23.50	25.13
236.00	33.60	38.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4C72

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay

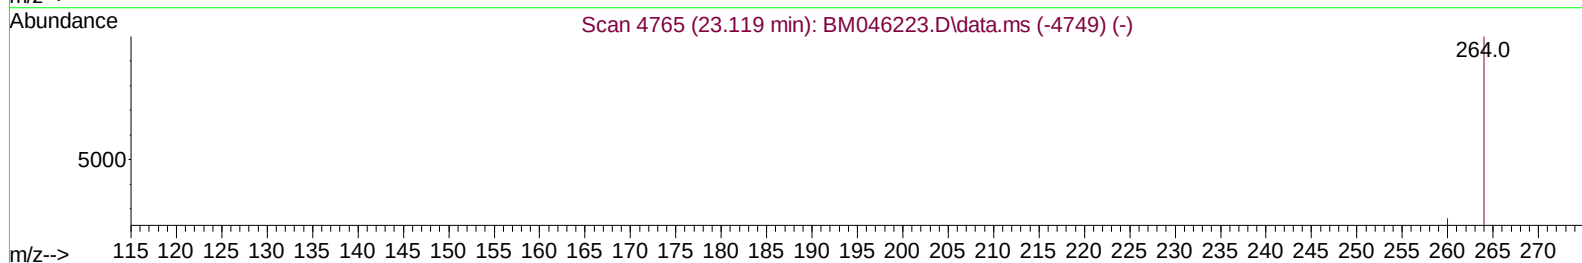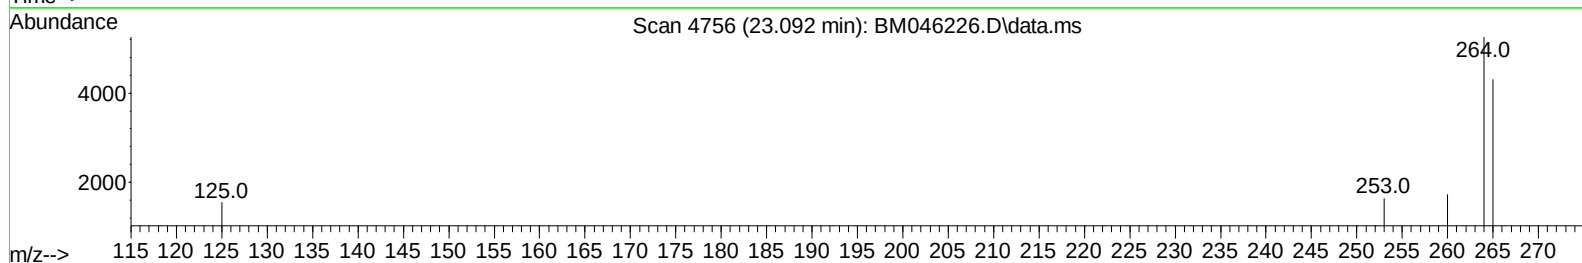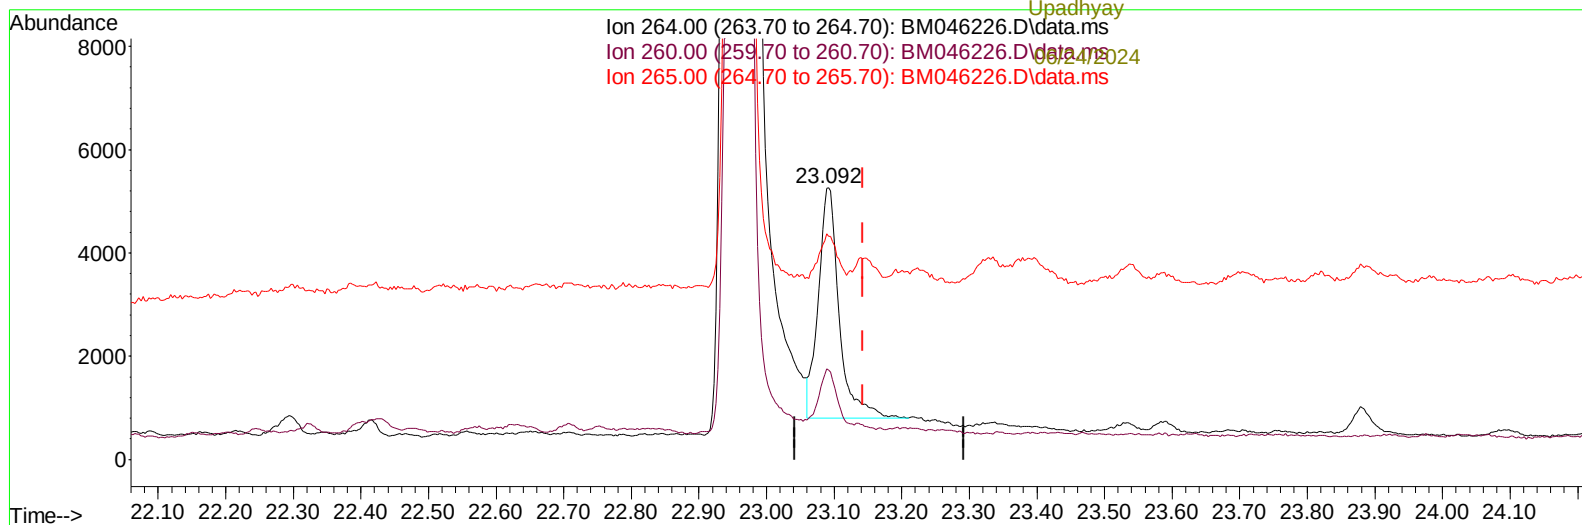

TIC: BM046226.D\data.ms

(23) Perylene-d12 (I)

23.092min (-0.050) 0.40 ng/u1

response 9516

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	32.80
265.00	110.60	82.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4C72

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

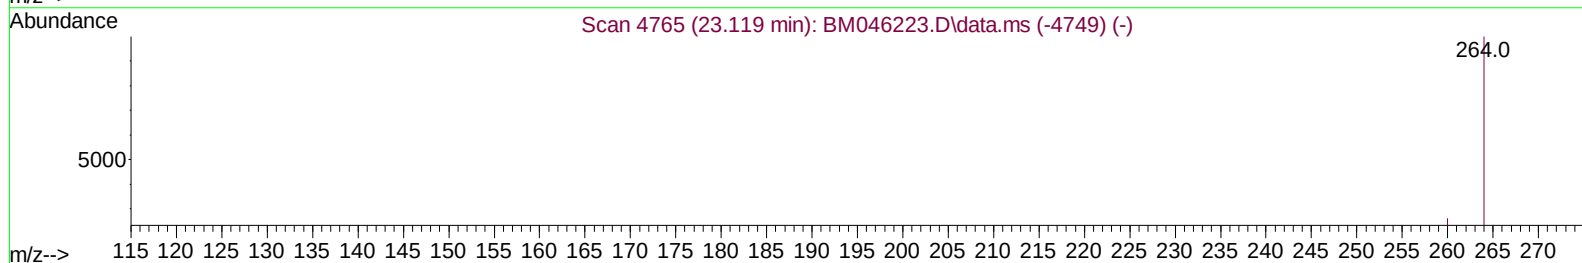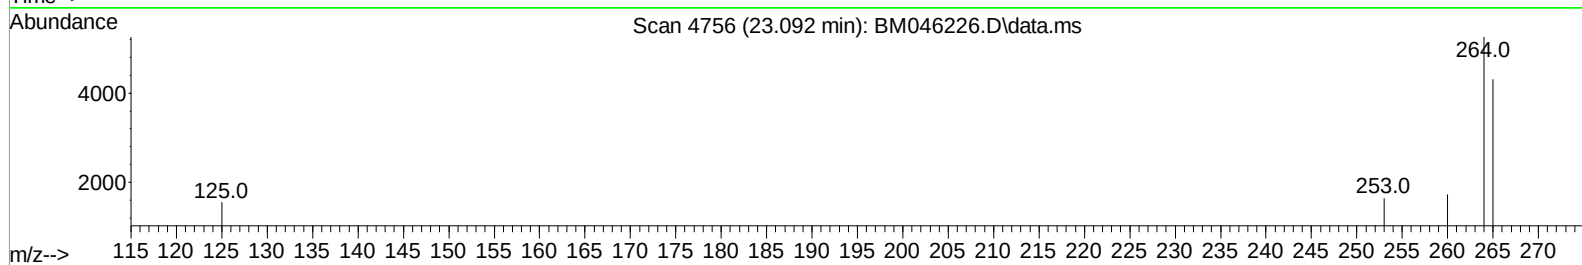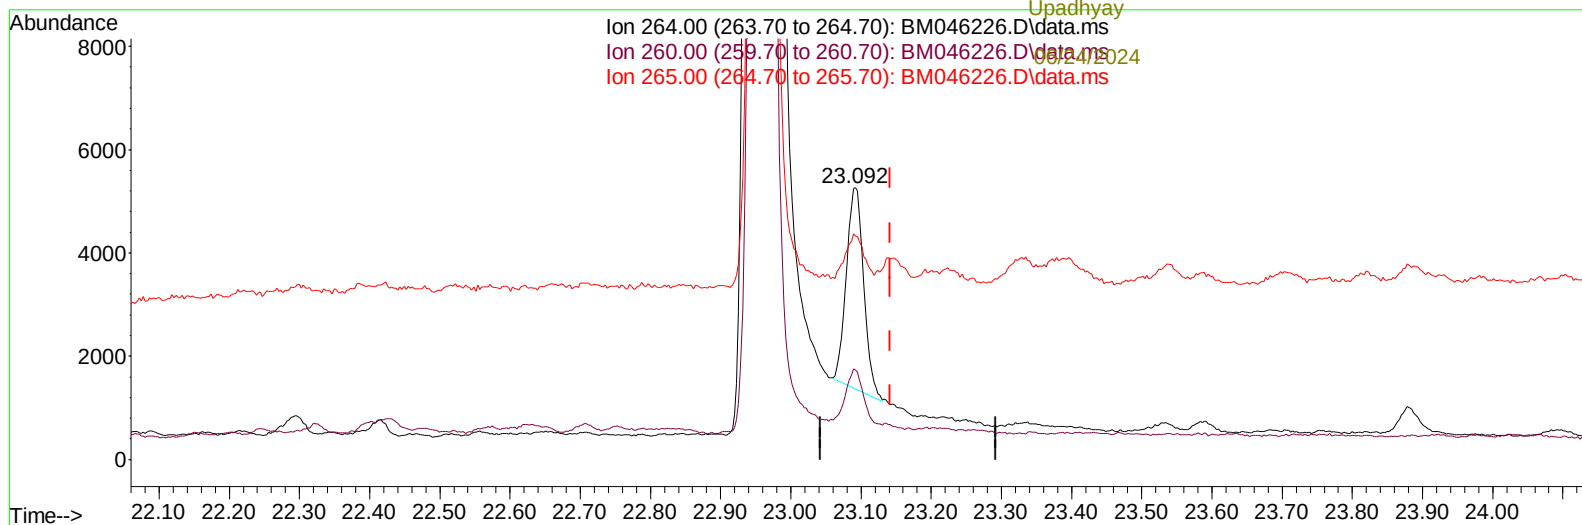

TIC: BM046226.D\data.ms

(23) Perylene-d12 (I)

23.092min (-0.050) 0.40 ng/ul m

response 6661

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	32.80
265.00	110.60	82.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72


Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024


Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay


Ion 252.00 (251.70 to 252.70): BM046226.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046226.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046226.D\data.ms

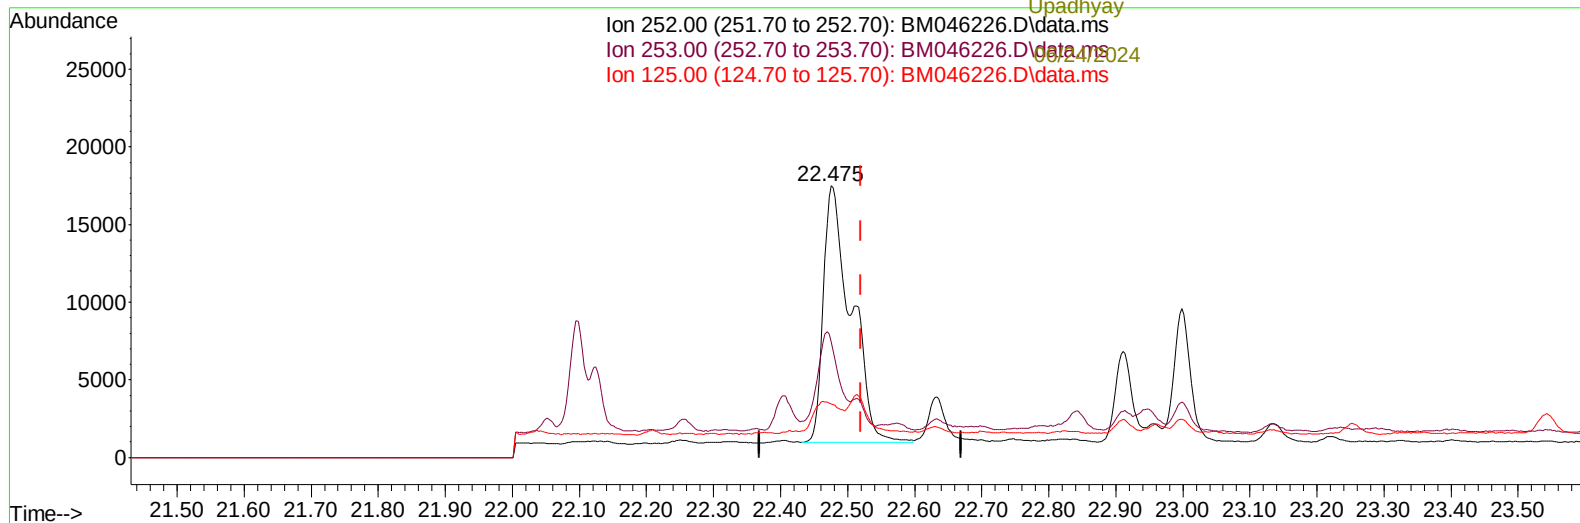

Scan 4545 (22.475 min): BM046226.D\data.ms

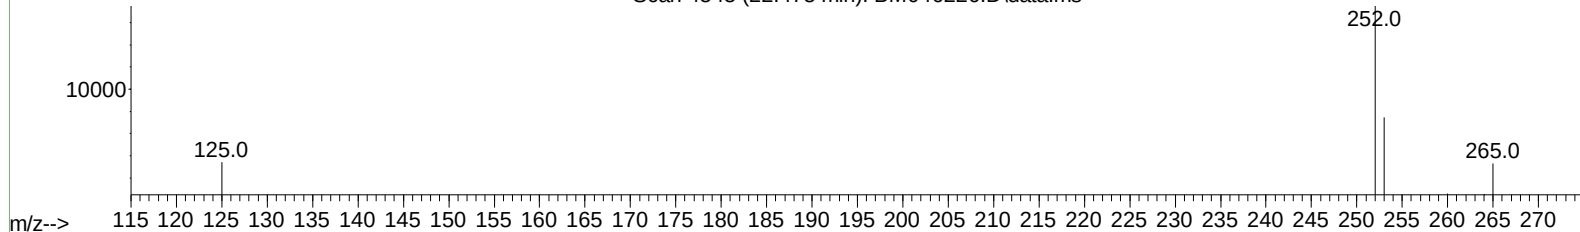

Scan 4554 (22.502 min): BM046223.D\data.ms (-4539) (-)

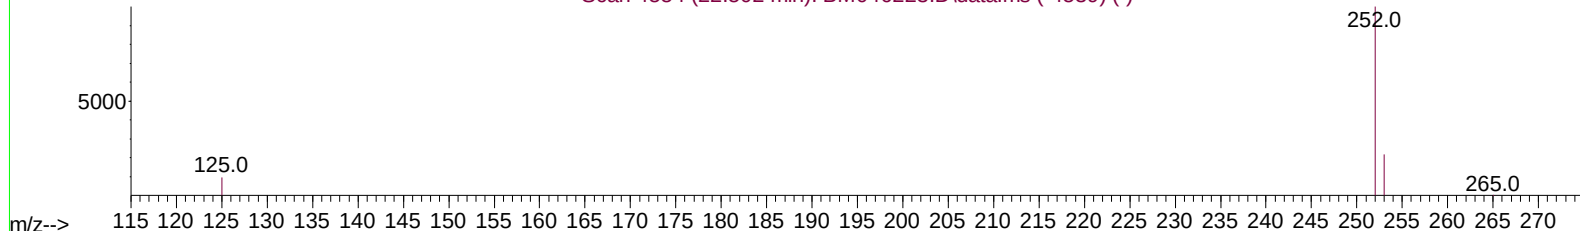

TIC: BM046226.D\data.ms

(24) Benzo(b)fluoranthene

22.475min (-0.044) 1.97 ng/u l

response 47174

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	42.58
125.00	20.10	19.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 252.00 (251.70 to 252.70): BM046226.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046226.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046226.D\data.ms

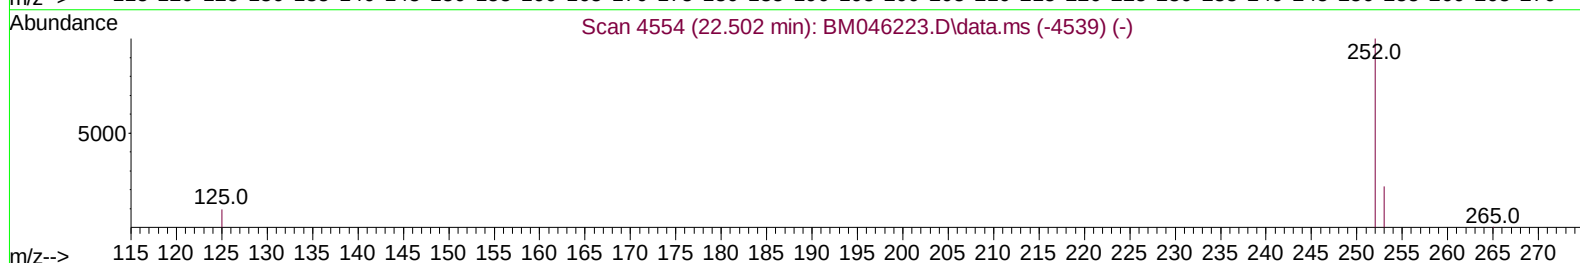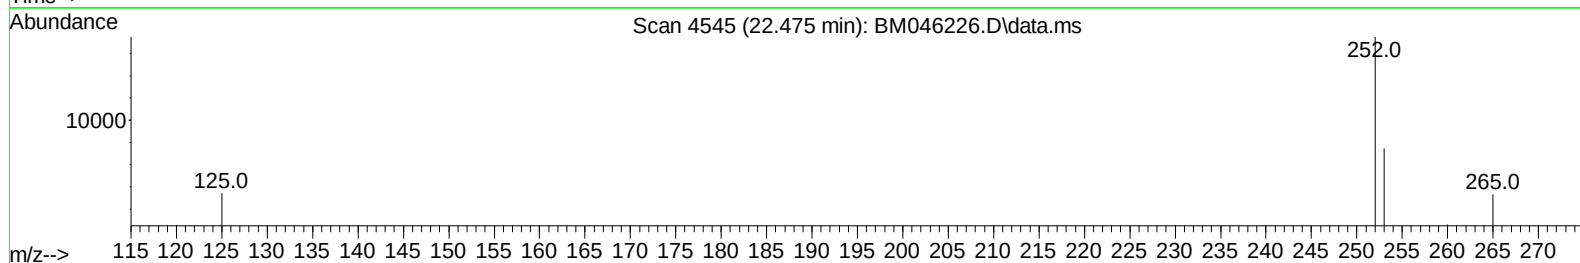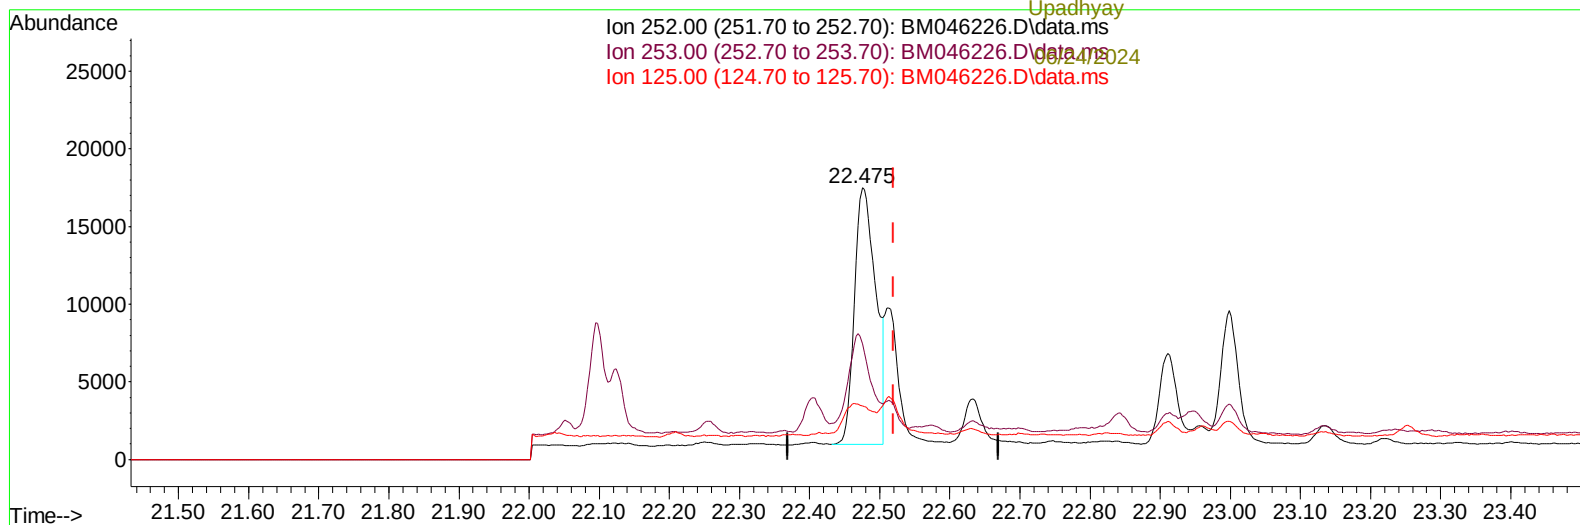

TIC: BM046226.D\data.ms

(24) Benzo(b)fluoranthene

22.475min (-0.044) 1.45 ng/ul m

response 34872

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	42.58
125.00	20.10	19.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 252.00 (251.70 to 252.70): BM046226.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046226.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046226.D\data.ms

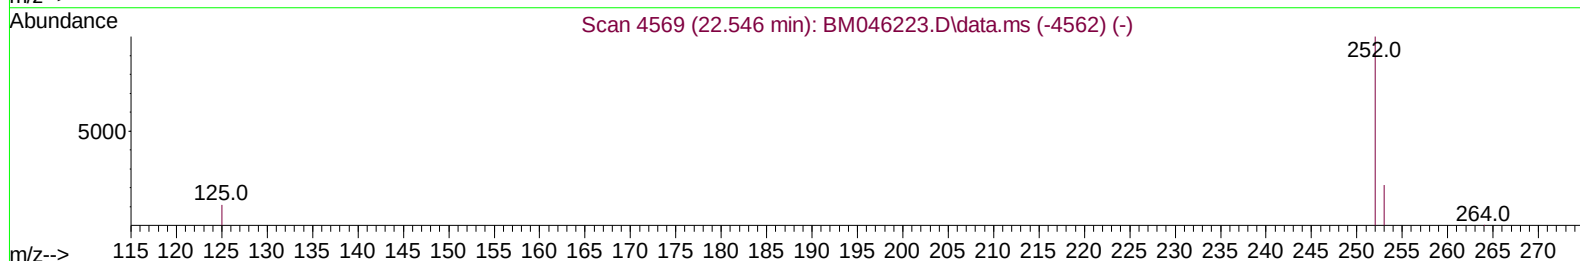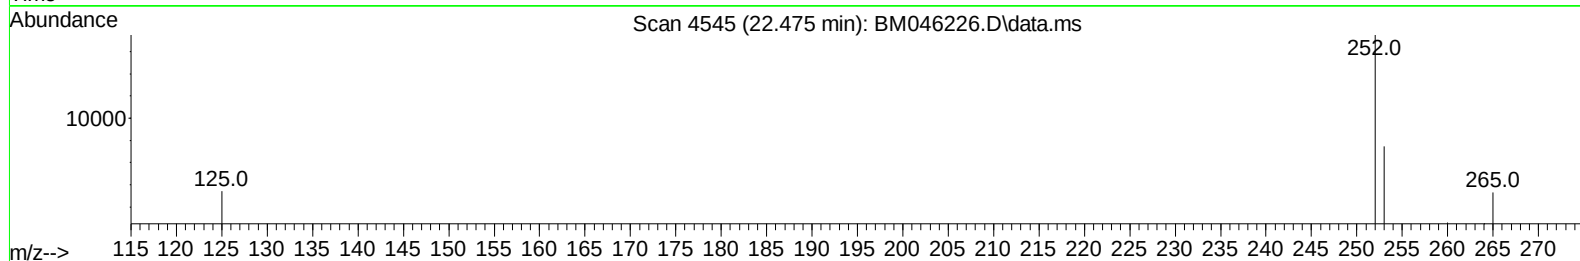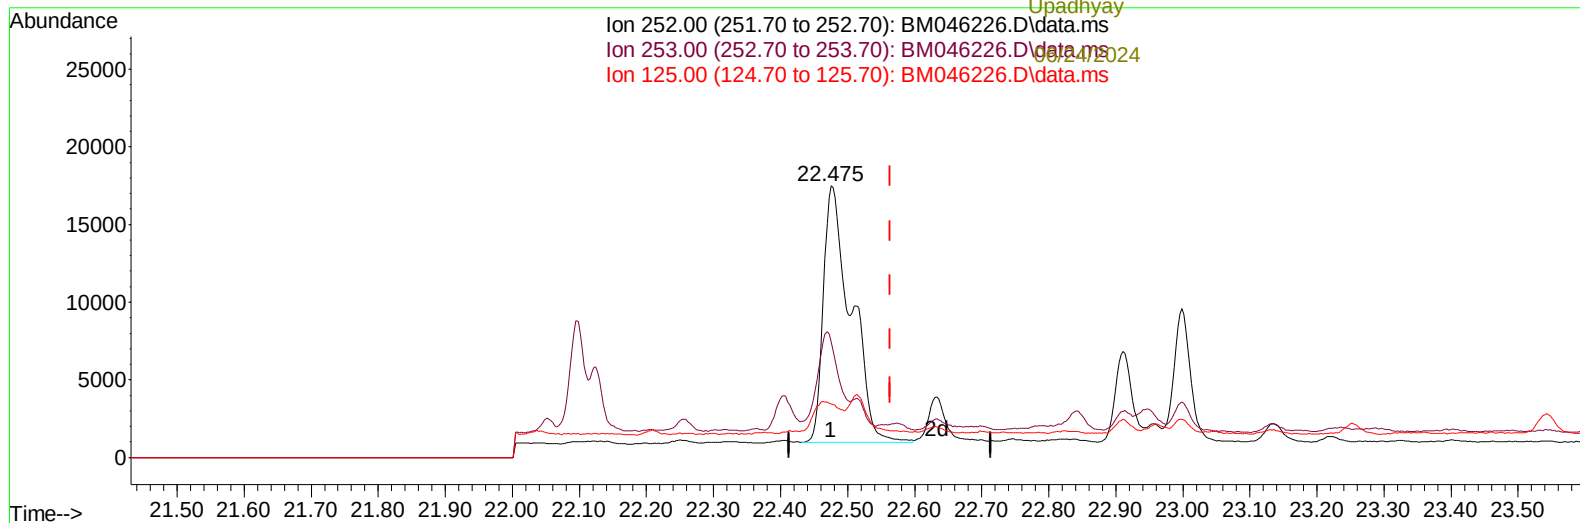

TIC: BM046226.D\data.ms

(25) Benzo(k)fluoranthene

22.475min (-0.088) 1.65 ng/u1

response 47174

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	42.58#
125.00	20.80	19.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 252.00 (251.70 to 252.70): BM046226.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046226.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046226.D\data.ms

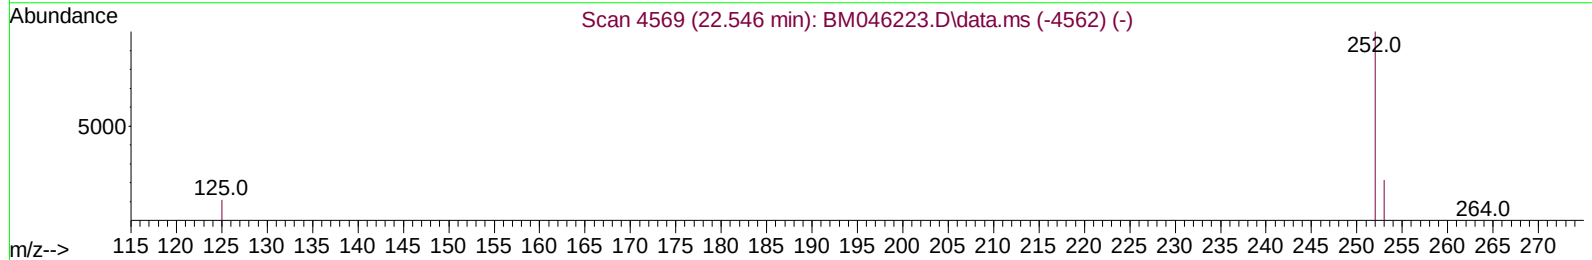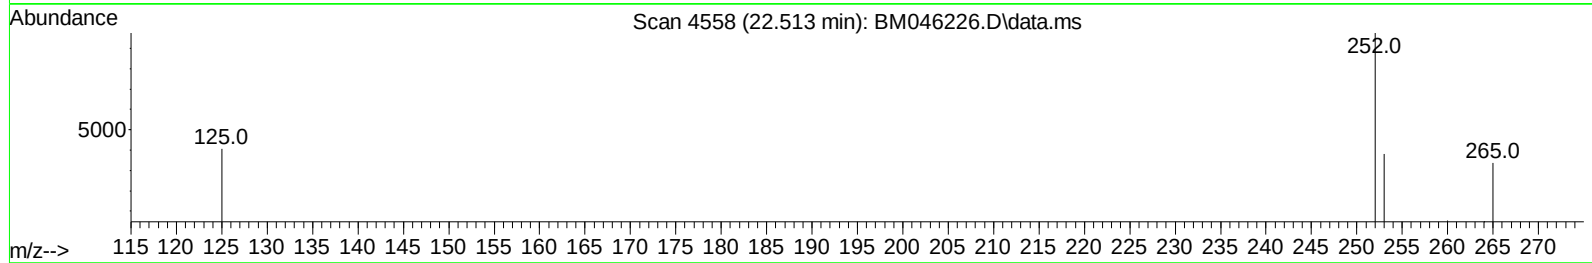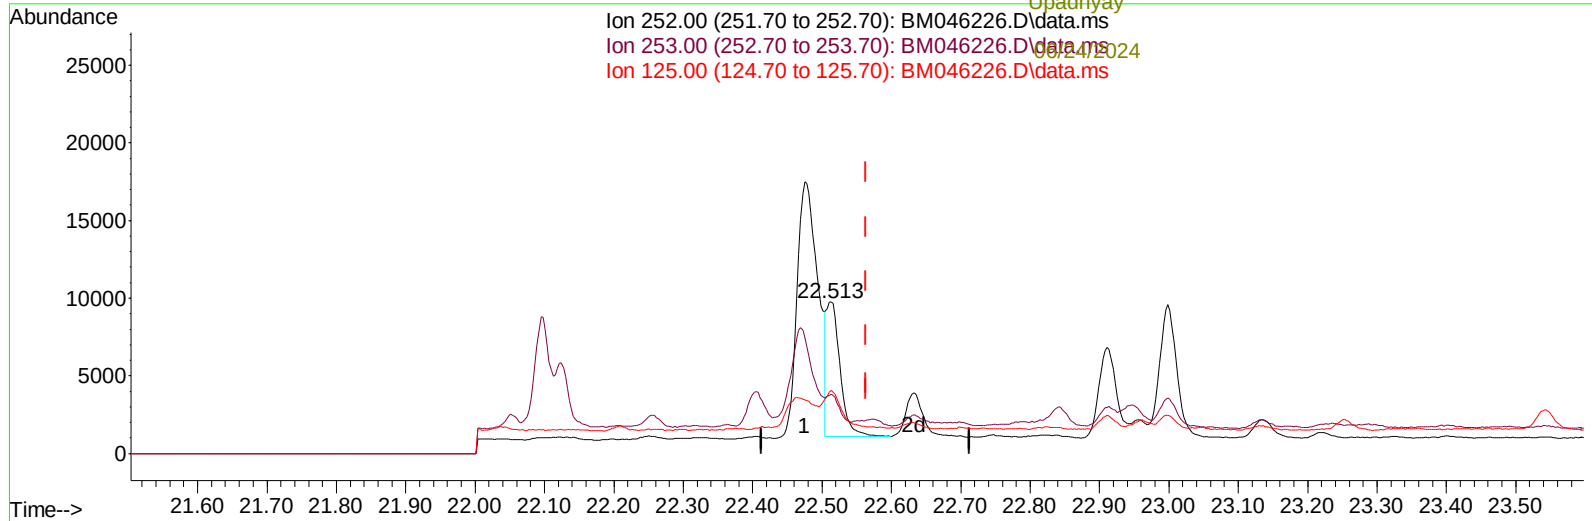

TIC: BM046226.D\data.ms

(25) Benzo(k)fluoranthene

22.513min (-0.050) 0.41 ng/ul m

response 11703

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	39.17
125.00	20.80	41.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
 Data File : BM046226.D
 Acq On : 23 Jun 2024 09:35
 Operator : MA/JU
 Sample : P2776-19
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4C72

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:29:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 02:25:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----06/24/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.409	152	1894	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.183	136	5723	0.400	ng/ul	-0.07
9) Acenaphthene-d10	14.058	164	3190	0.400	ng/ul	#-0.05
13) Phenanthrene-d10	16.799	188	6820m	0.400	ng/ul	-0.06
17) Chrysene-d12	21.003	240	5741m	0.400	ng/ul	-0.04
23) Perylene-d12	23.092	264	6661m	0.400	ng/ul	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.021	96	9599	3.694	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.811	152	2194	0.286	ng/ul	-0.05
18) Fluoranthene-d10	18.835	212	5321	0.309	ng/ul	-0.05
Target Compounds						
						Qvalue
5) Naphthalene	10.233	128	794	0.050	ng/ul#	72
7) 2-Methylnaphthalene	11.882	142	291	0.032	ng/ul	95
8) 1-Methylnaphthalene	12.097	142	237	0.024	ng/ul	90
10) Acenaphthylene	13.776	152	2597	0.172	ng/ul#	93
11) Acenaphthene	14.118	153	435	0.040	ng/ul	94
12) Fluorene	15.113	166	600	0.051	ng/ul#	95
15) Phenanthrene	16.842	178	13716m	0.716	ng/ul	
16) Anthracene	16.934	178	3345m	0.234	ng/ul	
19) Fluoranthene	18.863	202	40630	1.635	ng/ul	98
20) Pyrene	19.225	202	33994	1.265	ng/ul	99
21) Benzo(a)anthracene	20.985	228	20099	0.906	ng/ul	93
22) Chrysene	21.038	228	23951	0.846	ng/ul	94
24) Benzo(b)fluoranthene	22.475	252	34872m	1.453	ng/ul	
25) Benzo(k)fluoranthene	22.513	252	11703m	0.410	ng/ul	
26) Benzo(a)pyrene	22.998	252	14894	0.670	ng/ul	97
27) Indeno(1,2,3-cd)pyrene	25.128	276	14615	0.402	ng/ul#	96
28) Dibenzo(a,h)anthracene	25.135	278	4417	0.163	ng/ul#	40
29) Benzo(g,h,i)perylene	25.755	276	4593	0.147	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046226.D
Acq On : 23 Jun 2024 09:35
Operator : MA/JU
Sample : P2776-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C72

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

06/24/2024

Quant Time: Jun 24 02:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

