

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 188.00 (187.70 to 188.70): BM046233.D\data.ms
Ion 94.00 (93.70 to 94.70): BM046233.D\data.ms
Ion 80.00 (79.70 to 80.70): BM046233.D\data.ms

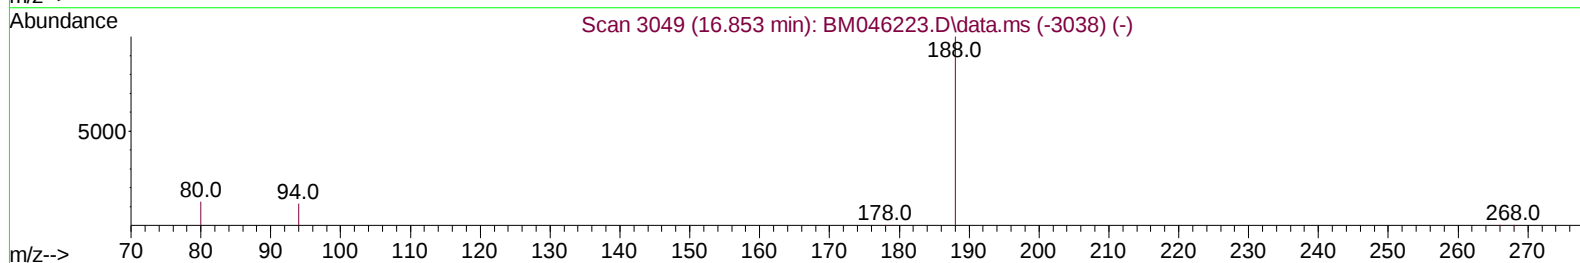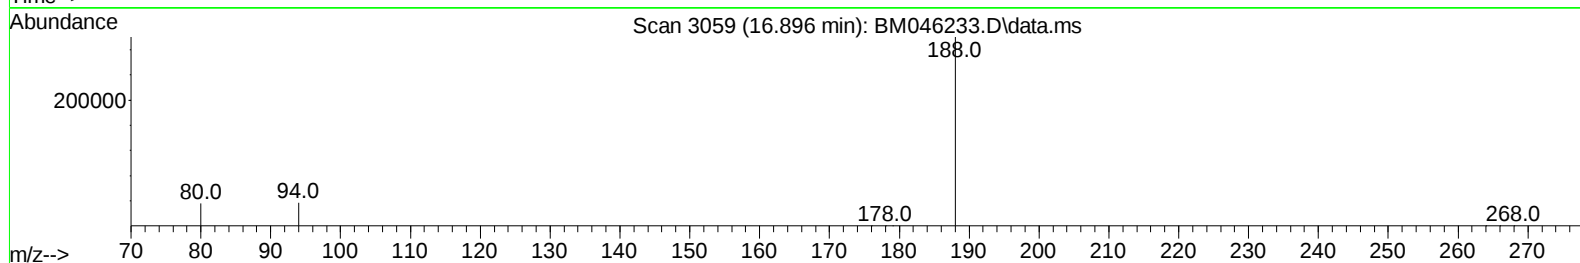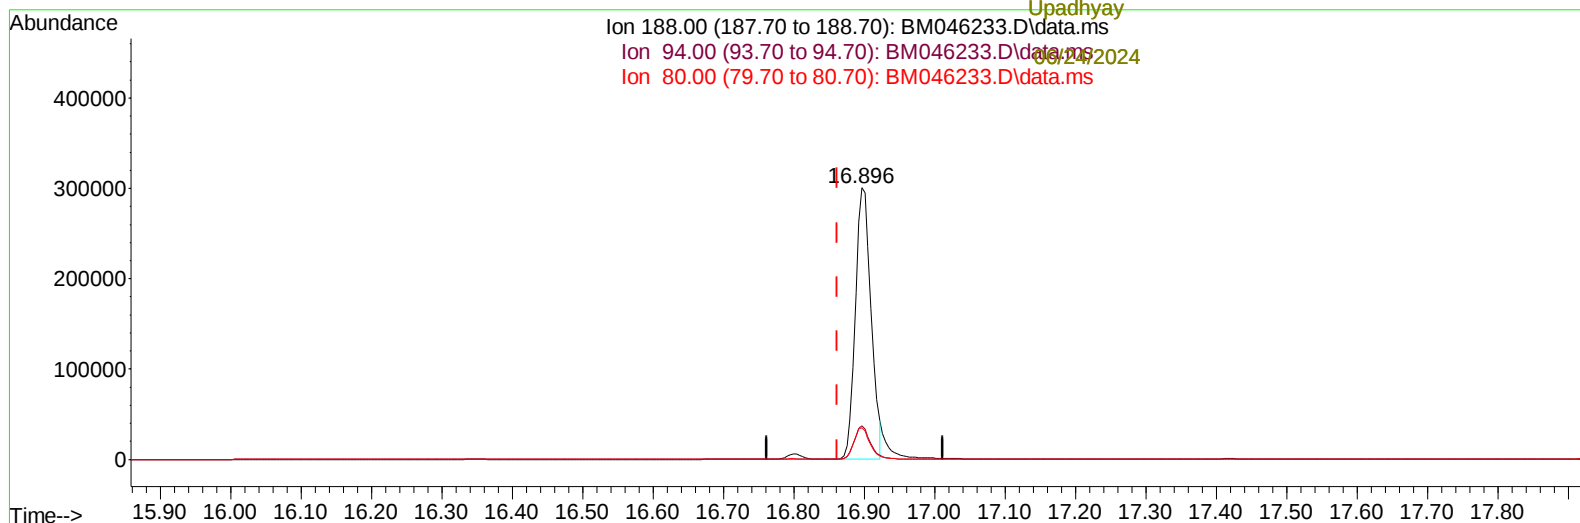

TIC: BM046233.D\data.ms

(13) Phenanthrene-d10 (I)**16.896min (+ 0.035) 0.40 ng/u1****response 461863**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	12.32
80.00	15.20	11.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4CA9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

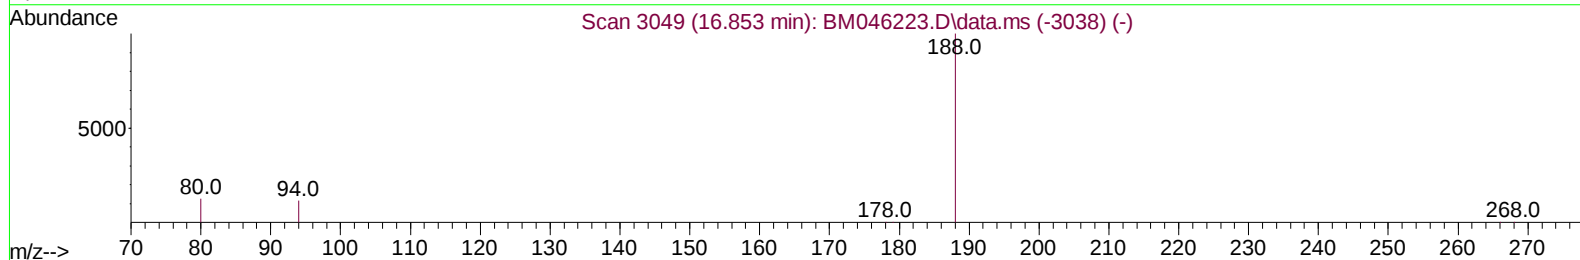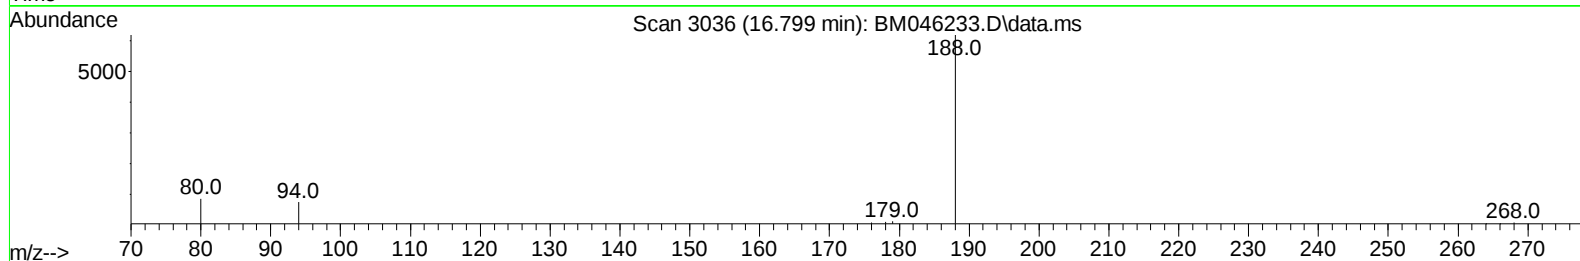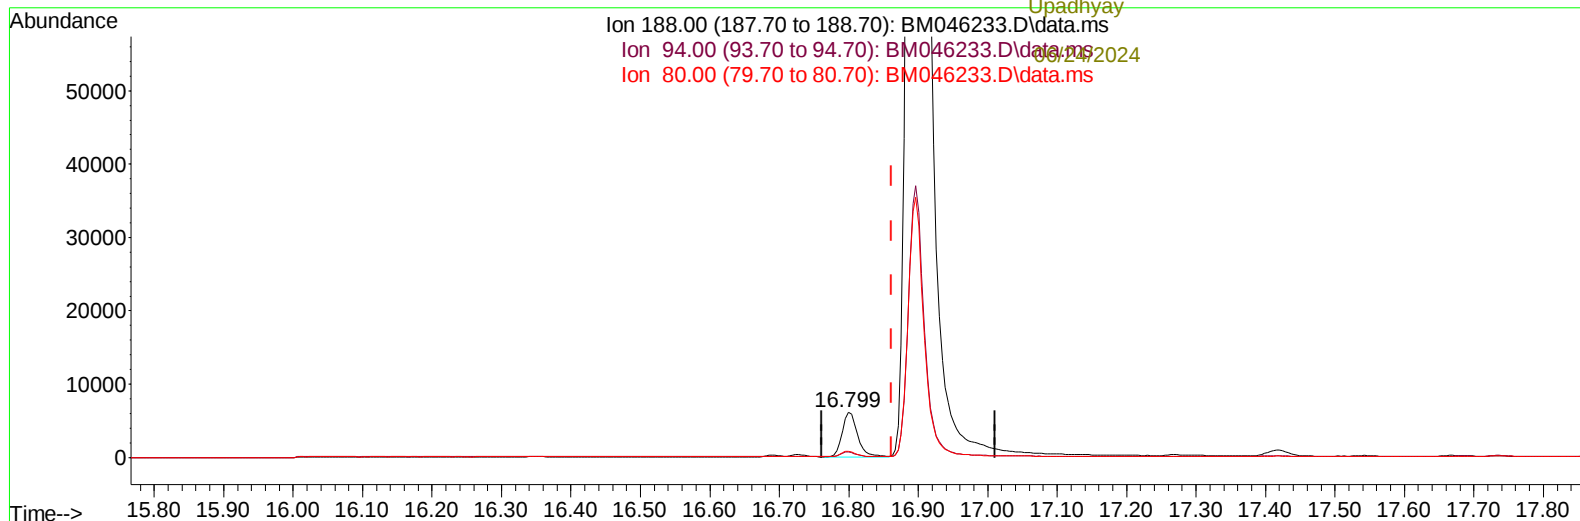

TIC: BM046233.D\data.ms

(13) Phenanthrene-d10 (I)

16.799min (-0.062) 0.40 ng/u1 m

response 9332

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	12.25
80.00	15.20	13.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4CA9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

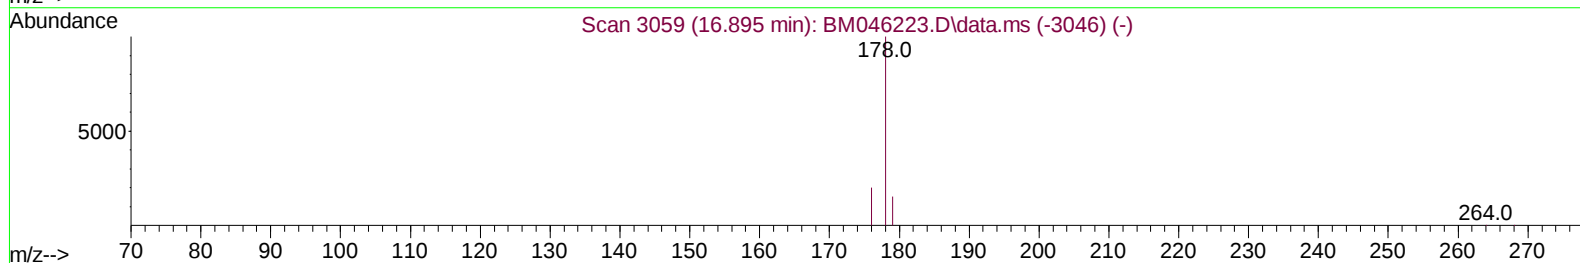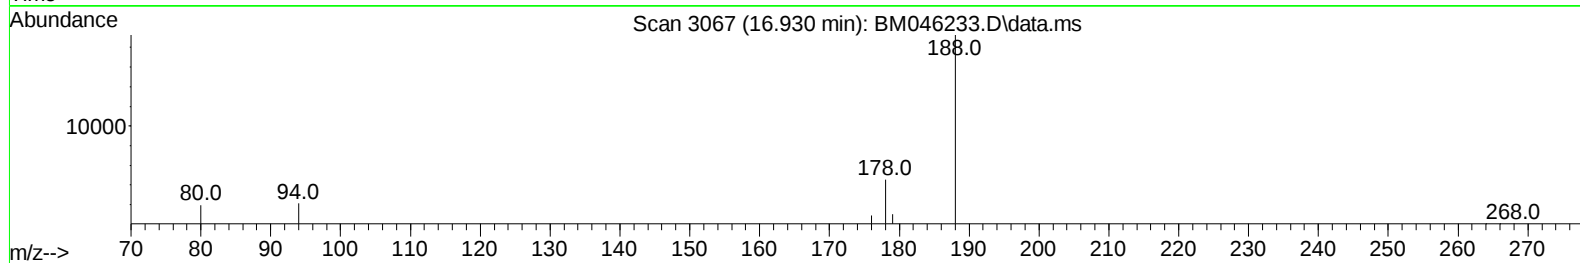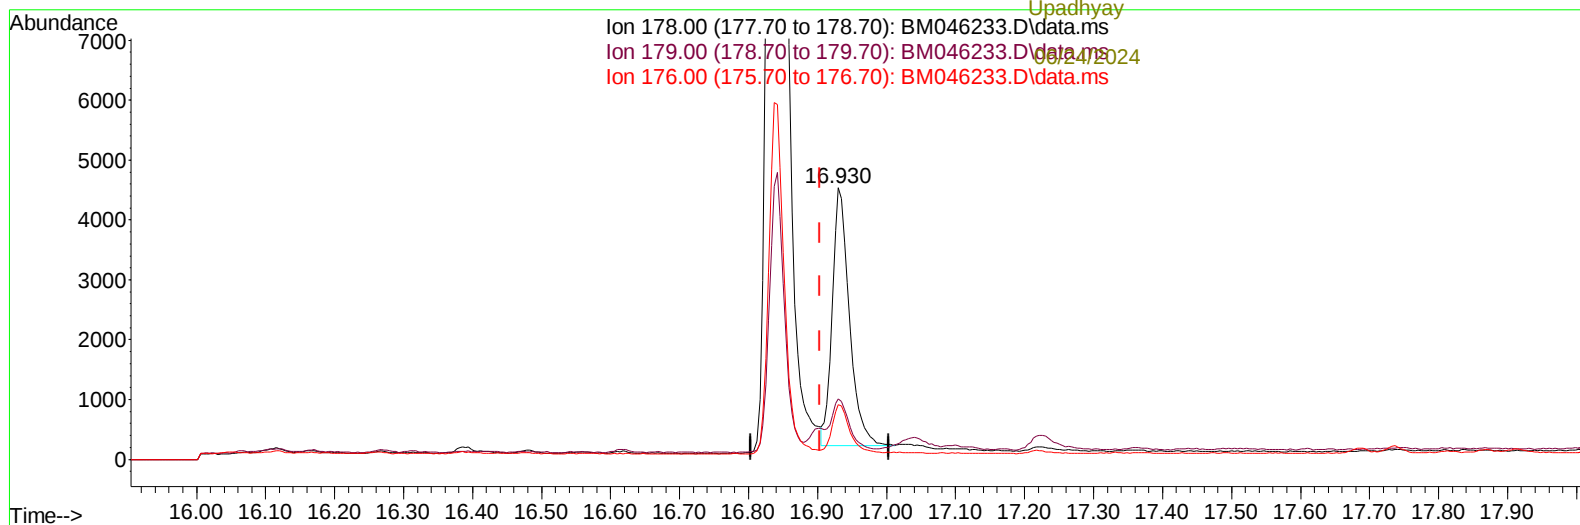

TIC: BM046233.D\data.ms

(15) Phenanthrene

16.930min (+ 0.027) 0.28 ng/u1

response 7387

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	22.36#
176.00	21.40	20.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9


Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration


Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay


Ion 178.00 (177.70 to 178.70): BM046233.D\data.ms
Ion 179.00 (178.70 to 179.70): BM046233.D\data.ms
Ion 176.00 (175.70 to 176.70): BM046233.D\data.ms

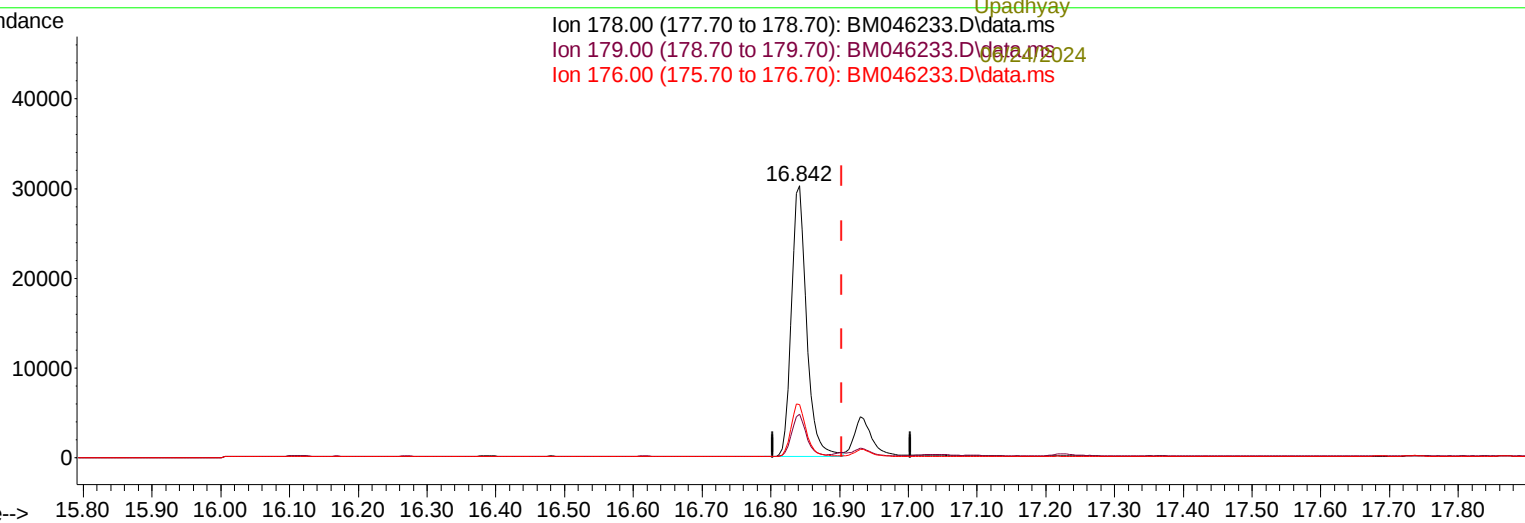

Scan 3046 (16.842 min): BM046233.D\data.ms

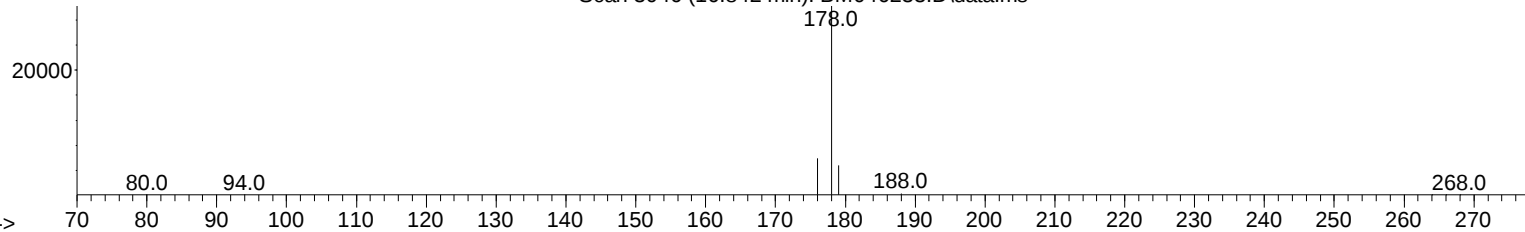

Scan 3059 (16.895 min): BM046223.D\data.ms (-3046) (-)

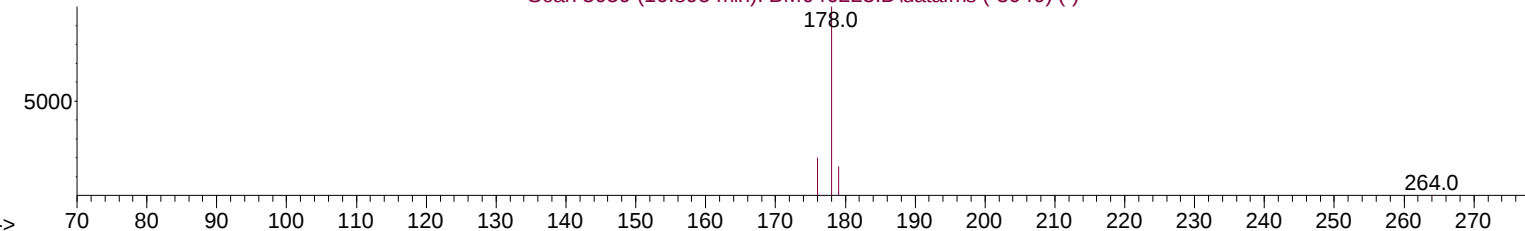

TIC: BM046233.D\data.ms

(15) Phenanthrene

16.842min (-0.062) 1.78 ng/u1 m

response 46576

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	15.82
176.00	21.40	19.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 178.00 (177.70 to 178.70): BM046233.D\data.ms
Ion 179.00 (178.70 to 179.70): BM046233.D\data.ms
Ion 176.00 (175.70 to 176.70): BM046233.D\data.ms

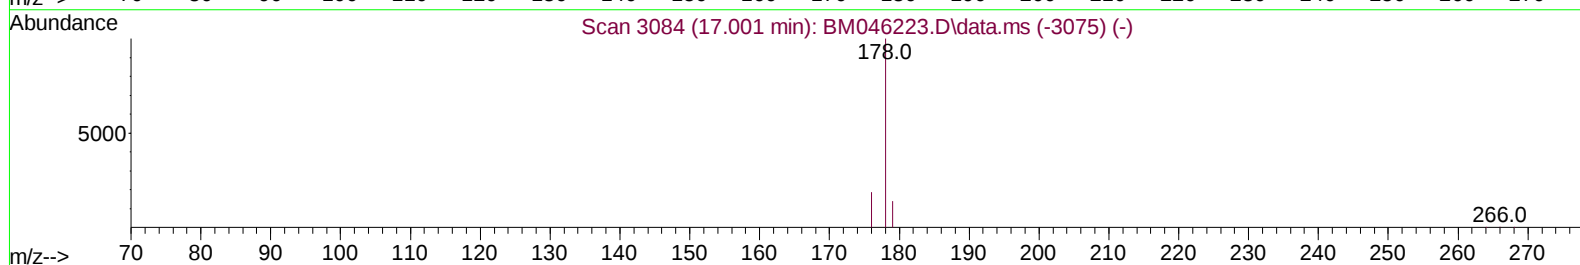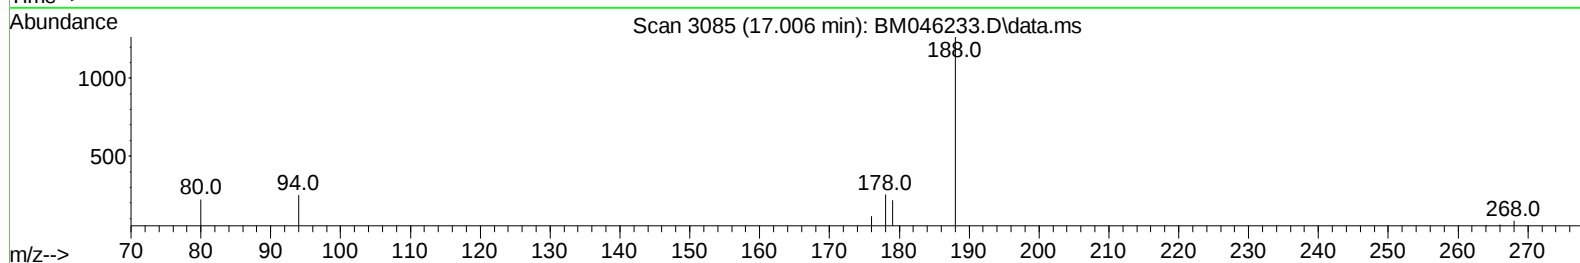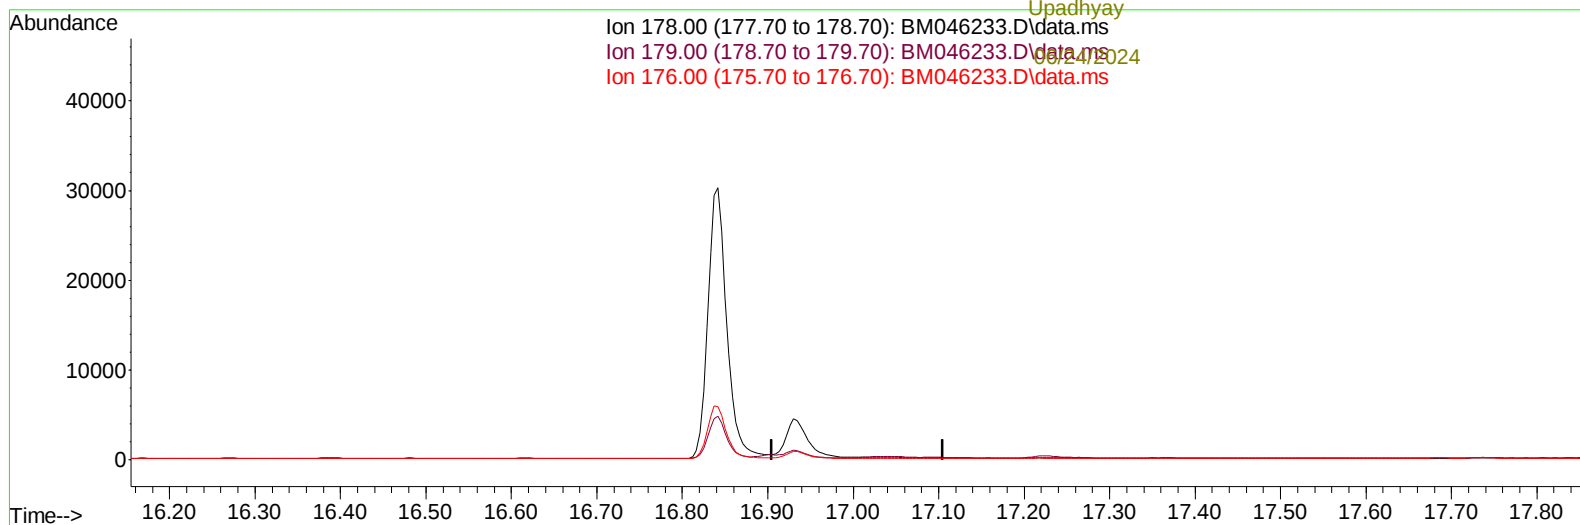

TIC: BM046233.D\data.ms

(16) Anthracene

17.005min (-17.005) 0.00 ng/u1

response 0

Ion	Exp%	Act%
178.00	100.00	0.00
179.00	18.60	0.00#
176.00	21.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4CA9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

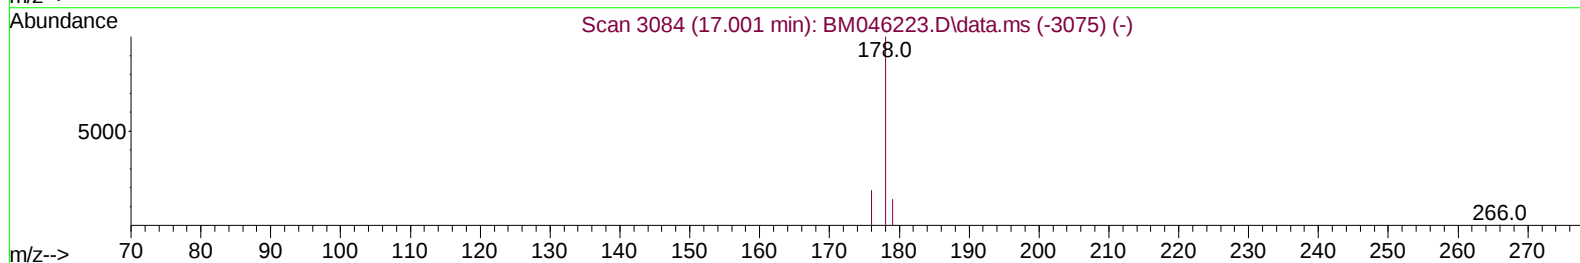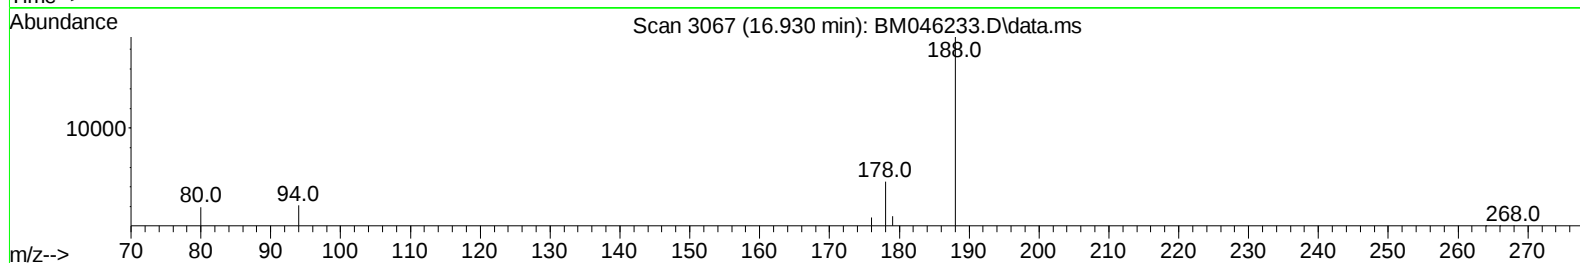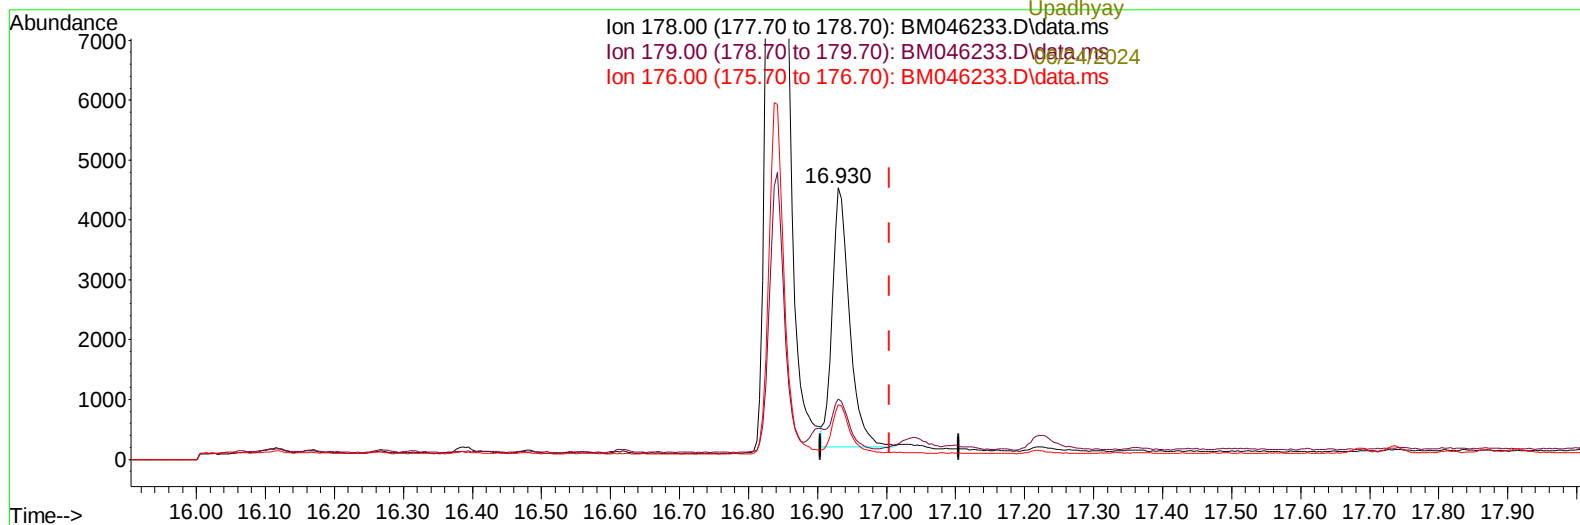

TIC: BM046233.D\data.ms

(16) Anthracene

16.930min (-0.075) 0.38 ng/ul m

response 7494

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.60	22.36#
176.00	21.20	20.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9


Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration


Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay


Ion 240.00 (239.70 to 240.70): BM046233.D\data.ms
Ion 120.00 (119.70 to 120.70): BM046233.D\data.ms
Ion 236.00 (235.70 to 236.70): BM046233.D\data.ms

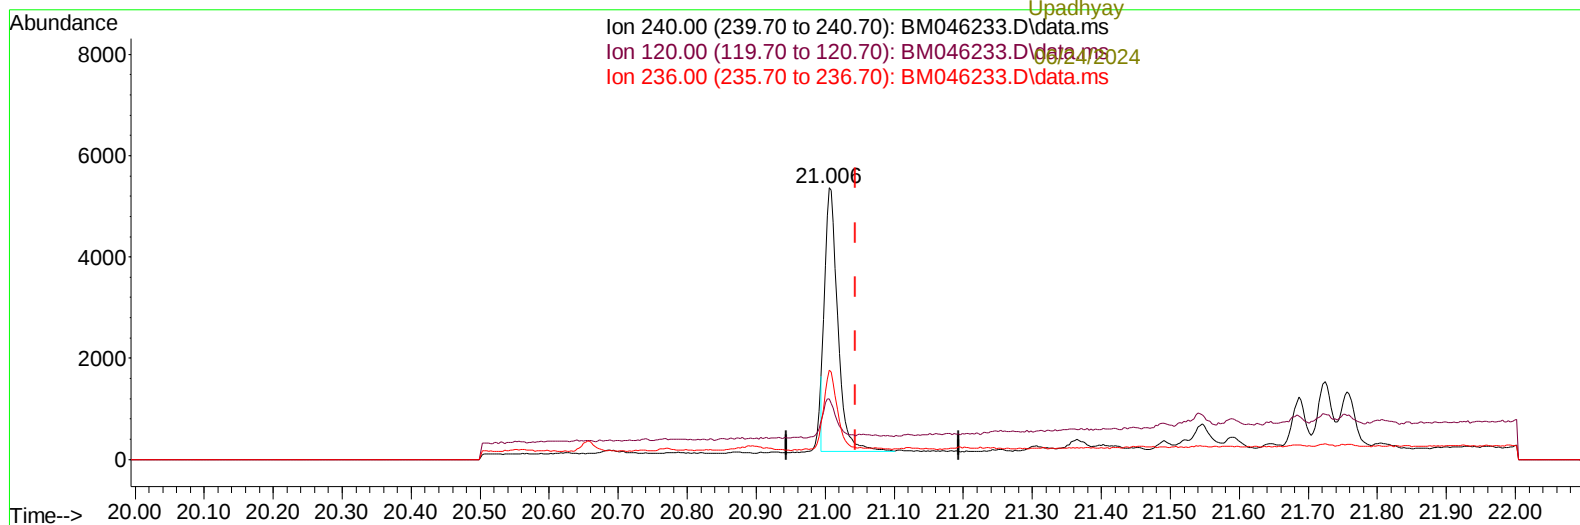

Scan 4042 (21.006 min): BM046233.D\data.ms

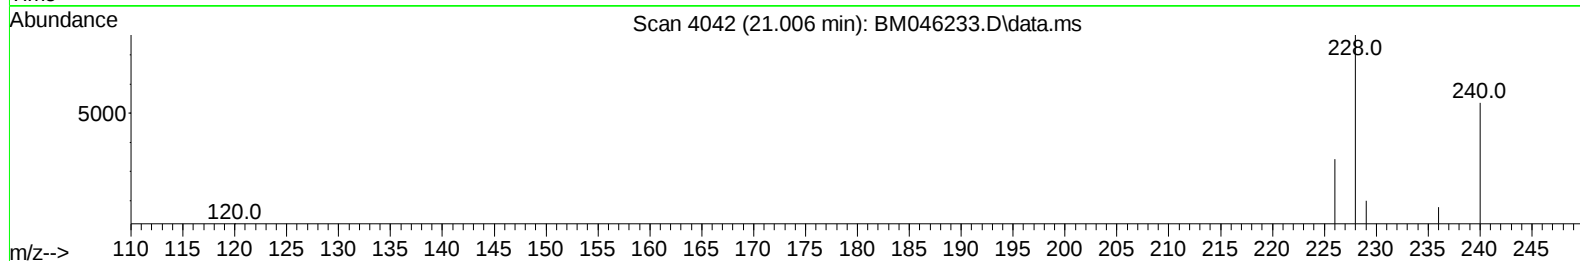

Scan 4051 (21.032 min): BM046223.D\data.ms (-4038) (-)

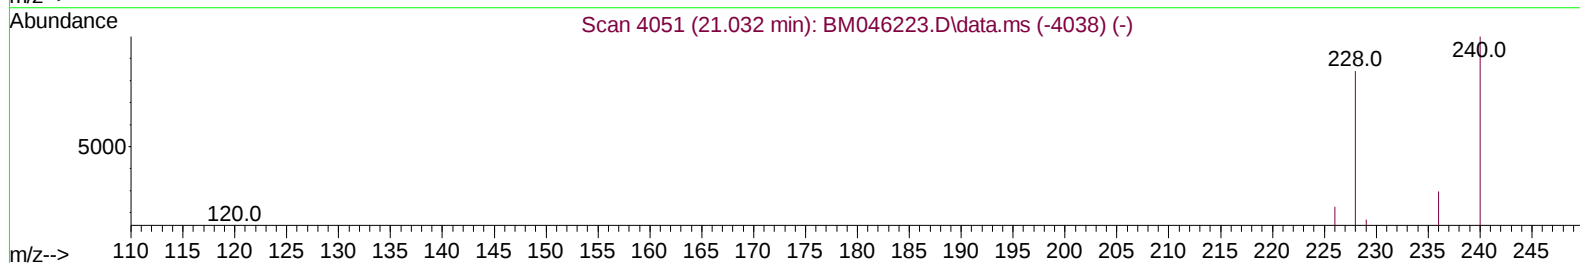

TIC: BM046233.D\data.ms

(17) Chrysene-d12

21.006min (-0.038) 0.40 ng/u1

response 6870

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	23.50	22.41
236.00	33.60	32.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9


Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration


Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay


Ion 240.00 (239.70 to 240.70): BM046233.D\data.ms
Ion 120.00 (119.70 to 120.70): BM046233.D\data.ms
Ion 236.00 (235.70 to 236.70): BM046233.D\data.ms

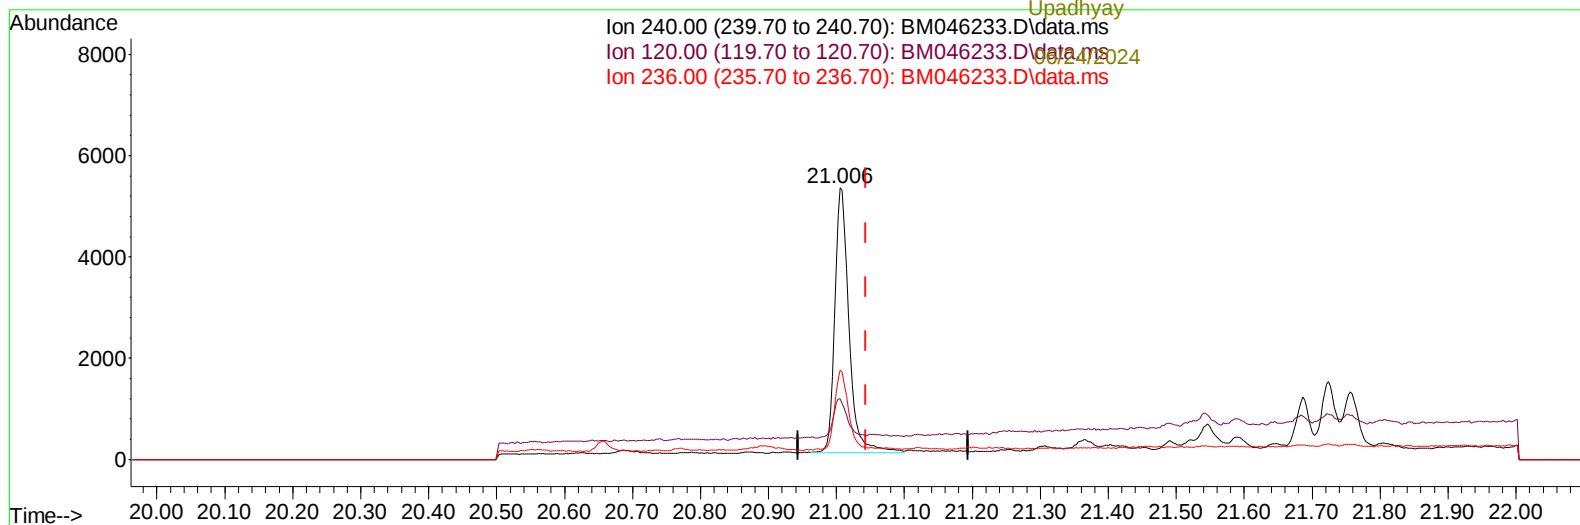

Scan 4042 (21.006 min): BM046233.D\data.ms

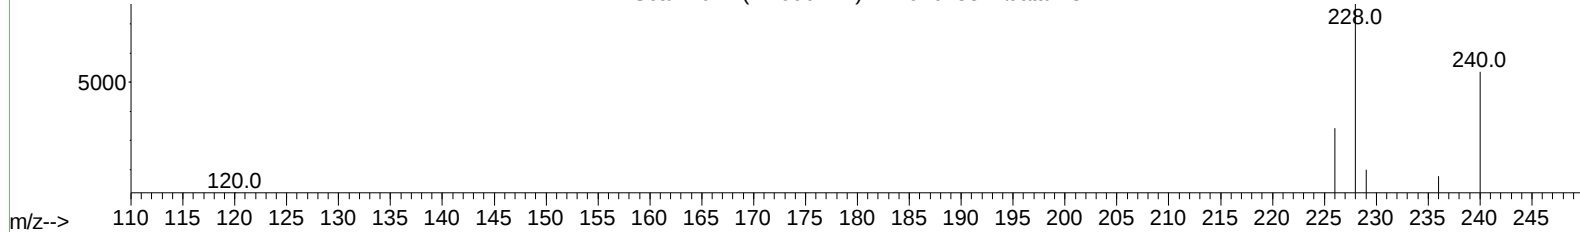

Scan 4051 (21.032 min): BM046223.D\data.ms (-4038) (-)

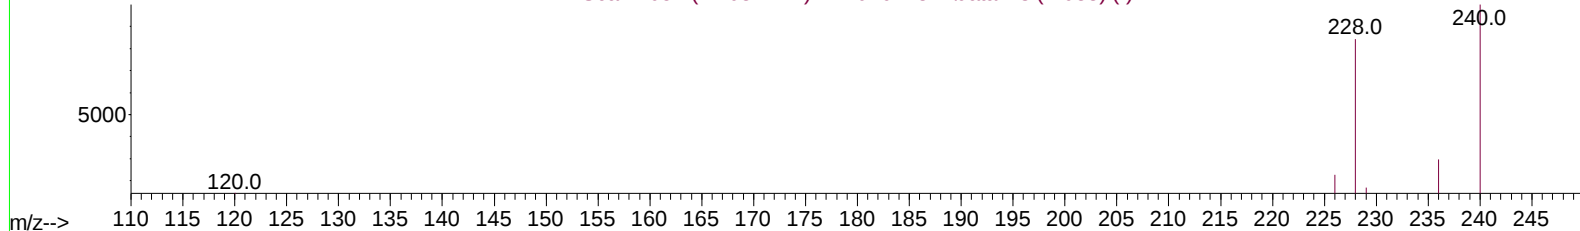

TIC: BM046233.D\data.ms

(17) Chrysene-d12

21.006min (-0.038) 0.40 ng/u1 m

response 7548

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	23.50	22.41
236.00	33.60	32.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4CA9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay

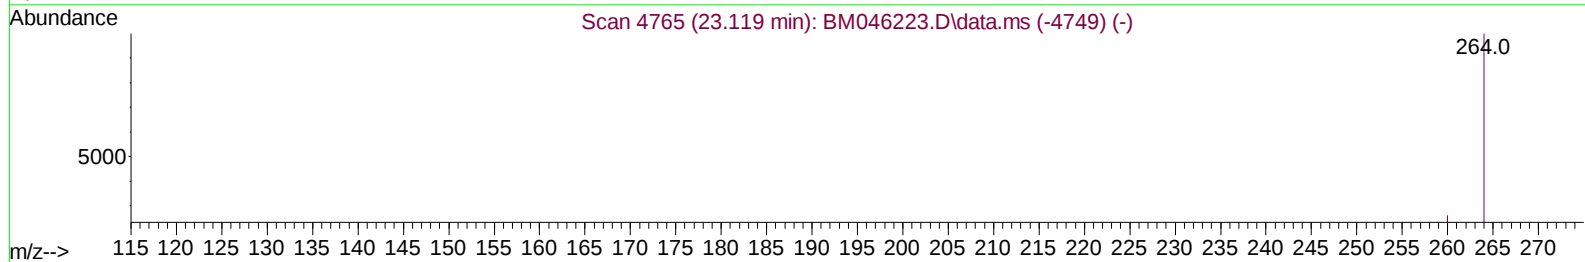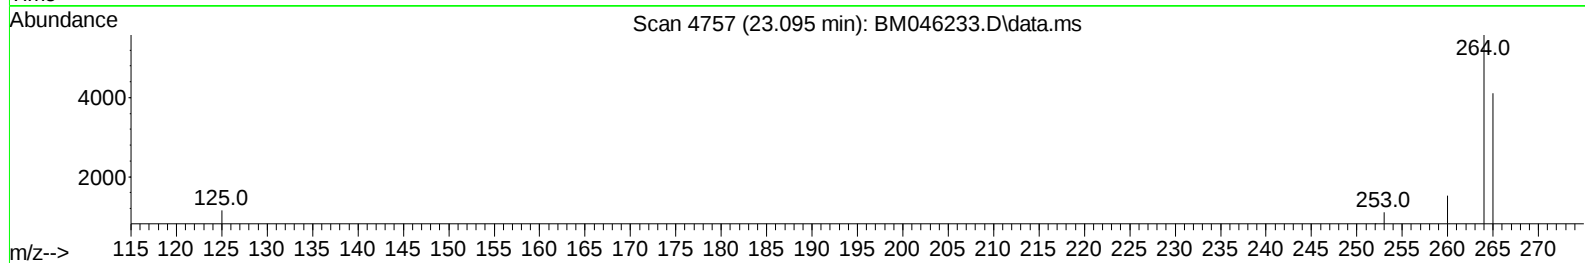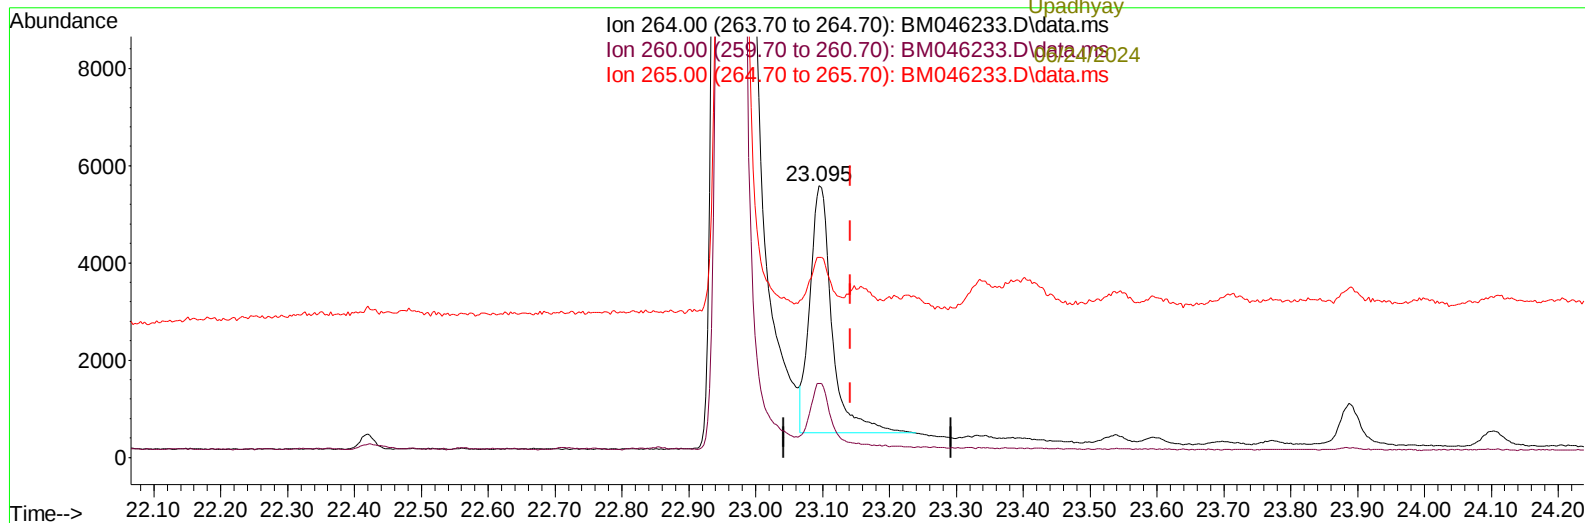

TIC: BM046233.D\data.ms

(23) Perylene-d12 (I)

23.095min (-0.047) 0.40 ng/u1

response 11641

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	27.23
265.00	110.60	73.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4CA9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

06/24/2024
Supervised By :Jagrut
Upadhyay

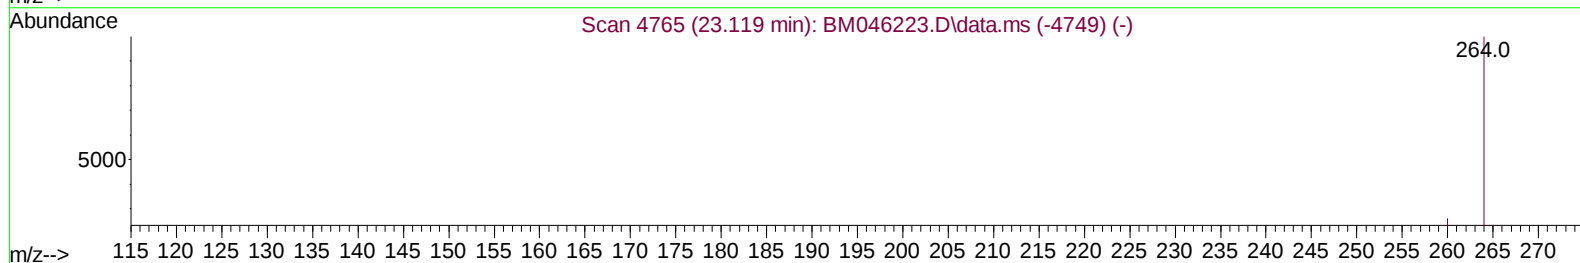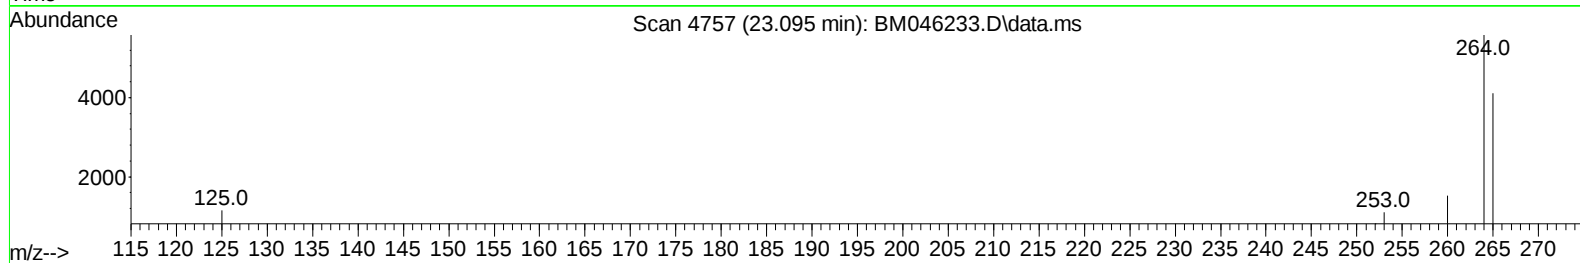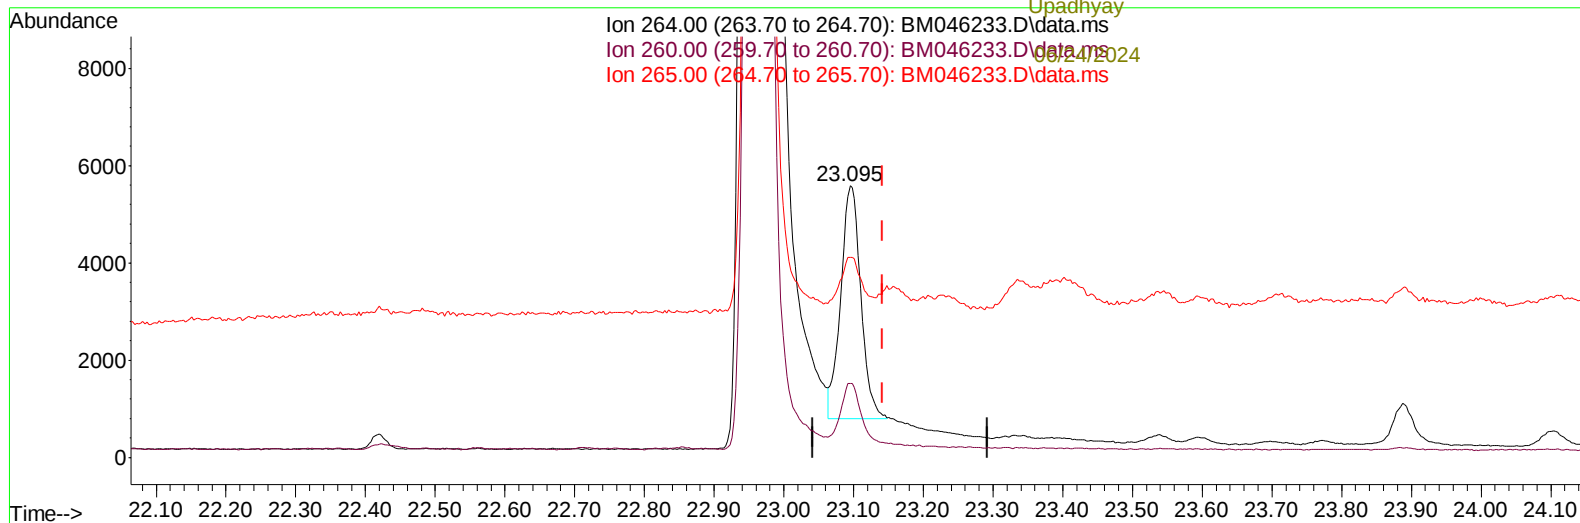

TIC: BM046233.D\data.ms

(23) Perylene-d12 (I)

23.095min (-0.047) 0.40 ng/ul m

response 9596

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	27.23
265.00	110.60	73.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 252.00 (251.70 to 252.70): BM046233.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046233.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046233.D\data.ms

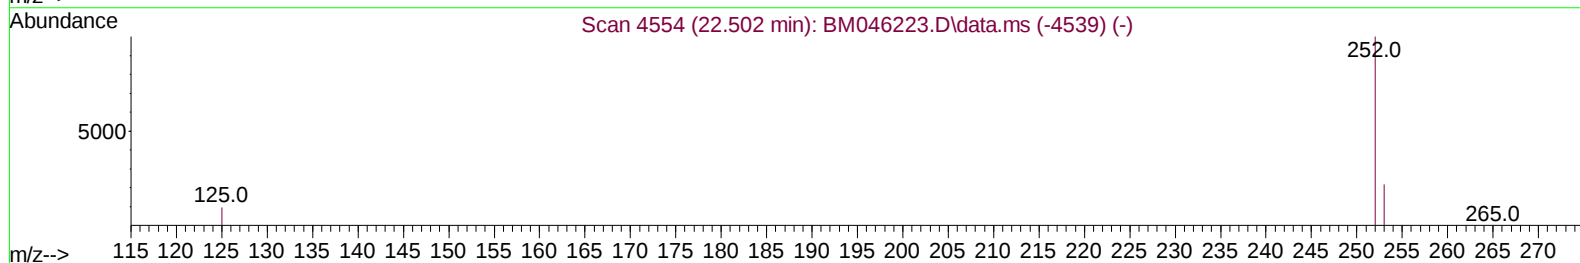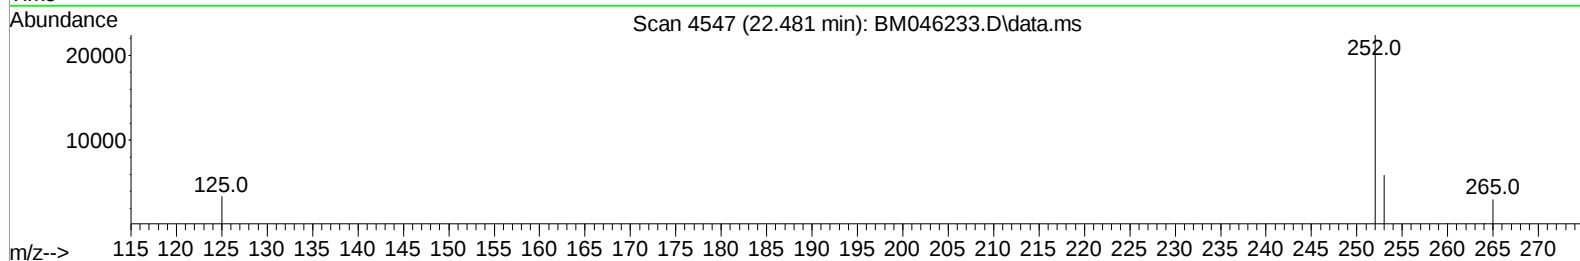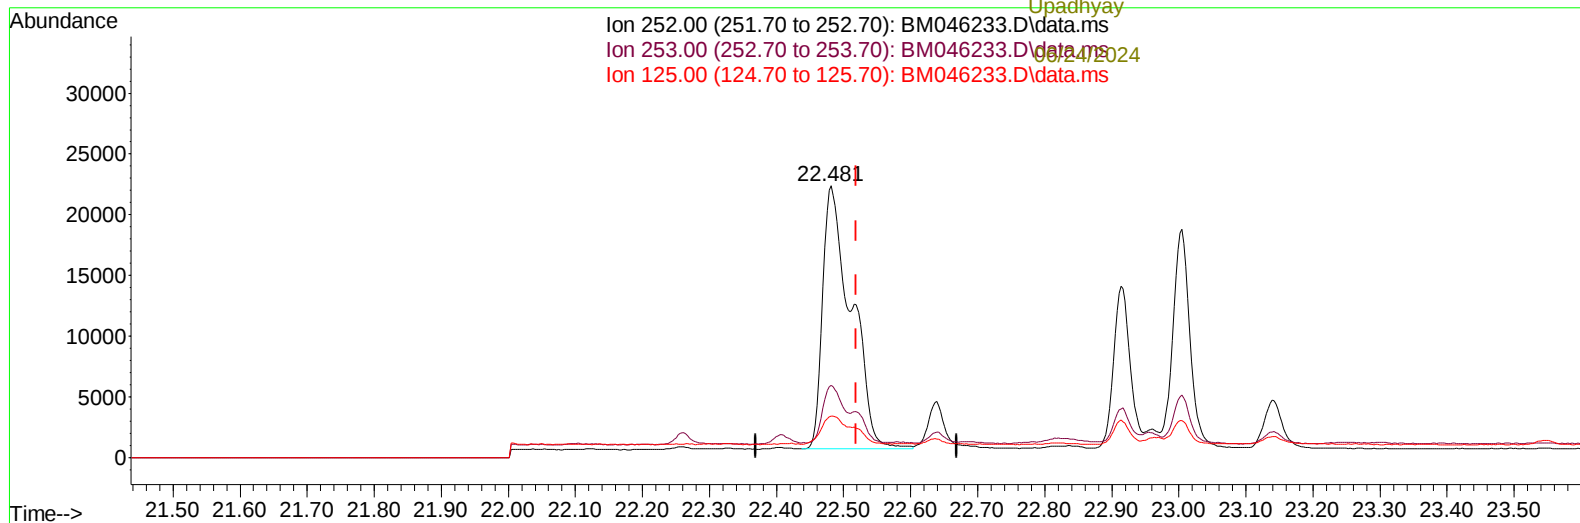

TIC: BM046233.D\data.ms

(24) Benzo(b)fluoranthene

22.481min (-0.038) 1.84 ng/u1

response 63714

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	26.46
125.00	20.10	15.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
 Data File : BM046233.D
 Acq On : 23 Jun 2024 13:50
 Operator : MA/JU
 Sample : P2776-14
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4CA9




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 02:25:34 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
 Supervised By :Jagrut
 Upadhyay

Ion 252.00 (251.70 to 252.70): BM046233.D\data.ms
 Ion 253.00 (252.70 to 253.70): BM046233.D\data.ms
 Ion 125.00 (124.70 to 125.70): BM046233.D\data.ms

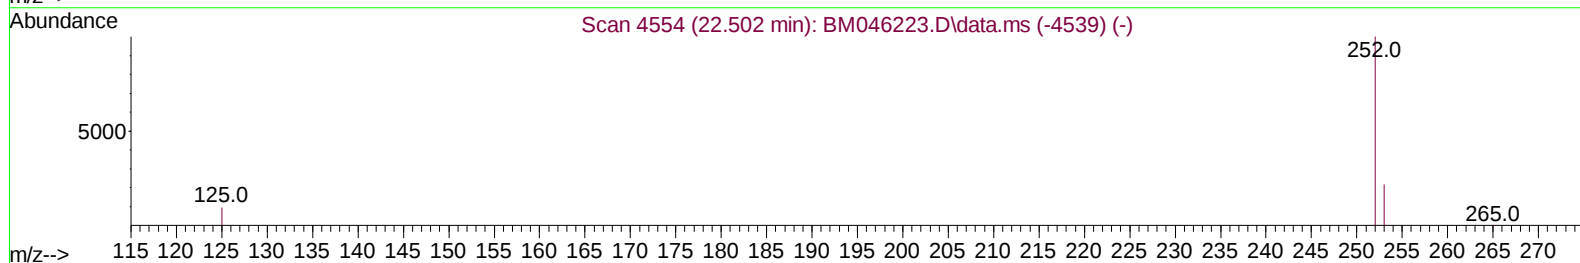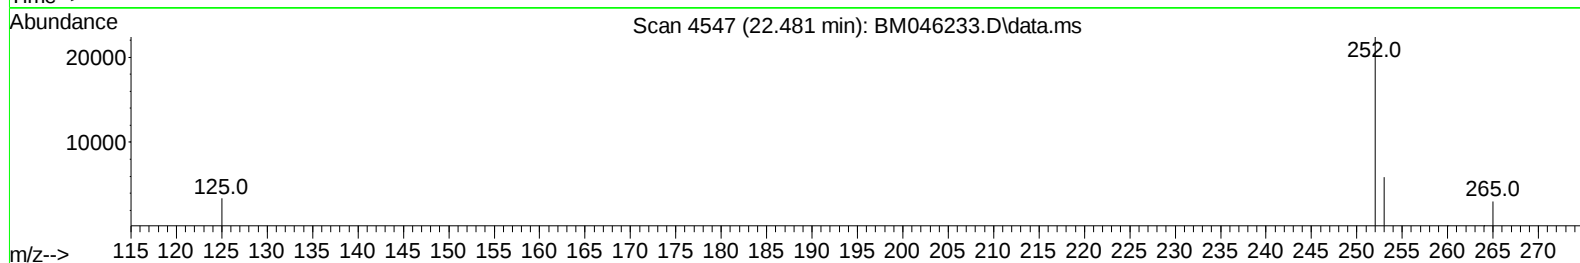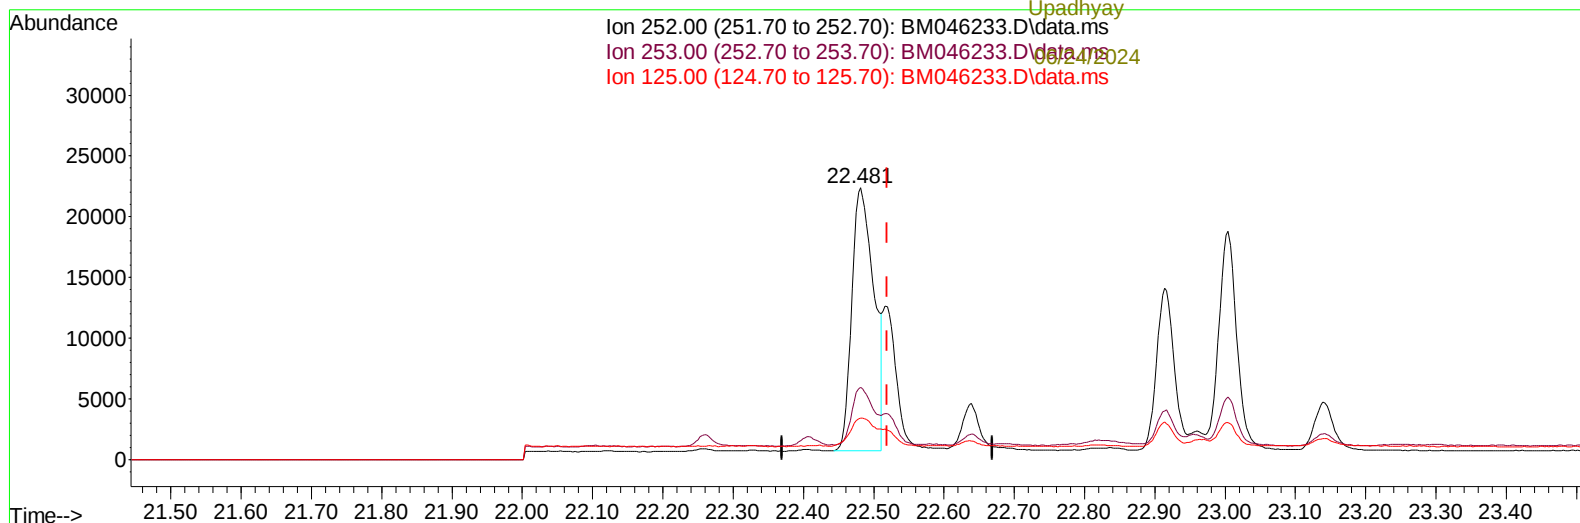

TIC: BM046233.D\data.ms

(24) Benzo(b)fluoranthene

22.481min (-0.038) 1.36 ng/ul m

response 47046

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	26.46
125.00	20.10	15.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 252.00 (251.70 to 252.70): BM046233.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046233.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046233.D\data.ms

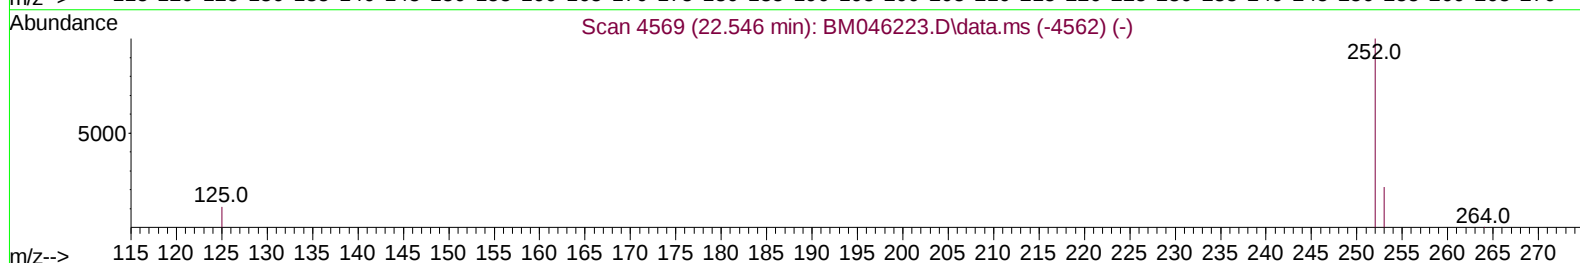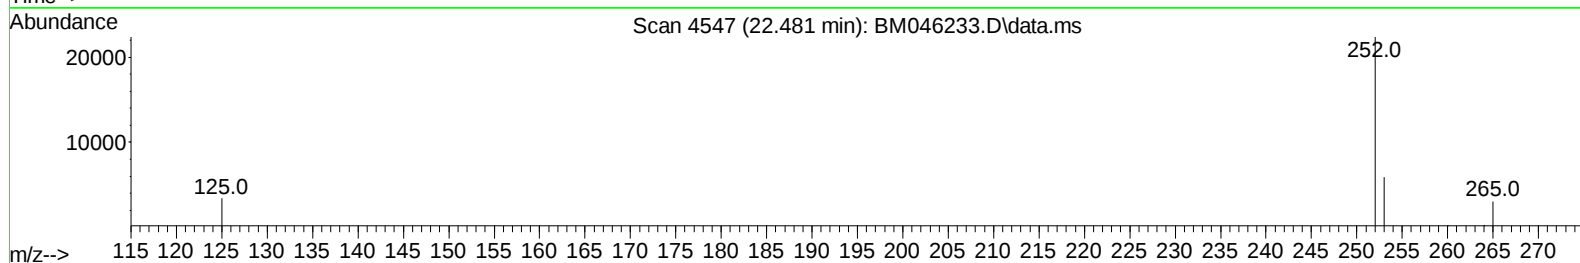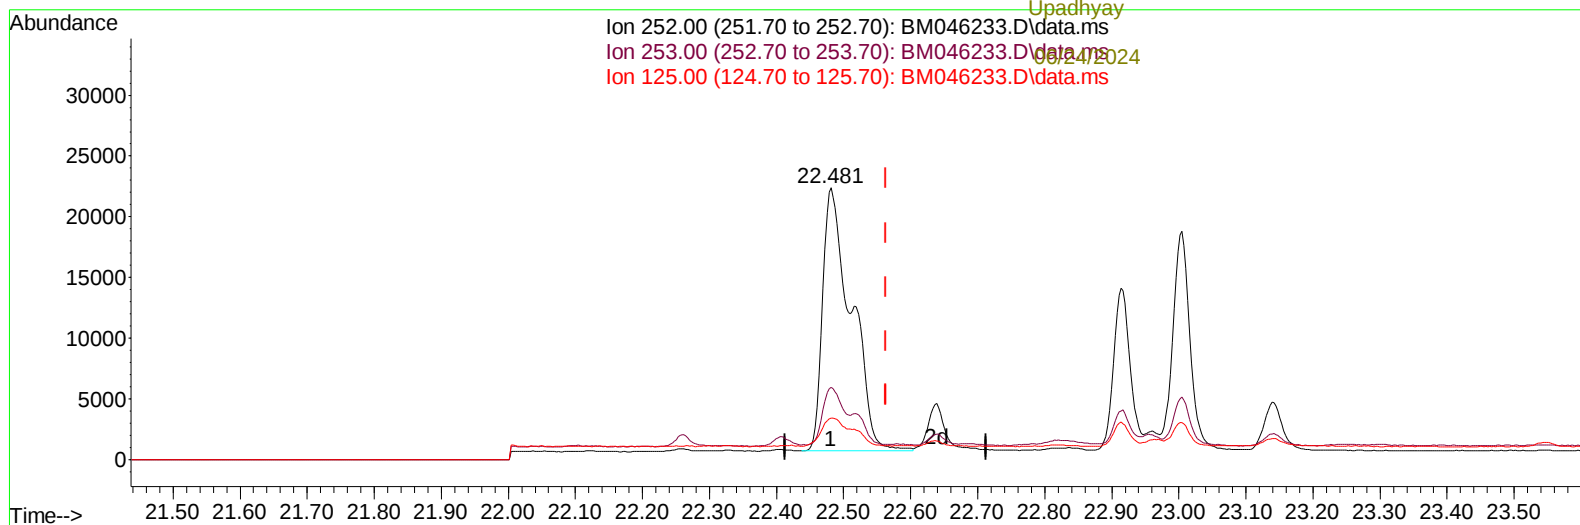

TIC: BM046233.D\data.ms

(25) Benzo(k)fluoranthene

22.481min (-0.082) 1.55 ng/u1

response 63714

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	26.46#
125.00	20.80	15.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9




Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

Ion 252.00 (251.70 to 252.70): BM046233.D\data.ms
Ion 253.00 (252.70 to 253.70): BM046233.D\data.ms
Ion 125.00 (124.70 to 125.70): BM046233.D\data.ms

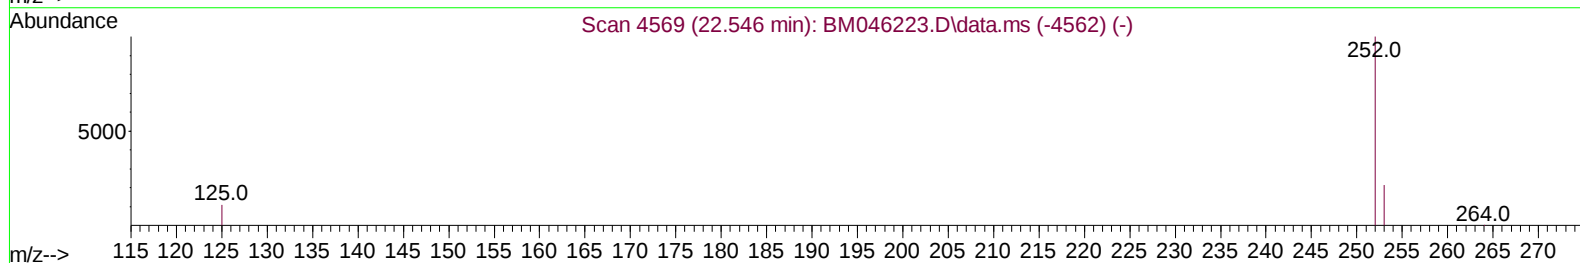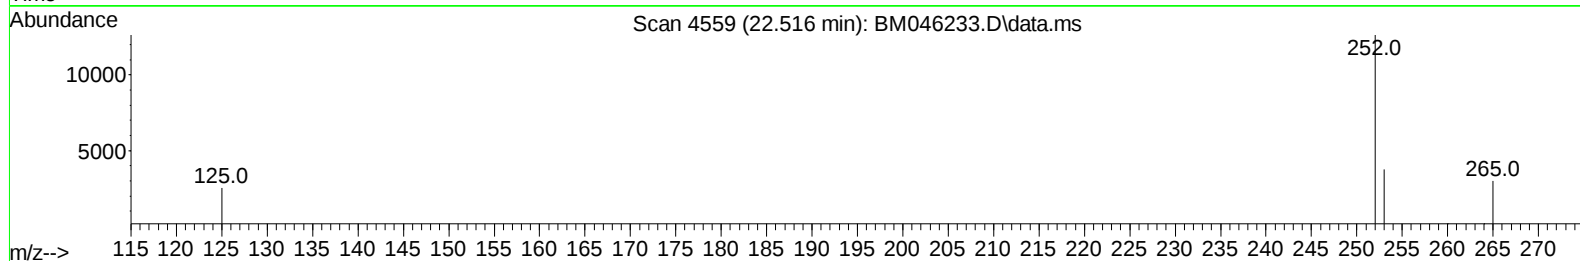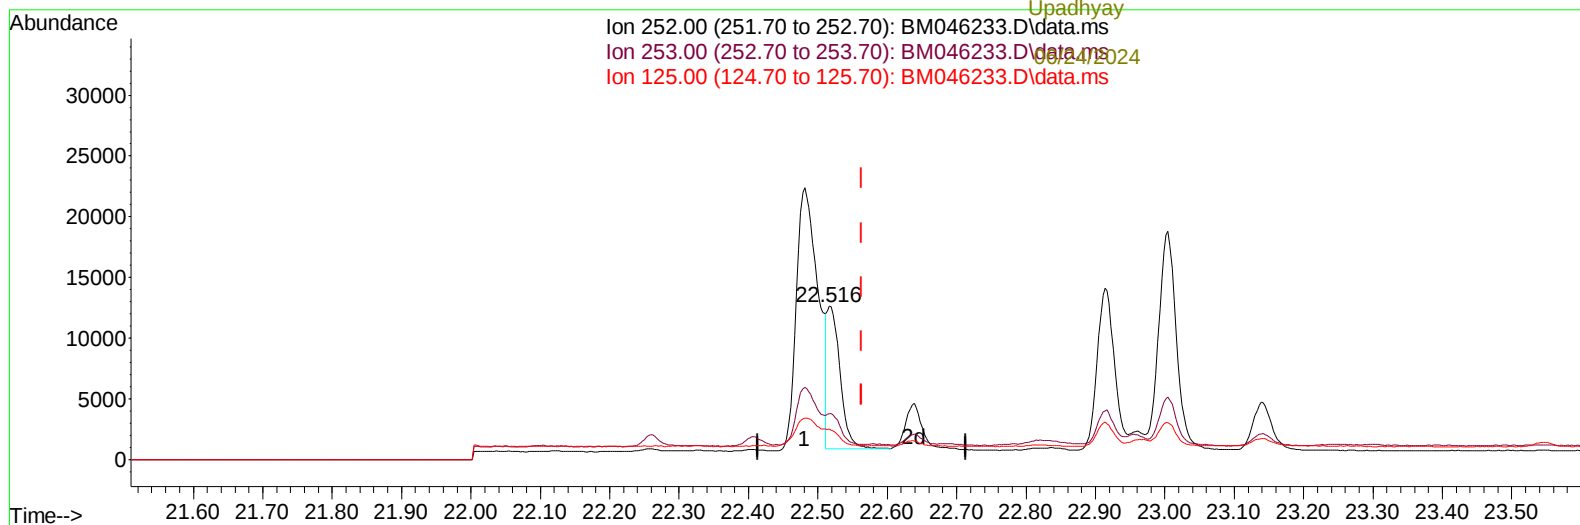

TIC: BM046233.D\data.ms

(25) Benzo(k)fluoranthene

22.516min (-0.047) 0.38 ng/u1 m

response 15737

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	29.82
125.00	20.80	19.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
 Data File : BM046233.D
 Acq On : 23 Jun 2024 13:50
 Operator : MA/JU
 Sample : P2776-14
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4CA9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :Jagrut Upadhyay 06/24/2024

Quant Time: Jun 24 02:30:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 02:25:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
-----06/24/2024							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.405	152	2578	0.400	ng/ul	-0.06	
4) Naphthalene-d8	10.172	136	8122	0.400	ng/ul	-0.08	
9) Acenaphthene-d10	14.053	164	4453	0.400	ng/ul	-0.06	
13) Phenanthrene-d10	16.799	188	9332m	0.400	ng/ul	-0.06	
17) Chrysene-d12	21.006	240	7548m	0.400	ng/ul	-0.04	
23) Perylene-d12	23.095	264	9596m	0.400	ng/ul	-0.05	
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.021	96	11975	3.386	ng/ul	-0.03	
6) 2-Methylnaphthalene-d10	11.794	152	2800	0.257	ng/ul	-0.07	
18) Fluoranthene-d10	18.835	212	5962	0.264	ng/ul	-0.05	
Target Compounds							
						Qvalue	
5) Naphthalene	10.222	128	1462	0.065	ng/ul#	84	
7) 2-Methylnaphthalene	11.871	142	543	0.043	ng/ul	98	
8) 1-Methylnaphthalene	12.086	142	531	0.038	ng/ul	99	
10) Acenaphthylene	13.771	152	3576	0.169	ng/ul#	94	
11) Acenaphthene	14.118	153	1954	0.128	ng/ul	98	
12) Fluorene	15.108	166	2095	0.128	ng/ul	98	
15) Phenanthrene	16.842	178	46576m	1.776	ng/ul		
16) Anthracene	16.930	178	7494m	0.384	ng/ul		
19) Fluoranthene	18.867	202	77609	2.375	ng/ul	96	
20) Pyrene	19.230	202	72478	2.051	ng/ul	95	
21) Benzo(a)anthracene	20.991	228	33933	1.164	ng/ul	98	
22) Chrysene	21.044	228	34080	0.916	ng/ul	99	
24) Benzo(b)fluoranthene	22.481	252	47046m	1.361	ng/ul		
25) Benzo(k)fluoranthene	22.516	252	15737m	0.383	ng/ul		
26) Benzo(a)pyrene	23.004	252	32008	0.999	ng/ul#	80	
27) Indeno(1,2,3-cd)pyrene	25.142	276	24287	0.463	ng/ul#	93	
28) Dibenzo(a,h)anthracene	25.145	278	5644	0.145	ng/ul#	79	
29) Benzo(g,h,i)perylene	25.765	276	24083	0.536	ng/ul	97	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046233.D
Acq On : 23 Jun 2024 13:50
Operator : MA/JU
Sample : P2776-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4CA9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :Jagrut Upadhyay 06/24/2024

06/24/2024
Supervised By :Jagrut
Upadhyay

06/24/2024

Quant Time: Jun 24 02:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

