
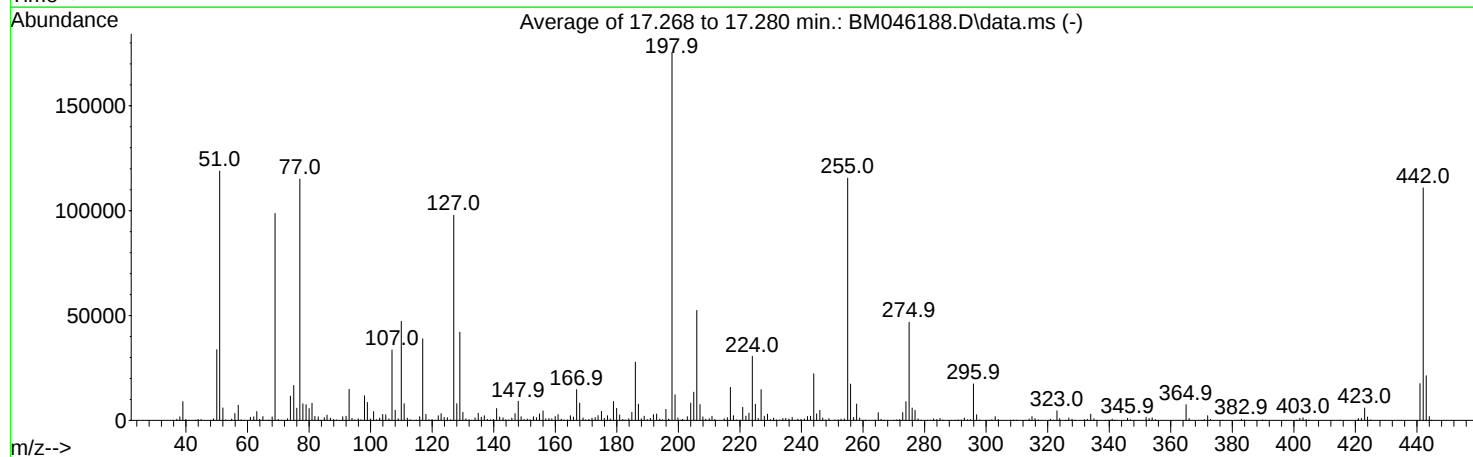


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062224\
Data File : BM046188.D
Acq On : 22 Jun 2024 09:07
Operator : MA/JU
Sample : DFTPP034
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP034

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 24 02:25:34 2024

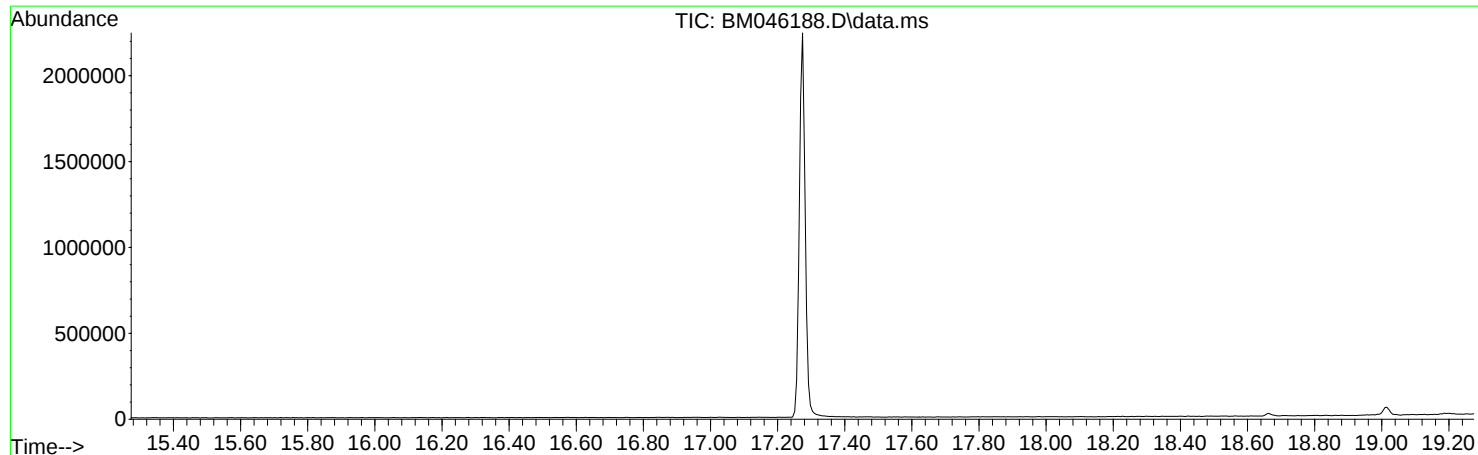

AutoFind: Scans 2428, 2429, 2430; Background Corrected with Scan 2421

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.8	118883	PASS
68	69	0.00	2	1.7	1717	PASS
69	198	0.00	100	56.2	98667	PASS
70	69	0.00	2	0.5	516	PASS
127	198	10	80	55.7	97803	PASS
197	198	0.00	2	0.4	629	PASS
198	198	100	100	100.0	175445	PASS
199	198	5	9	7.0	12195	PASS
275	198	10	60	26.7	46763	PASS
365	198	1	100	4.3	7514	PASS
441	198	0.01	100	10.0	17580	PASS
442	198	50	100	63.2	110856	PASS
443	442	15	24	19.2	21325	PASS

m/z	Abundance
40.00	1582.0
40.90	245.0
42.90	203.0
43.90	1967.0
47.00	185.0
48.90	662.0
50.80	274.0
54.90	195.0
73.00	828.0
73.90	235.0
77.00	199.0
83.80	467.0
85.80	228.0
132.90	275.0
135.00	181.0
146.80	213.0
190.90	231.0
192.80	249.0
207.00	1308.0
208.00	312.0
208.90	394.0
220.90	272.0
281.00	459.0
281.90	161.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

m/z	Abundance
35.90	167.0
37.00	616.0
38.00	1977.0
39.00	10093.0
40.00	2147.0
40.90	335.0
42.00	171.0
43.00	173.0
44.00	2584.0
44.80	311.0
47.00	185.0
48.00	198.0
48.90	1737.0
50.00	37072.0
51.00	135808.0
52.00	6722.0
53.00	230.0
54.80	747.0
55.90	3614.0
57.00	8085.0
57.80	265.0
61.00	1762.0
62.00	2043.0
63.00	4793.0
64.00	515.0
65.00	1950.0
66.00	188.0
66.80	209.0
68.00	2131.0
68.90	110088.0
70.00	728.0
73.00	1850.0
74.00	12603.0
75.00	18560.0
76.00	6302.0
77.00	125944.0
78.00	8650.0
79.00	8164.0
80.00	5944.0
80.90	9710.0
81.90	2073.0
82.90	1964.0
83.90	539.0
84.90	1482.0
85.90	2906.0
87.00	1272.0
88.00	447.0
89.00	230.0
91.00	1808.0
92.00	2104.0
93.00	15713.0
94.00	966.0
94.90	272.0
96.00	841.0
97.00	209.0
98.00	12523.0
99.00	9599.0
99.90	822.0
100.90	4320.0
101.90	310.0
102.90	1255.0
104.00	3341.0
104.90	2925.0
105.90	828.0
106.90	36600.0
108.00	5161.0
108.90	726.0
109.90	50824.0
110.90	8942.0
111.90	1333.0
112.80	362.0
114.90	228.0
116.00	1578.0
116.90	41104.0
117.90	3023.0
118.80	441.0
120.00	390.0
122.00	2591.0
122.90	3106.0
124.00	1443.0
125.00	1331.0
126.10	331.0
127.00	101912.0
128.00	8492.0
129.00	43464.0
129.90	4144.0
130.90	786.0
132.10	412.0
132.90	358.0
133.90	1377.0
134.90	4001.0
135.90	1676.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

137.00	2388.0
137.90	517.0
138.90	197.0
139.90	479.0
141.00	5588.0
142.00	1448.0
143.00	1163.0
144.00	307.0
144.80	264.0
145.90	1172.0
147.00	3315.0
147.90	8581.0
148.90	1847.0
149.90	466.0
150.90	545.0
152.00	326.0
152.90	1875.0
153.90	1403.0
154.90	2796.0
156.00	4605.0
156.90	685.0
158.00	998.0
158.90	802.0
159.90	2003.0
160.90	2811.0
162.00	715.0
162.80	211.0
163.90	168.0
164.90	2191.0
165.90	1652.0
167.00	14428.0
167.90	8675.0
169.00	1071.0
169.80	183.0
170.80	568.0
172.00	892.0
172.90	1533.0
173.90	2304.0
175.00	4353.0
175.90	898.0
177.00	2121.0
177.90	620.0
178.90	8740.0
180.00	5761.0
180.90	2762.0
181.90	482.0
183.90	885.0
184.90	3600.0
186.00	27016.0
187.00	7857.0
187.90	846.0
188.90	1808.0
189.90	336.0
190.90	1039.0
191.90	2817.0
193.00	3469.0
194.00	517.0
194.90	300.0
195.90	4828.0
196.90	931.0
197.90	170752.0
198.90	11790.0
199.80	989.0
201.20	587.0
201.90	286.0
202.90	1571.0
204.00	7868.0
205.00	13243.0
206.00	49624.0
207.00	8117.0
208.00	2245.0
209.00	725.0
210.00	840.0
210.90	2173.0
211.90	368.0
214.90	636.0
215.90	1293.0
216.90	14418.0
217.90	2166.0
219.00	247.0
221.00	6042.0
221.90	1830.0
222.90	3089.0
224.00	28248.0
225.00	7476.0
225.90	977.0
226.90	13423.0
227.90	1839.0
229.00	2748.0
230.00	482.0
231.00	1112.0
231.80	182.0
233.00	217.0
234.00	845.0
234.90	933.0
236.00	635.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

237.00	1401.0
238.00	218.0
238.80	637.0
239.80	523.0
240.90	630.0
242.00	1832.0
243.00	2004.0
244.00	21304.0
245.00	2820.0
245.90	4279.0
246.90	1110.0
247.80	261.0
248.90	815.0
250.90	272.0
251.90	268.0
252.90	532.0
253.90	591.0
255.00	106488.0
255.90	16840.0
257.00	1152.0
257.90	6980.0
258.90	1130.0
260.90	249.0
264.00	156.0
265.00	3003.0
265.90	621.0
266.90	231.0
271.00	322.0
271.90	287.0
272.90	3292.0
273.90	8193.0
275.00	42624.0
276.00	5473.0
276.90	3974.0
278.00	627.0
280.90	545.0
282.00	295.0
282.90	677.0
284.00	349.0
285.00	796.0
290.80	210.0
292.90	804.0
294.00	332.0
294.80	166.0
295.90	14571.0
296.90	2662.0
297.90	291.0
301.80	270.0
302.90	1587.0
304.00	376.0
308.90	217.0
309.90	198.0
314.00	557.0
314.90	1558.0
315.90	782.0
316.90	180.0
320.90	508.0
323.00	4295.0
323.90	675.0
326.90	843.0
327.90	429.0
332.00	291.0
332.90	426.0
334.00	2298.0
335.00	606.0
338.80	164.0
340.90	386.0
345.90	784.0
346.90	206.0
351.90	1379.0
352.90	793.0
353.90	1211.0
355.00	314.0
364.90	5967.0
366.00	664.0
370.80	279.0
372.00	1922.0
373.00	432.0
383.00	507.0
384.00	158.0
389.80	187.0
401.90	769.0
403.00	970.0
403.90	269.0
404.80	166.0
415.00	161.0
420.70	543.0
421.00	536.0
422.00	743.0
423.00	4613.0
424.00	1418.0
425.00	214.0
441.00	12827.0
442.00	80664.0
443.00	16976.0
444.00	1634.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

m/z	Abundance
35.90	167.0
37.00	616.0
38.00	1977.0
39.00	10093.0
40.00	2147.0
40.90	335.0
42.00	171.0
43.00	173.0
44.00	2584.0
44.80	311.0
47.00	185.0
48.00	198.0
48.90	1737.0
50.00	37072.0
51.00	135808.0
52.00	6722.0
53.00	230.0
54.80	747.0
55.90	3614.0
57.00	8085.0
57.80	265.0
61.00	1762.0
62.00	2043.0
63.00	4793.0
64.00	515.0
65.00	1950.0
66.00	188.0
66.80	209.0
68.00	2131.0
68.90	110088.0
70.00	728.0
73.00	1850.0
74.00	12603.0
75.00	18560.0
76.00	6302.0
77.00	125944.0
78.00	8650.0
79.00	8164.0
80.00	5944.0
80.90	9710.0
81.90	2073.0
82.90	1964.0
83.90	539.0
84.90	1482.0
85.90	2906.0
87.00	1272.0
88.00	447.0
89.00	230.0
91.00	1808.0
92.00	2104.0
93.00	15713.0
94.00	966.0
94.90	272.0
96.00	841.0
97.00	209.0
98.00	12523.0
99.00	9599.0
99.90	822.0
100.90	4320.0
101.90	310.0
102.90	1255.0
104.00	3341.0
104.90	2925.0
105.90	828.0
106.90	36600.0
108.00	5161.0
108.90	726.0
109.90	50824.0
110.90	8942.0
111.90	1333.0
112.80	362.0
114.90	228.0
116.00	1578.0
116.90	41104.0
117.90	3023.0
118.80	441.0
120.00	390.0
122.00	2591.0
122.90	3106.0
124.00	1443.0
125.00	1331.0
126.10	331.0
127.00	101912.0
128.00	8492.0
129.00	43464.0
129.90	4144.0
130.90	786.0
132.10	412.0
132.90	358.0
133.90	1377.0
134.90	4001.0
135.90	1676.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

137.00	2388.0
137.90	517.0
138.90	197.0
139.90	479.0
141.00	5588.0
142.00	1448.0
143.00	1163.0
144.00	307.0
144.80	264.0
145.90	1172.0
147.00	3315.0
147.90	8581.0
148.90	1847.0
149.90	466.0
150.90	545.0
152.00	326.0
152.90	1875.0
153.90	1403.0
154.90	2796.0
156.00	4605.0
156.90	685.0
158.00	998.0
158.90	802.0
159.90	2003.0
160.90	2811.0
162.00	715.0
162.80	211.0
163.90	168.0
164.90	2191.0
165.90	1652.0
167.00	14428.0
167.90	8675.0
169.00	1071.0
169.80	183.0
170.80	568.0
172.00	892.0
172.90	1533.0
173.90	2304.0
175.00	4353.0
175.90	898.0
177.00	2121.0
177.90	620.0
178.90	8740.0
180.00	5761.0
180.90	2762.0
181.90	482.0
183.90	885.0
184.90	3600.0
186.00	27016.0
187.00	7857.0
187.90	846.0
188.90	1808.0
189.90	336.0
190.90	1039.0
191.90	2817.0
193.00	3469.0
194.00	517.0
194.90	300.0
195.90	4828.0
196.90	931.0
197.90	170752.0
198.90	11790.0
199.80	989.0
201.20	587.0
201.90	286.0
202.90	1571.0
204.00	7868.0
205.00	13243.0
206.00	49624.0
207.00	8117.0
208.00	2245.0
209.00	725.0
210.00	840.0
210.90	2173.0
211.90	368.0
214.90	636.0
215.90	1293.0
216.90	14418.0
217.90	2166.0
219.00	247.0
221.00	6042.0
221.90	1830.0
222.90	3089.0
224.00	28248.0
225.00	7476.0
225.90	977.0
226.90	13423.0
227.90	1839.0
229.00	2748.0
230.00	482.0
231.00	1112.0
231.80	182.0
233.00	217.0
234.00	845.0
234.90	933.0
236.00	635.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

237.00	1401.0
238.00	218.0
238.80	637.0
239.80	523.0
240.90	630.0
242.00	1832.0
243.00	2004.0
244.00	21304.0
245.00	2820.0
245.90	4279.0
246.90	1110.0
247.80	261.0
248.90	815.0
250.90	272.0
251.90	268.0
252.90	532.0
253.90	591.0
255.00	106488.0
255.90	16840.0
257.00	1152.0
257.90	6980.0
258.90	1130.0
260.90	249.0
264.00	156.0
265.00	3003.0
265.90	621.0
266.90	231.0
271.00	322.0
271.90	287.0
272.90	3292.0
273.90	8193.0
275.00	42624.0
276.00	5473.0
276.90	3974.0
278.00	627.0
280.90	545.0
282.00	295.0
282.90	677.0
284.00	349.0
285.00	796.0
290.80	210.0
292.90	804.0
294.00	332.0
294.80	166.0
295.90	14571.0
296.90	2662.0
297.90	291.0
301.80	270.0
302.90	1587.0
304.00	376.0
308.90	217.0
309.90	198.0
314.00	557.0
314.90	1558.0
315.90	782.0
316.90	180.0
320.90	508.0
323.00	4295.0
323.90	675.0
326.90	843.0
327.90	429.0
332.00	291.0
332.90	426.0
334.00	2298.0
335.00	606.0
338.80	164.0
340.90	386.0
345.90	784.0
346.90	206.0
351.90	1379.0
352.90	793.0
353.90	1211.0
355.00	314.0
364.90	5967.0
366.00	664.0
370.80	279.0
372.00	1922.0
373.00	432.0
383.00	507.0
384.00	158.0
389.80	187.0
401.90	769.0
403.00	970.0
403.90	269.0
404.80	166.0
415.00	161.0
420.70	543.0
421.00	536.0
422.00	743.0
423.00	4613.0
424.00	1418.0
425.00	214.0
441.00	12827.0
442.00	80664.0
443.00	16976.0
444.00	1634.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

m/z	Abundance
35.00	155.0
36.00	700.0
38.00	2001.0
39.00	10245.0
39.00	2031.0
41.00	422.0
43.00	273.0
44.00	2667.0
44.00	410.0
49.00	1530.0
50.00	39536.0
51.00	138560.0
52.00	7069.0
53.00	215.0
54.00	973.0
55.00	3930.0
57.00	8633.0
58.00	470.0
58.00	169.0
61.00	1493.0
62.00	1923.0
63.00	4861.0
63.00	560.0
65.00	2258.0
67.00	217.0
68.00	1786.0
69.00	114912.0
70.10	474.0
71.00	186.0
73.00	1664.0
74.00	14881.0
75.00	19272.0
76.00	6992.0
77.00	137728.0
78.00	9330.0
79.00	8715.0
80.00	7014.0
81.00	9043.0
81.00	2340.0
83.00	1909.0
83.00	579.0
85.00	1496.0
85.00	3074.0
86.00	1033.0
87.00	415.0
89.00	294.0
90.00	2317.0
92.00	2322.0
93.00	18608.0
94.00	1213.0
94.00	224.0
95.00	812.0
96.00	320.0
98.00	13759.0
98.00	10184.0
100.00	831.0
101.00	5062.0
101.00	323.0
103.00	1304.0
103.00	3206.0
104.00	3189.0
106.00	992.0
107.00	39032.0
108.00	5939.0
108.00	928.0
110.00	56312.0
110.00	9098.0
112.00	1027.0
112.00	348.0
114.00	178.0
116.00	2228.0
117.00	46960.0
118.00	3423.0
119.00	316.0
119.00	425.0
121.00	162.0
121.00	2419.0
122.00	4161.0
123.00	1953.0
124.00	1644.0
126.00	295.0
127.00	116488.0
128.00	9588.0
129.00	51696.0
130.00	4602.0
131.00	1034.0
131.00	378.0
132.00	479.0
133.00	1428.0
135.00	4256.0
136.00	1703.0
137.00	2426.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

138.00	546.0
138.90	420.0
139.90	550.0
140.90	6903.0
142.00	2073.0
143.00	1680.0
143.80	346.0
145.00	229.0
145.90	1350.0
146.90	4162.0
148.00	11098.0
148.90	2039.0
149.90	542.0
151.00	699.0
151.90	464.0
152.90	2077.0
153.90	1336.0
154.90	3755.0
156.00	4840.0
156.90	1046.0
157.90	908.0
158.90	917.0
160.00	2186.0
160.90	3576.0
161.90	684.0
162.90	316.0
163.90	386.0
164.90	2640.0
165.90	2051.0
166.90	18080.0
168.00	9424.0
169.00	1608.0
169.90	534.0
171.00	685.0
171.90	1508.0
173.00	1547.0
173.90	2889.0
175.00	5065.0
176.00	1370.0
177.00	2910.0
177.80	848.0
178.90	11077.0
180.00	6853.0
180.90	2915.0
182.00	529.0
182.70	232.0
183.90	931.0
184.90	4567.0
186.00	32880.0
187.00	9310.0
187.90	937.0
188.90	2438.0
189.90	405.0
190.90	1378.0
191.90	3229.0
193.00	3889.0
193.90	904.0
194.80	273.0
196.00	6462.0
196.70	956.0
197.90	214016.0
198.90	14472.0
199.90	1496.0
201.40	836.0
202.90	2226.0
204.00	9743.0
205.00	15806.0
206.00	63264.0
207.00	10129.0
207.90	2221.0
208.90	1265.0
210.00	880.0
210.90	2144.0
211.70	502.0
214.90	1064.0
215.90	1604.0
216.90	19240.0
217.90	2732.0
218.90	191.0
221.00	7580.0
222.00	2718.0
222.90	4292.0
224.00	37416.0
225.00	9367.0
226.00	1031.0
226.90	17496.0
227.90	2487.0
228.90	3517.0
230.00	326.0
230.90	1079.0
231.90	278.0
232.90	333.0
233.90	1058.0
234.90	1209.0
235.90	652.0
236.90	1777.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

237.90	196.0
238.90	594.0
239.90	696.0
240.90	899.0
241.90	2211.0
243.00	2189.0
244.00	26200.0
245.00	3809.0
246.00	5814.0
246.90	1418.0
247.90	227.0
249.00	891.0
250.90	238.0
251.90	179.0
252.90	826.0
253.90	972.0
255.00	140416.0
256.00	20352.0
257.00	1658.0
257.90	9594.0
258.90	1553.0
259.80	325.0
260.80	175.0
263.90	212.0
264.90	4457.0
265.90	448.0
270.80	366.0
271.90	409.0
272.90	4425.0
273.90	10111.0
274.90	56488.0
275.90	7033.0
276.90	6042.0
277.90	1046.0
278.80	349.0
280.90	624.0
281.90	240.0
283.00	937.0
283.90	538.0
285.00	1218.0
285.90	204.0
288.80	159.0
289.90	215.0
290.90	232.0
291.90	381.0
292.90	1372.0
294.00	301.0
294.90	449.0
295.90	20432.0
296.90	3332.0
298.00	350.0
301.90	389.0
303.00	2028.0
303.90	559.0
307.90	252.0
308.90	169.0
310.00	183.0
312.90	243.0
314.00	708.0
314.90	2100.0
315.90	941.0
316.90	193.0
320.90	754.0
321.90	253.0
323.00	5178.0
323.90	1044.0
325.80	151.0
326.90	1277.0
327.90	655.0
328.90	185.0
331.90	658.0
332.90	545.0
334.00	3797.0
335.00	1001.0
335.90	151.0
338.80	176.0
340.90	760.0
342.00	241.0
346.00	1199.0
347.00	351.0
352.00	1592.0
353.00	980.0
354.00	1277.0
355.00	366.0
365.00	9044.0
366.00	1185.0
370.90	397.0
372.00	2538.0
373.00	613.0
376.90	160.0
382.90	632.0
383.90	275.0
389.80	241.0
390.80	321.0
392.00	227.0
400.80	209.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

402.00	1111.0
403.00	1466.0
404.00	579.0
404.90	218.0
420.90	1101.0
421.80	1183.0
423.00	6642.0
423.90	1968.0
424.90	268.0
441.00	21408.0
442.00	132672.0
443.00	24296.0
444.00	2031.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

m/z	Abundance
37.10	321.0
38.00	1112.0
39.00	6371.0
40.00	1693.0
41.00	242.0
43.00	253.0
44.00	2040.0
45.00	354.0
46.90	266.0
49.00	1097.0
50.00	24560.0
51.00	83104.0
52.00	3986.0
52.80	243.0
54.90	611.0
55.90	2268.0
56.90	4970.0
57.90	323.0
60.90	1153.0
62.00	1114.0
63.00	2982.0
64.00	532.0
65.00	1270.0
65.90	158.0
67.90	1233.0
68.90	71000.0
69.90	346.0
73.00	1337.0
74.00	8031.0
75.00	12127.0
76.00	4063.0
77.00	82264.0
78.00	5847.0
79.00	5486.0
80.00	4103.0
81.00	5711.0
81.90	1268.0
82.90	1138.0
83.80	581.0
84.90	980.0
85.90	2208.0
86.90	819.0
87.90	372.0
88.80	164.0
91.00	1257.0
91.90	1451.0
93.00	10184.0
93.90	753.0
94.90	239.0
96.00	732.0
96.80	304.0
98.00	8961.0
99.00	5880.0
99.80	368.0
100.90	3187.0
102.00	216.0
102.90	709.0
103.90	1961.0
105.00	1963.0
106.00	370.0
107.00	25080.0
108.00	3377.0
109.00	722.0
110.00	34504.0
110.90	5870.0
111.90	840.0
112.90	221.0
115.90	1379.0
116.90	28800.0
118.00	2108.0
119.00	297.0
119.90	273.0
121.90	1683.0
122.90	2426.0
123.80	1072.0
125.00	1006.0
125.90	215.0
127.00	75008.0
128.00	5795.0
129.00	30928.0
129.90	2619.0
130.90	506.0
132.00	233.0
132.80	244.0
133.90	930.0
134.90	2539.0
135.90	1298.0
136.90	1814.0
137.90	275.0
138.90	275.0
139.90	447.0
140.90	4384.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

141.90	1272.0
142.90	869.0
143.90	297.0
144.80	279.0
145.90	993.0
146.90	2808.0
147.90	7469.0
148.90	1315.0
149.90	322.0
150.90	517.0
151.70	397.0
152.90	1392.0
153.90	1274.0
154.90	2614.0
156.00	3982.0
156.80	519.0
157.90	816.0
158.90	659.0
159.90	1269.0
160.90	1986.0
162.00	442.0
162.90	254.0
163.90	216.0
164.90	1728.0
166.00	1125.0
166.90	11485.0
167.90	6709.0
169.00	878.0
170.90	515.0
171.90	836.0
172.90	835.0
173.90	1716.0
175.00	3457.0
176.00	819.0
176.90	1681.0
177.90	548.0
178.90	7232.0
179.90	4473.0
180.90	2074.0
181.80	404.0
182.80	213.0
183.90	557.0
184.90	3405.0
186.00	23416.0
187.00	6043.0
188.00	600.0
188.90	1760.0
189.90	315.0
190.90	997.0
191.90	2270.0
193.00	2609.0
194.00	687.0
194.80	175.0
195.00	173.0
195.90	4517.0
197.00	739.0
197.90	141568.0
198.90	10322.0
199.90	875.0
200.80	213.0
201.30	515.0
202.90	1390.0
204.00	7090.0
205.00	11240.0
206.00	44304.0
207.00	8420.0
207.90	1595.0
208.90	987.0
210.10	842.0
210.90	1728.0
211.90	261.0
214.90	577.0
216.00	911.0
216.90	13580.0
217.90	1686.0
218.90	189.0
220.10	257.0
220.90	6059.0
221.90	1592.0
223.00	2995.0
224.00	25888.0
225.00	6374.0
226.00	722.0
226.90	13063.0
227.90	1648.0
228.90	2777.0
229.90	277.0
230.90	950.0
231.80	191.0
232.90	212.0
233.90	869.0
234.90	695.0
235.90	680.0
237.00	1127.0
237.80	168.0
238.90	606.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

239.90	442.0
240.90	633.0
241.90	1590.0
242.90	1683.0
244.00	19032.0
244.90	2672.0
246.00	4452.0
246.90	994.0
247.70	172.0
248.90	734.0
250.80	223.0
251.90	266.0
252.90	482.0
254.00	409.0
255.00	99640.0
256.00	14676.0
256.90	1318.0
257.90	6768.0
258.90	973.0
263.80	176.0
264.90	3598.0
265.90	510.0
266.90	160.0
270.00	176.0
271.00	326.0
271.90	377.0
272.90	3409.0
274.00	8567.0
275.00	41176.0
276.00	5052.0
276.90	4388.0
277.80	747.0
278.90	220.0
280.90	518.0
282.00	211.0
282.90	553.0
284.00	235.0
285.00	760.0
286.00	172.0
288.80	187.0
291.00	157.0
291.90	247.0
292.90	1231.0
293.80	216.0
294.90	287.0
295.90	17224.0
296.90	2139.0
300.90	173.0
301.90	240.0
303.00	1593.0
304.00	339.0
307.90	258.0
313.90	671.0
314.90	1778.0
315.90	759.0
317.10	251.0
320.90	417.0
321.90	191.0
323.00	4243.0
323.90	750.0
325.80	163.0
326.80	1233.0
327.90	469.0
331.80	228.0
333.00	304.0
334.00	2827.0
335.00	760.0
335.90	169.0
339.80	166.0
341.00	636.0
341.80	230.0
345.90	1005.0
347.00	333.0
352.00	1546.0
353.00	933.0
354.00	1209.0
355.00	392.0
364.90	7532.0
365.90	1026.0
369.90	250.0
371.00	385.0
372.00	2266.0
372.90	462.0
382.90	582.0
384.00	262.0
390.00	180.0
401.00	235.0
402.00	762.0
403.00	1228.0
403.90	398.0
421.00	793.0
422.00	866.0
423.00	6362.0
424.00	1381.0
424.90	227.0
441.00	18504.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034

442.00	119232.0
443.00	22704.0
444.00	1860.0
444.80	165.0

Instrument :
BNA_M
ClientSampleId :
DFTPP034