

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
 Data File : BM005947.D
 Acq On : 24 Jun 2016 01:48
 Operator : UM/SJ
 Sample : H3612-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z35

Quant Time: Jun 24 04:25:38 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 00:58:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	311675	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1348237	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	753965	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1734698	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	2035439	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	2094368	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	15166	1.94	ng/uL	0.00
5) Phenol-d5	6.83	99	593195	22.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	385177	23.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	465977	22.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	478933	22.78	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	226999	22.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	237203	22.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	437352	21.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	623830	28.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1380141	23.04	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1760368	23.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	235869	20.14	ng/ul	0.00
57) Fluorene-d10	15.30	176	1240982	23.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	173931	20.13	ng/ul	0.00
70) Anthracene-d10	17.16	188	1931059	24.44	ng/ul	0.00
76) Pyrene-d10	19.45	212	2265431	23.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	2404909	25.49	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.77	163	410602	6.79 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005947.D
Acq On : 24 Jun 2016 01:48
Operator : UM/SJ
Sample : H3612-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z35

Quant Time: Jun 24 04:25:38 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 00:58:22 2016
Response via : Initial Calibration

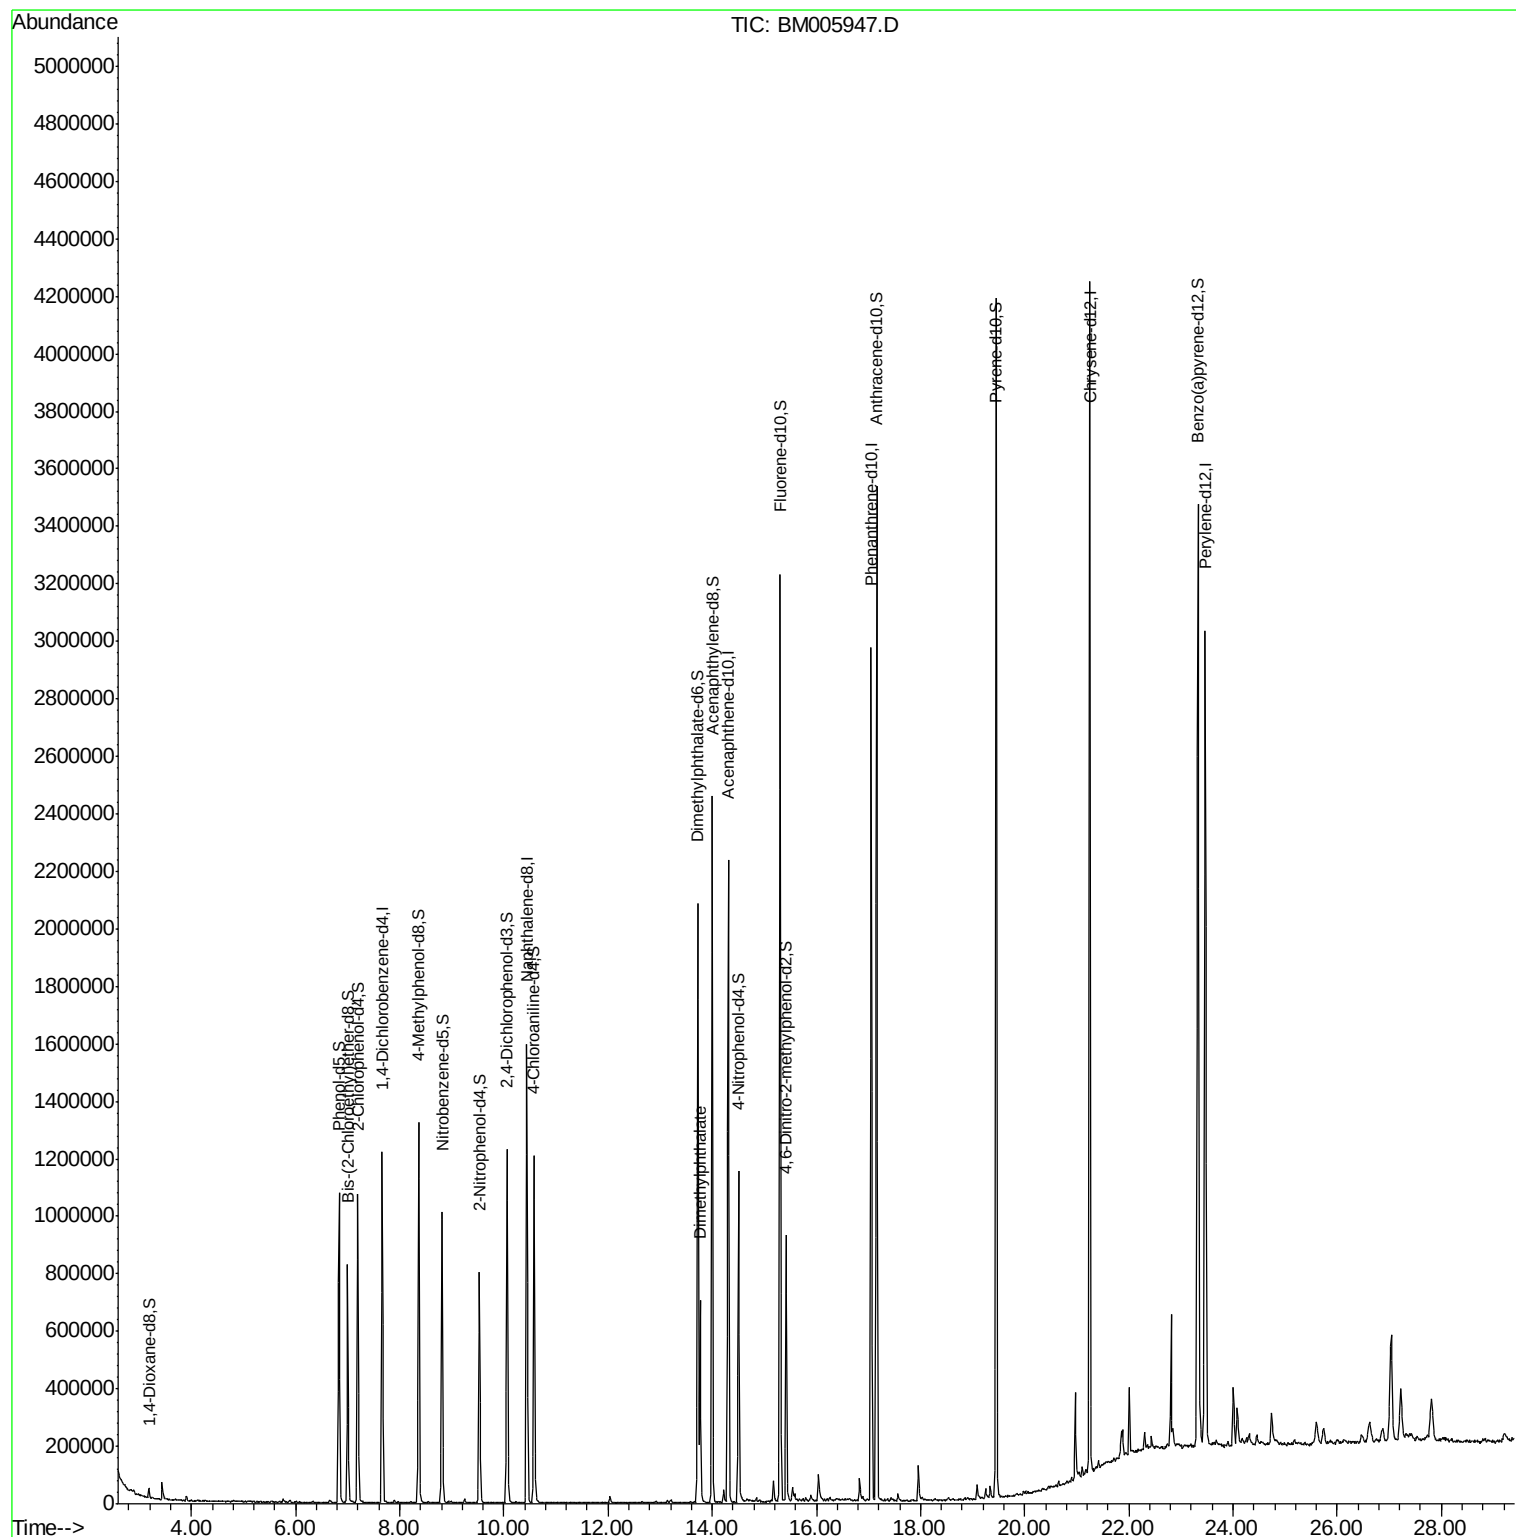


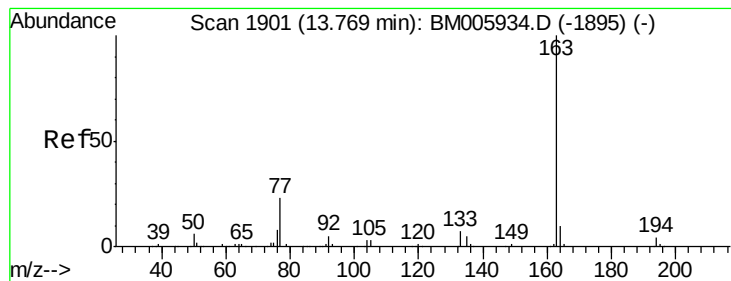

#44
 Dimethylphthalate
 Concen: 6.79 ng/ul
 RT: 13.77 min Scan# 1901
 Delta R.T. -0.00 min
 Lab File: BM005947.D
 Acq: 24 Jun 2016 01:48

Instrument :
 BNA_M
 ClientSampleId :
 D9Z35

Tgt Ion:	163	Resp:	410602
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.1	4.7
164	9.4	7.9	11.9

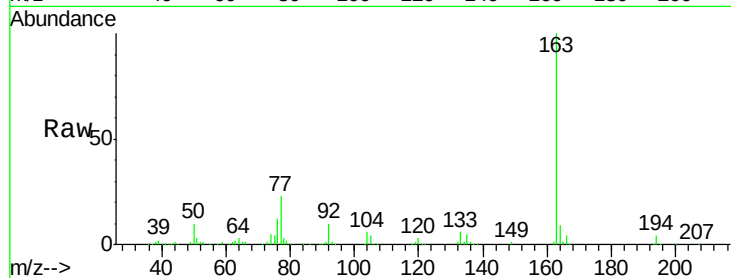

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

