

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
 Data File : BM005948.D
 Acq On : 24 Jun 2016 02:24
 Operator : UM/SJ
 Sample : H3612-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z36

Quant Time: Jun 24 04:31:43 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 00:58:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	248168	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1074919	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	612249	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1445124	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1693508	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1713578	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	13592	2.18	ng/uL	0.00
5) Phenol-d5	6.83	99	491345	22.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	317595	24.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	385435	22.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	380968	22.76	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	179612	22.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	190435	23.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	357203	22.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	308999	17.81	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1122491	23.07	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1428684	23.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	161693	17.00	ng/ul	0.00
57) Fluorene-d10	15.30	176	998132	23.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	142682	19.82	ng/ul	0.00
70) Anthracene-d10	17.16	188	1549899	23.54	ng/ul	0.00
76) Pyrene-d10	19.45	212	1868419	23.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	1903446	24.65	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	345337	7.03	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005948.D
Acq On : 24 Jun 2016 02:24
Operator : UM/SJ
Sample : H3612-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z36

Quant Time: Jun 24 04:31:43 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 00:58:22 2016
Response via : Initial Calibration

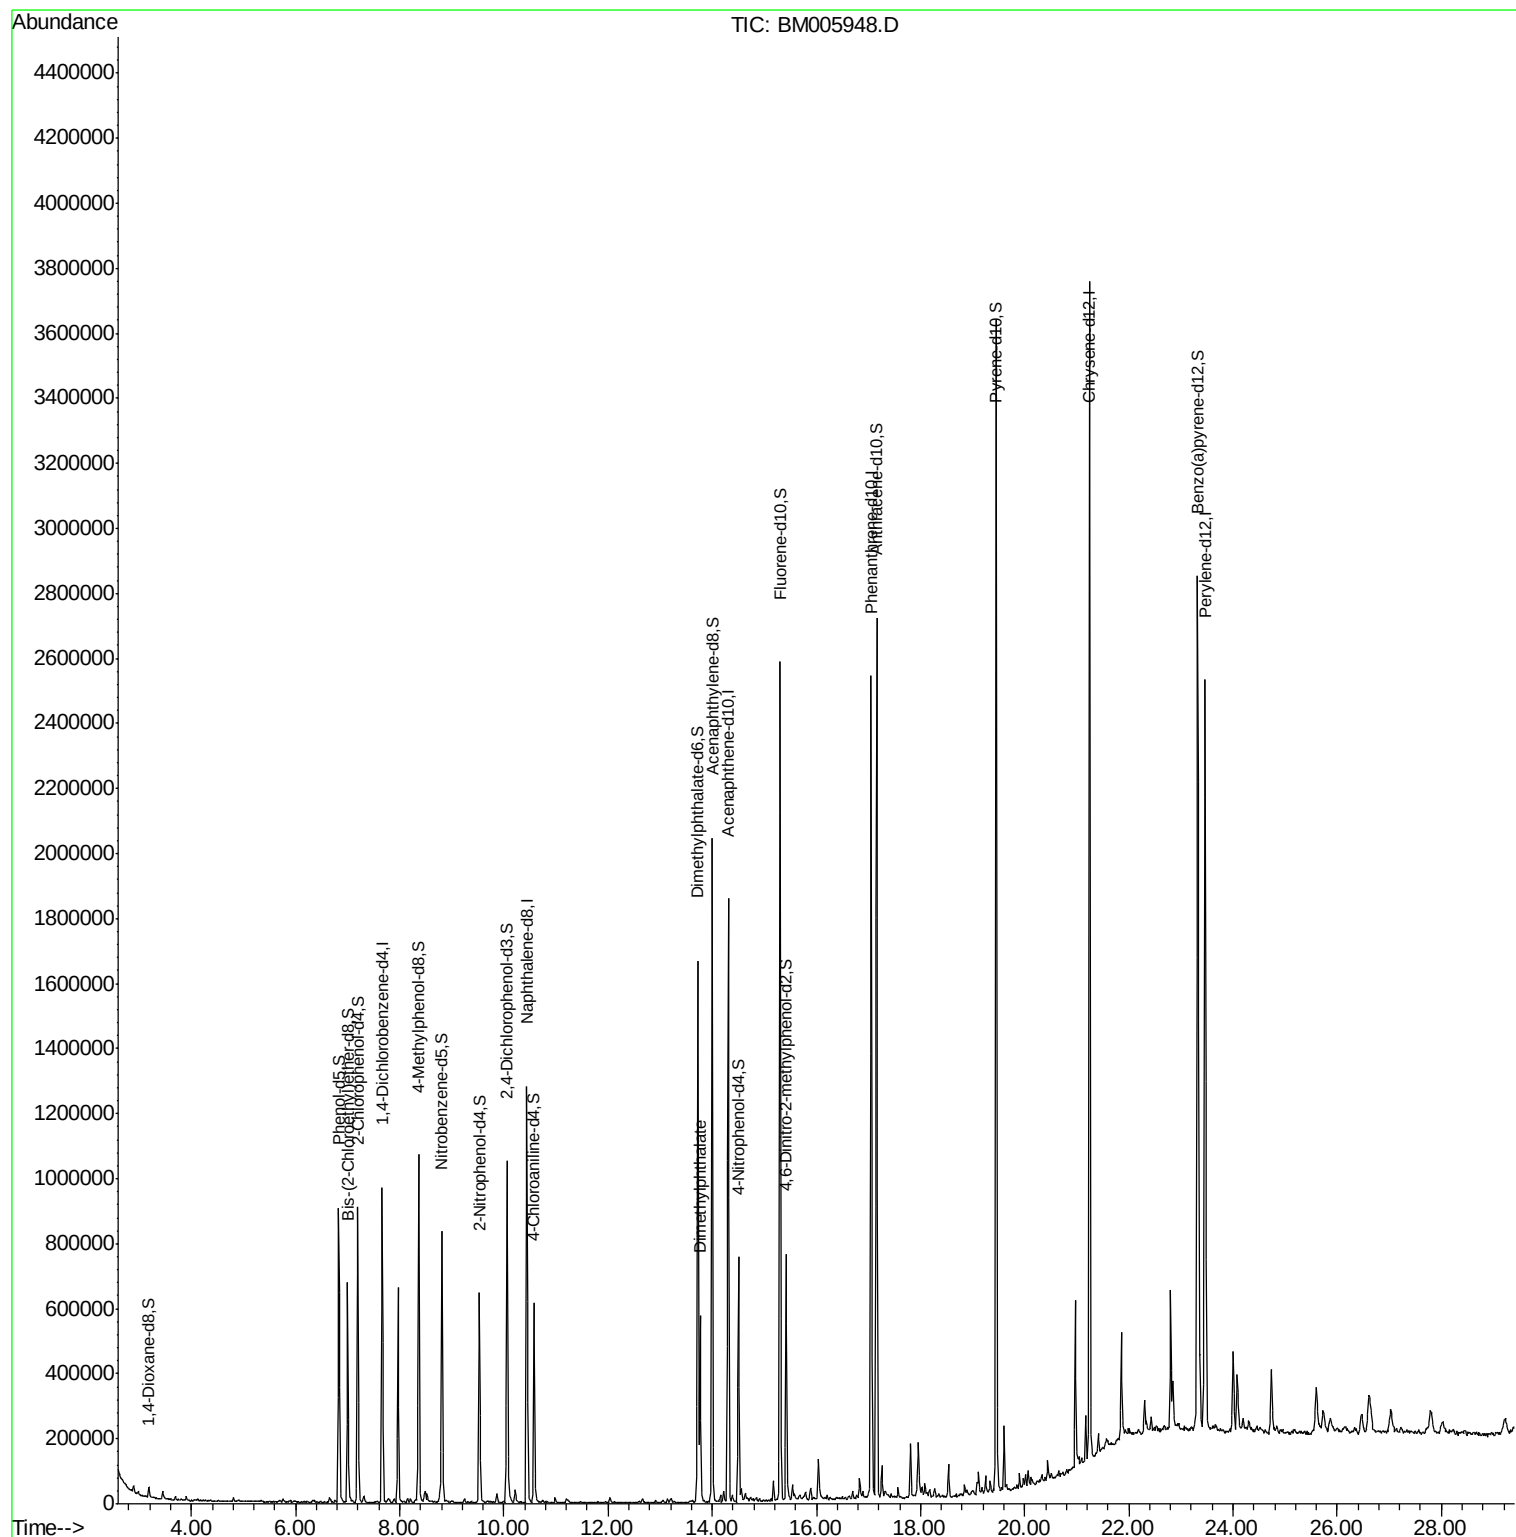

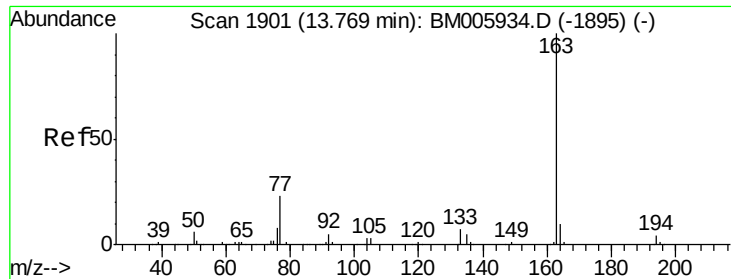

#44
 Dimethylphthalate
 Concen: 7.03 ng/ul
 RT: 13.77 min Scan# 1901
 Delta R.T. -0.00 min
 Lab File: BM005948.D
 Acq: 24 Jun 2016 02:24

Instrument :
 BNA_M
 ClientSampleId :
 D9Z36

Tot Ion:163	Resp:	345337
Ion Ratio	Lower	Upper
163	100	
194	4.3	3.1 4.7
164	10.1	7.9 11.9

