

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
 Data File : BM005952.D
 Acq On : 24 Jun 2016 04:47
 Operator : UM/SJ
 Sample : H3639-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z41

Quant Time: Jun 24 06:01:28 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 00:58:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	416876	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	2054571	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	1228332	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	2581338	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	2341645	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	2309456	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	19554	1.87	ng/uL	0.00
5) Phenol-d5	6.83	99	833590	23.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	546954	24.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	641680	22.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	688172	24.47	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	328682	21.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	366982	23.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	657442	21.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	934906	28.19	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	2199295	22.53	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	2679567	21.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	348858	18.29	ng/ul	0.00
57) Fluorene-d10	15.30	176	1846048	21.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	271998	21.15	ng/ul	0.00
70) Anthracene-d10	17.16	188	2654693	22.58	ng/ul	0.00
76) Pyrene-d10	19.45	212	2742272	25.23	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	2491277	23.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	1581110	16.05	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005952.D
Acq On : 24 Jun 2016 04:47
Operator : UM/SJ
Sample : H3639-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z41

Quant Time: Jun 24 06:01:28 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 00:58:22 2016
Response via : Initial Calibration

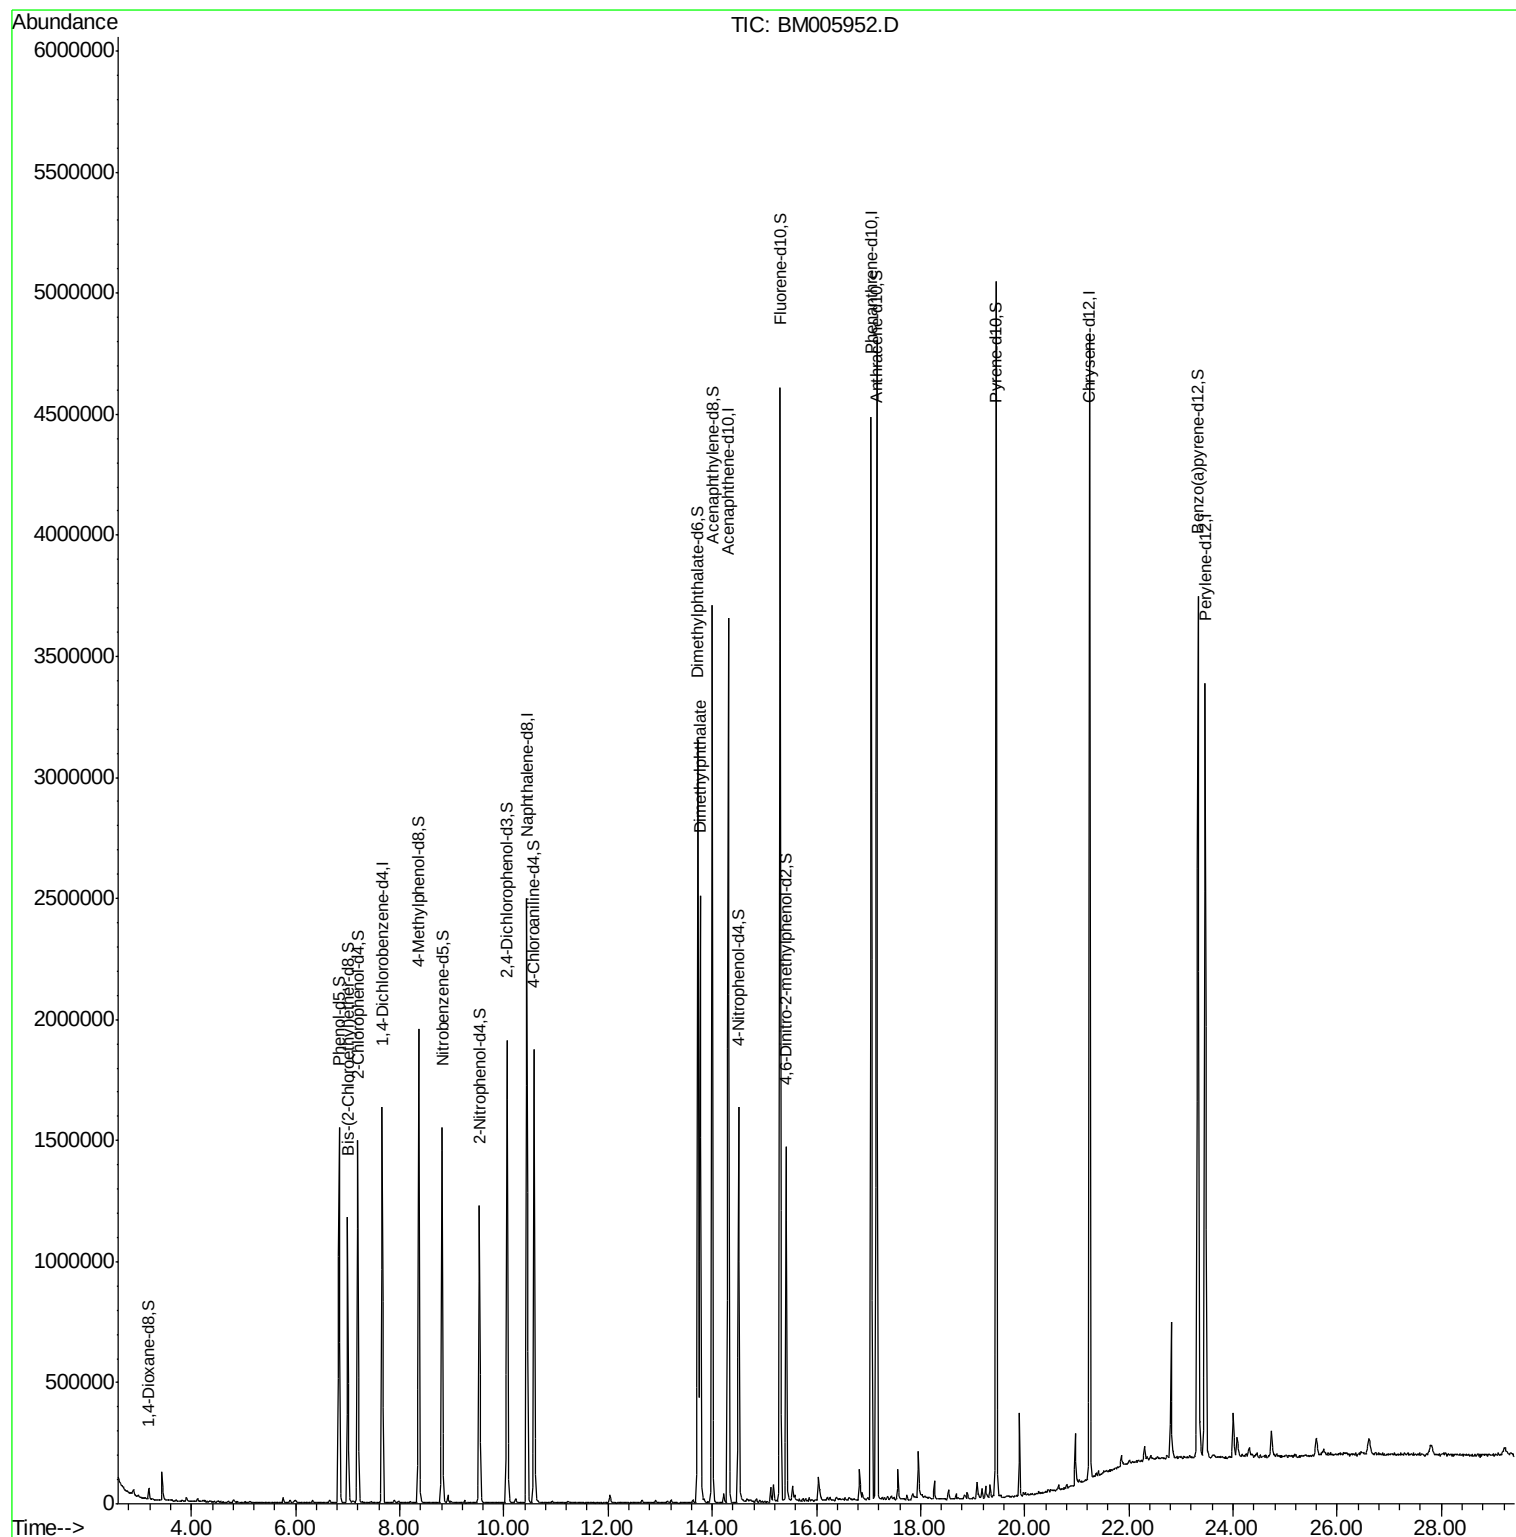


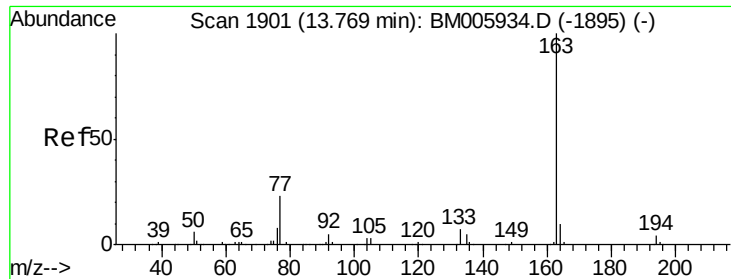

#44
 Dimethylphthalate
 Concen: 16.05 ng/ul
 RT: 13.77 min Scan# 1901
 Delta R.T. -0.00 min
 Lab File: BM005952.D
 Acq: 24 Jun 2016 04:47

Instrument :
 BNA_M
 ClientSampleId :
 D9Z41

Tot Ion:163 Resp: 1581110
 Ion Ratio Lower Upper
 163 100
 194 3.8 3.1 4.7
 164 10.1 7.9 11.9

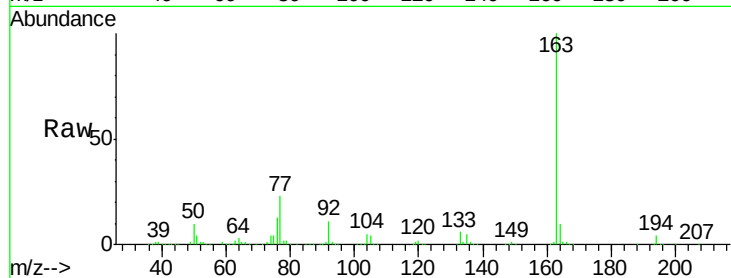

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

