

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
 Data File : BM005955.D
 Acq On : 24 Jun 2016 06:35
 Operator : UM/SJ
 Sample : H3639-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z46

Quant Time: Jun 24 15:33:34 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 00:58:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	289606	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	1264986	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	708700	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1615795	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	1893814	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	1945516	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	12797	1.76	ng/uL	0.00
5) Phenol-d5	6.83	99	486156	19.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	319521	20.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	379808	19.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	378214	19.36	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	178320	19.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	185017	18.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	353527	18.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	509716	24.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1085774	19.28	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1373903	19.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	154268	14.01	ng/ul	0.00
57) Fluorene-d10	15.30	176	982145	20.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	113189	14.06	ng/ul	0.00
70) Anthracene-d10	17.15	188	1487181	20.20	ng/ul	0.00
76) Pyrene-d10	19.45	212	1676865	19.08	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	1740006	19.85	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.77	163	288195	5.07	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005955.D
Acq On : 24 Jun 2016 06:35
Operator : UM/SJ
Sample : H3639-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z46

Quant Time: Jun 24 15:33:34 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 00:58:22 2016
Response via : Initial Calibration

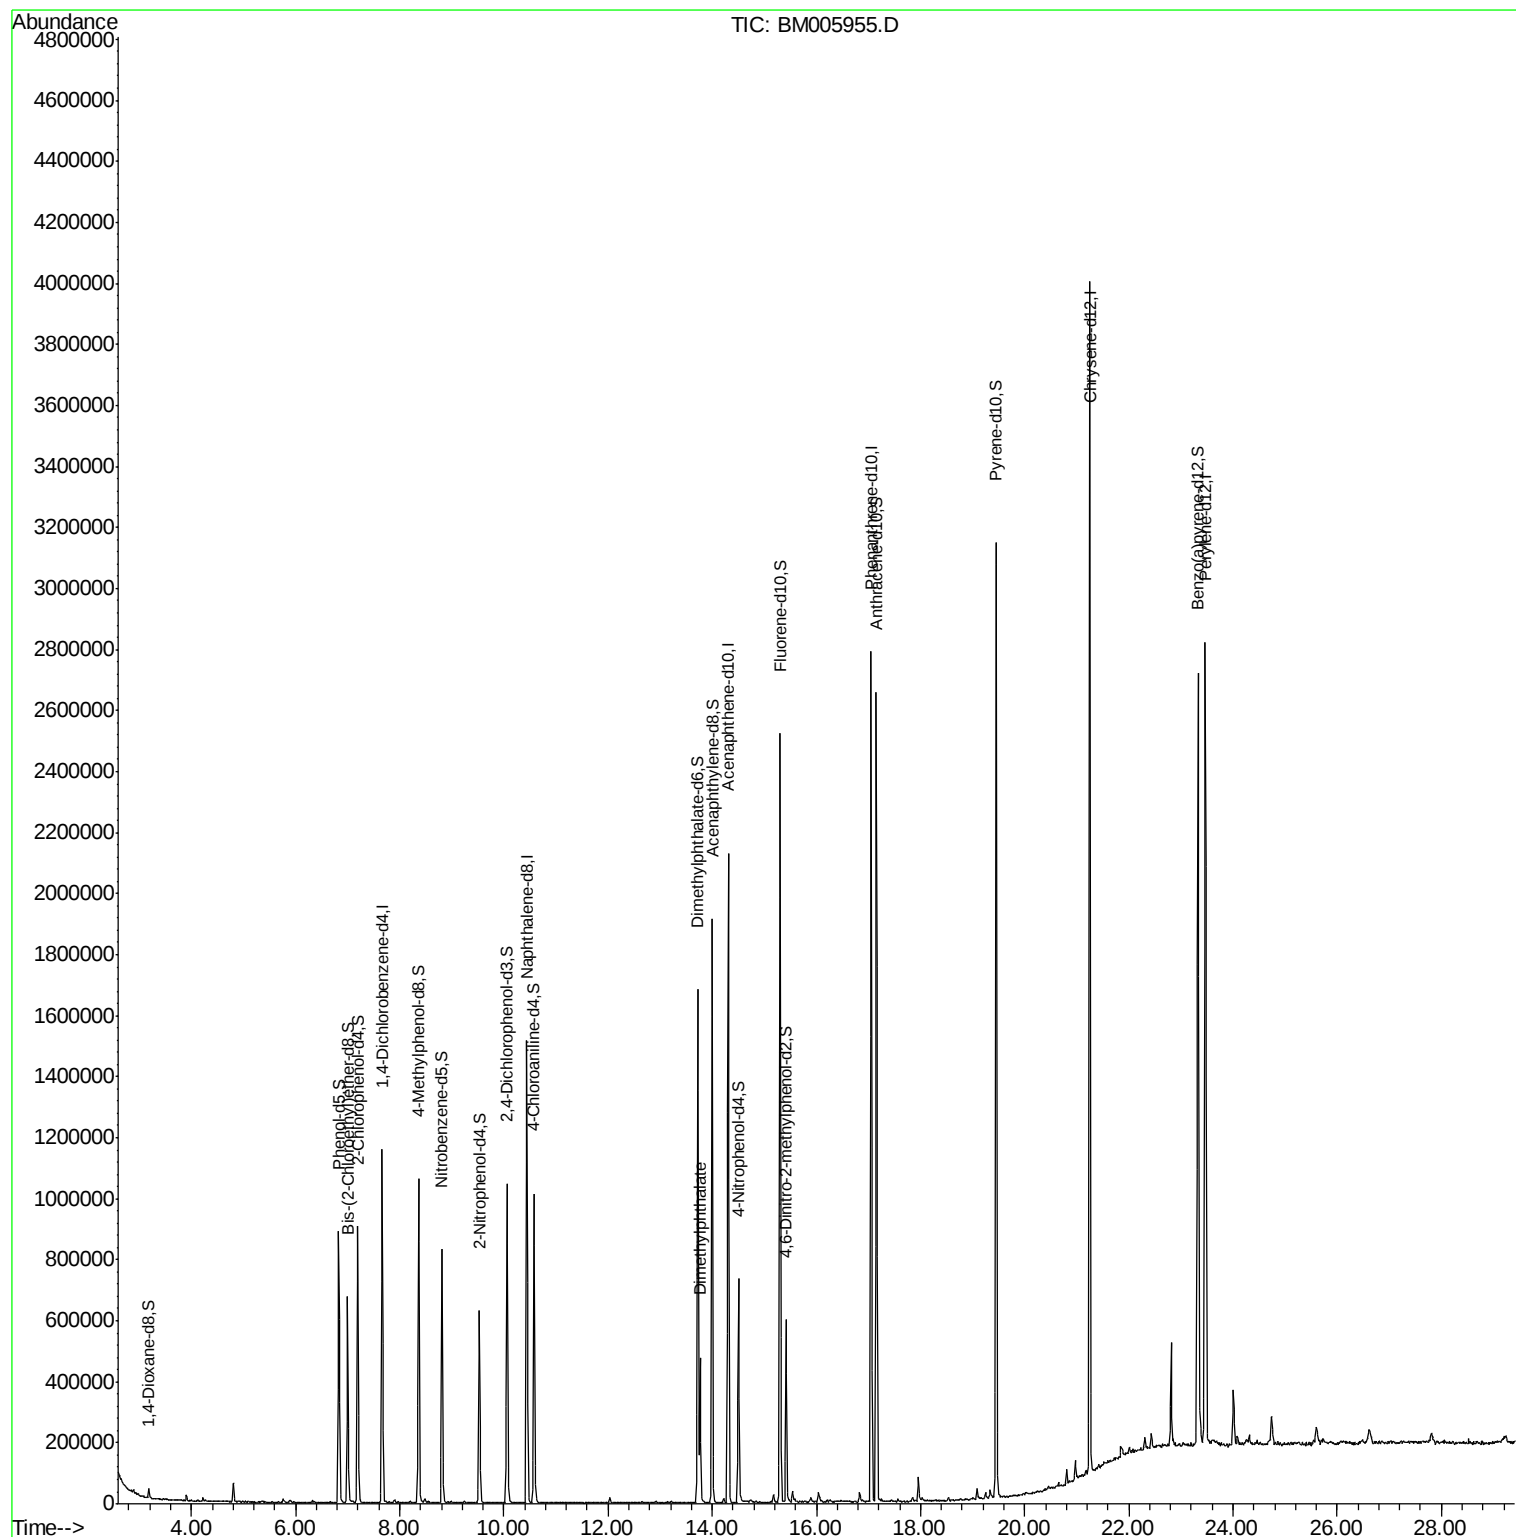

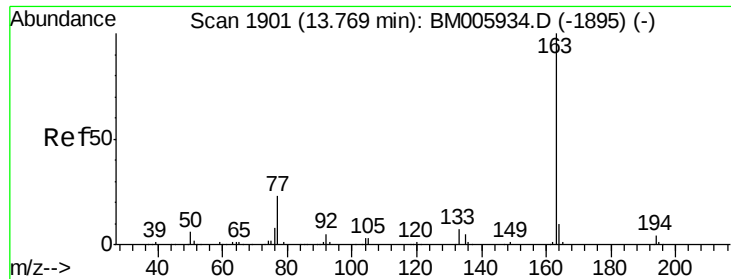

#44
 Dimethylphthalate
 Concen: 5.07 ng/ul
 RT: 13.77 min Scan# 1901
 Delta R.T. -0.00 min
 Lab File: BM005955.D
 Acq: 24 Jun 2016 06:35

Instrument :
 BNA_M
 ClientSampleId :
 D9Z46

Tot Ion:	163	Resp:	288195
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.1	4.7
164	9.8	7.9	11.9

