

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
 Data File : BM005937.D
 Acq On : 23 Jun 2016 19:48
 Operator : UM/SJ
 Sample : H3608-17
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC391

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.234	614	620	625	rVB	43410	68684	1.01%	0.110%
2	6.828	713	721	729	rBV	262378	430268	6.30%	0.687%
3	6.998	744	750	763	rBV	861235	1399234	20.48%	2.233%
4	7.193	777	783	795	rBV	989733	1618622	23.69%	2.583%
5	7.663	855	863	871	rBV	1030877	1645461	24.09%	2.626%
6	8.363	972	982	993	rBV	677468	1139963	16.69%	1.819%
7	8.816	1051	1059	1073	rBV	1079199	1837477	26.90%	2.933%
8	9.528	1173	1180	1191	rBV	844801	1469267	21.51%	2.345%
9	10.063	1264	1271	1283	rBV	1238182	2121844	31.06%	3.386%
10	10.445	1327	1336	1347	rBV	1304099	2314252	33.88%	3.694%
11	13.722	1886	1893	1910	rBV	2302336	3346046	48.98%	5.340%
12	13.998	1933	1940	1950	rBV	2507714	3767232	55.15%	6.013%
13	14.310	1986	1993	2001	rBV2	1835186	2893651	42.36%	4.618%
14	14.504	2020	2026	2036	rBV	230458	366733	5.37%	0.585%
15	15.304	2155	2162	2170	rBV	3336364	4962931	72.65%	7.921%
16	15.421	2176	2182	2198	rBV	1116013	1566954	22.94%	2.501%
17	17.057	2453	2460	2468	rBV	2398075	3436861	50.31%	5.485%
18	17.157	2470	2477	2490	rBV2	3718117	5462992	79.97%	8.719%
19	19.086	2800	2805	2809	rBV	52104	68982	1.01%	0.110%
20	19.456	2861	2868	2878	rBV2	4455140	6519450	95.43%	10.405%
21	21.250	3167	3173	3185	rBV	3375902	4391513	64.28%	7.009%
22	22.809	3435	3438	3444	rVB	73012	99429	1.46%	0.159%
23	23.327	3518	3526	3540	rBV2	3528476	6831393	100.00%	10.903%
24	23.468	3543	3550	3565	rVB	2269309	4356261	63.77%	6.953%
25	24.009	3638	3642	3650	rVB	137997	250262	3.66%	0.399%
26	24.744	3763	3767	3777	rVB	134191	290658	4.25%	0.464%


Sum of corrected areas: 62656420

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005937.D
Acq On : 23 Jun 2016 19:48
Operator : UM/SJ
Sample : H3608-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC391

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

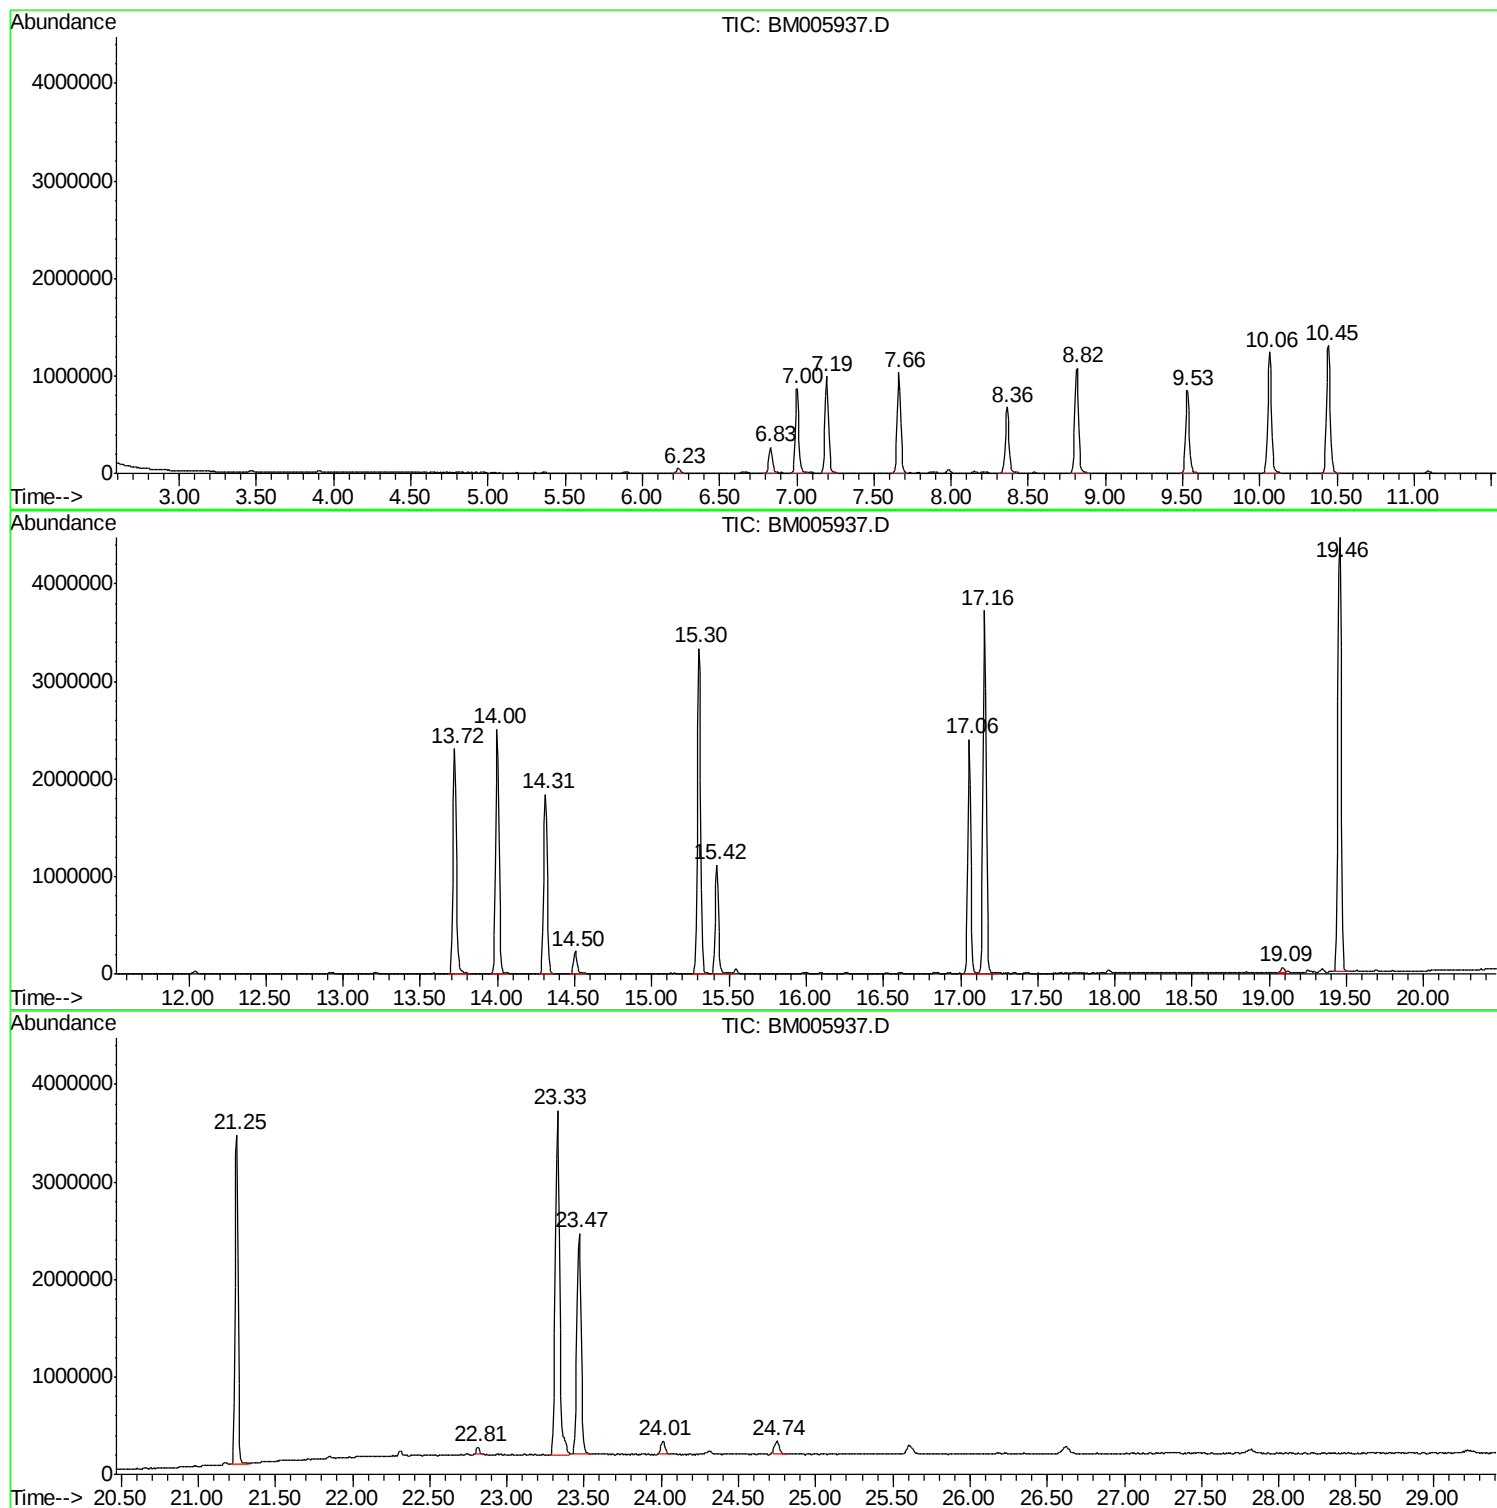

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005937.D
Acq On : 23 Jun 2016 19:48
Operator : UM/SJ
Sample : H3608-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC391

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005937.D
Acq On : 23 Jun 2016 19:48
Operator : UM/SJ
Sample : H3608-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC391

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc