

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005938.D
Acq On : 23 Jun 2016 20:24
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.828	715	721	730	rBV	272401	443014	7.65%	0.831%
2	7.004	742	751	762	rBV	754756	1230326	21.25%	2.308%
3	7.192	776	783	797	rVB	850984	1385551	23.93%	2.599%
4	7.663	855	863	873	rVB	795886	1264460	21.84%	2.372%
5	8.363	974	982	993	rBV	713209	1153859	19.93%	2.164%
6	8.810	1051	1058	1073	rBV	897804	1590811	27.48%	2.984%
7	9.528	1172	1180	1195	rBV	731136	1275371	22.03%	2.392%
8	10.063	1264	1271	1285	rBV	1088974	1886304	32.58%	3.538%
9	10.445	1328	1336	1347	rBV	1017253	1786165	30.85%	3.350%
10	10.580	1353	1359	1366	rBV	95515	157471	2.72%	0.295%
11	13.721	1885	1893	1910	rBV	1959406	2908985	50.25%	5.456%
12	13.998	1931	1940	1953	rBV	2306239	3500538	60.47%	6.565%
13	14.310	1986	1993	2006	rVB2	1491570	2314875	39.99%	4.342%
14	14.504	2020	2026	2041	rBV	215378	348865	6.03%	0.654%
15	15.304	2155	2162	2173	rBV	2893402	4355036	75.23%	8.168%
16	15.421	2176	2182	2196	rBV	877212	1252602	21.64%	2.349%
17	17.057	2453	2460	2468	rBV2	1906490	2820237	48.72%	5.289%
18	17.156	2470	2477	2490	rBV2	3125535	4771555	82.42%	8.949%
19	19.456	2861	2868	2877	rBV	3929879	5579358	96.38%	10.464%
20	21.250	3167	3173	3182	rBV	2717907	3576111	61.77%	6.707%
21	23.327	3519	3526	3540	rVB2	2984008	5789092	100.00%	10.858%
22	23.468	3543	3550	3559	rVB	1869452	3478853	60.09%	6.525%
23	24.015	3638	3643	3650	rVB	111120	211372	3.65%	0.396%
24	24.750	3764	3768	3776	rVB	109821	236969	4.09%	0.444%


Sum of corrected areas: 53317780

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005938.D
Acq On : 23 Jun 2016 20:24
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

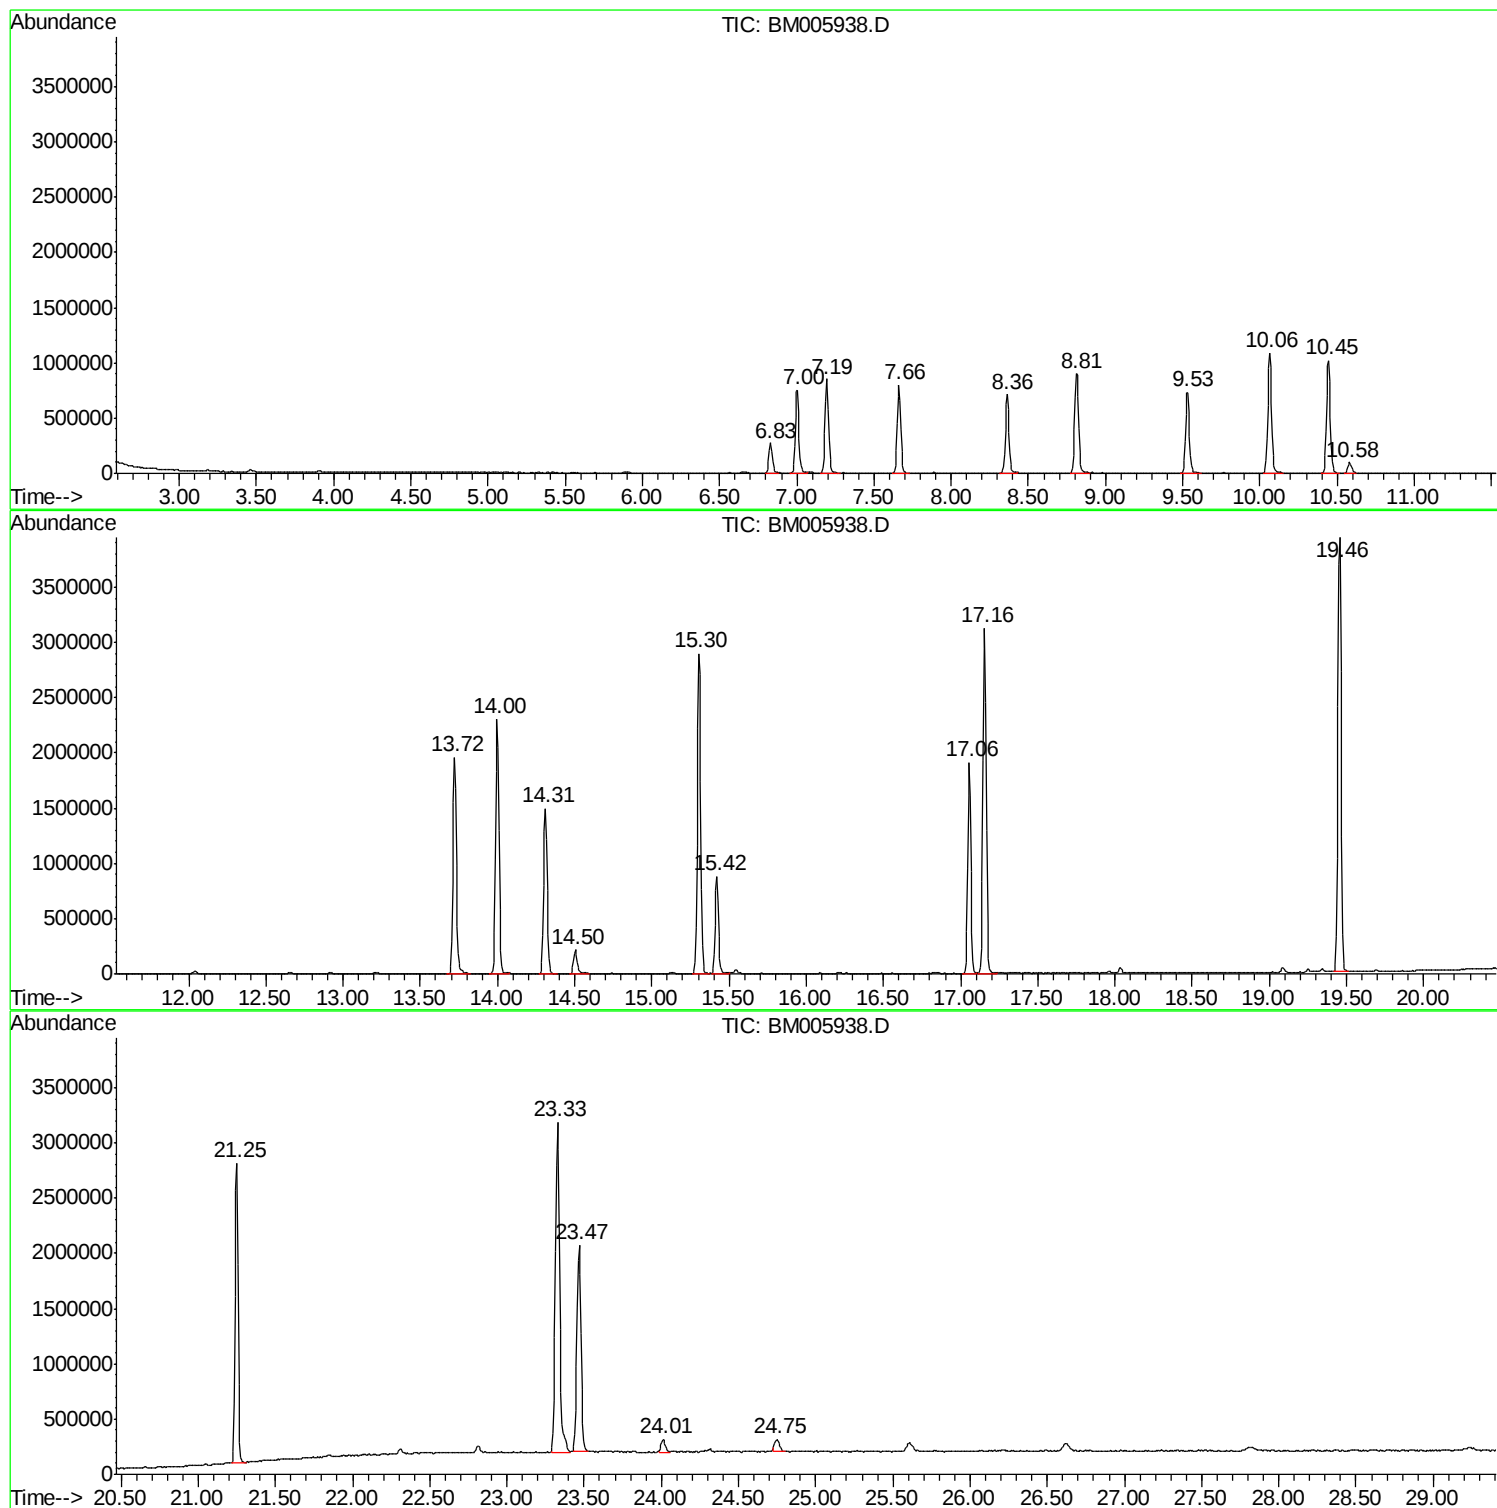

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005938.D
Acq On : 23 Jun 2016 20:24
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005938.D
Acq On : 23 Jun 2016 20:24
Operator : UM/SJ
Sample : H3608-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC385

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc