

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
 Data File : BM005942.D
 Acq On : 23 Jun 2016 22:48
 Operator : UM/SJ
 Sample : H3612-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.828	714	721	736	rVB	700639	1188124	22.16%	2.190%
2	6.999	743	750	761	rBV	536205	859703	16.03%	1.584%
3	7.193	774	783	796	rBV	687652	1142572	21.31%	2.106%
4	7.663	856	863	873	rBV	1105683	1804123	33.64%	3.325%
5	8.363	972	982	997	rBV	819568	1376258	25.66%	2.536%
6	8.810	1051	1058	1070	rBV	613578	1067999	19.92%	1.968%
7	9.528	1172	1180	1194	rBV	473630	831416	15.50%	1.532%
8	10.063	1264	1271	1282	rBV	793656	1346493	25.11%	2.482%
9	10.445	1328	1336	1348	rVB	1447068	2603686	48.55%	4.798%
10	10.581	1351	1359	1374	rVV	742488	1346047	25.10%	2.481%
11	13.722	1887	1893	1897	rBV	1274327	1882960	35.11%	3.470%
12	13.769	1897	1901	1920	rVB	1270750	1912296	35.66%	3.524%
13	13.998	1930	1940	1952	rBV	1510095	2333223	43.51%	4.300%
14	14.310	1986	1993	2003	rVB2	2226298	3403403	63.47%	6.272%
15	14.504	2019	2026	2041	rBV	603606	920290	17.16%	1.696%
16	15.304	2156	2162	2170	rBV	1987278	2944482	54.91%	5.427%
17	15.422	2176	2182	2193	rBV	451160	682880	12.73%	1.259%
18	16.833	2417	2422	2428	rBV2	33744	61771	1.15%	0.114%
19	17.057	2453	2460	2468	rBV	2884050	4184926	78.04%	7.713%
20	17.157	2469	2477	2488	rVV2	2087979	3207813	59.82%	5.912%
21	17.957	2609	2613	2619	rBV2	60107	90111	1.68%	0.166%
22	19.451	2861	2867	2877	rBV	2743113	3906482	72.85%	7.199%
23	20.968	3122	3125	3132	rBV4	76178	110751	2.07%	0.204%
24	21.174	3157	3160	3166	rBV	106527	139041	2.59%	0.256%
25	21.251	3167	3173	3181	rVV	3838412	5362448	100.00%	9.883%
26	23.327	3519	3526	3532	rBV	2025330	3823501	71.30%	7.047%
27	23.468	3542	3550	3562	rBV	2717906	5289025	98.63%	9.747%
28	24.009	3638	3642	3649	rVB2	121134	218227	4.07%	0.402%
29	24.750	3764	3768	3775	rVB3	117385	220416	4.11%	0.406%


Sum of corrected areas: 54260467

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062316\
Data File : BM005942.D
Acq On : 23 Jun 2016 22:48
Operator : UM/SJ
Sample : H3612-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z37

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

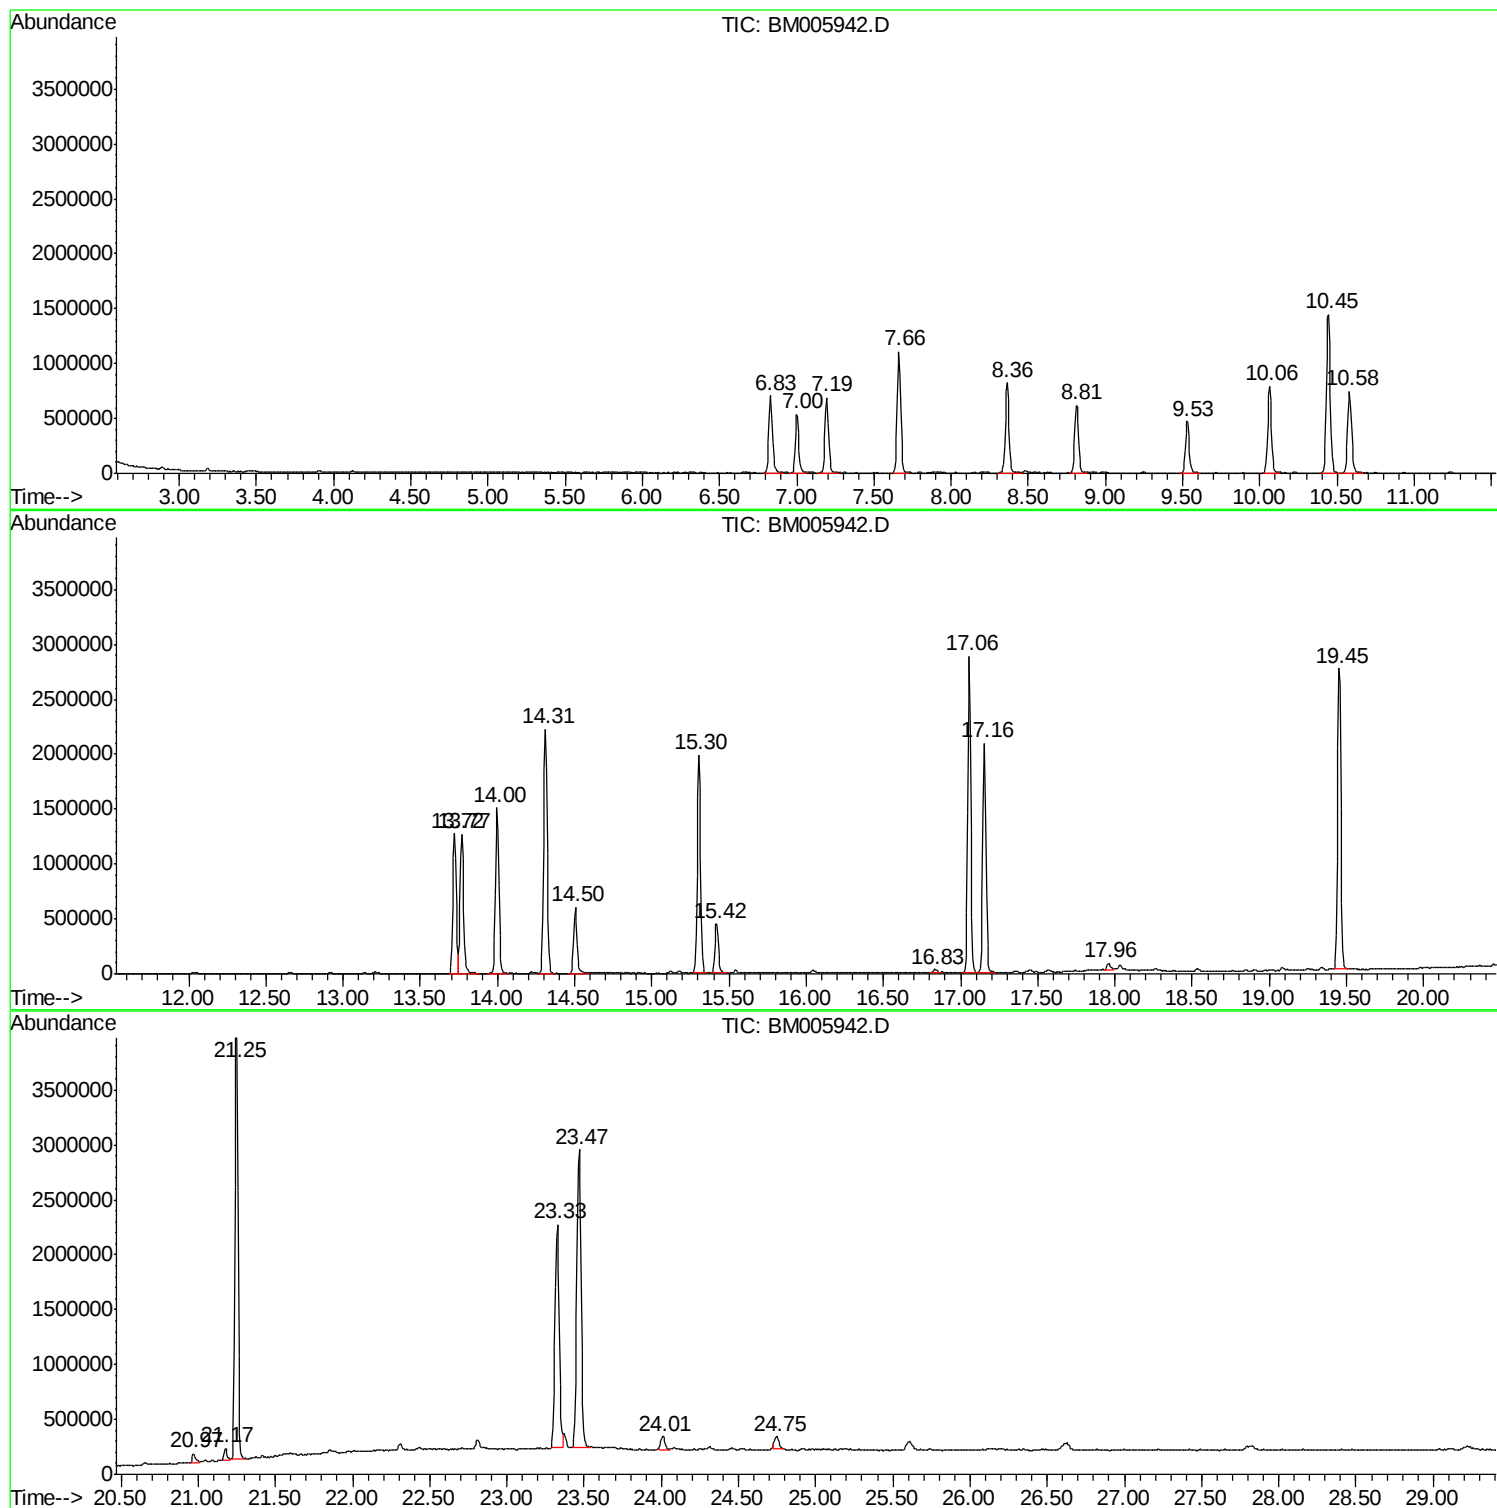

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005942.D
Acq On : 23 Jun 2016 22:48
Operator : UM/SJ
Sample : H3612-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z37

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062316\
Data File : BM005942.D
Acq On : 23 Jun 2016 22:48
Operator : UM/SJ
Sample : H3612-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z37

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc