

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010688.D
 Acq On : 23 Jun 2017 12:51
 Operator : SJ/JU
 Sample : I3625-19
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5A01

Quant Time: Jun 24 03:37:22 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 24 03:35:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	75966	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	347450	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	226337	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.87	188	547188	20.00	ng/ul	0.00
75) Chrysene-d12	21.09	240	578640	20.00	ng/ul	0.00
83) Perylene-d12	23.23	264	421834	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	6135	4.63	ng/uL	0.00
5) Phenol-d5	6.65	99	151679	20.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	85146	20.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	118592	23.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	134767	22.46	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	61602	24.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	72839	25.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	154514	25.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	168962	26.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	525904	26.47	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	599553	25.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	69679	19.93	ng/ul	0.00
57) Fluorene-d10	15.12	176	431759	25.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	73604	21.90	ng/ul	0.00
70) Anthracene-d10	16.87	188	547188	20.71	ng/ul	-0.09
76) Pyrene-d10	19.28	212	834121	31.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.10	264	550728	27.01	ng/ul	0.01

Target Compounds

					Qvalue	
6) Phenol	6.67	94	18008	2.416	ng/ul#	87
28) Naphthalene	10.27	128	50397	2.915	ng/ul	98
30) 4-Chloroaniline	10.27	127	7012	1.101	ng/ul#	12
34) 2-Methylnaphthalene	11.89	142	55544	3.996	ng/ul	90
44) Dimethylphthalate	13.58	163	164282	8.435	ng/ul	99
47) Acenaphthylene	13.83	152	30552	1.388	ng/ul#	87
49) Acenaphthene	14.17	153	101765	6.853	ng/ul	96
53) Dibenzofuran	14.52	168	84826	3.772	ng/ul	98
58) Fluorene	15.17	166	138048	7.332	ng/ul	97
69) Phenanthrene	16.92	178	2989160	102.754	ng/ul	98
71) Anthracene	17.00	178	435150	14.519	ng/ul	99
72) Carbazole	17.27	167	273862	10.474	ng/ul	99
74) Fluoranthene	18.94	202	4139425	110.412	ng/ul#	96
77) Pyrene	19.32	202	3351465	100.276	ng/ul#	97
80) Benzo(a)anthracene	21.07	228	1597098	47.397	ng/ul	97
82) Chrysene	21.13	228	1580261	52.599	ng/ul	97
85) Benzo(b)fluoranthene	22.60	252	1495622	54.619	ng/ul#	98
86) Benzo(k)fluoranthene	22.60	252	1495622	57.614	ng/ul#	96
88) Benzo(a)pyrene	23.14	252	929141	36.857	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.34	276	520994	19.927	ng/ul#	96
90) Dibenzo(a,h)anthracene	25.34	278	155827	7.152	ng/ul#	96
91) Benzo(g,h,i)perylene	25.99	276	386929	18.591	ng/ul	99

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010688.D
Acq On : 23 Jun 2017 12:51
Operator : SJ/JU
Sample : I3625-19
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A01

Quant Time: Jun 24 03:37:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 24 03:35:21 2017
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010688.D
Acq On : 23 Jun 2017 12:51
Operator : SJ/JU
Sample : I3625-19
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A01

Quant Time: Jun 24 03:37:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 24 03:35:21 2017
Response via : Initial Calibration

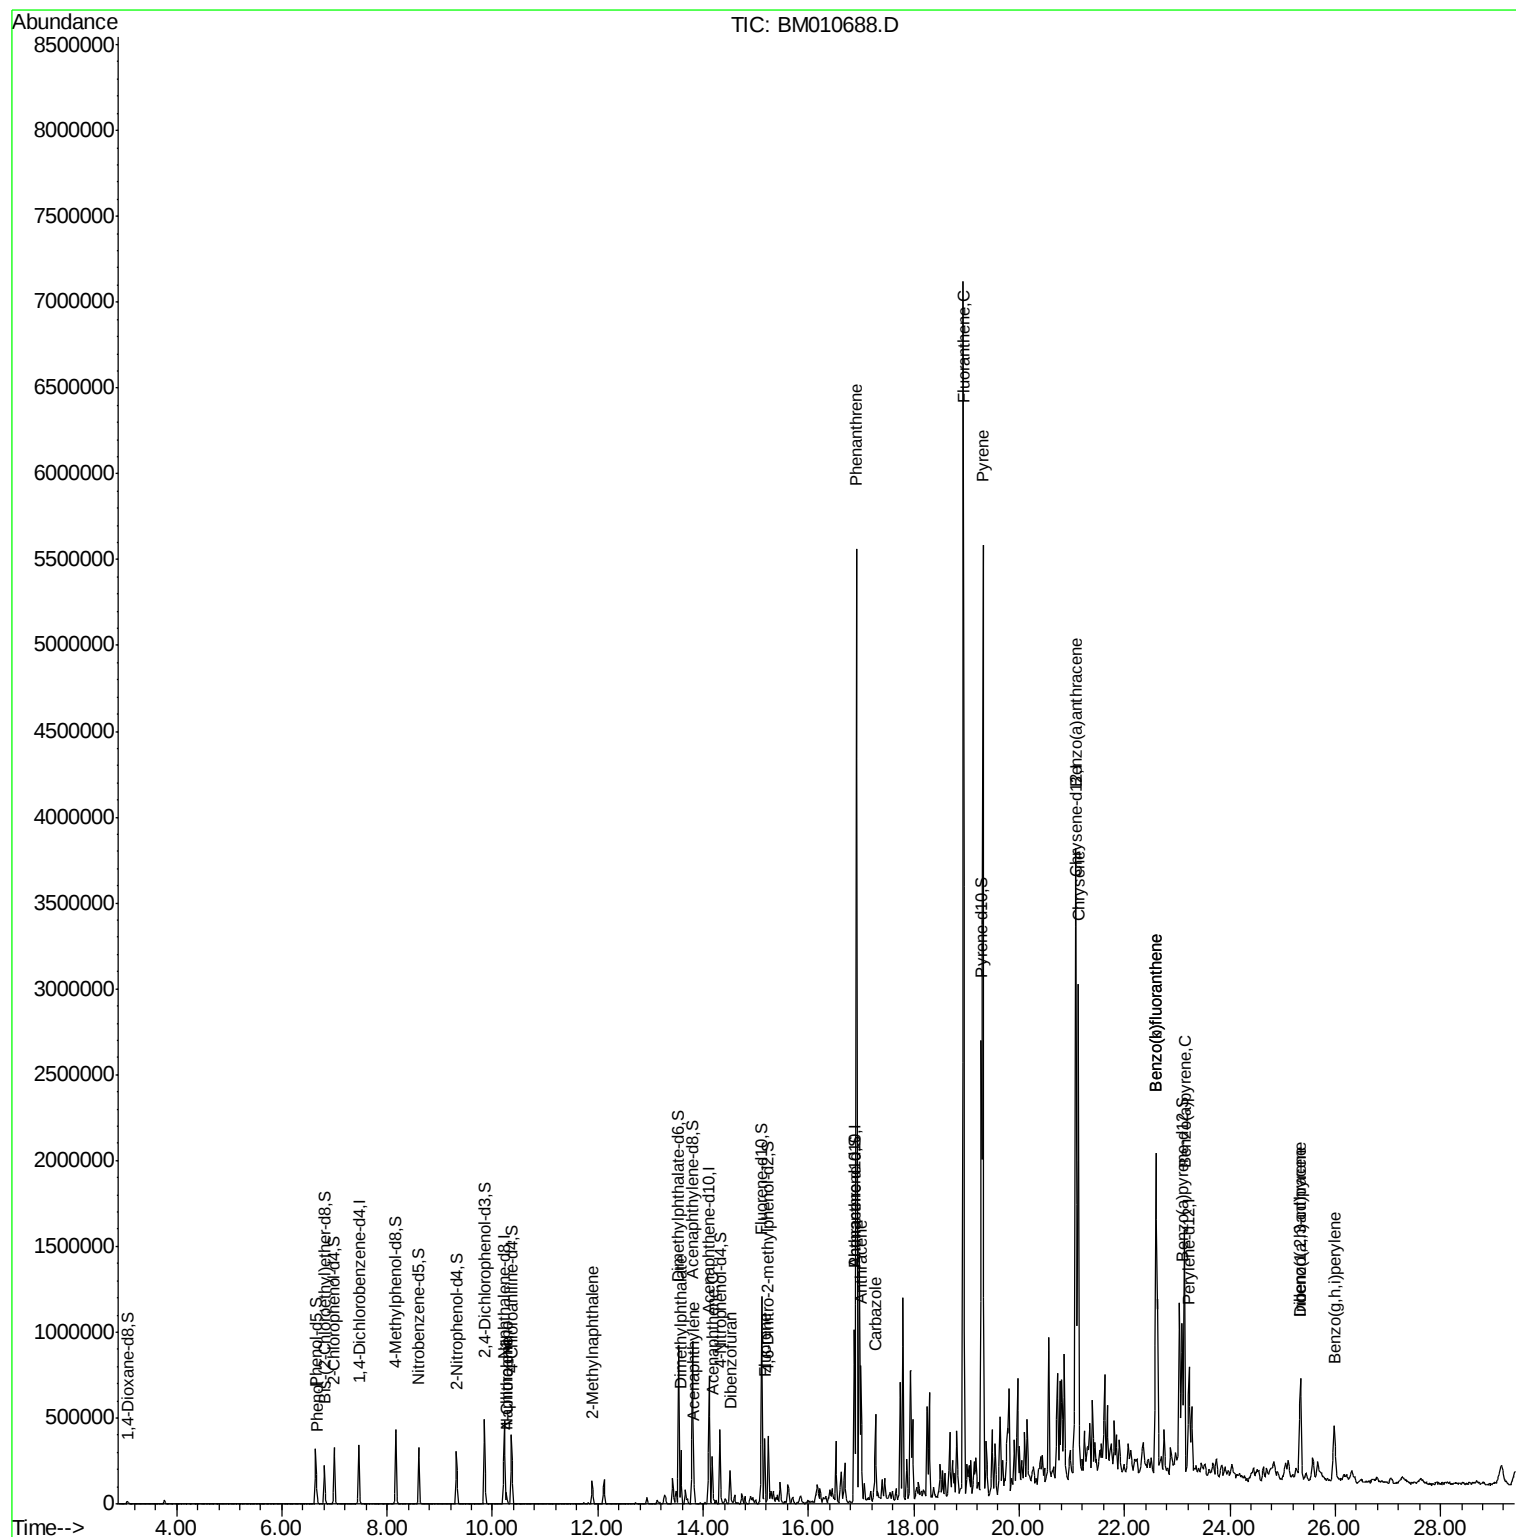



#6

Phenol

Concen: 2.416 ng/ul

RT: 6.67 min Scan# 644

Delta R.T. -0.00 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01





Tgt Ion: 94 Resp: 18008

Ion Ratio Lower Upper

94 100

65 26.2 28.2 42.4#

66 50.4 47.2 70.8

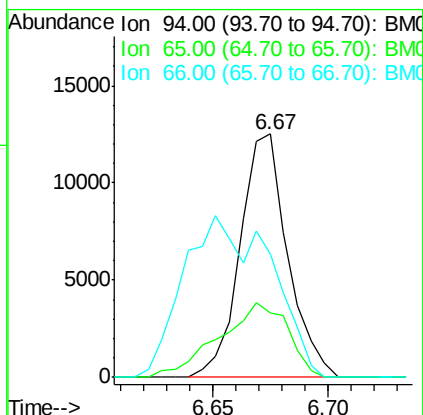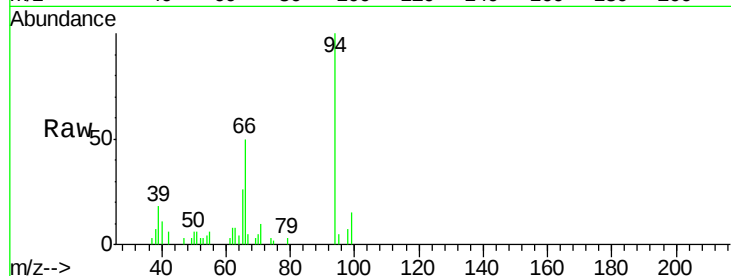

#28

Naphthalene

Concen: 2.915 ng/ul

RT: 10.27 min Scan# 1255

Delta R.T. -0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51




Tgt Ion: 128 Resp: 50397


Ion Ratio Lower Upper

128 100

129 11.6 8.8 13.2

127 12.2 10.6 16.0



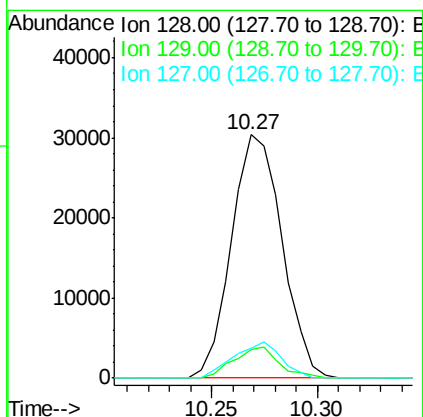





#30
4-Chloroaniline
Concen: 1.101 ng/ul
RT: 10.27 min Scan# 1256
Delta R.T. -0.11 min
Lab File: BM010688.D
Acq: 23 Jun 2017 12:51




Instrument :
BNA_M
ClientSampleId :
F5A01


Tgt Ion:127 Resp: 7012
Ion Ratio Lower Upper
127 100
129 87.0 28.4 42.6#

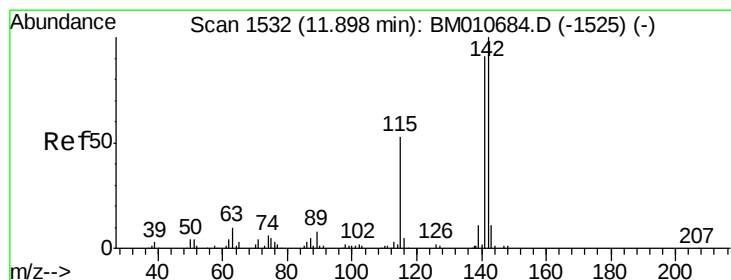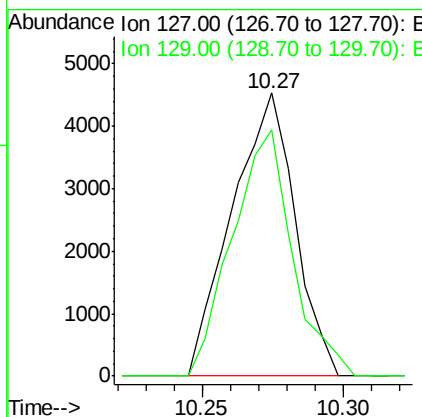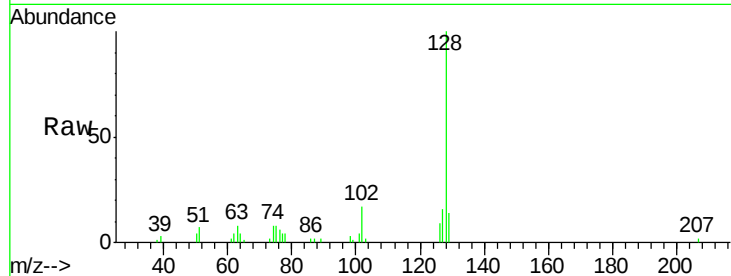

#34
2-Methylnaphthalene
Concen: 3.996 ng/ul
RT: 11.89 min Scan# 1531
Delta R.T. -0.01 min
Lab File: BM010688.D
Acq: 23 Jun 2017 12:51

Tgt Ion:142 Resp: 55544
Ion Ratio Lower Upper
142 100
141 83.3 74.1 111.1


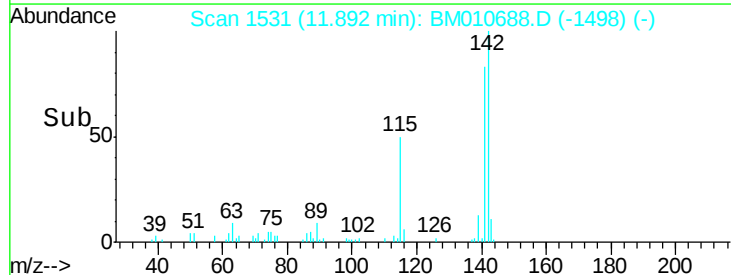
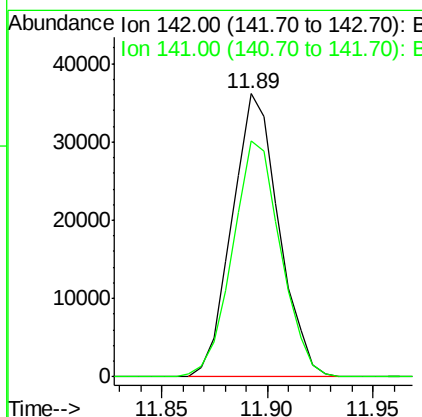





#44
Dimethylphthalate
Concen: 8.435 ng/ul
RT: 13.58 min Scan# 1818
Delta R.T. -0.00 min
Lab File: BM010688.D
Acq: 23 Jun 2017 12:51




Instrument :
BNA_M
ClientSampleId :
F5A01


Tgt Ion:163 Resp: 164282
Ion Ratio Lower Upper
163 100
194 4.9 3.5 5.3
164 10.5 8.2 12.4

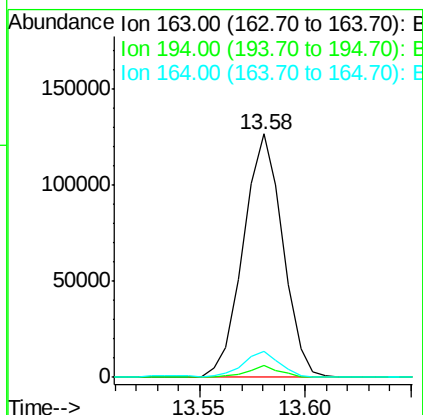

#47
Acenaphthylene
Concen: 1.388 ng/ul
RT: 13.83 min Scan# 1860
Delta R.T. -0.00 min
Lab File: BM010688.D
Acq: 23 Jun 2017 12:51

Tgt Ion:152 Resp: 30552
Ion Ratio Lower Upper
152 100
151 15.5 16.3 24.5#
153 19.6 10.2 15.4#

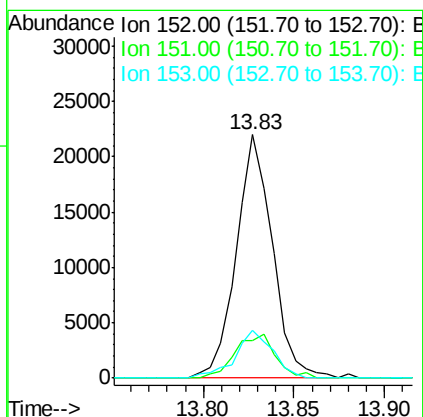

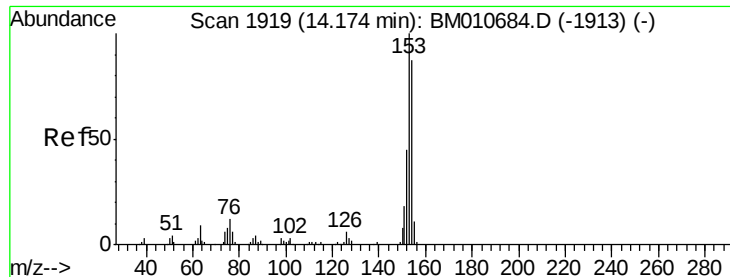

#49

Acenaphthene

Concen: 6.853 ng/ul

RT: 14.17 min Scan# 1919

Delta R.T. -0.00 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:153 Resp: 101765

Ion Ratio Lower Upper

153 100

152 47.9 37.6 56.4




154 83.3 70.4 105.6

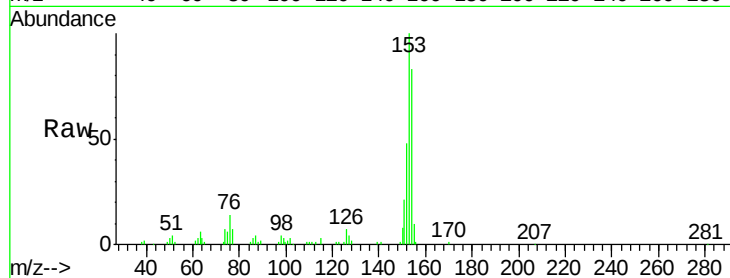

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

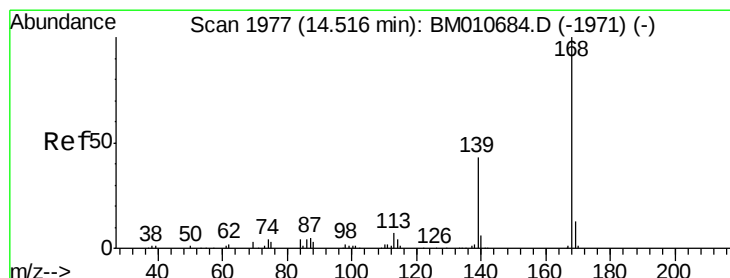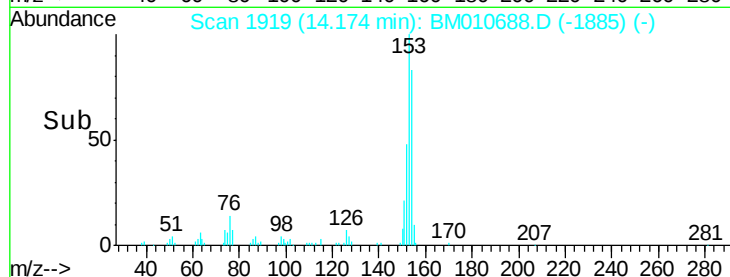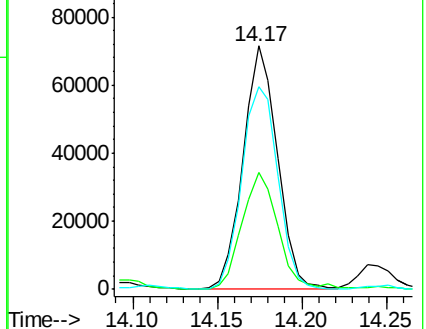

#53

Dibenzofuran

Concen: 3.772 ng/ul

RT: 14.52 min Scan# 1977

Delta R.T. -0.00 min

Lab File: BM010688.D


Acq: 23 Jun 2017 12:51

Tgt Ion:168 Resp: 84826

Ion Ratio Lower Upper



168 100


139 37.4 30.8 46.2

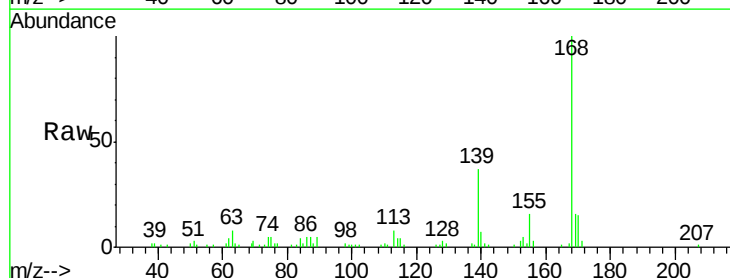

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

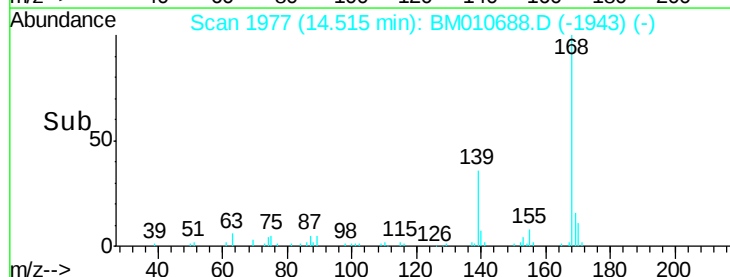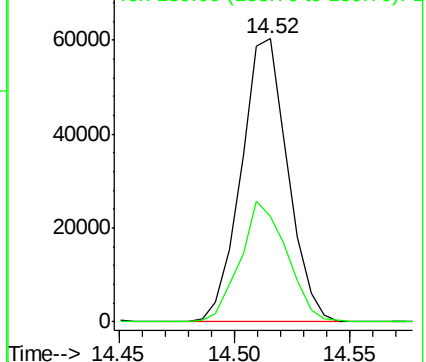



#58

Fluorene

Concen: 7.332 ng/ul

RT: 15.17 min Scan# 2088

Delta R.T. -0.00 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:166 Resp: 138048

Ion Ratio Lower Upper

166 100

165 95.0 77.9 116.9




167 14.6 10.6 16.0

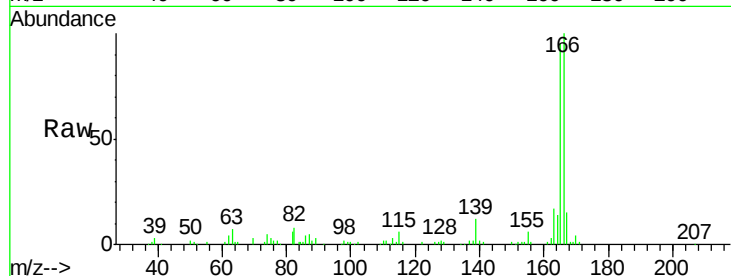

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

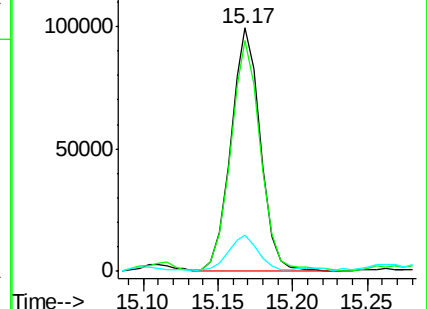

#69

Phenanthrene

Concen: 102.754 ng/ul

RT: 16.92 min Scan# 2385

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51


Tgt Ion:178 Resp: 2989160

Ion Ratio Lower Upper

178 100

179 15.2 12.6 19.0



176 19.9 14.9 22.3




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

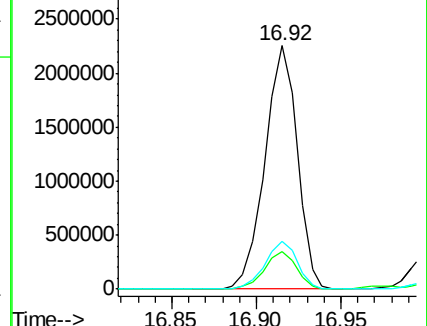







#71
 Anthracene
 Concen: 14.519 ng/ul
 RT: 17.00 min Scan# 2399
 Delta R.T. -0.00 min
 Lab File: BM010688.D
 Acq: 23 Jun 2017 12:51

Instrument :
 BNA_M
 ClientSampleId :
 F5A01

Tgt Ion:178 Resp: 435150
 Ion Ratio Lower Upper
 178 100
 179 15.7 11.7 17.5
 176 18.1 14.6 21.8




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

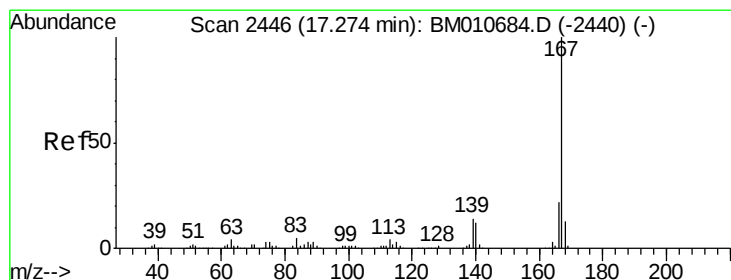
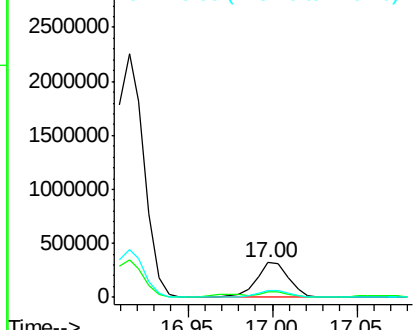



#72
 Carbazole
 Concen: 10.474 ng/ul
 RT: 17.27 min Scan# 2446
 Delta R.T. -0.00 min
 Lab File: BM010688.D
 Acq: 23 Jun 2017 12:51

Tgt Ion:167 Resp: 273862
 Ion Ratio Lower Upper
 167 100
 166 21.5 17.1 25.7
 139 13.8 10.0 15.0



Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E

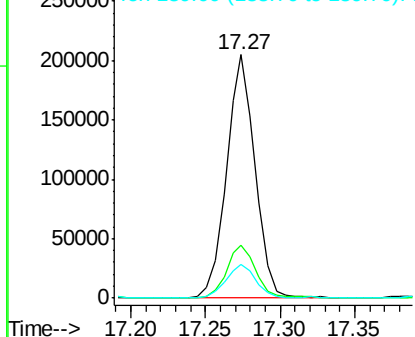

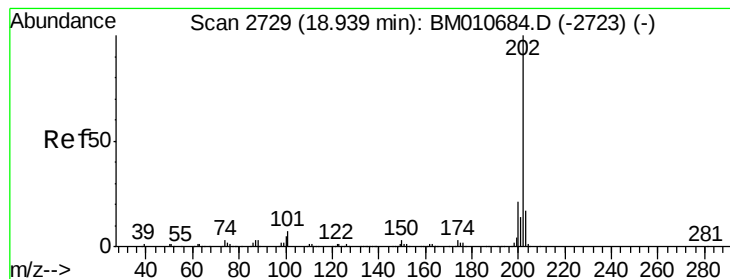

#74

Fluoranthene

Concen: 110.412 ng/ul

RT: 18.94 min Scan# 2730

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:202 Resp: 4139425

Ion Ratio Lower Upper

202 100

101 7.4 4.6 7.0#


100 5.4 3.4 5.2#

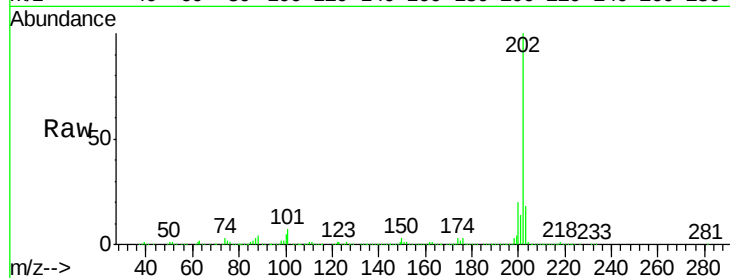



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

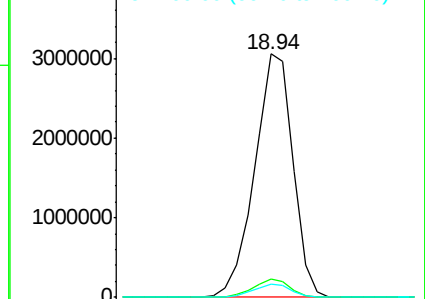

Time-->

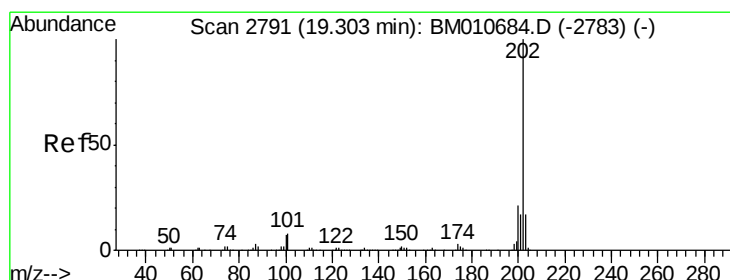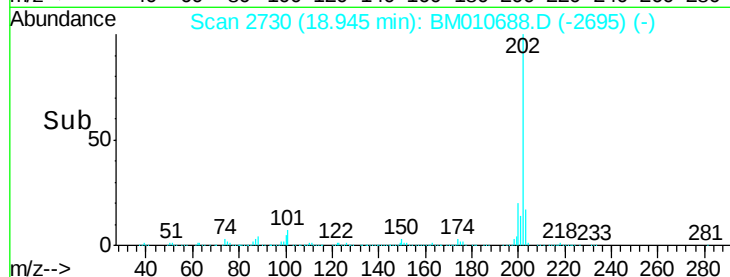

#77

Pyrene

Concen: 100.276 ng/ul

RT: 19.32 min Scan# 2793

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51


Tgt Ion:202 Resp: 3351465

Ion Ratio Lower Upper

202 100

101 7.9 5.1 7.7#


100 6.4 4.9 7.3

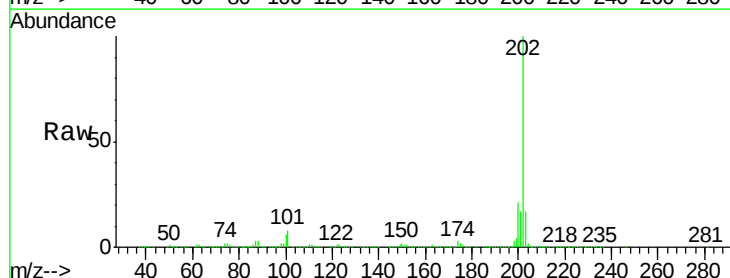


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

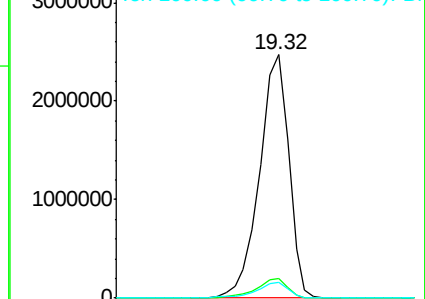

Time-->

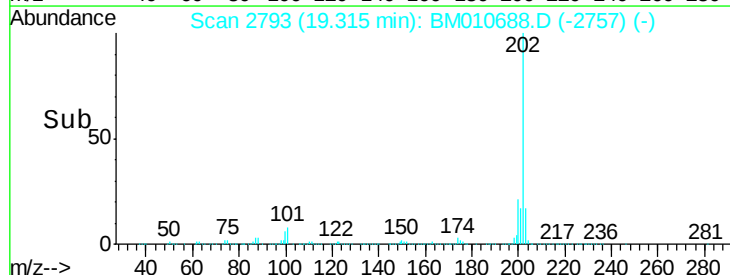



#80

Benzo(a)anthracene

Concen: 47.397 ng/ul

RT: 21.07 min Scan# 3091

Delta R.T. -0.00 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:228 Resp: 1597098

Ion Ratio Lower Upper




228 100

229 20.8 15.4 23.0

226 27.7 21.4 32.0



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

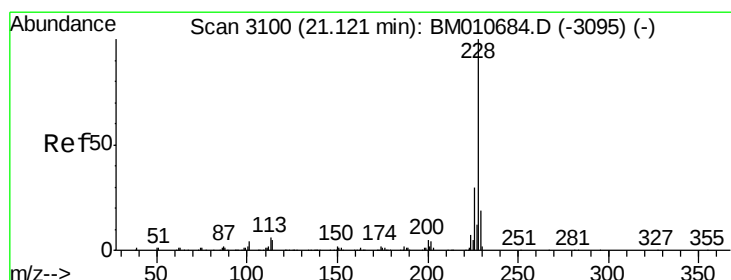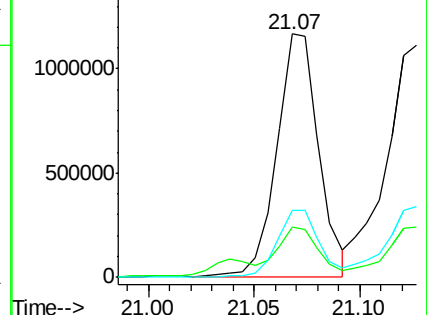

#82

Chrysene

Concen: 52.599 ng/ul

RT: 21.13 min Scan# 3101

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51


Tgt Ion:228 Resp: 1580261

Ion Ratio Lower Upper



228 100


226 30.4 23.4 35.2

229 21.6 15.5 23.3



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

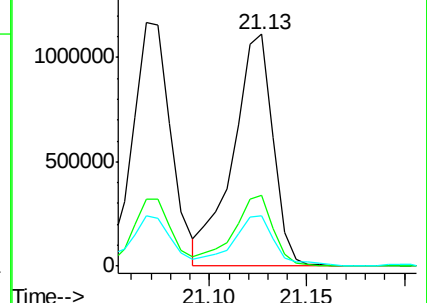



#85

Benzo(b)fluoranthene

Concen: 54.619 ng/ul

RT: 22.60 min Scan# 3351

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:252 Resp: 1495622

Ion Ratio Lower Upper

252 100

253 22.9 17.9 26.9




125 5.9 3.6 5.4#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

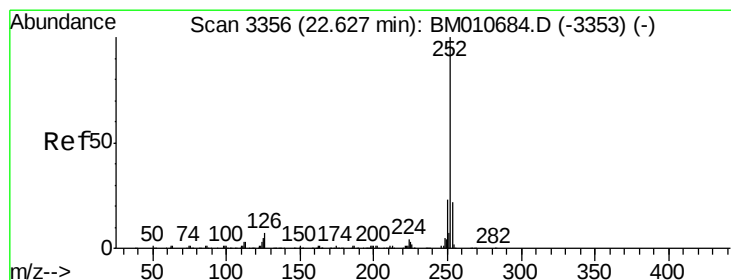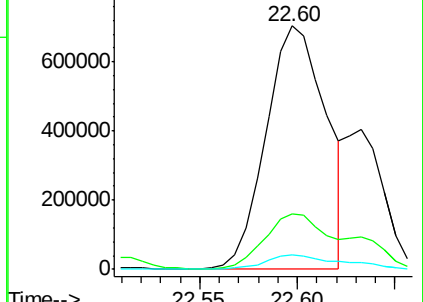

#86

Benzo(k)fluoranthene

Concen: 57.614 ng/ul

RT: 22.60 min Scan# 3351

Delta R.T. -0.03 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51


Tgt Ion:252 Resp: 1495622

Ion Ratio Lower Upper

252 100

253 22.9 17.1 25.7



125 5.9 3.4 5.2#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

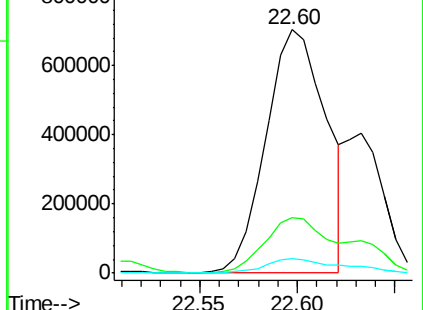

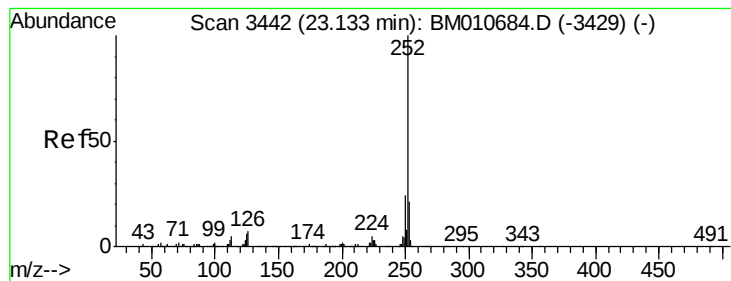

#88

Benzo(a)pyrene

Concen: 36.857 ng/ul

RT: 23.14 min Scan# 3443

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:252 Resp: 929141

Ion Ratio Lower Upper

252 100

253 22.9 18.2 27.2




125 5.9 4.0 6.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

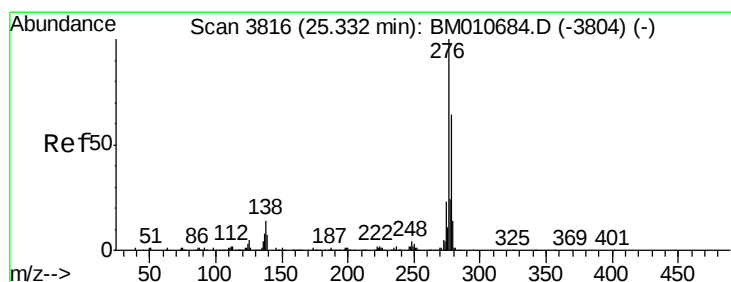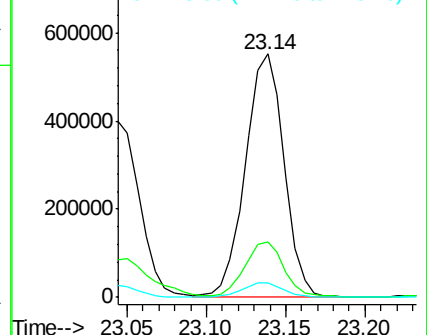

#89

Indeno(1,2,3-cd)pyrene

Concen: 19.927 ng/ul

RT: 25.34 min Scan# 3817

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51


Tgt Ion:276 Resp: 520994

Ion Ratio Lower Upper

276 100

138 15.8 9.3 13.9#



277 24.4 19.9 29.9

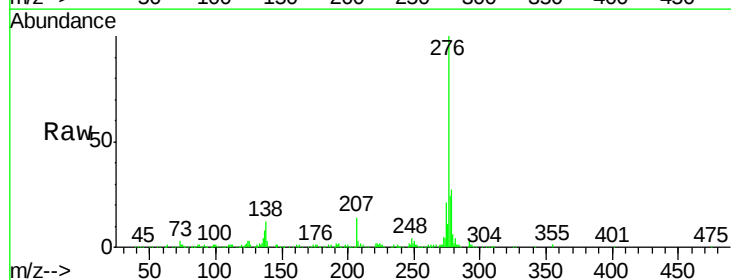


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

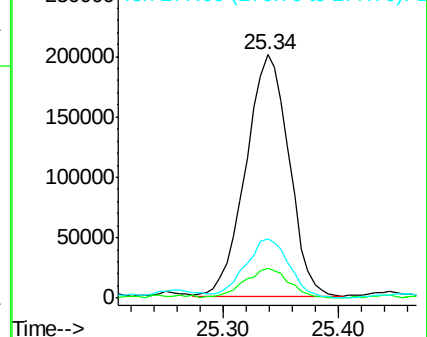



#90

Dibenzo(a,h)anthracene

Concen: 7.152 ng/ul

RT: 25.34 min Scan# 3817

Delta R.T. -0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51

Instrument :

BNA_M

ClientSampleId :

F5A01


Tgt Ion:278 Resp: 155827

Ion Ratio Lower Upper

278 100

139 13.0 5.8 8.8#




279 23.3 18.6 27.8

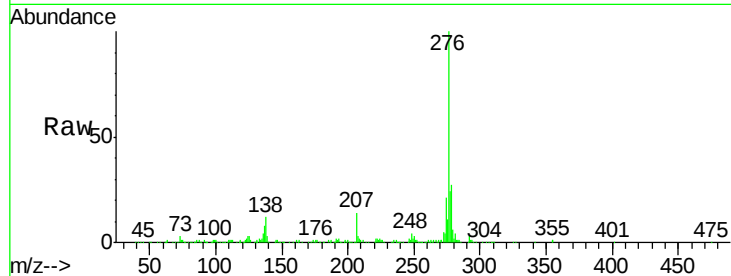

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

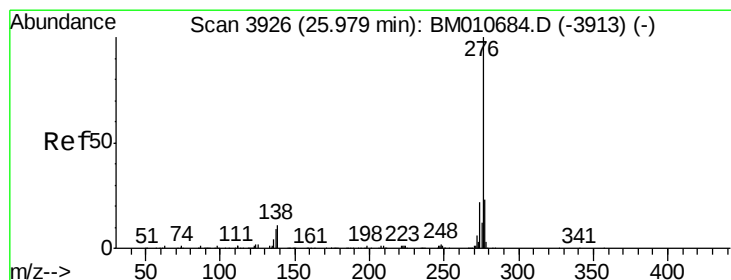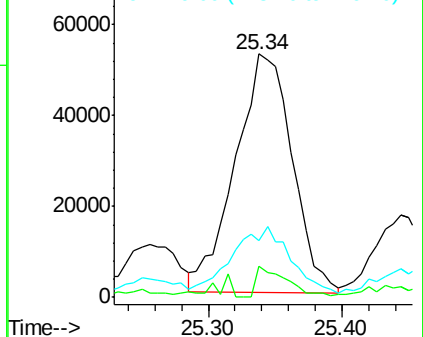

#91

Benzo(g,h,i)perylene

Concen: 18.591 ng/ul

RT: 25.99 min Scan# 3927

Delta R.T. 0.01 min

Lab File: BM010688.D

Acq: 23 Jun 2017 12:51


Tgt Ion:276 Resp: 386929

Ion Ratio Lower Upper

276 100

138 12.2 8.5 12.7

277 23.4 18.6 28.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

