

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010701.D
 Acq On : 23 Jun 2017 21:50
 Operator : SJ/JU
 Sample : I3657-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H2TR7

Quant Time: Jun 24 04:41:09 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 24 04:37:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	72153	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	339004	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	238450	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.87	188	589307	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	620618	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	471342	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.07	96	2514	2.00	ng/uL	0.00
5) Phenol-d5	6.65	99	64057	9.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	37271	9.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	51170	10.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	57378	10.07	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	26380	10.91	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.32	143	32814	11.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	62047	10.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	43463	7.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	243072	11.61	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	271274	11.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	26910	7.31	ng/ul	0.00
57) Fluorene-d10	15.11	176	206890	11.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	35685	9.86	ng/ul	0.00
70) Anthracene-d10	16.96	188	345971	12.16	ng/ul	0.00
76) Pyrene-d10	19.27	212	392155	13.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.09	264	273601	12.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.58	163	124068	6.047	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010701.D
Acq On : 23 Jun 2017 21:50
Operator : SJ/JU
Sample : I3657-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H2TR7

Quant Time: Jun 24 04:41:09 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 24 04:37:39 2017
Response via : Initial Calibration

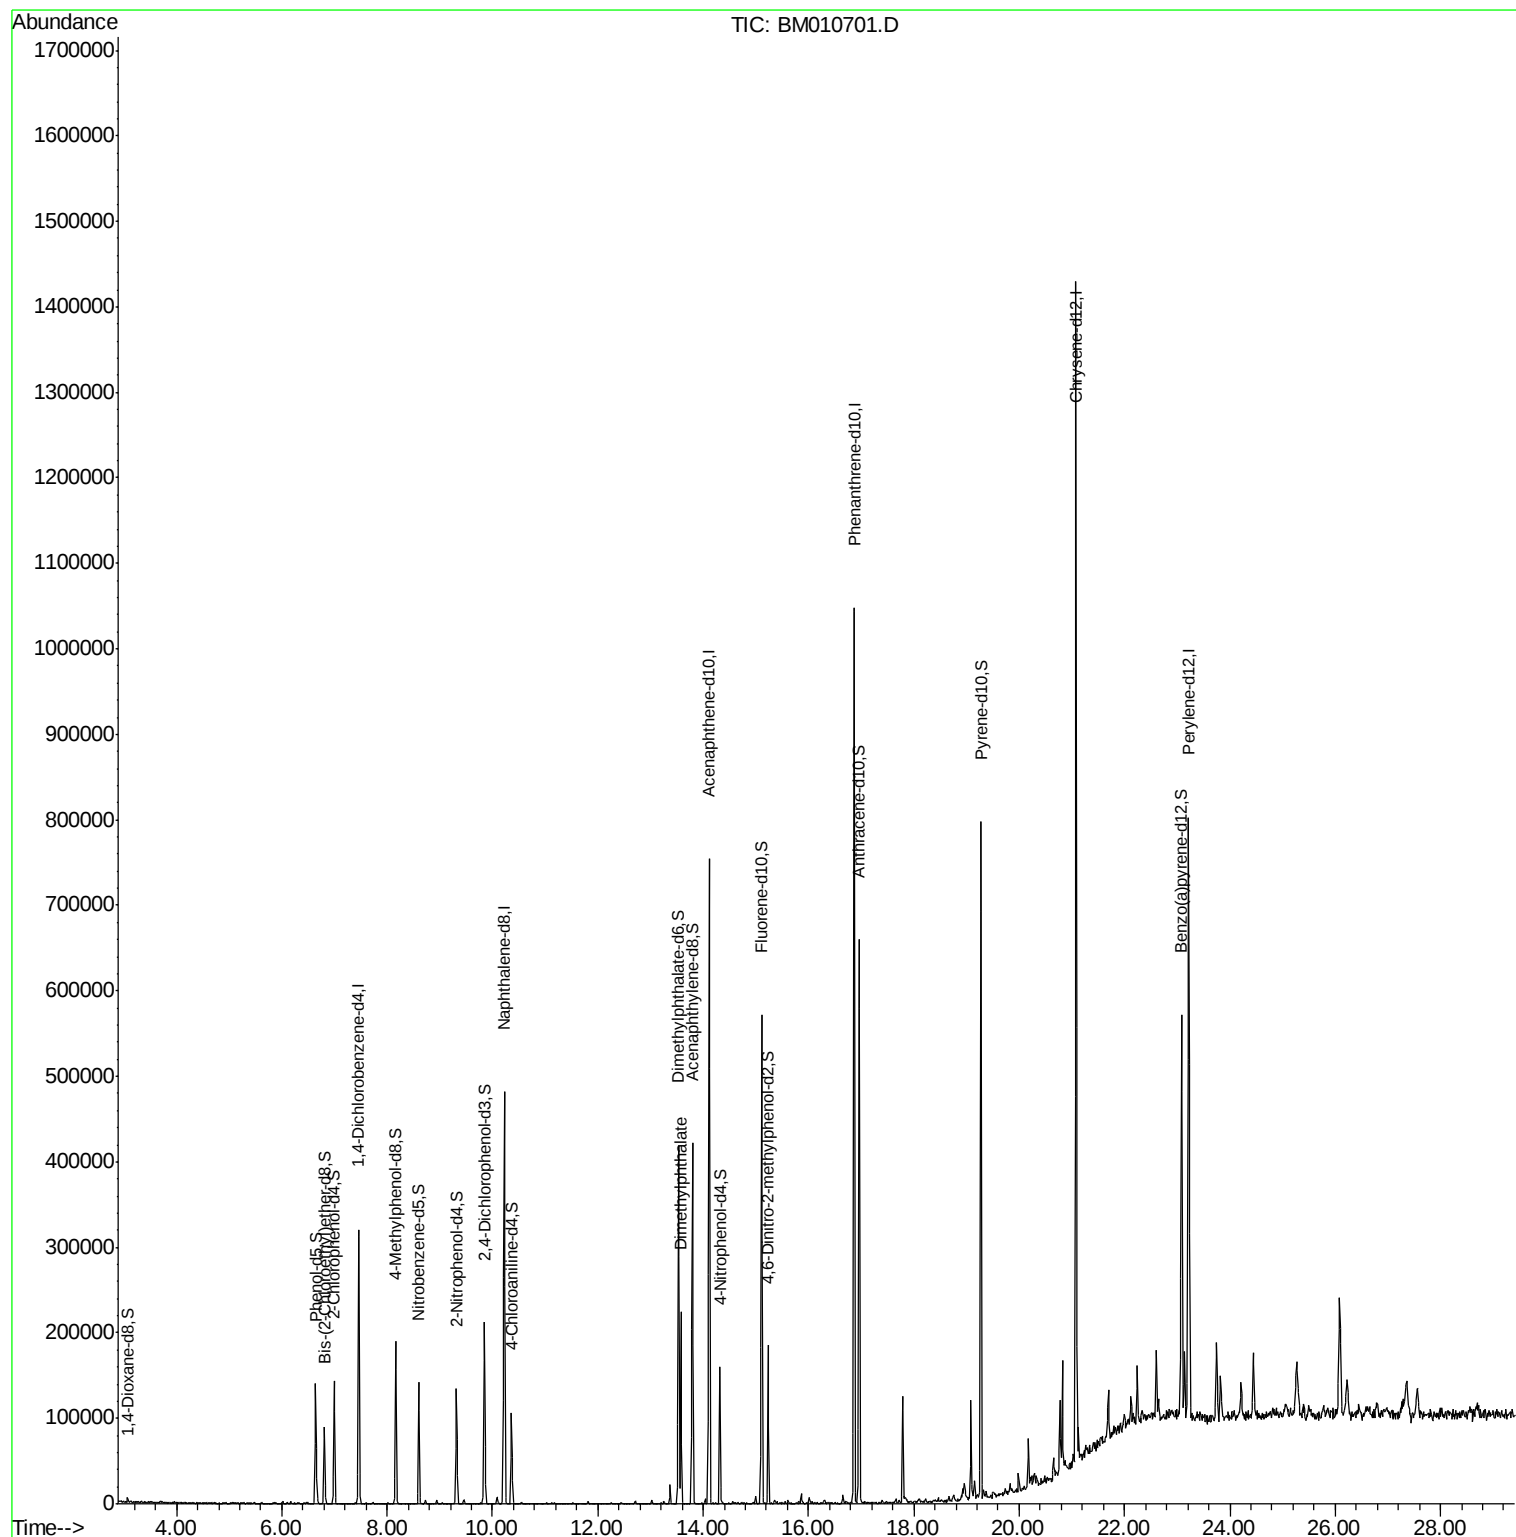

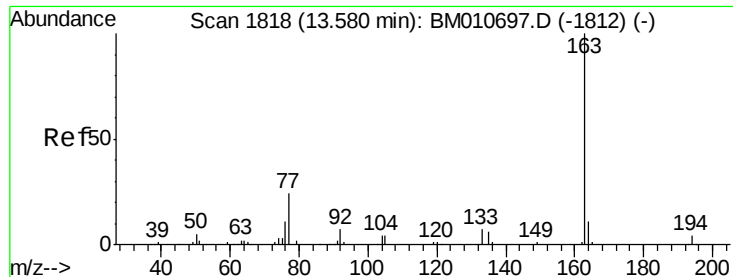

#44

Dimethylphthalate

Concen: 6.047 ng/ul

RT: 13.58 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM010701.D


Acq: 23 Jun 2017 21:50

Instrument :

BNA_M

ClientSampleId :

H2TR7

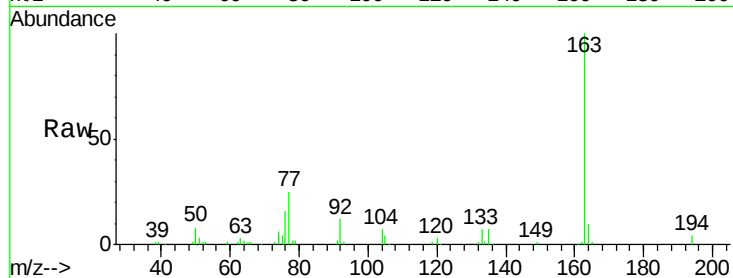

Tgt Ion:163 Resp: 124068

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.0 8.2 12.4

