

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010702.D
 Acq On : 23 Jun 2017 22:26
 Operator : SJ/JU
 Sample : I3657-02MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H2TR7MS

Quant Time: Jun 24 04:41:17 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 24 04:37:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	71546	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	337415	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	238101	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	576529	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	604244	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	445289	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	4521	3.62	ng/uL	0.00
5) Phenol-d5	6.65	99	114466	16.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	63194	16.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	87033	18.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	101585	17.98	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	46517	19.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	55370	19.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	112839	19.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	112399	18.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	412358	19.73	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	461591	18.99	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	59929	16.29	ng/ul	0.00
57) Fluorene-d10	15.11	176	341508	18.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	68658	19.39	ng/ul	0.00
70) Anthracene-d10	16.96	188	556075	19.97	ng/ul	0.00
76) Pyrene-d10	19.27	212	631513	22.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.09	264	428066	19.89	ng/ul	0.00

Target Compounds


					Qvalue	
6) Phenol	6.68	94	124100	17.678	ng/ul	96
8) Bis(2-Chloroethyl)ether	6.90	93	5257	1.029	ng/ul#	23
10) 2-Chlorophenol	7.03	128	83876	17.550	ng/ul	97
15) N-Nitroso-di-n-propylamine	8.26	70	91286	18.361	ng/ul#	89
33) 4-Chloro-3-methylphenol	11.52	107	137535	18.973	ng/ul	96
44) Dimethylphthalate	13.58	163	170039	8.299	ng/ul	98
49) Acenaphthene	14.17	153	294923	18.880	ng/ul	99
52) 4-Nitrophenol	14.34	109	93752	20.089	ng/ul	81
54) 2,4-Dinitrotoluene	14.49	165	108766	19.755	ng/ul	96
67) Atrazine	16.52	200	15627	2.320	ng/ul#	39
68) Pentachlorophenol	16.52	266	94335	19.247	ng/ul	93
77) Pyrene	19.30	202	768939	22.032	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010702.D
Acq On : 23 Jun 2017 22:26
Operator : SJ/JU
Sample : I3657-02MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H2TR7MS

Quant Time: Jun 24 04:41:17 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 24 04:37:39 2017
Response via : Initial Calibration

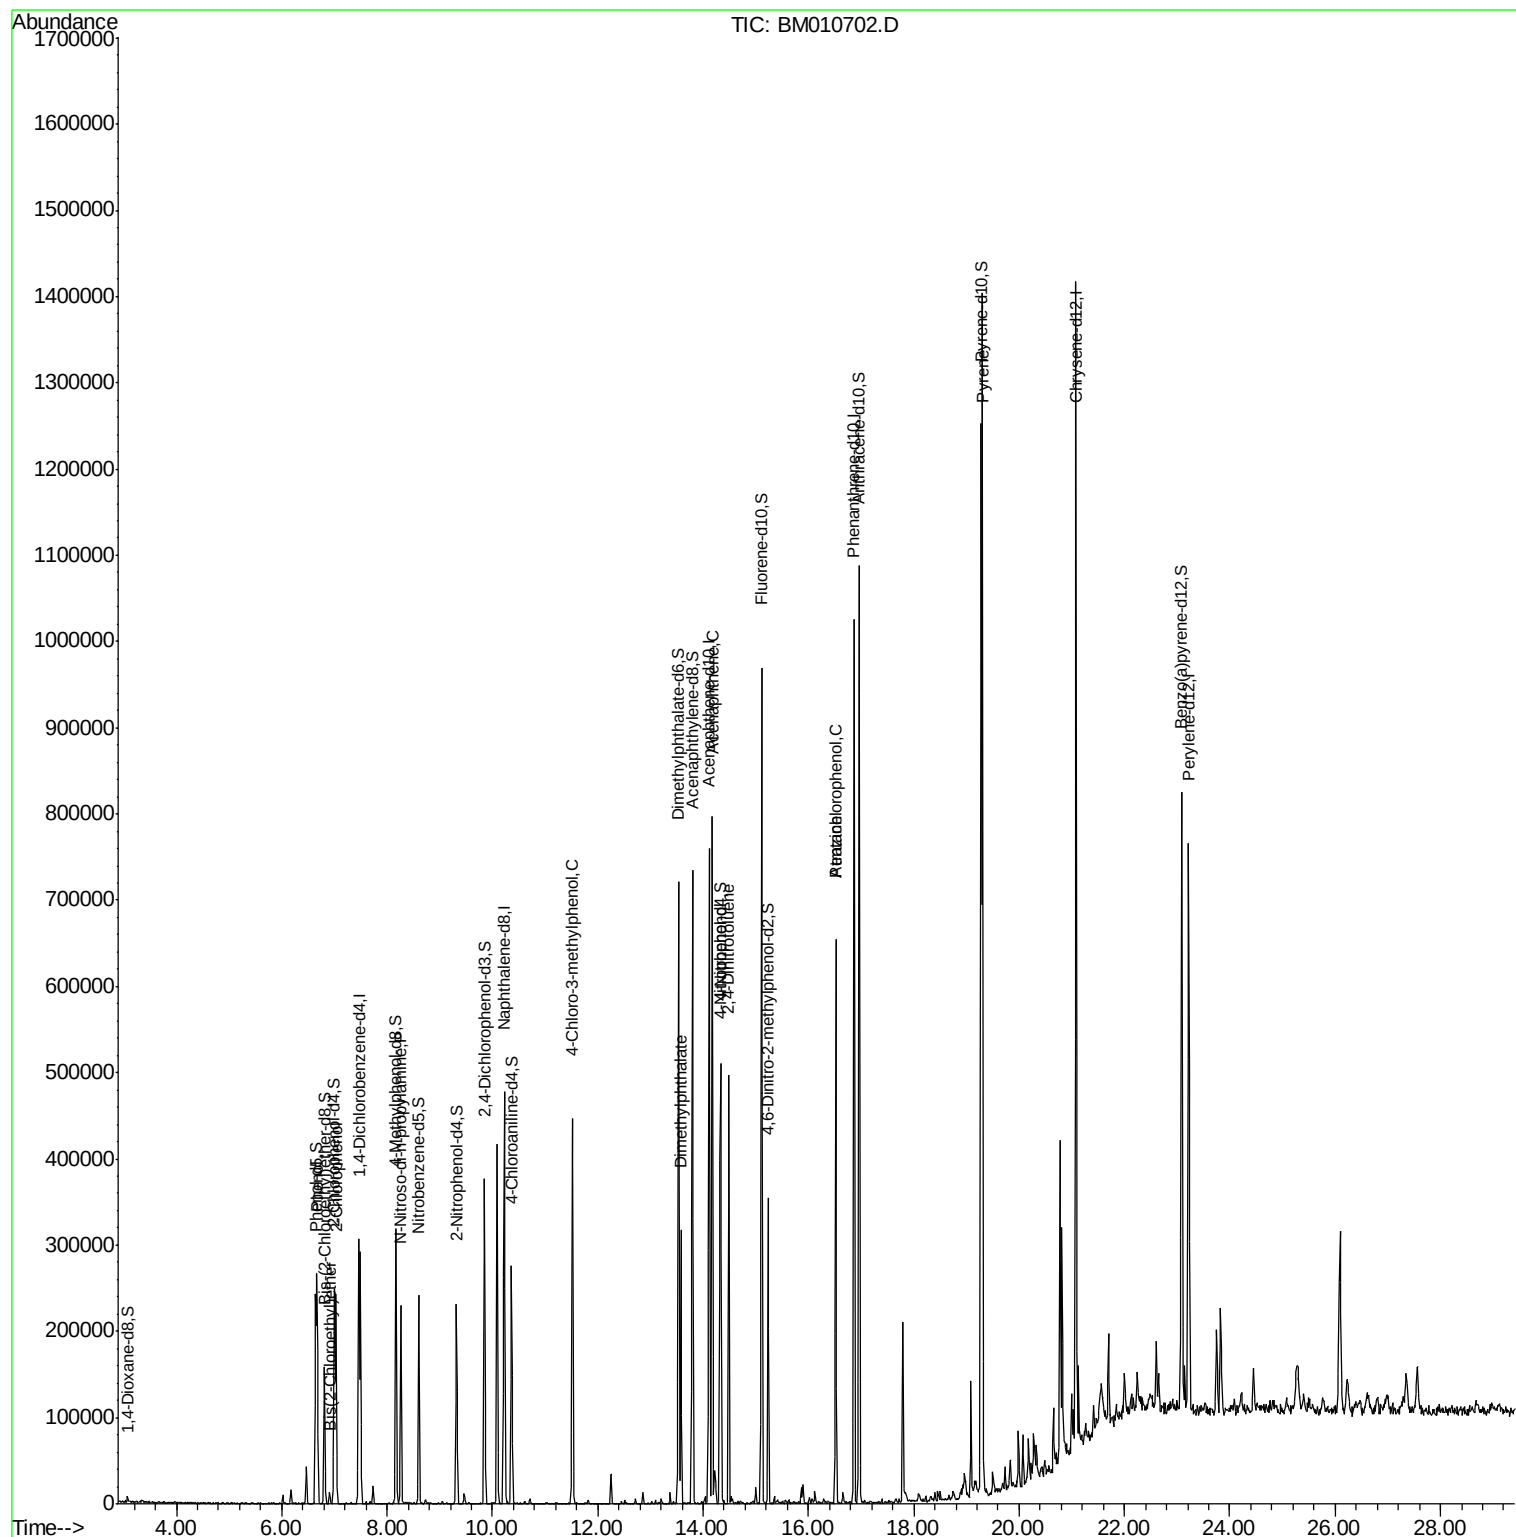

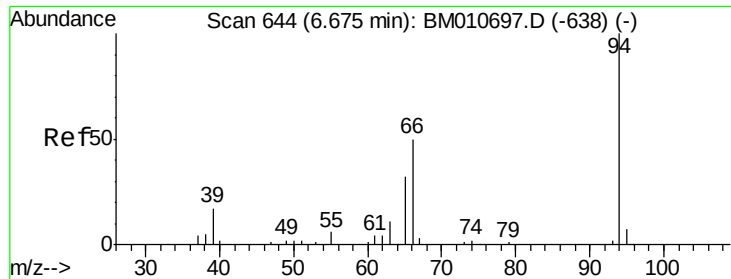





#6

Phenol

Concen: 17.678 ng/ul
 RT: 6.68 min Scan# 644
 Delta R.T. 0.00 min
 Lab File: BM010702.D
 Acq: 23 Jun 2017 22:26

Instrument :
 BNA_M
 ClientSampleId :
 H2TR7MS

Tgt Ion: 94 Resp: 124100
 Ion Ratio Lower Upper
 94 100
 65 32.8 28.2 42.4
 66 56.5 47.2 70.8

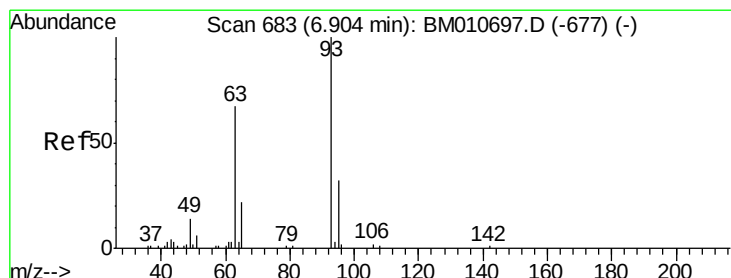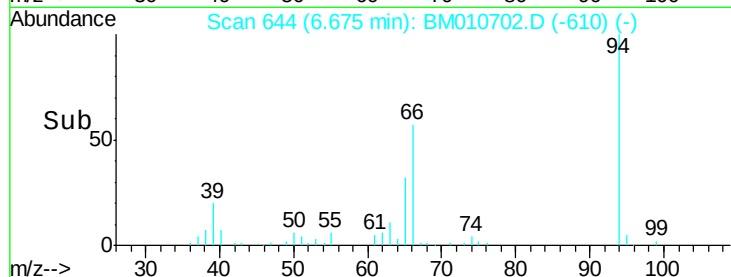
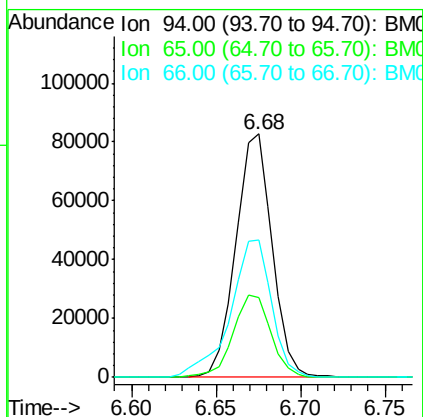
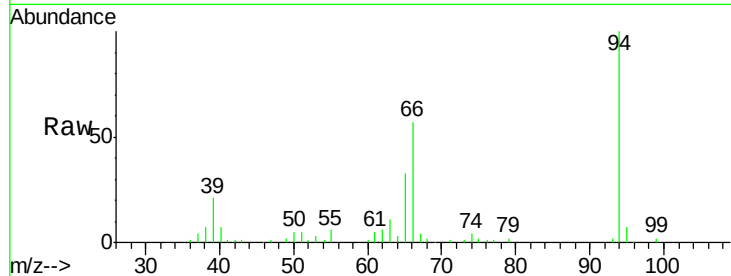



#8

Bis(2-Chloroethyl)ether

Concen: 1.029 ng/ul
 RT: 6.90 min Scan# 683
 Delta R.T. 0.00 min
 Lab File: BM010702.D
 Acq: 23 Jun 2017 22:26

Tgt Ion: 93 Resp: 5257
 Ion Ratio Lower Upper
 93 100
 63 0.0 57.3 85.9#
 95 0.0 26.6 39.8#


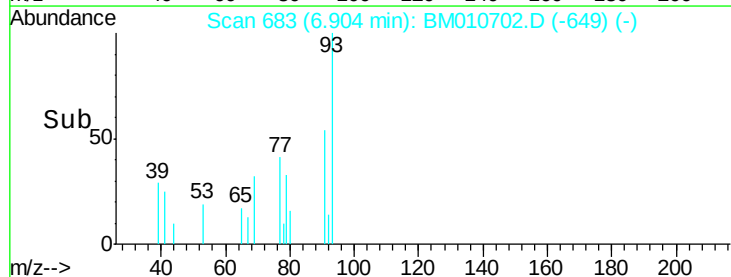
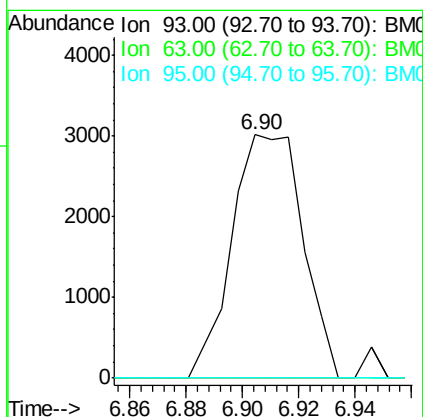
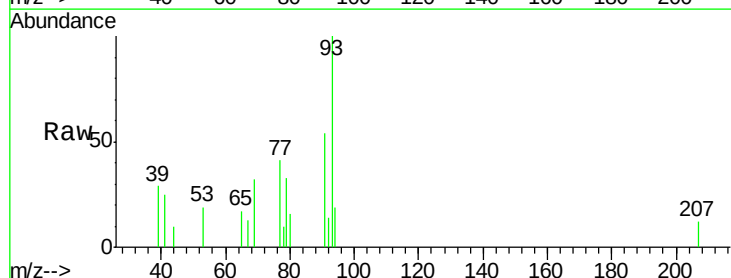


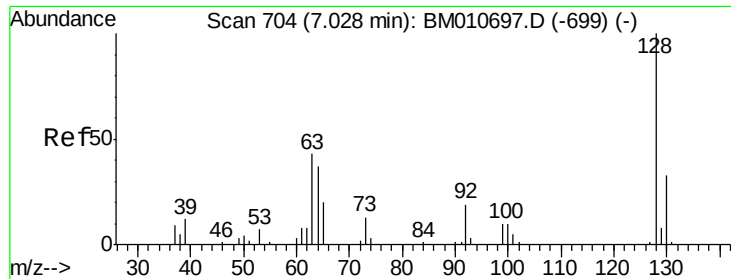

#10
2-Chlorophenol
Concen: 17.550 ng/ul
RT: 7.03 min Scan# 704
Delta R.T. 0.00 min
Lab File: BM010702.D
Acq: 23 Jun 2017 22:26




Instrument :
BNA_M
ClientSampleId :
H2TR7MS


Tgt Ion: 128 Resp: 83876
Ion Ratio Lower Upper
128 100
64 49.3 38.0 57.0
130 32.7 24.4 36.6

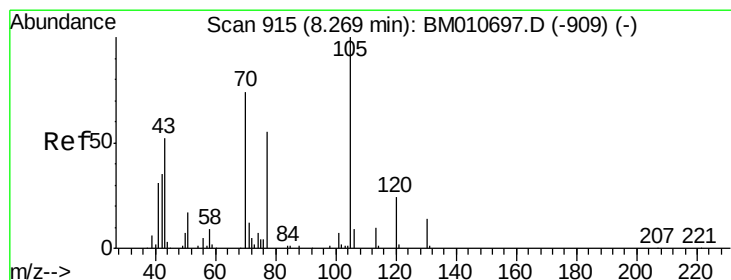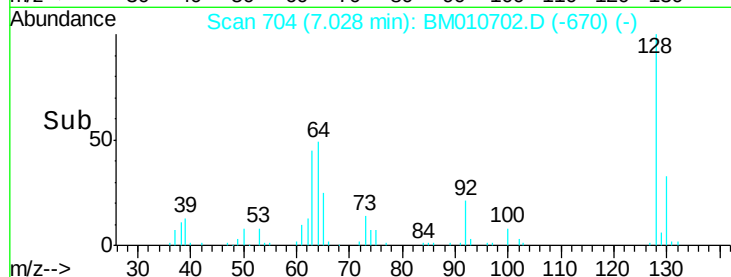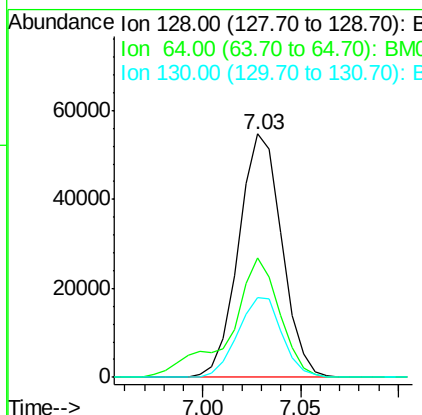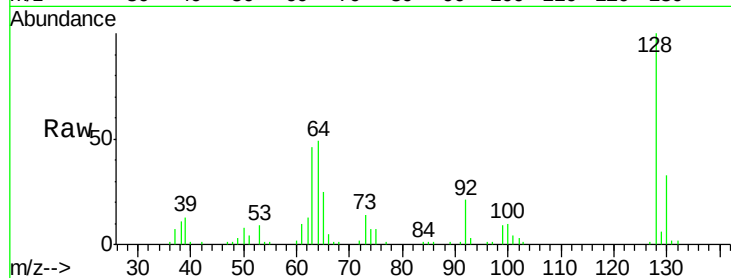

#15
N-Nitroso-di-n-propylamine
Concen: 18.361 ng/ul
RT: 8.26 min Scan# 914
Delta R.T. -0.01 min
Lab File: BM010702.D
Acq: 23 Jun 2017 22:26

Tgt Ion: 70 Resp: 91286
Ion Ratio Lower Upper
70 100
42 40.6 41.1 61.7#
101 9.2 6.7 10.1
130 18.6 14.6 22.0


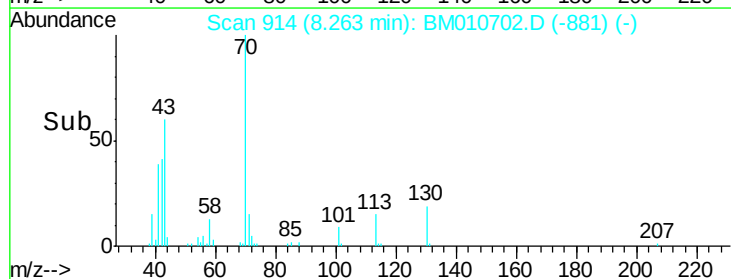
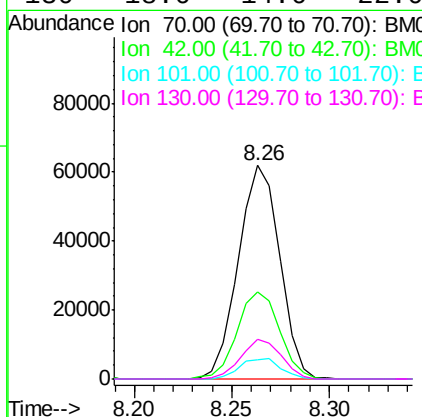
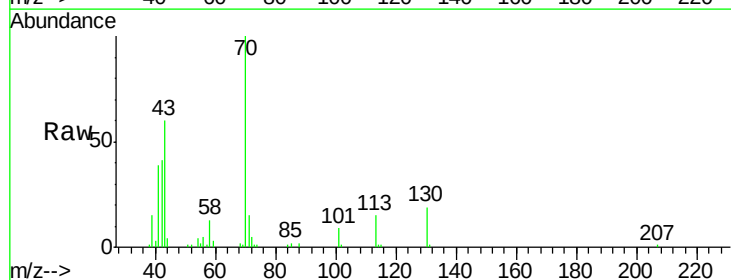


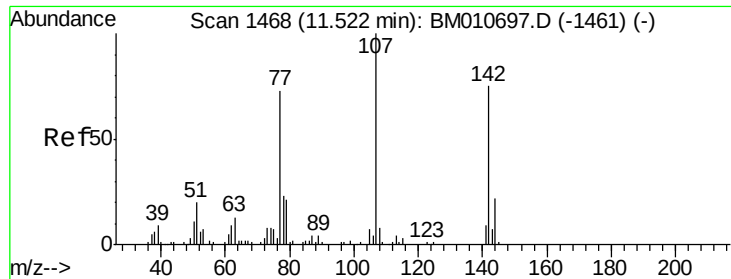

#33
4-Chloro-3-methylphenol
Concen: 18.973 ng/ul
RT: 11.52 min Scan# 1467
Delta R.T. -0.01 min
Lab File: BM010702.D
Acq: 23 Jun 2017 22:26




Instrument :
BNA_M
ClientSampleId :
H2TR7MS


Tgt Ion	Ratio	Lower	Upper
107	100		
144	21.2	20.4	30.6
142	73.7	60.5	90.7

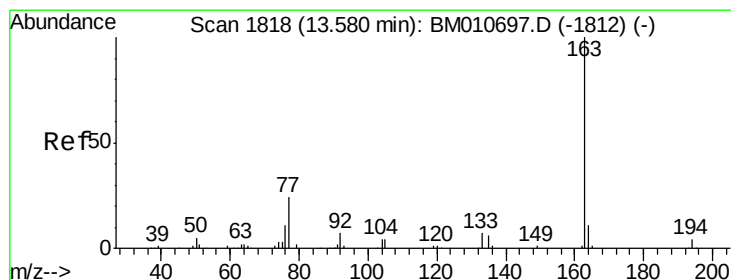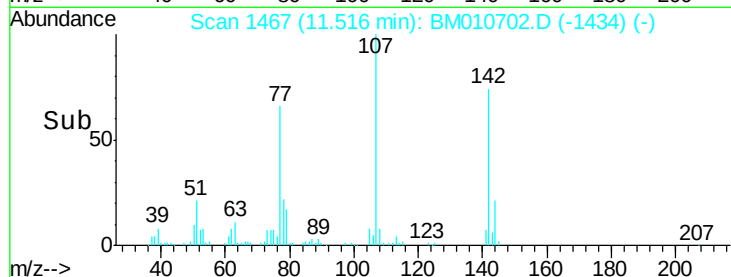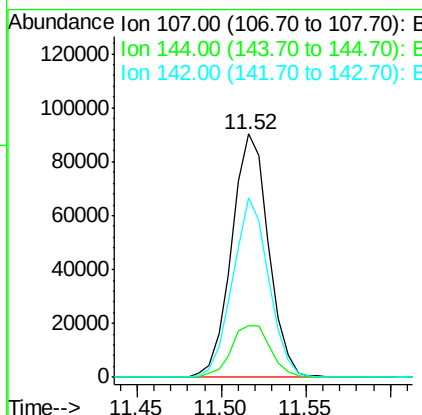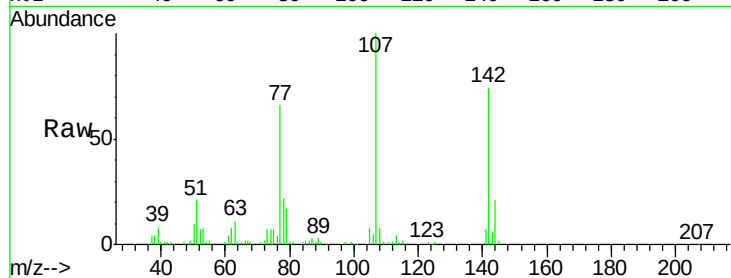

#44
Dimethylphthalate
Concen: 8.299 ng/ul
RT: 13.58 min Scan# 1818
Delta R.T. 0.00 min
Lab File: BM010702.D
Acq: 23 Jun 2017 22:26

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.1	3.5	5.3
164	9.8	8.2	12.4

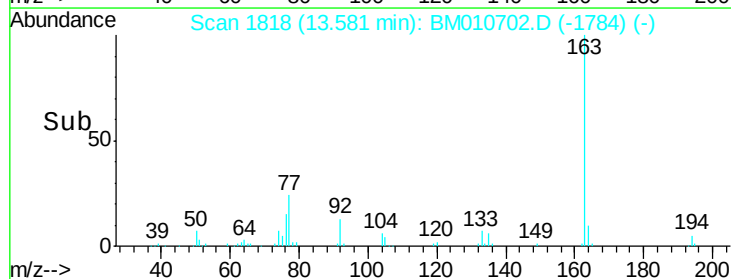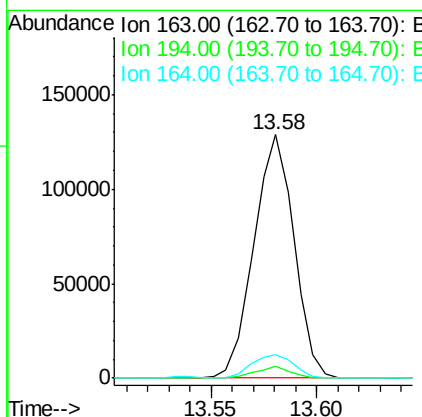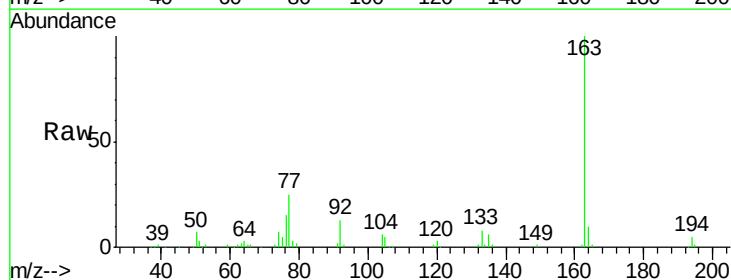

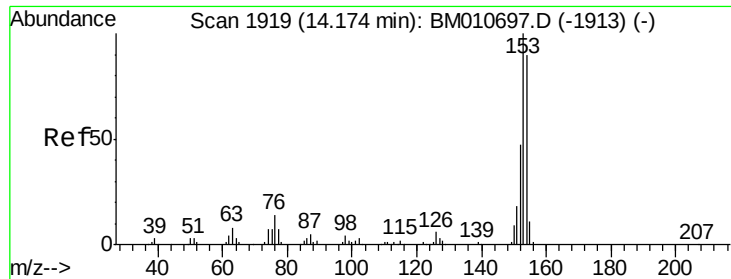

#49

Acenaphthene

Concen: 18.880 ng/ul

RT: 14.17 min Scan# 1919

Delta R.T. 0.00 min

Lab File: BM010702.D

Acq: 23 Jun 2017 22:26

Instrument :

BNA_M

ClientSampleId :

H2TR7MS


Tgt Ion:153 Resp: 294923

Ion Ratio Lower Upper

153 100

152 45.8 37.6 56.4




154 87.9 70.4 105.6

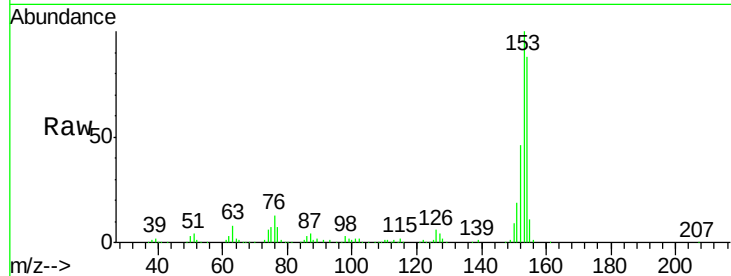

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

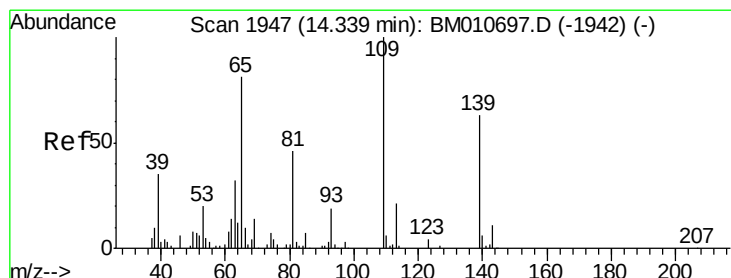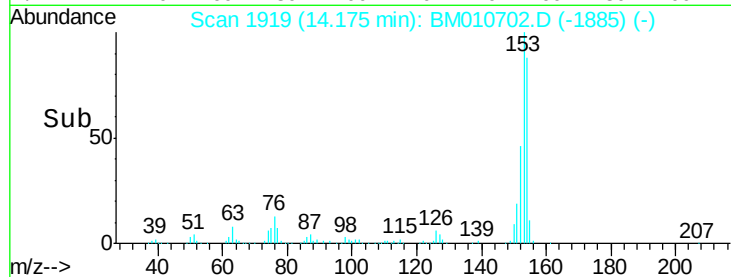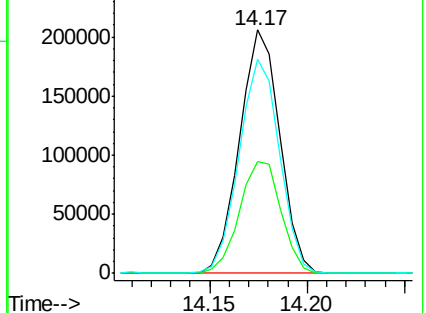

#52

4-Nitrophenol

Concen: 20.089 ng/ul

RT: 14.34 min Scan# 1947

Delta R.T. 0.00 min

Lab File: BM010702.D

Acq: 23 Jun 2017 22:26


Tgt Ion:109 Resp: 93752

Ion Ratio Lower Upper

109 100

139 67.2 66.6 100.0



65 78.8 78.3 117.5

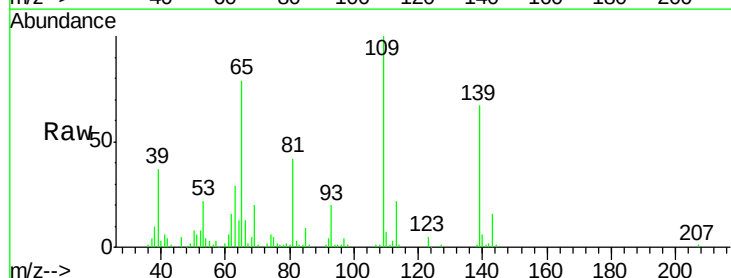


Abundance Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM

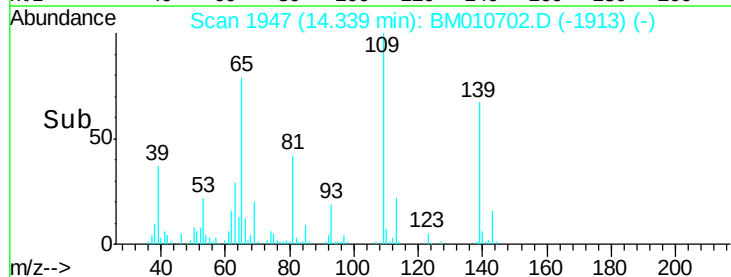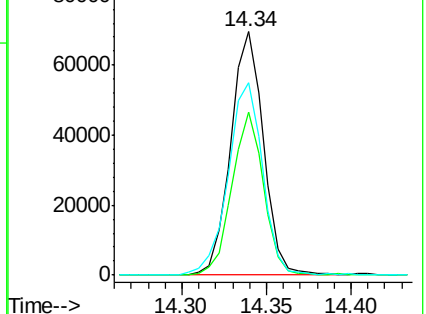

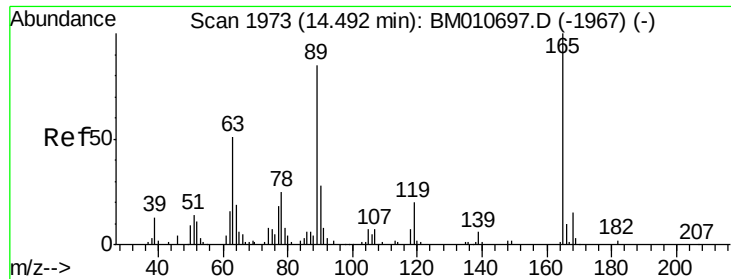

#54

2,4-Dinitrotoluene

Concen: 19.755 ng/ul

RT: 14.49 min Scan# 1972

Delta R.T. -0.01 min

Lab File: BM010702.D

Acq: 23 Jun 2017 22:26

Instrument :

BNA_M

ClientSampleId :

H2TR7MS


Tgt Ion:165 Resp: 108766

Ion Ratio Lower Upper

165 100

63 54.2 45.8 68.8




182 3.4 2.6 4.0

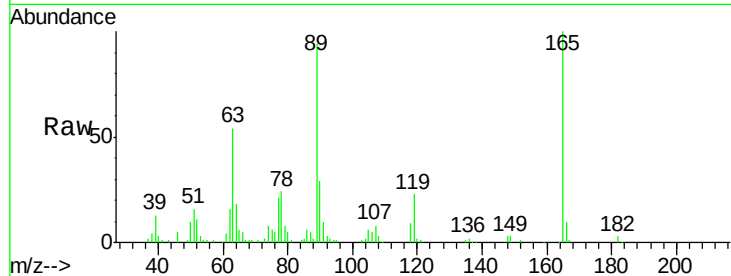

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM

Ion 182.00 (181.70 to 182.70): E

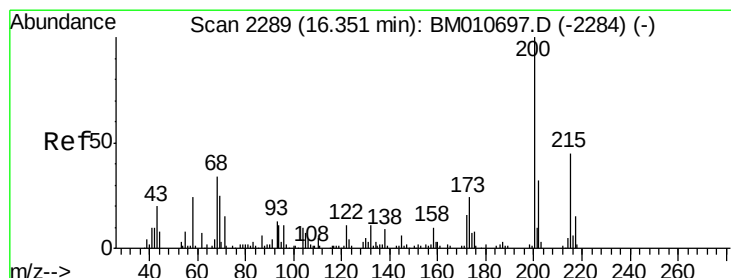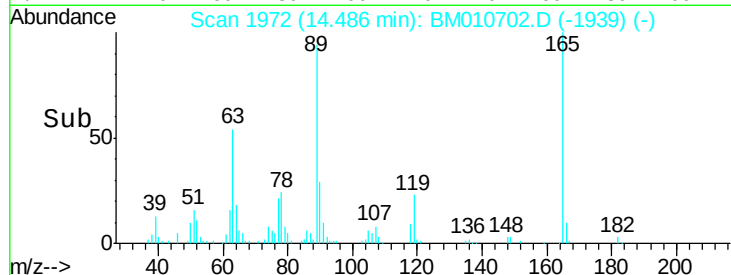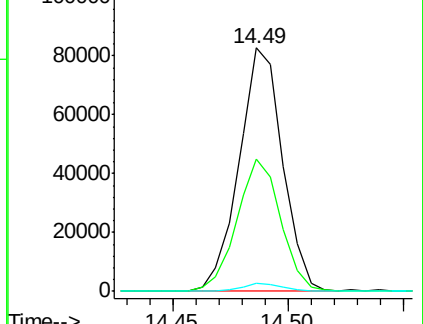

#67

Atrazine

Concen: 2.320 ng/ul

RT: 16.52 min Scan# 2317

Delta R.T. 0.16 min

Lab File: BM010702.D

Acq: 23 Jun 2017 22:26


Tgt Ion:200 Resp: 15627

Ion Ratio Lower Upper

200 100

173 0.0 18.2 27.2#



215 0.0 35.0 52.4#

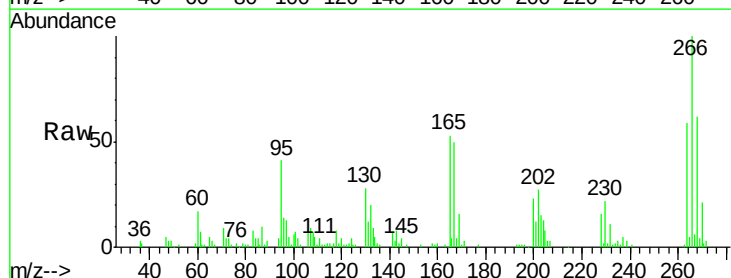


Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

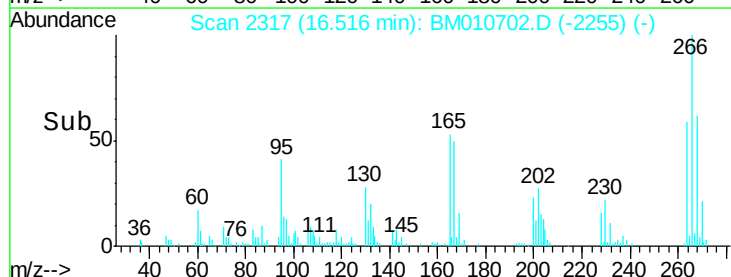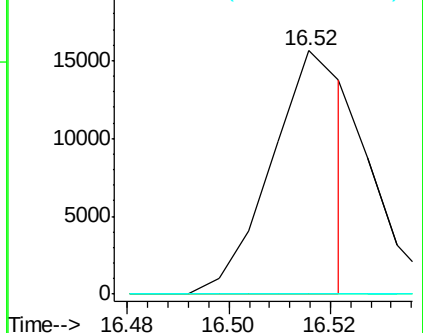


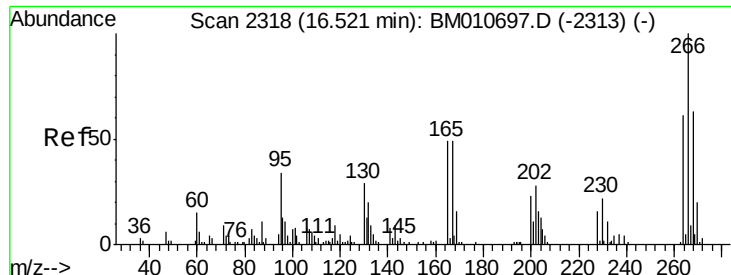




#68
 Pentachlorophenol
 Concen: 19.247 ng/ul
 RT: 16.52 min Scan# 2318
 Delta R.T. 0.00 min
 Lab File: BM010702.D
 Acq: 23 Jun 2017 22:26

Instrument :
 BNA_M
 ClientSampleId :
 H2TR7MS

Tgt Ion:266 Resp: 94335
 Ion Ratio Lower Upper
 266 100
 264 55.6 49.3 73.9
 268 60.3 52.6 78.8

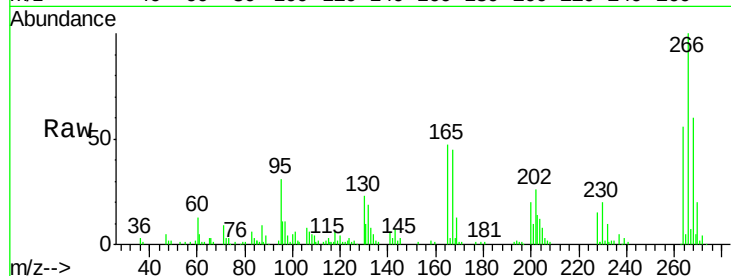


Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

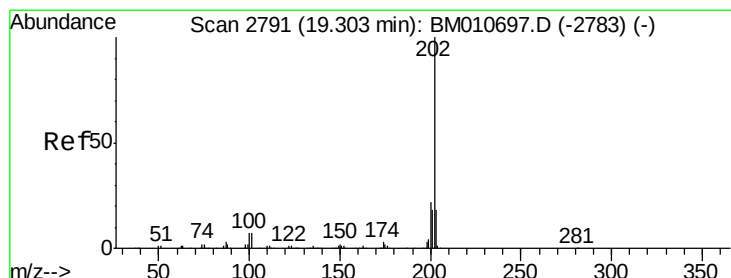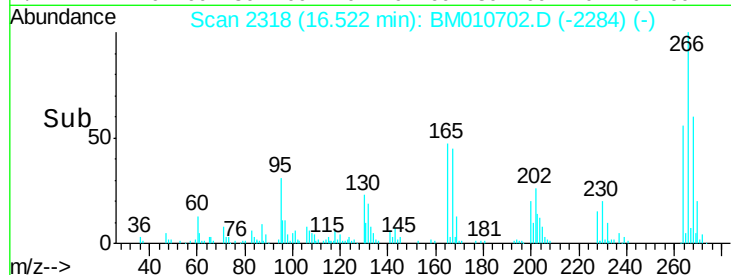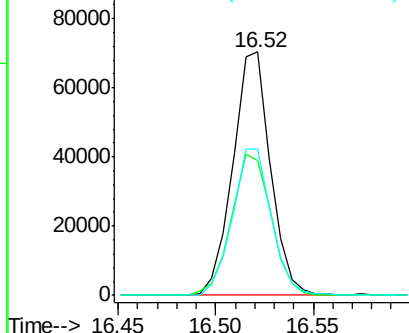

#77
 Pyrene
 Concen: 22.032 ng/ul
 RT: 19.30 min Scan# 2791
 Delta R.T. 0.00 min
 Lab File: BM010702.D
 Acq: 23 Jun 2017 22:26

Tgt Ion:202 Resp: 768939
 Ion Ratio Lower Upper
 202 100
 101 7.5 5.1 7.7
 100 5.9 4.9 7.3

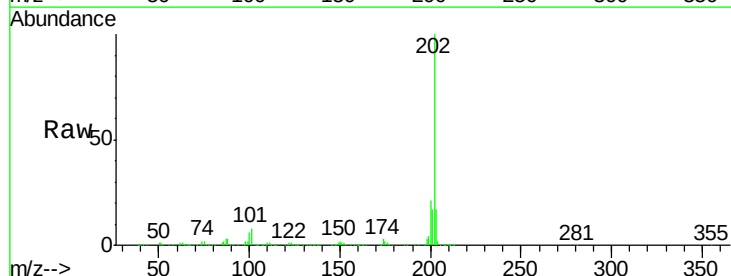

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

