

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010710.D
 Acq On : 24 Jun 2017 03:14
 Operator : SJ/JU
 Sample : I3625-14ME 20X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C81ME

Quant Time: Jun 24 04:43:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 24 04:37:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	64856	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	302085	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	214886	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	529785	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	581890	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	427570	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.65	99	4070	0.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	2090	0.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	2890	0.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	3927	0.77	ng/ul	-0.01
19) Nitrobenzene-d5	8.60	128	1710	0.79	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.31	143	1902	0.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	4075	0.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	3902	0.71	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	15777	0.84	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	16684	0.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	1295	0.39	ng/ul	0.00
57) Fluorene-d10	15.11	176	14411	0.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	1796	0.55	ng/ul	0.00
70) Anthracene-d10	16.86	188	529785	20.71	ng/ul	-0.11
76) Pyrene-d10	19.27	212	25377	0.94	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.08	264	15983	0.77	ng/ul	0.00

Target Compounds


					Qvalue	
28) Naphthalene	10.27	128	967451	64.355	ng/ul	99
30) 4-Chloroaniline	10.27	127	129543	23.385	ng/ul#	26
34) 2-Methylnaphthalene	11.89	142	194942	16.132	ng/ul	94
40) 1,1'-Biphenyl	12.93	154	51984	3.094	ng/ul	98
49) Acenaphthene	14.17	153	164443	11.665	ng/ul	93
53) Dibenzofuran	14.52	168	211271	9.896	ng/ul	91
58) Fluorene	15.17	166	229183	12.821	ng/ul	99
69) Phenanthrene	16.91	178	1011714	35.921	ng/ul	99
71) Anthracene	17.00	178	504751	17.395	ng/ul	98
72) Carbazole	17.27	167	218668	8.638	ng/ul	97
74) Fluoranthene	18.94	202	596702	16.439	ng/ul#	96
77) Pyrene	19.30	202	395634	11.771	ng/ul#	97
80) Benzo(a)anthracene	21.06	228	124647	3.678	ng/ul	96
82) Chrysene	21.12	228	101077	3.346	ng/ul	97
85) Benzo(b)fluoranthene	22.59	252	50115	1.806	ng/ul#	94
86) Benzo(k)fluoranthene	22.59	252	50115	1.905	ng/ul#	95
88) Benzo(a)pyrene	23.12	252	30592	1.197	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010710.D
Acq On : 24 Jun 2017 03:14
Operator : SJ/JU
Sample : I3625-14ME 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C81ME

Quant Time: Jun 24 04:43:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 24 04:37:39 2017
Response via : Initial Calibration

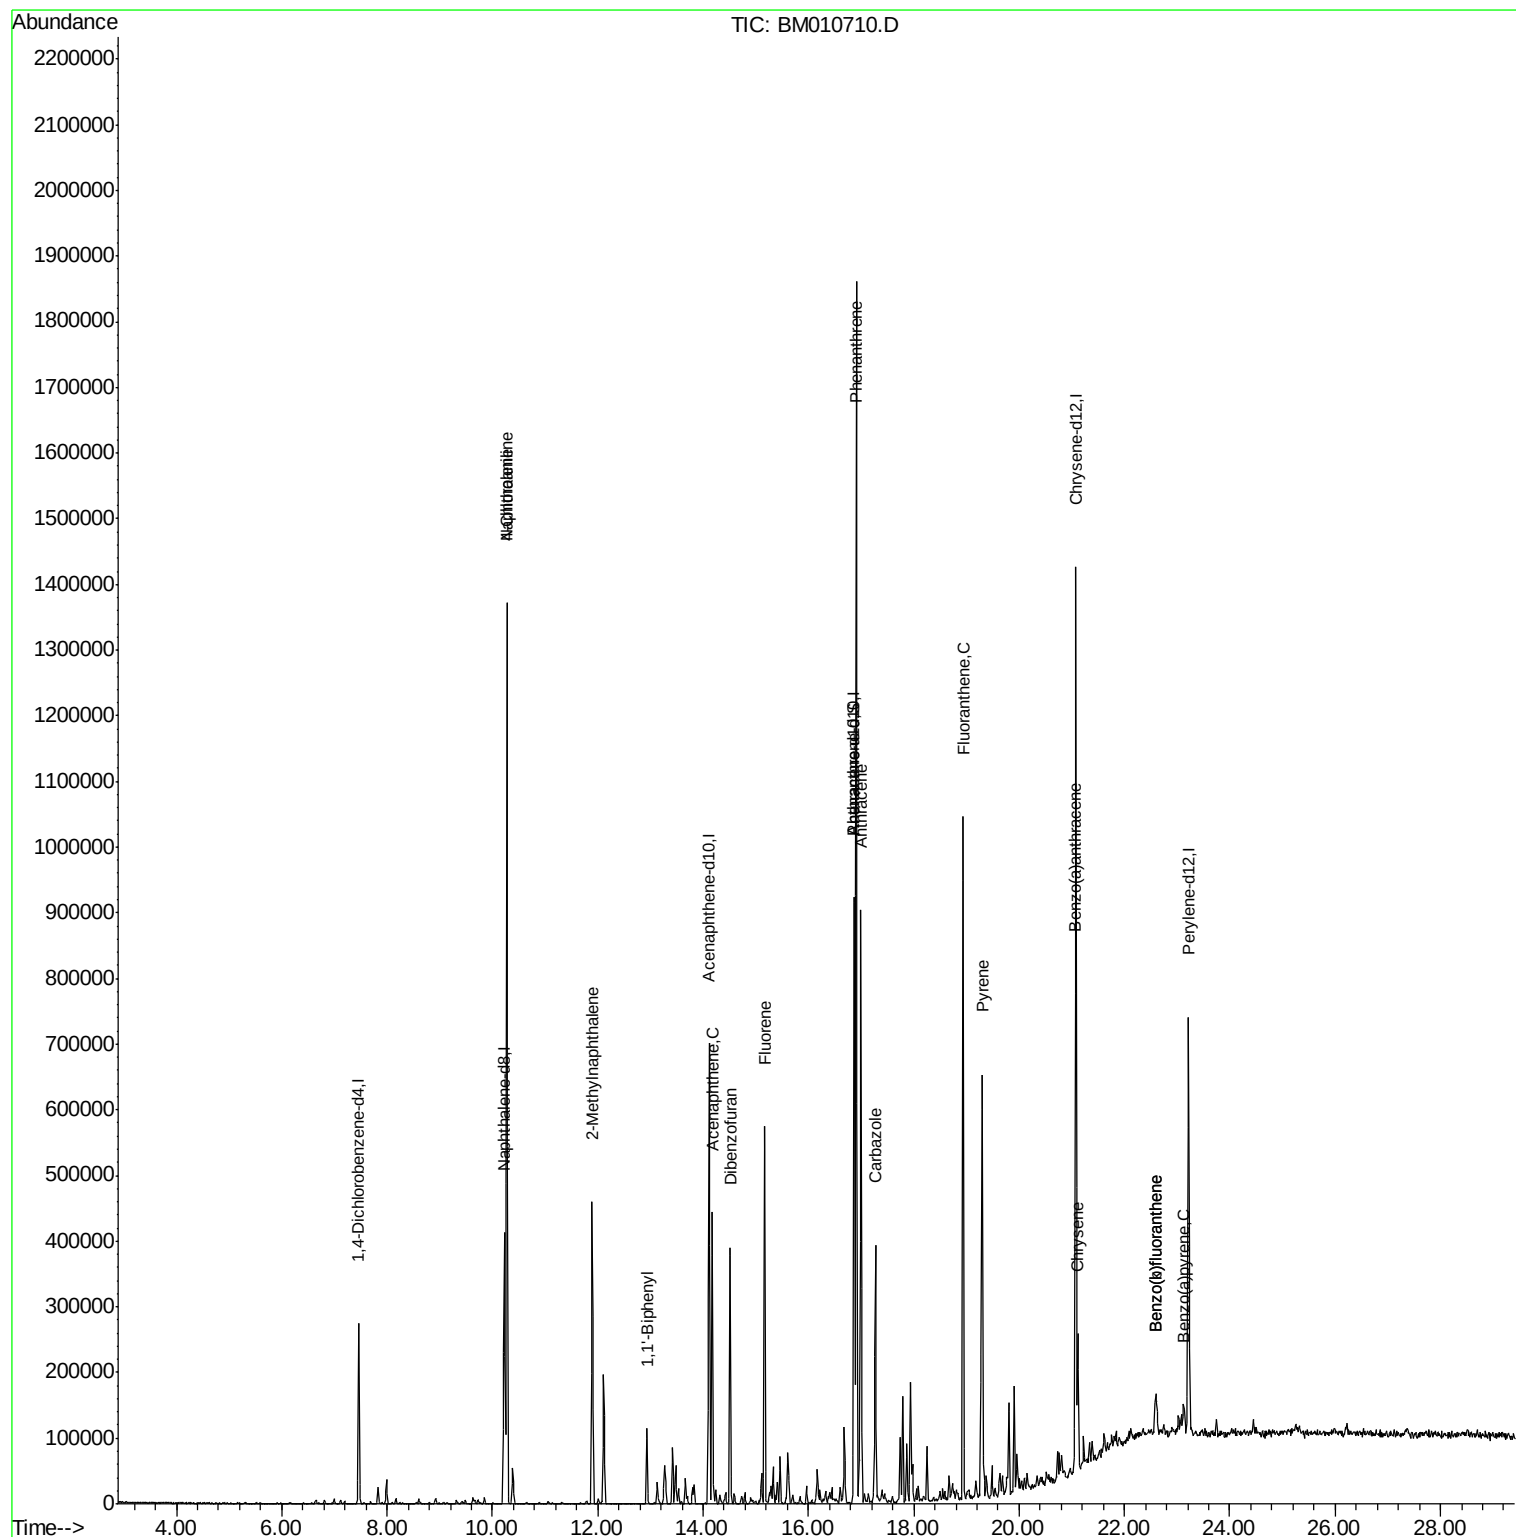



#28

Naphthalene

Concen: 64.355 ng/ul

RT: 10.27 min Scan# 1256

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:128 Resp: 967451

Ion Ratio Lower Upper

128 100

129 10.4 8.8 13.2




127 13.2 10.6 16.0

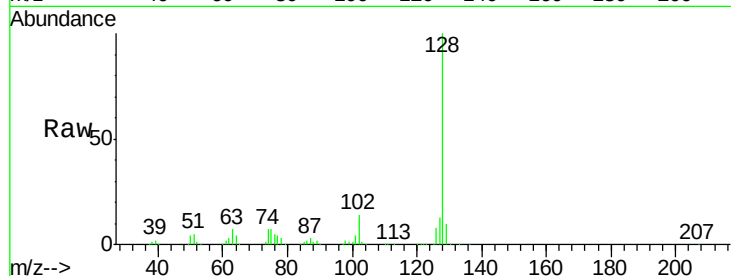

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

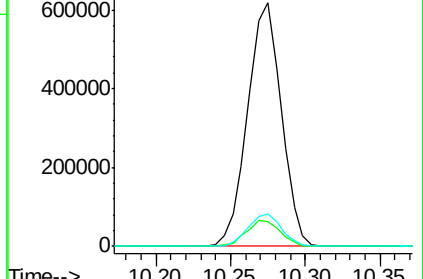

#30

4-Chloroaniline

Concen: 23.385 ng/ul

RT: 10.27 min Scan# 1256

Delta R.T. -0.12 min

Lab File: BM010710.D


Acq: 24 Jun 2017 03:14

Tgt Ion:127 Resp: 129543

Ion Ratio Lower Upper



127 100


129 78.9 28.4 42.6#



Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

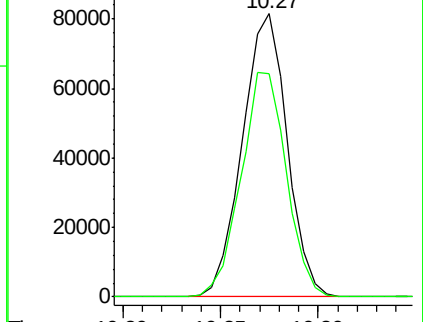


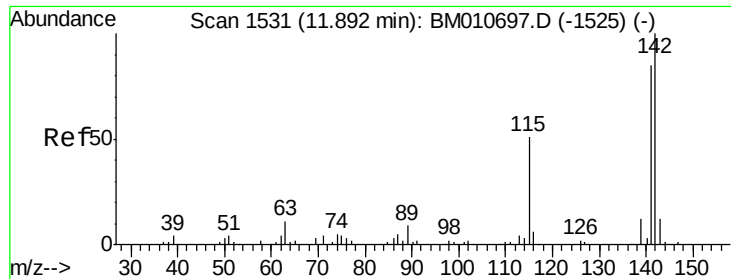




#34
 2-Methylnaphthalene
 Concen: 16.132 ng/ul
 RT: 11.89 min Scan# 1531
 Delta R.T. 0.00 min
 Lab File: BM010710.D
 Acq: 24 Jun 2017 03:14

Instrument :
 BNA_M
 ClientSampled :
 F5C81ME

Tgt Ion:142 Resp: 194942
 Ion Ratio Lower Upper
 142 100
 141 86.7 74.1 111.1

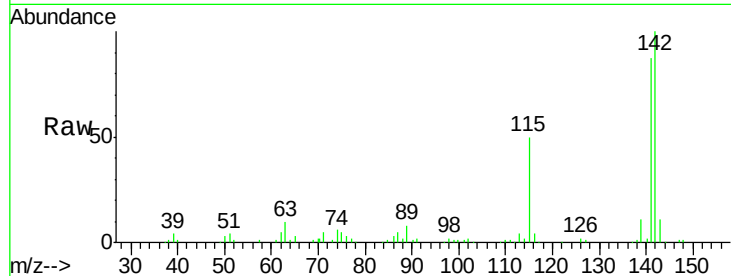


Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E

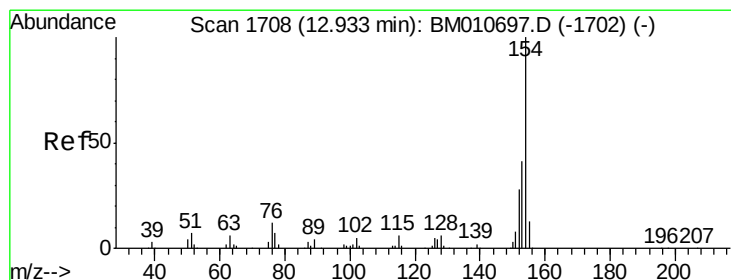
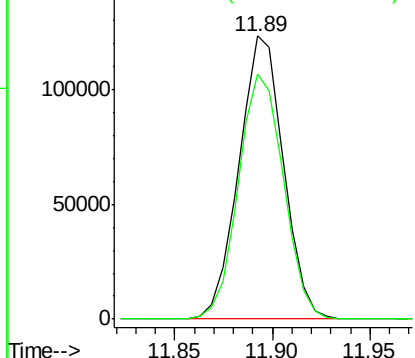



#40
 1,1'-Biphenyl
 Concen: 3.094 ng/ul
 RT: 12.93 min Scan# 1708
 Delta R.T. 0.00 min
 Lab File: BM010710.D
 Acq: 24 Jun 2017 03:14

Tgt Ion:154 Resp: 51984
 Ion Ratio Lower Upper
 154 100
 153 42.0 32.6 48.8
 76 11.4 8.5 12.7



Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BM

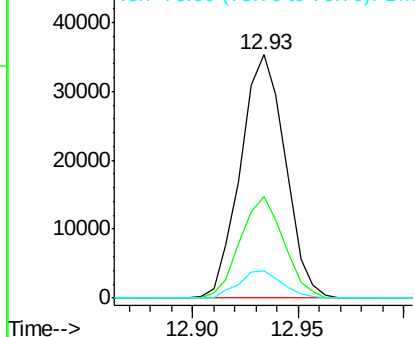

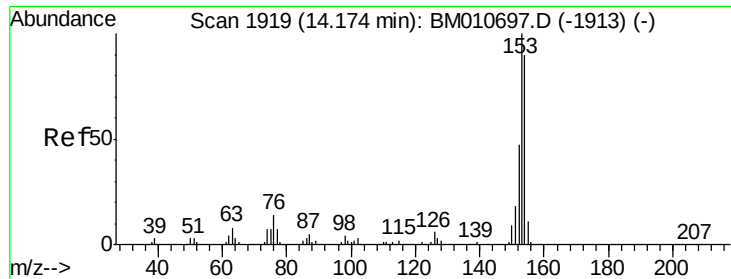

#49

Acenaphthene

Concen: 11.665 ng/ul

RT: 14.17 min Scan# 1919

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:153 Resp: 164443

Ion Ratio Lower Upper

153 100

152 49.9 37.6 56.4




154 95.8 70.4 105.6



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

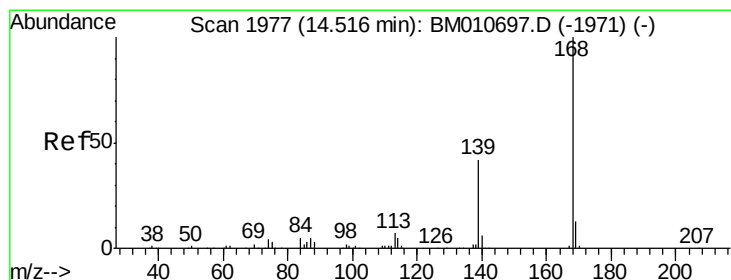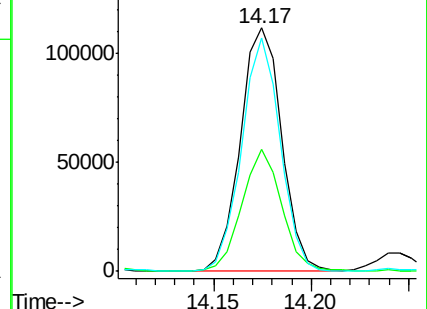

#53

Dibenzofuran

Concen: 9.896 ng/ul

RT: 14.52 min Scan# 1977

Delta R.T. 0.00 min

Lab File: BM010710.D


Acq: 24 Jun 2017 03:14

Tgt Ion:168 Resp: 211271

Ion Ratio Lower Upper



168 100


139 43.7 30.8 46.2

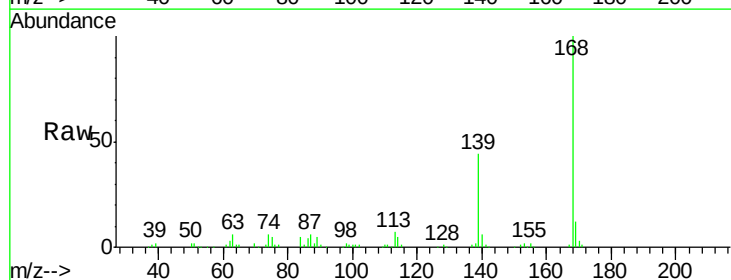

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

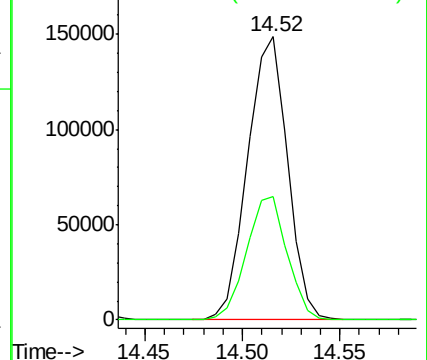

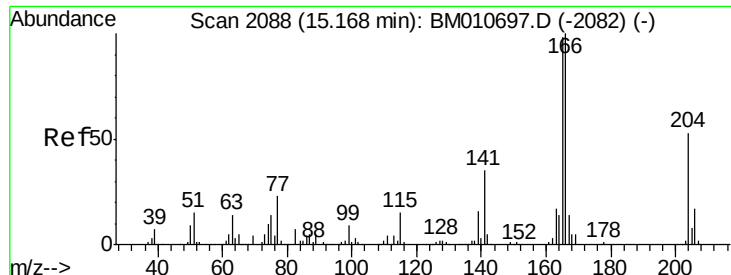

#58

Fluorene

Concen: 12.821 ng/ul

RT: 15.17 min Scan# 2088

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:166 Resp: 229183

Ion Ratio Lower Upper

166 100

165 96.9 77.9 116.9




167 12.4 10.6 16.0

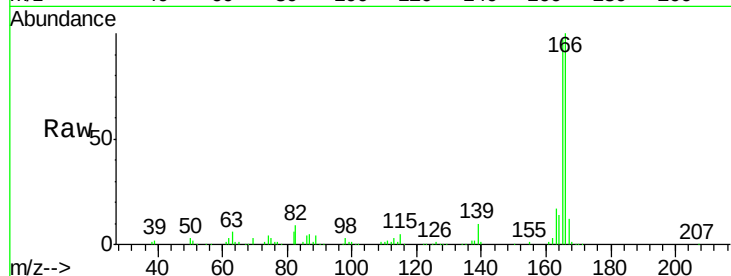

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

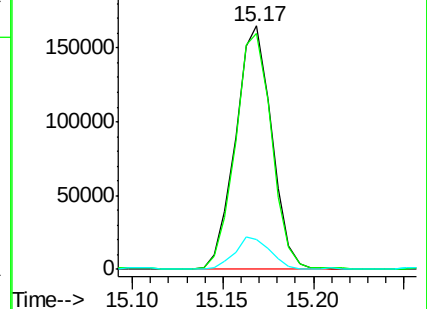

#69

Phenanthrene

Concen: 35.921 ng/ul

RT: 16.91 min Scan# 2384

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14


Tgt Ion:178 Resp: 1011714

Ion Ratio Lower Upper

178 100

179 14.9 12.6 19.0



176 18.2 14.9 22.3




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

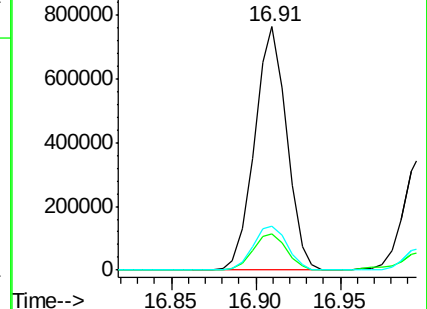

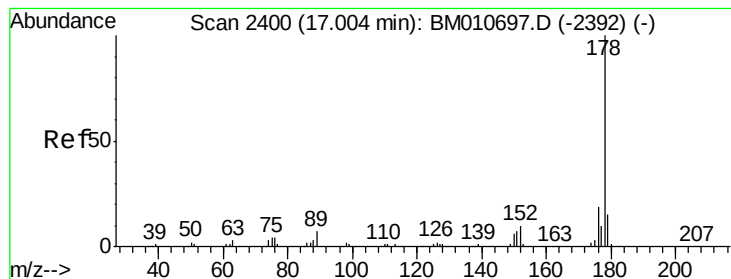

#71

Anthracene

Concen: 17.395 ng/ul

RT: 17.00 min Scan# 2399

Delta R.T. -0.01 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:178 Resp: 504751

Ion Ratio Lower Upper

178 100

179 15.2 11.7 17.5




176 19.0 14.6 21.8



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

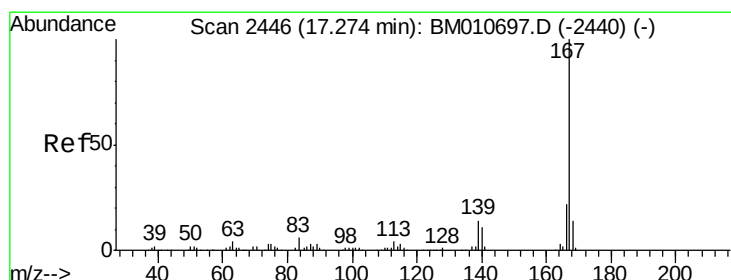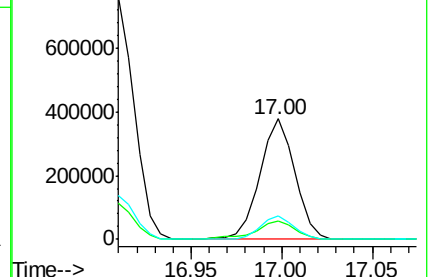

#72

Carbazole

Concen: 8.638 ng/ul

RT: 17.27 min Scan# 2446

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14


Tgt Ion:167 Resp: 218668

Ion Ratio Lower Upper

167 100

166 22.6 17.1 25.7



139 14.4 10.0 15.0




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

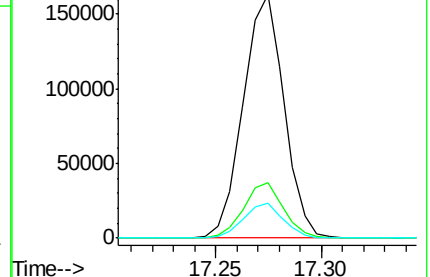

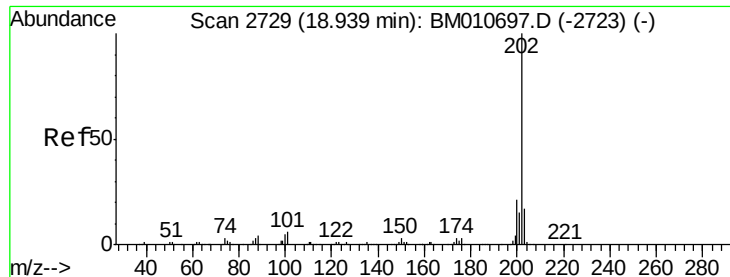

#74

Fluoranthene

Concen: 16.439 ng/ul

RT: 18.94 min Scan# 2729

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:202 Resp: 596702

Ion Ratio Lower Upper

202 100

101 7.2 4.6 7.0#




100 5.4 3.4 5.2#

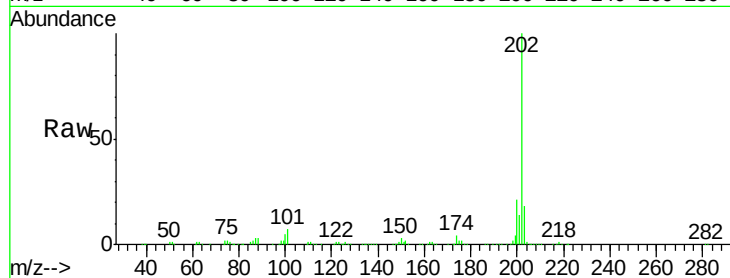

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

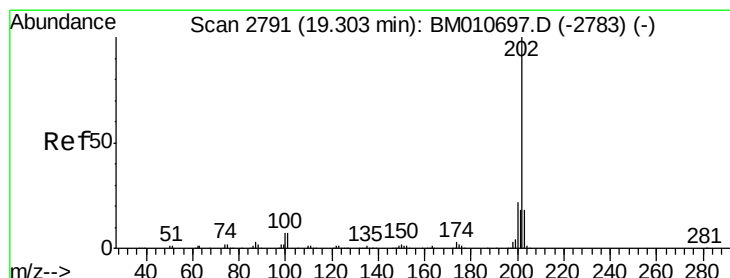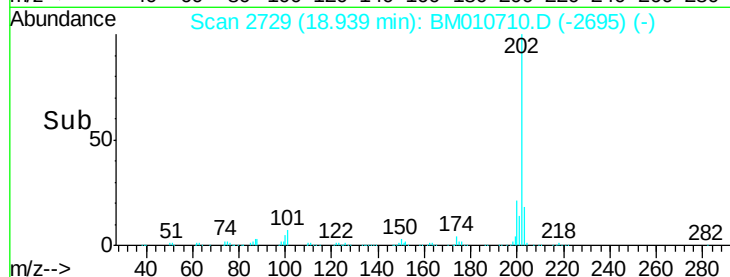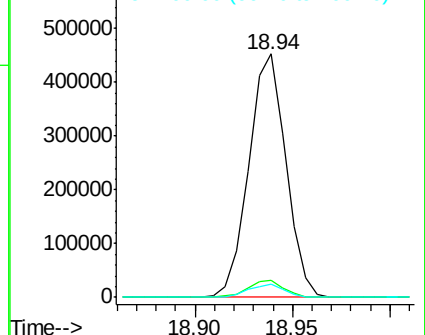

#77

Pyrene

Concen: 11.771 ng/ul

RT: 19.30 min Scan# 2791

Delta R.T. 0.00 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14


Tgt Ion:202 Resp: 395634

Ion Ratio Lower Upper

202 100

101 8.3 5.1 7.7#



100 6.4 4.9 7.3

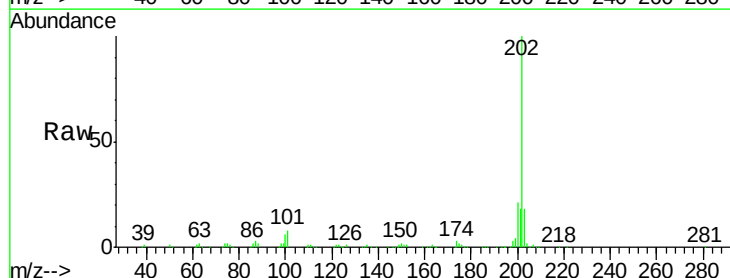


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

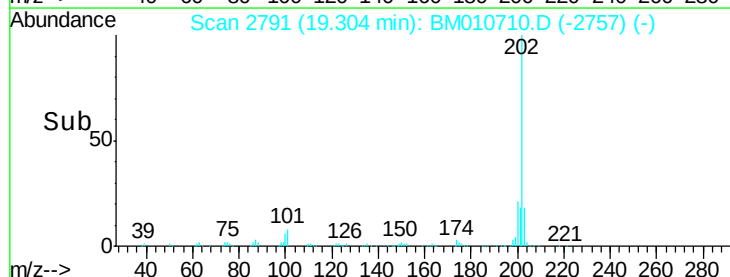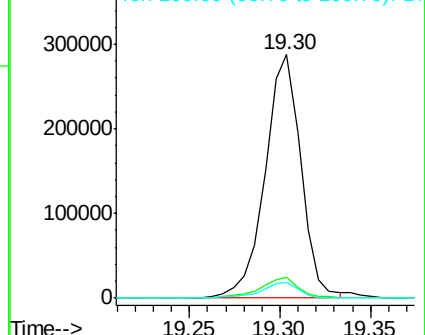



#80

Benzo(a)anthracene

Concen: 3.678 ng/ul

RT: 21.06 min Scan# 3090

Delta R.T. -0.01 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:228 Resp: 124647

Ion Ratio Lower Upper

228 100

229 20.1 15.4 23.0




226 23.5 21.4 32.0



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

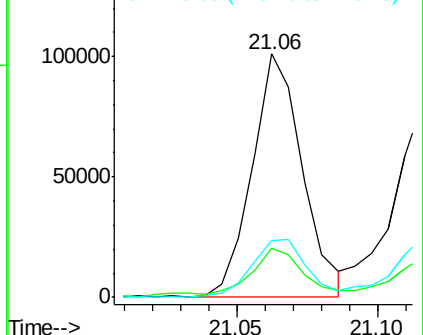

#82

Chrysene

Concen: 3.346 ng/ul

RT: 21.12 min Scan# 3099

Delta R.T. -0.01 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14


Tgt Ion:228 Resp: 101077

Ion Ratio Lower Upper

228 100

226 30.9 23.4 35.2



229 20.6 15.5 23.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

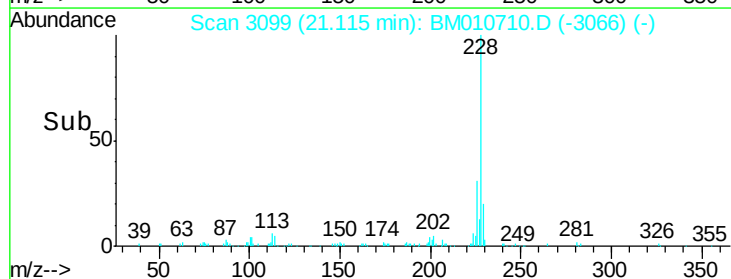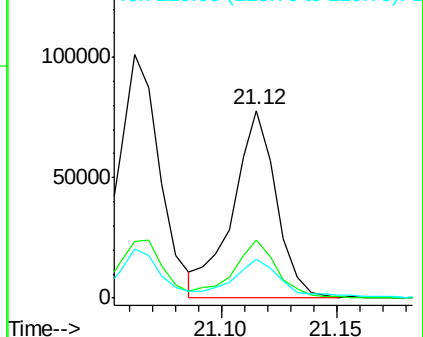

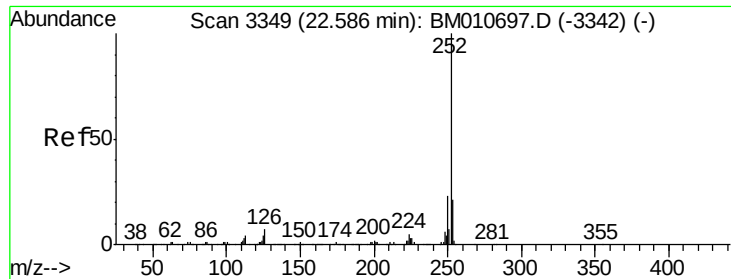

#85

Benzo(b)fluoranthene

Concen: 1.806 ng/ul

RT: 22.59 min Scan# 3350

Delta R.T. 0.01 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME


Tgt Ion:252 Resp: 50115

Ion Ratio Lower Upper

252 100

253 20.1 17.9 26.9

125 9.0 3.6 5.4#

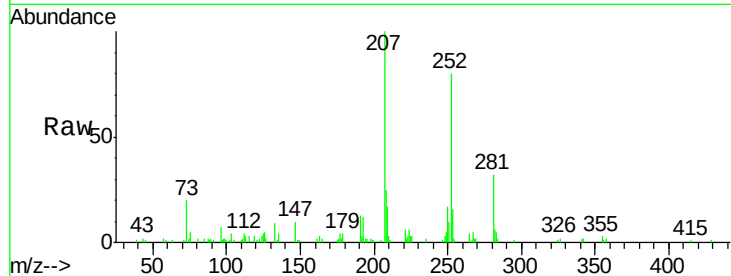


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->

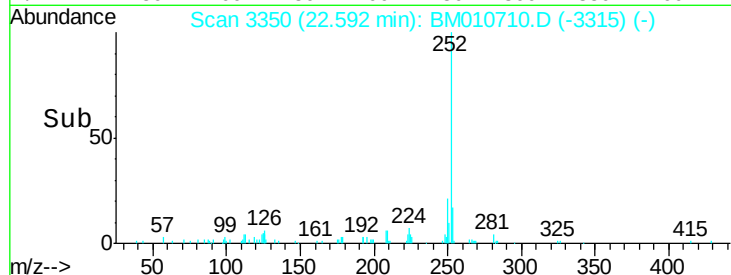


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->



#86

Benzo(k)fluoranthene

Concen: 1.905 ng/ul

RT: 22.59 min Scan# 3350

Delta R.T. -0.04 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14


Tgt Ion:252 Resp: 50115

Ion Ratio Lower Upper

252 100

253 20.1 17.1 25.7

125 9.0 3.4 5.2#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->




Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->

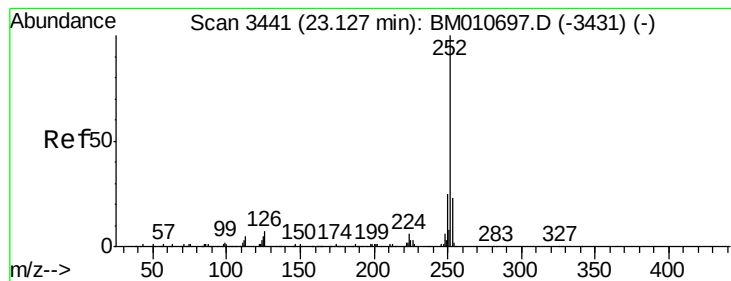

#88

Benzo(a)pyrene

Concen: 1.197 ng/ul

RT: 23.12 min Scan# 3440

Delta R.T. -0.01 min

Lab File: BM010710.D

Acq: 24 Jun 2017 03:14

Instrument :

BNA_M

ClientSampleId :

F5C81ME

Tgt Ion:252 Resp: 30592

Ion Ratio Lower Upper

252 100

253 24.2 18.2 27.2

125 9.9 4.0 6.0#

