

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010715.D
 Acq On : 24 Jun 2017 06:14
 Operator : SJ/JU
 Sample : I3627-17DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5A90DL

Quant Time: Jun 26 01:50:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 01:49:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	77598	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	349546	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	248732	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	617599	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	678266	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	502974	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	690	0.51	ng/uL	0.00
5) Phenol-d5	6.65	99	25884	3.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	14617	3.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	19030	3.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	22053	3.60	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	9758	3.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	11288	3.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	22971	3.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	26450	4.15	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	91073	4.17	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	103794	4.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	10384	2.70	ng/ul	0.00
57) Fluorene-d10	15.11	176	82416	4.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	11562	3.05	ng/ul	0.00
70) Anthracene-d10	16.86	188	617599	20.71	ng/ul	-0.10
76) Pyrene-d10	19.27	212	155036	4.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.08	264	106749	4.39	ng/ul	0.00

Target Compounds


						Qvalue
28) Naphthalene	10.27	128	701237	40.31	ng/ul	100
30) 4-Chloroaniline	10.27	127	94676	14.77	ng/ul#	27
34) 2-Methylnaphthalene	11.89	142	149460	10.69	ng/ul	96
40) 1,1'-Biphenyl	12.93	154	39665	2.04	ng/ul	93
44) Dimethylphthalate	13.58	163	36002	1.68	ng/ul	98
49) Acenaphthene	14.17	153	107101	6.56	ng/ul	96
53) Dibenzofuran	14.52	168	167088	6.76	ng/ul	91
58) Fluorene	15.17	166	113427	5.48	ng/ul	98
69) Phenanthrene	16.91	178	769836	23.45	ng/ul	98
71) Anthracene	17.00	178	94925	2.81	ng/ul	99
74) Fluoranthene	18.94	202	422658	9.99	ng/ul	99
77) Pyrene	19.30	202	244875	6.25	ng/ul	98
80) Benzo(a)anthracene	21.06	228	83183	2.11	ng/ul	98
82) Chrysene	21.12	228	65679	1.87	ng/ul	98
85) Benzo(b)fluoranthene	22.59	252	35389	1.08	ng/ul	94
86) Benzo(k)fluoranthene	22.59	252	35389	1.14	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010715.D
Acq On : 24 Jun 2017 06:14
Operator : SJ/JU
Sample : I3627-17DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5A90DL

Quant Time: Jun 26 01:50:16 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 26 01:49:13 2017
Response via : Initial Calibration




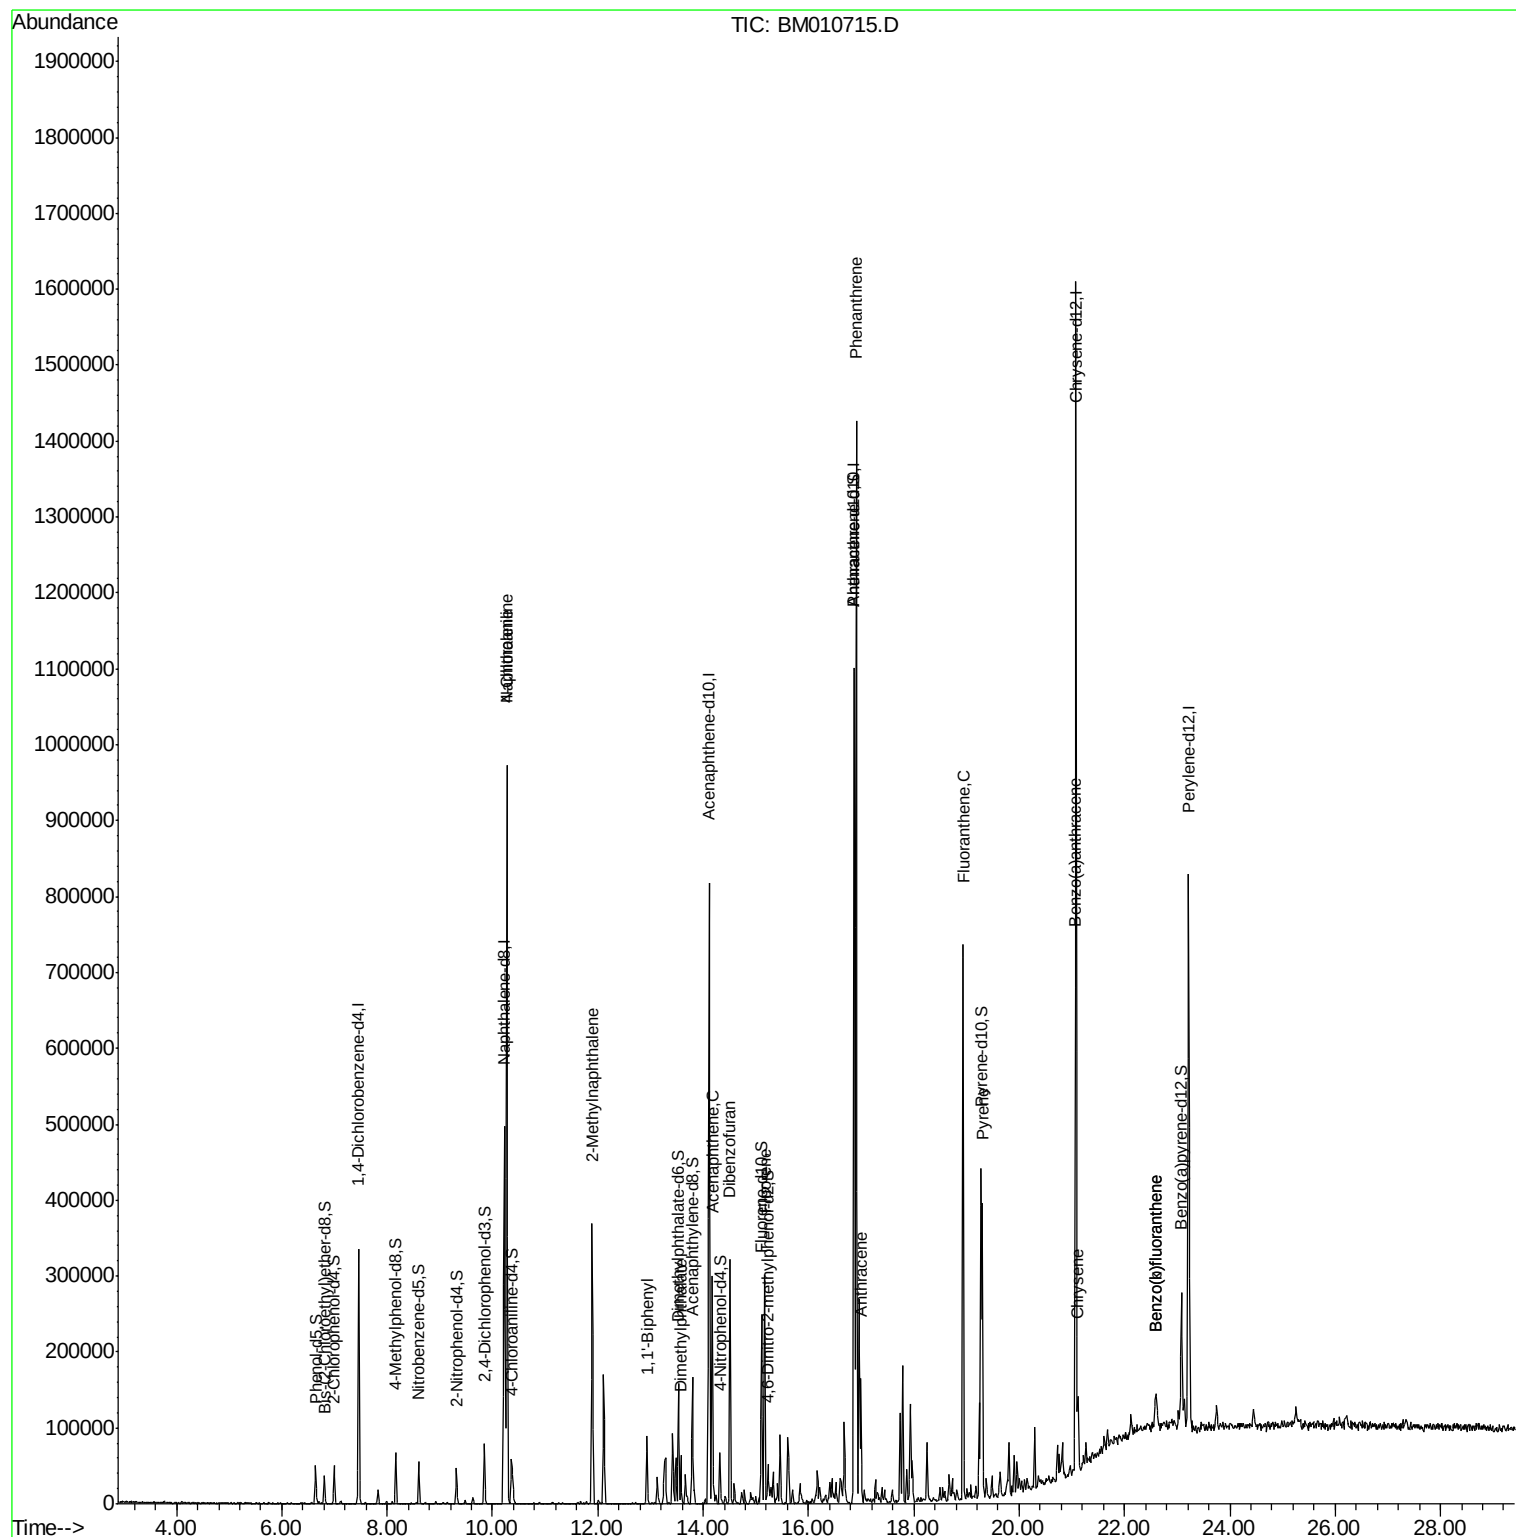


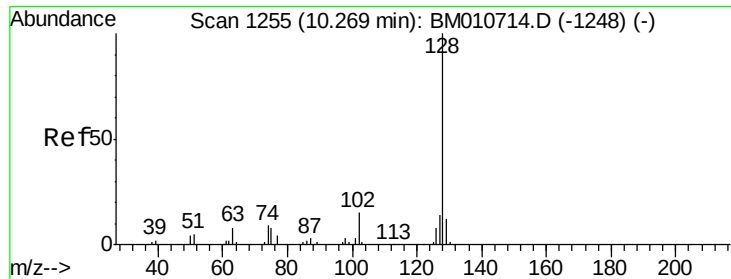

#28
Naphthalene
Concen: 40.31 ng/ul
RT: 10.27 min Scan# 1255
Delta R.T. 0.00 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14




Instrument :
BNA_M
ClientSampleId :
F5A90DL


Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.8	8.8	13.2
127	13.2	10.6	16.0

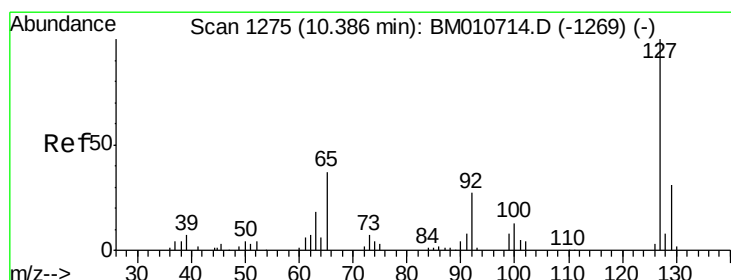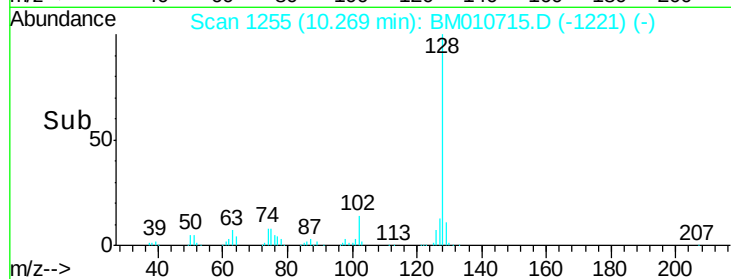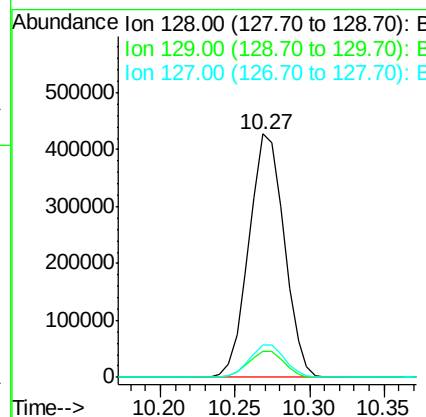

#30
4-Chloroaniline
Concen: 14.77 ng/ul
RT: 10.27 min Scan# 1256
Delta R.T. -0.11 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14

Tgt Ion	Ratio	Lower	Upper
127	100		
129	78.4	28.4	42.6

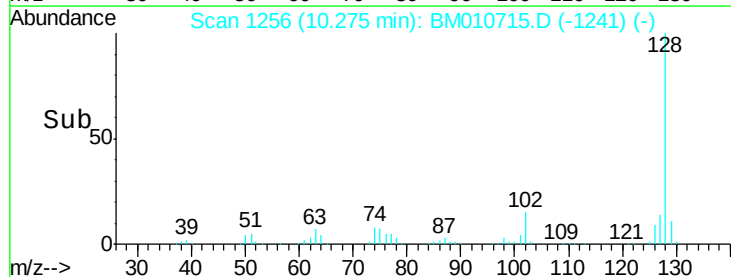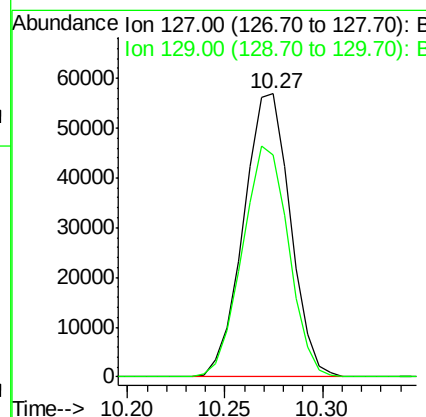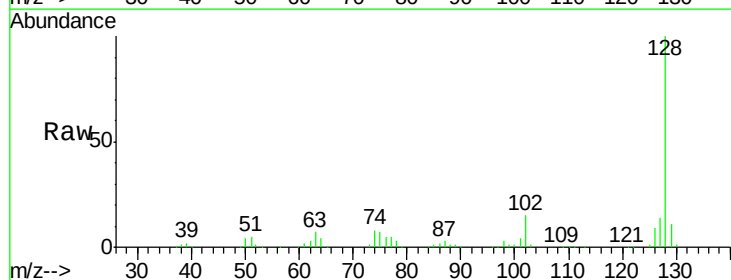

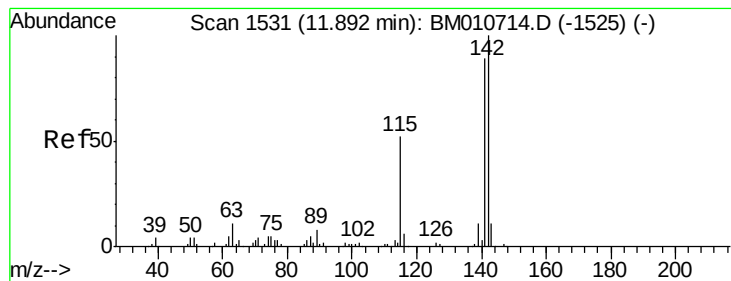

#34

2-Methylnaphthalene

Concen: 10.69 ng/ul

RT: 11.89 min Scan# 1531

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14

Instrument :

BNA_M

ClientSampled :


F5A90DL

Tgt Ion:142 Resp: 149460

Ion Ratio Lower Upper

142 100


141 88.4 74.1 111.1




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

11.89

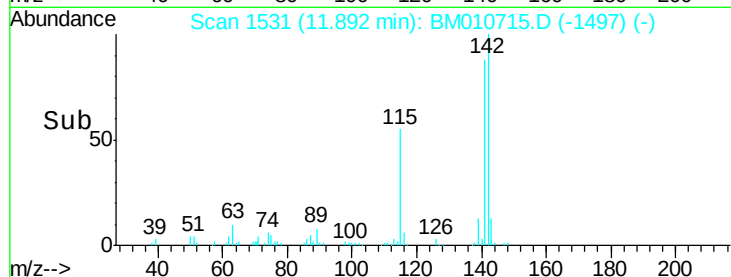

Time-->

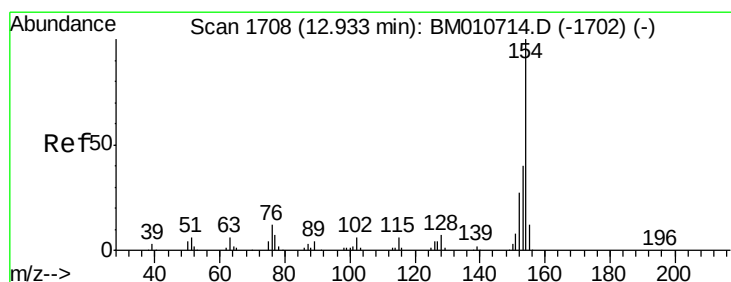

#40

1,1'-Biphenyl

Concen: 2.04 ng/ul

RT: 12.93 min Scan# 1708

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14


Tgt Ion:154 Resp: 39665

Ion Ratio Lower Upper

154 100

153 35.3 32.6 48.8

76 10.7 8.5 12.7

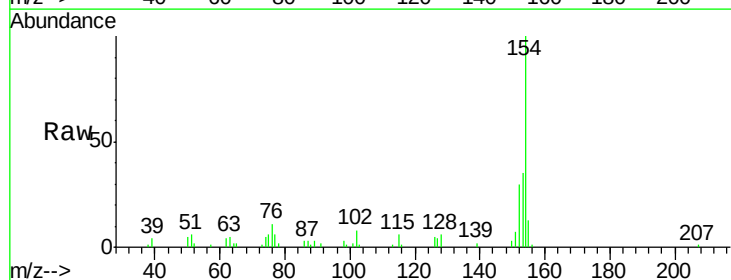


Abundance Ion 154.00 (153.70 to 154.70): E


Ion 153.00 (152.70 to 153.70): E

Ion 76.00 (75.70 to 76.70): BM

12.93

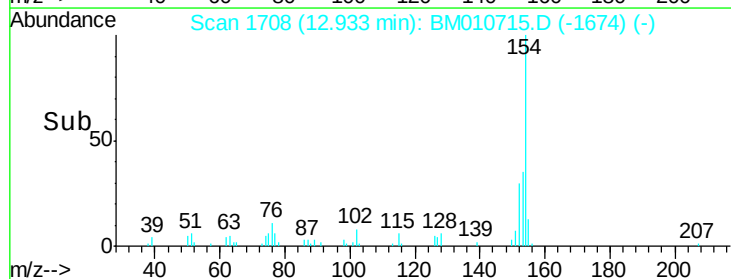





Time-->

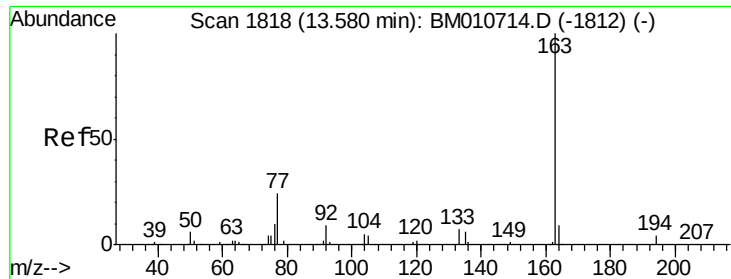

#44
Dimethylphthalate
Concen: 1.68 ng/ul
RT: 13.58 min Scan# 1818
Delta R.T. 0.00 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14




Instrument :
BNA_M
ClientSampleId :
F5A90DL


Tgt Ion:163 Resp: 36002
Ion Ratio Lower Upper
163 100
194 5.3 3.5 5.3
164 10.9 8.2 12.4

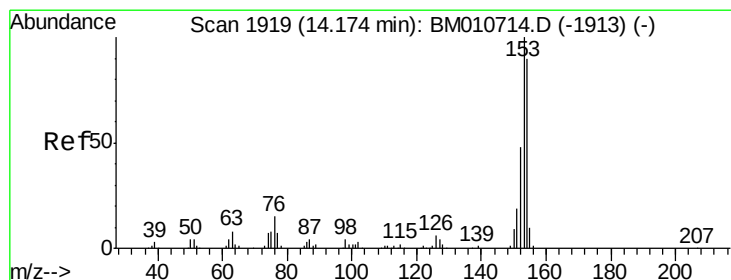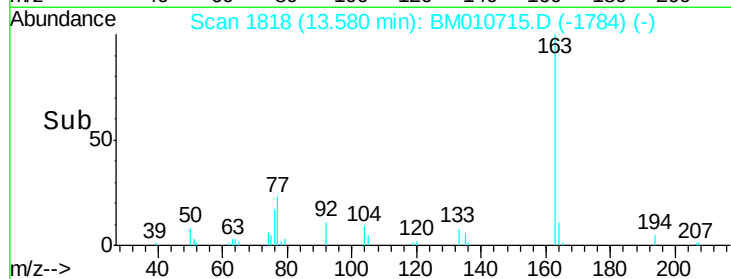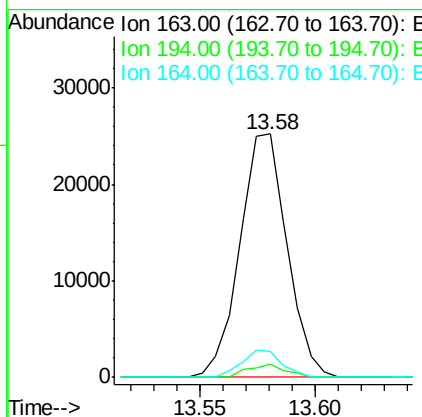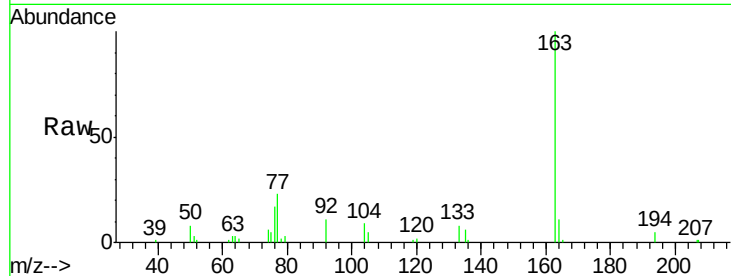

#49
Acenaphthene
Concen: 6.56 ng/ul
RT: 14.17 min Scan# 1919
Delta R.T. 0.00 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14

Tgt Ion:153 Resp: 107101
Ion Ratio Lower Upper
153 100
152 46.6 37.6 56.4
154 93.9 70.4 105.6

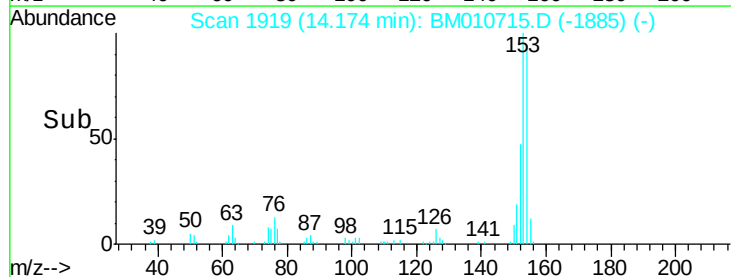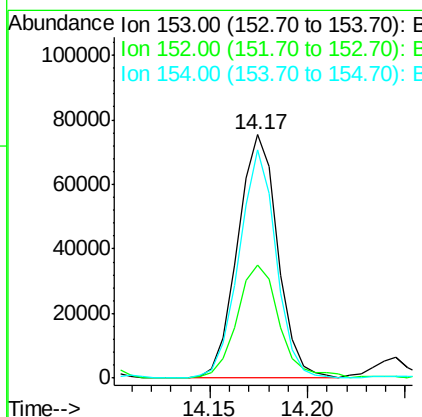

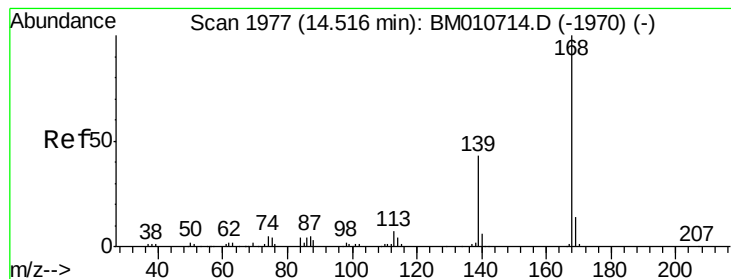

#53

Dibenzenofuran

Concen: 6.76 ng/ul

RT: 14.52 min Scan# 1977

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14

Instrument :

BNA_M

ClientSampleId :


F5A90DL

Tgt Ion:168 Resp: 167088

Ion Ratio Lower Upper

168 100

139 43.7 30.8 46.2



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E



14.52

100000

50000

0

Time--> 14.45 14.50 14.55

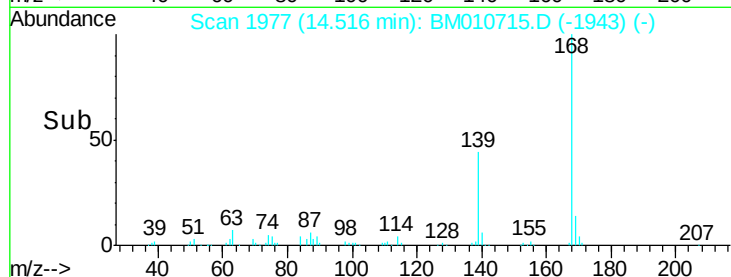

#58

Fluorene

Concen: 5.48 ng/ul

RT: 15.17 min Scan# 2088

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14


Tgt Ion:166 Resp: 113427

Ion Ratio Lower Upper

166 100

165 95.8 77.9 116.9

167 15.1 10.6 16.0



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.17

100000

80000


60000


40000

20000

0

Time--> 15.10 15.15 15.20

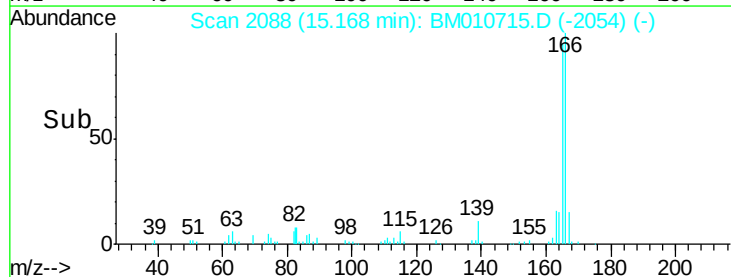

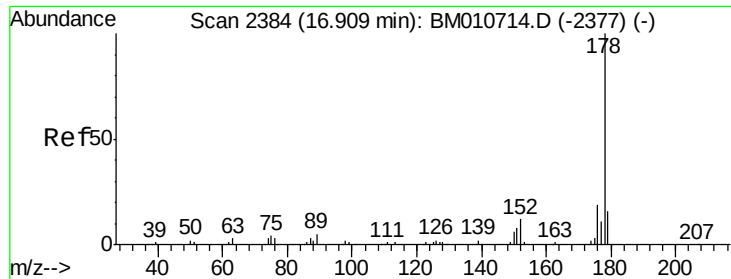

#69

Phenanthrene

Concen: 23.45 ng/ul

RT: 16.91 min Scan# 2384

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14

Instrument :

BNA_M

ClientSampleId :

F5A90DL


Tgt Ion:178 Resp: 769836

Ion Ratio Lower Upper

178 100

179 15.5 12.6 19.0




176 19.7 14.9 22.3



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

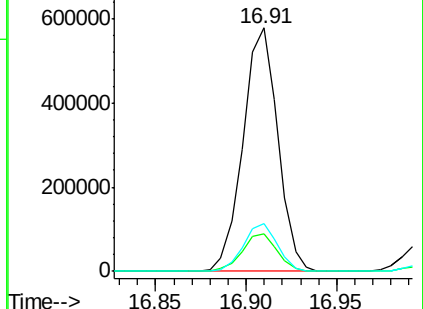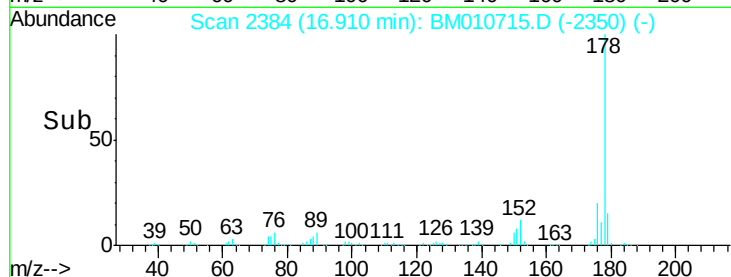

#71

Anthracene

Concen: 2.81 ng/ul

RT: 17.00 min Scan# 2399

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14


Tgt Ion:178 Resp: 94925

Ion Ratio Lower Upper

178 100

179 14.7 11.7 17.5



176 18.7 14.6 21.8




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

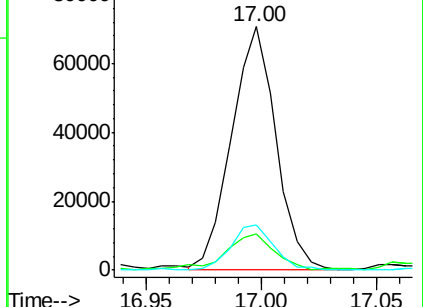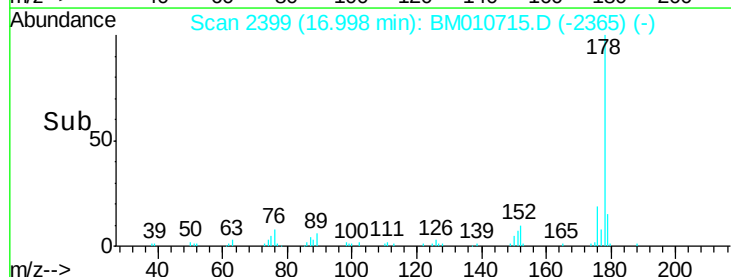

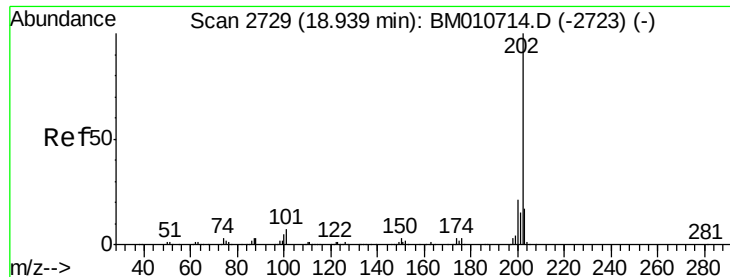

#74

Fluoranthene

Concen: 9.99 ng/ul

RT: 18.94 min Scan# 2729

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14

Instrument :

BNA_M

ClientSampleId :

F5A90DL


Tgt Ion:202 Resp: 422658

Ion Ratio Lower Upper

202 100

101 5.7 4.6 7.0




100 4.7 3.4 5.2

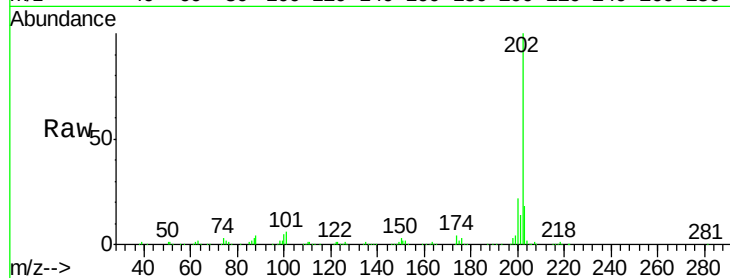

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

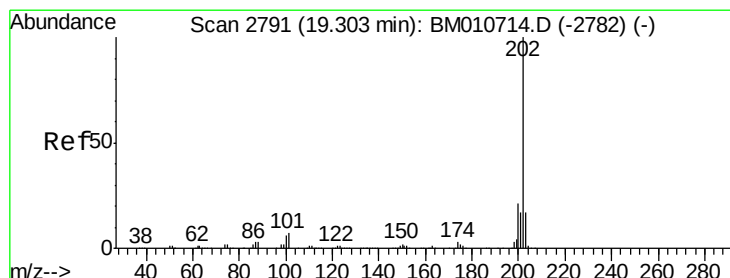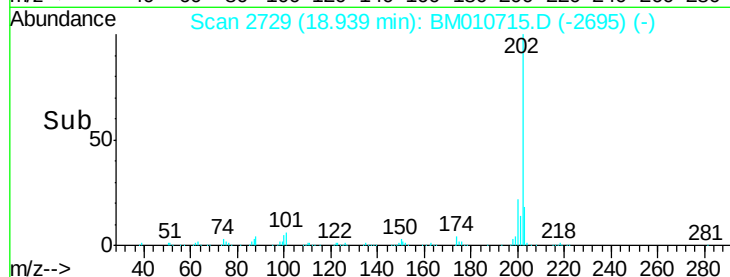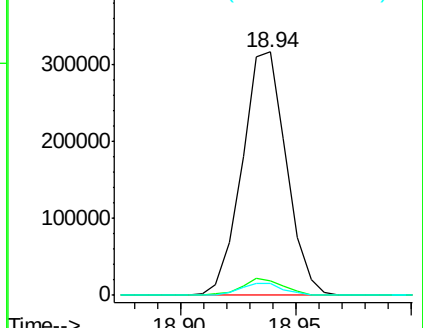

#77

Pyrene

Concen: 6.25 ng/ul

RT: 19.30 min Scan# 2791

Delta R.T. 0.00 min

Lab File: BM010715.D

Acq: 24 Jun 2017 06:14


Tgt Ion:202 Resp: 244875

Ion Ratio Lower Upper

202 100

101 7.4 5.1 7.7



100 5.6 4.9 7.3

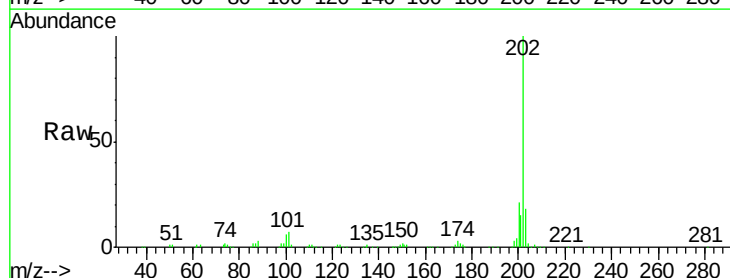


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



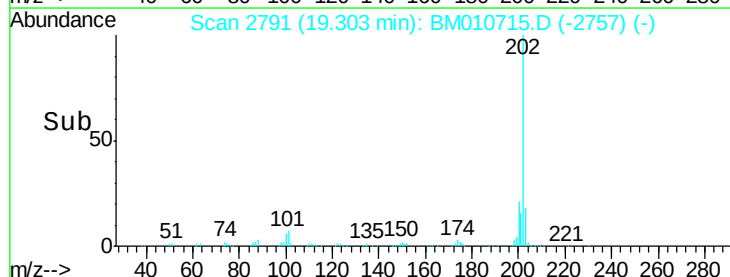
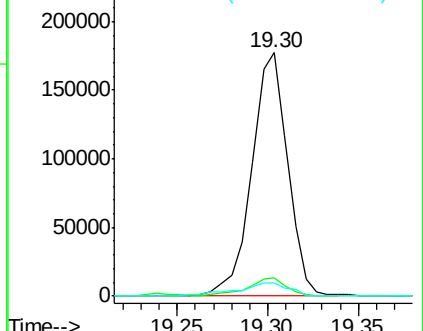


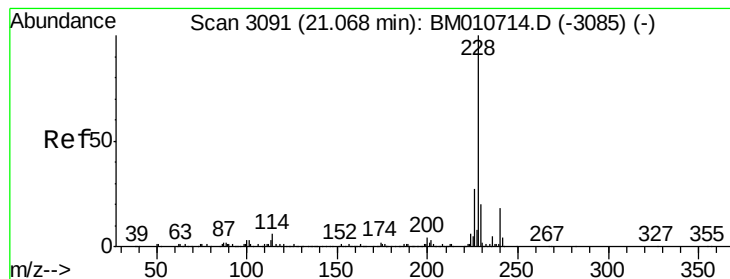

#80
Benzo(a)anthracene
Concen: 2.11 ng/ul
RT: 21.06 min Scan# 3090
Delta R.T. -0.01 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14




Instrument :
BNA_M
ClientSampleId :
F5A90DL


Tgt Ion:228 Resp: 83183
Ion Ratio Lower Upper
228 100
229 18.4 15.4 23.0
226 25.8 21.4 32.0

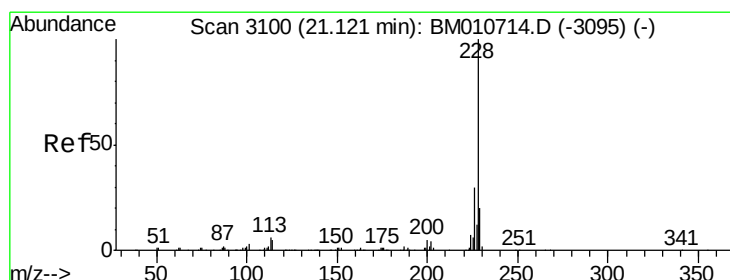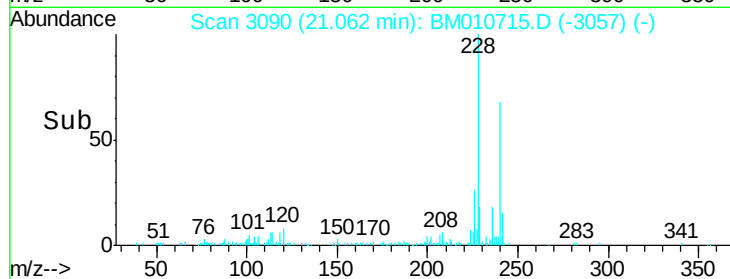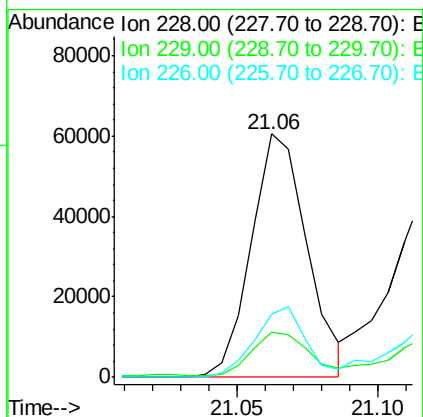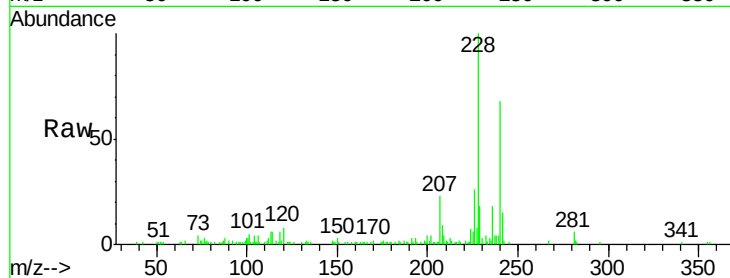

#82
Chrysene
Concen: 1.87 ng/ul
RT: 21.12 min Scan# 3099
Delta R.T. -0.01 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14

Tgt Ion:228 Resp: 65679
Ion Ratio Lower Upper
228 100
226 28.4 23.4 35.2
229 21.0 15.5 23.3


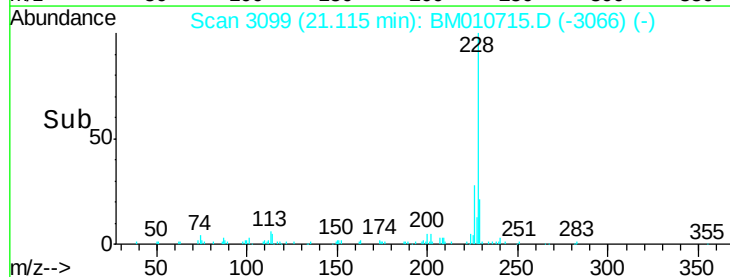
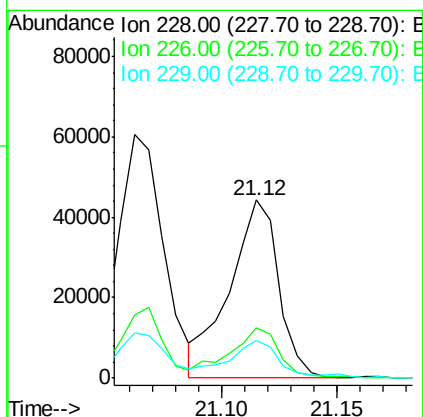
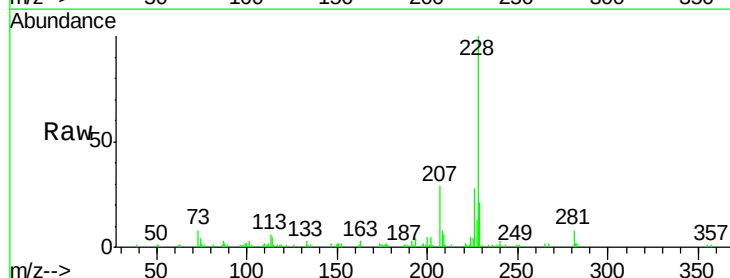


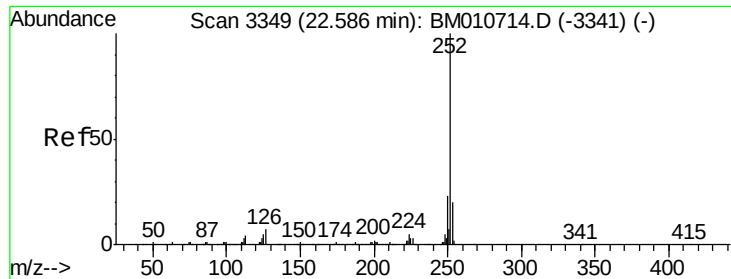

#85
Benzo(b)fluoranthene
Concen: 1.08 ng/ul
RT: 22.59 min Scan# 3349
Delta R.T. 0.00 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14

Instrument :
BNA_M
ClientSampleId :
F5A90DL

Tgt Ion:252 Resp: 35389
Ion Ratio Lower Upper
252 100
253 25.6 17.9 26.9
125 4.5 3.6 5.4

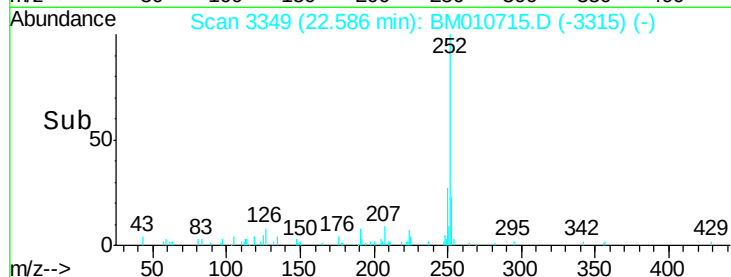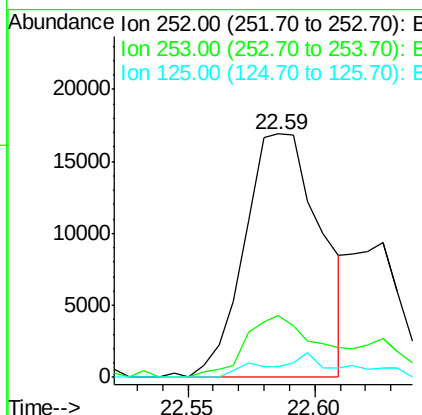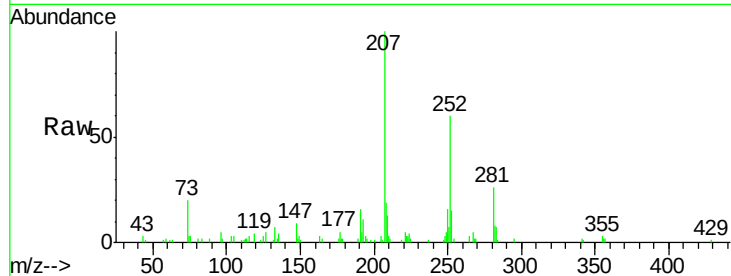

#86
Benzo(k)fluoranthene
Concen: 1.14 ng/ul
RT: 22.59 min Scan# 3349
Delta R.T. -0.04 min
Lab File: BM010715.D
Acq: 24 Jun 2017 06:14

Tgt Ion:252 Resp: 35389
Ion Ratio Lower Upper
252 100
253 25.6 17.1 25.7
125 4.5 3.4 5.2

